

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
 Data File : PD065059.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2021 19:48
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 03:31:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	20572407	162.6E6	20.014	20.529
28)	SA Decachlor...	8.240	9.083	21365691	90036215	18.857	19.025
Target Compounds							
9)	A Endosulfan I	5.546	6.251	10934411	72002938	10.251	10.224
10)	B gamma-Chl...	5.432	6.127	11575332	76077861	10.238	9.950
12)	B 4,4'-DDE	5.653	6.357	20094306	140.9E6	19.066	19.625
13)	MA Dieldrin	5.789	6.509	21929996	145.1E6	19.541	20.002
19)	B Endosulfa...	6.699	7.288	20513927	110.4E6	19.318	19.252
20)	A Methoxychlor	6.955	7.607	50571526	262.9E6	85.798	86.883
21)	B Endrin ke...	7.193	7.761	24412447	126.3E6	19.149	19.441



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
Data File : PD065059.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2021 19:48
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 03:31:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

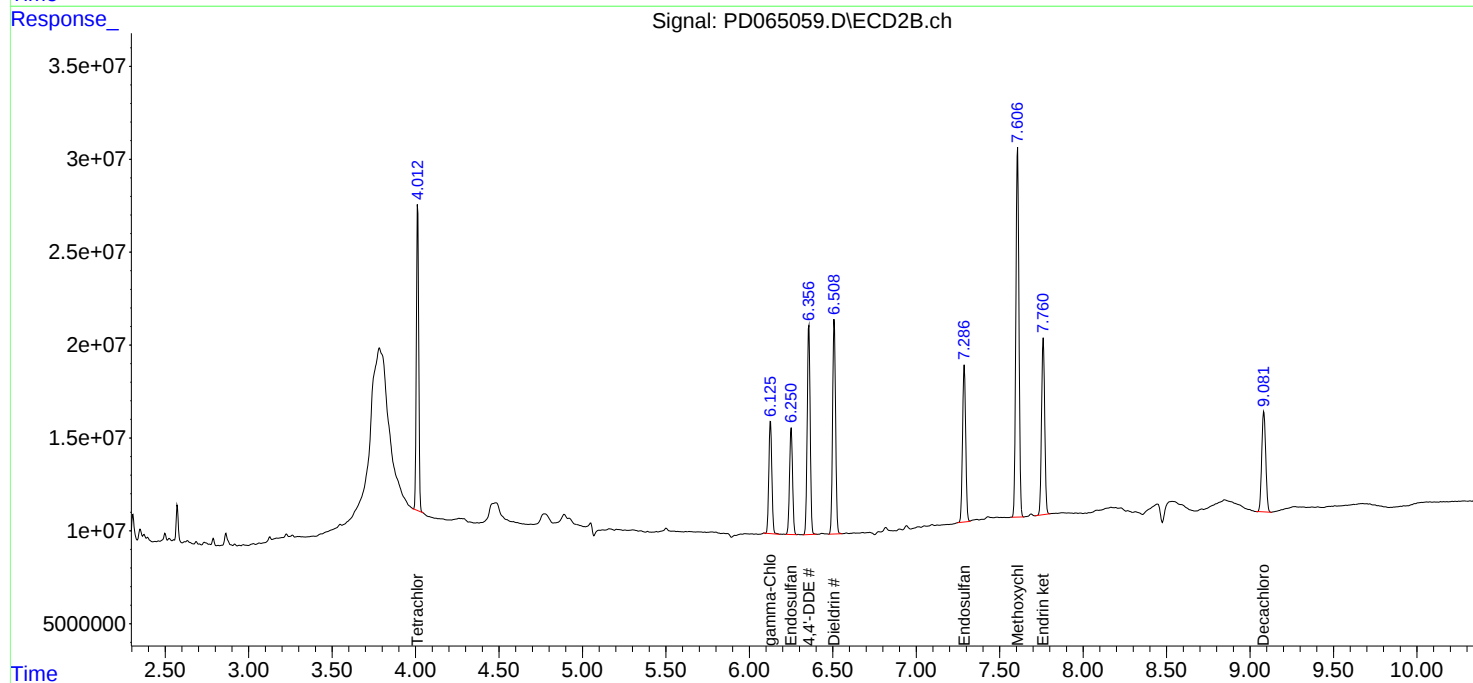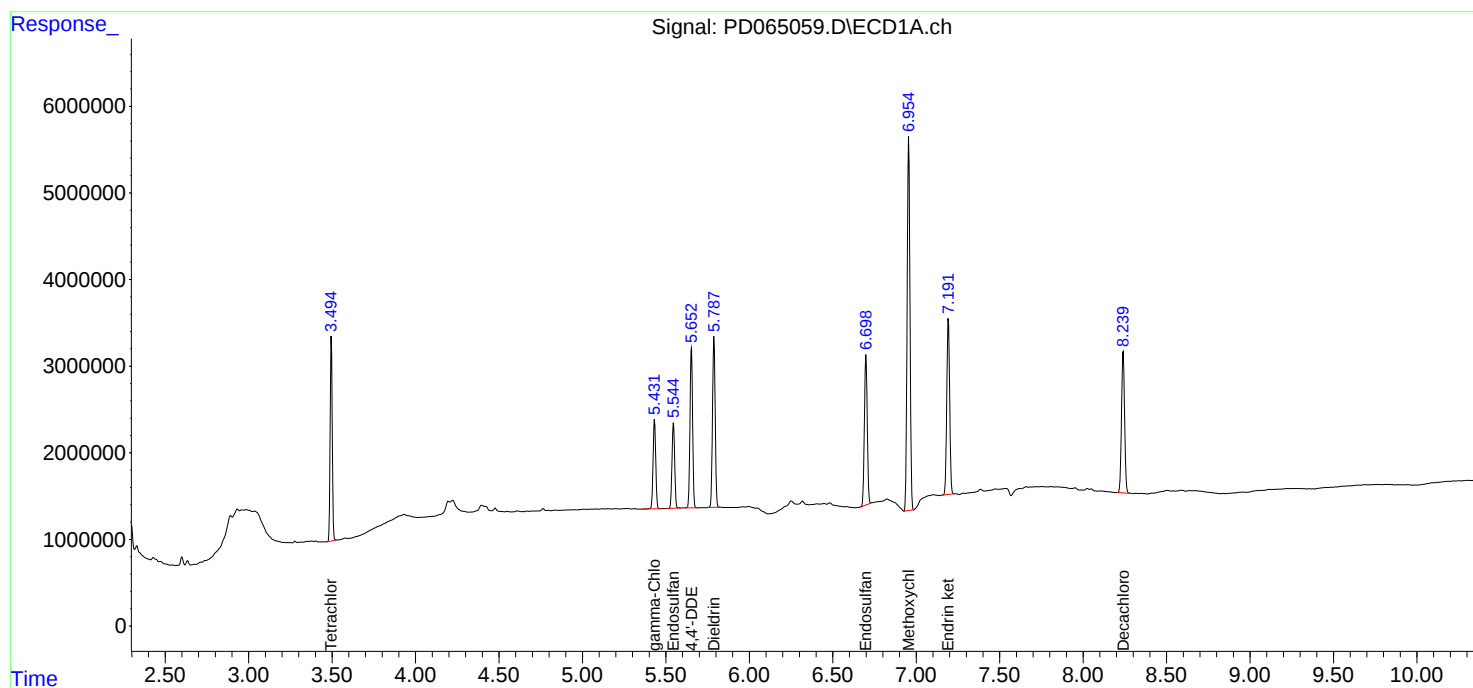


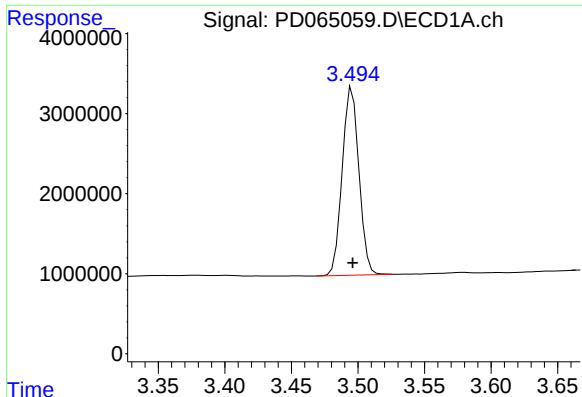

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 20572407
Conc: 20.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

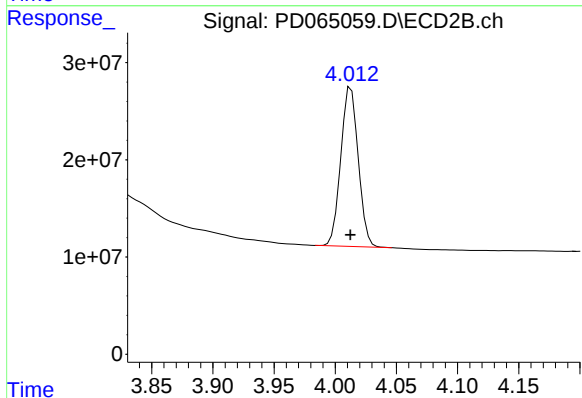


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 162602227
Conc: 20.53 ng/ml

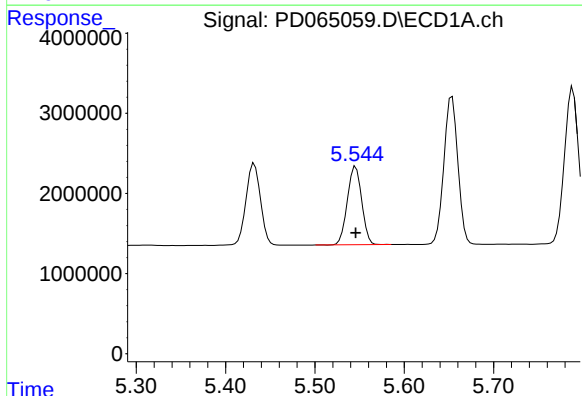


#9 Endosulfan I

R.T.: 5.546 min
Delta R.T.: 0.000 min
Response: 10934411
Conc: 10.25 ng/ml

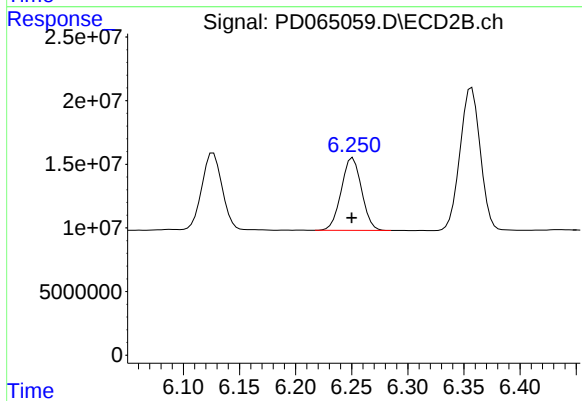

#9 Endosulfan I


R.T.: 6.251 min
Delta R.T.: 0.000 min
Response: 72002938
Conc: 10.22 ng/ml

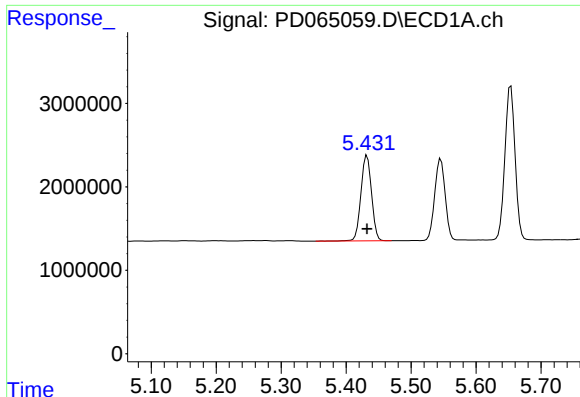

#10 gamma-Chlordane


R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 11575332
Conc: 10.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

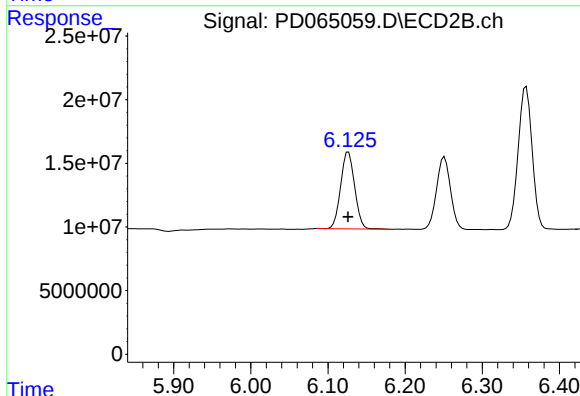


#10 gamma-Chlordane

R.T.: 6.127 min
Delta R.T.: 0.000 min
Response: 76077861
Conc: 9.95 ng/ml

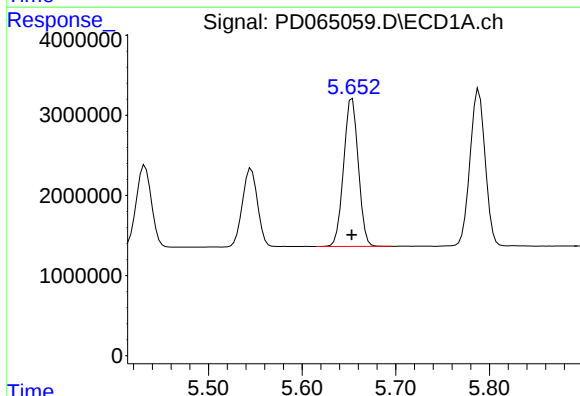


#12 4,4'-DDE

R.T.: 5.653 min
Delta R.T.: 0.000 min
Response: 20094306
Conc: 19.07 ng/ml

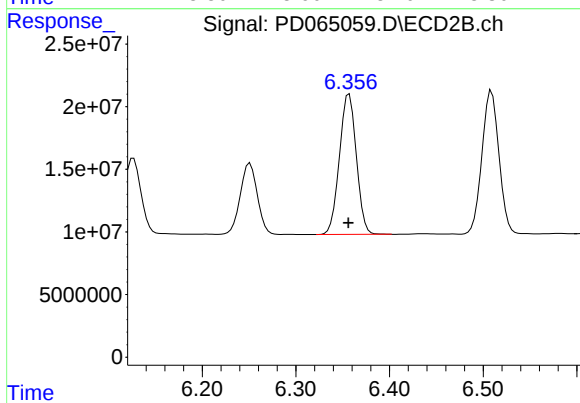

#12 4,4'-DDE


R.T.: 6.357 min
Delta R.T.: 0.000 min
Response: 140919870
Conc: 19.62 ng/ml

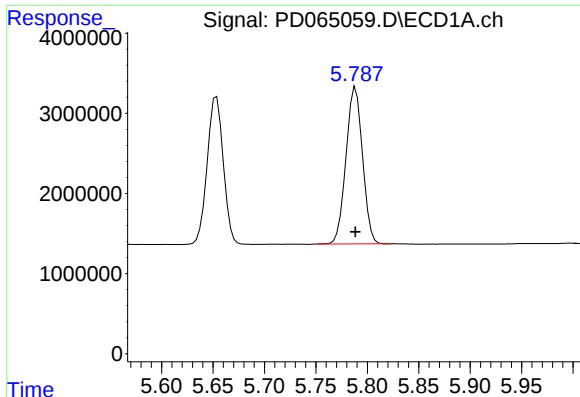

#13 Dieldrin


R.T.: 5.789 min
Delta R.T.: 0.000 min
Response: 21929996
Conc: 19.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

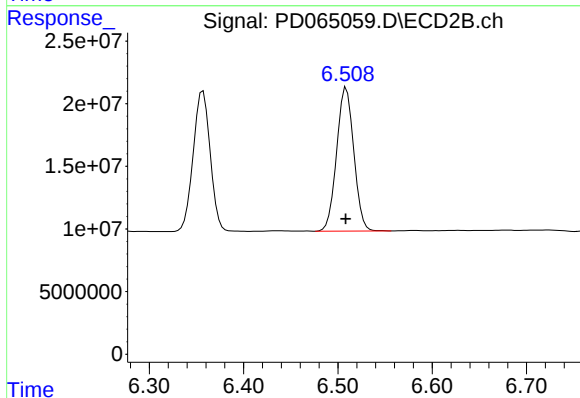


#13 Dieldrin

R.T.: 6.509 min
Delta R.T.: 0.000 min
Response: 145136094
Conc: 20.00 ng/ml

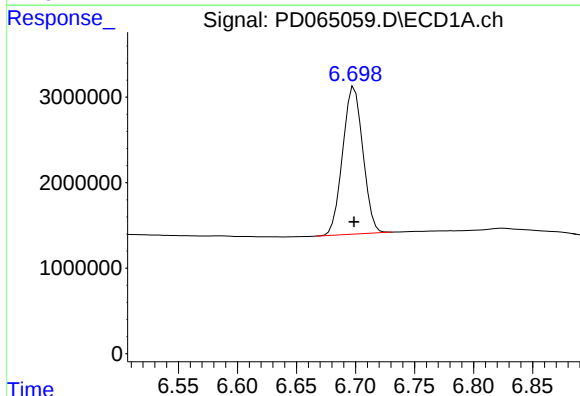


#19 Endosulfan Sulfate

R.T.: 6.699 min
Delta R.T.: 0.000 min
Response: 20513927
Conc: 19.32 ng/ml

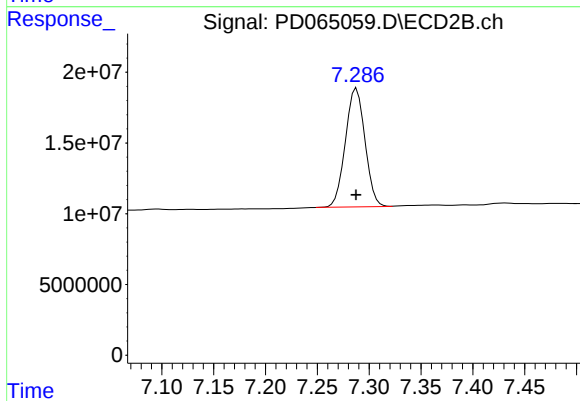

#19 Endosulfan Sulfate


R.T.: 7.288 min
Delta R.T.: 0.000 min
Response: 110404168
Conc: 19.25 ng/ml

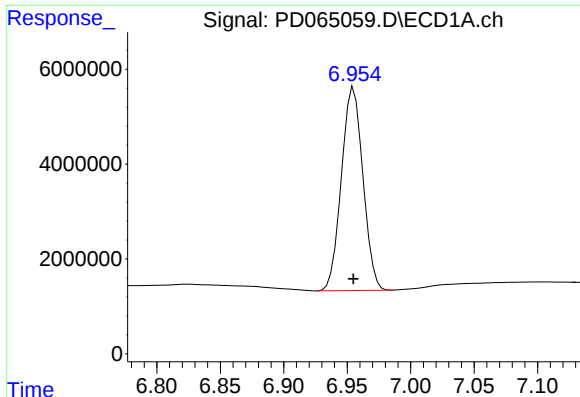

#20 Methoxychlor


R.T.: 6.955 min
Delta R.T.: 0.000 min
Response: 50571526
Conc: 85.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

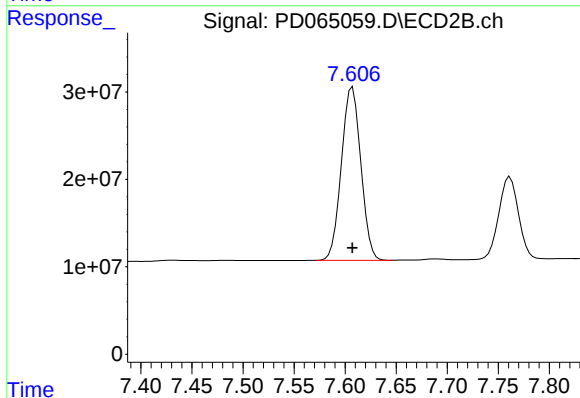


#20 Methoxychlor

R.T.: 7.607 min
Delta R.T.: 0.000 min
Response: 262917816
Conc: 86.88 ng/ml

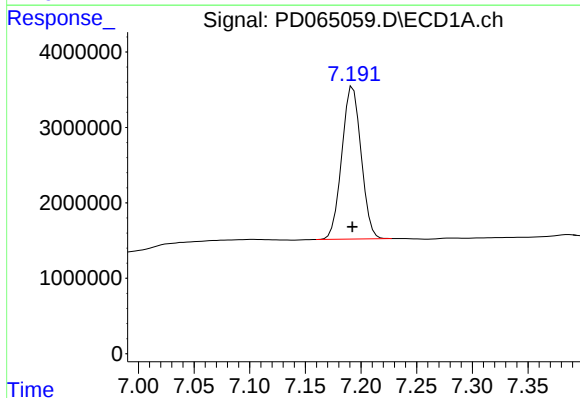


#21 Endrin ketone

R.T.: 7.193 min
Delta R.T.: 0.000 min
Response: 24412447
Conc: 19.15 ng/ml

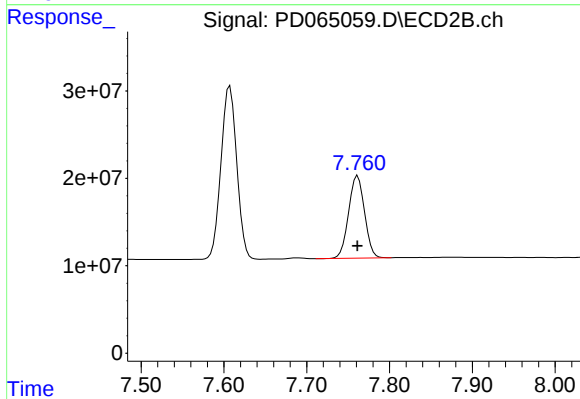

#21 Endrin ketone


R.T.: 7.761 min
Delta R.T.: 0.000 min
Response: 126344171
Conc: 19.44 ng/ml

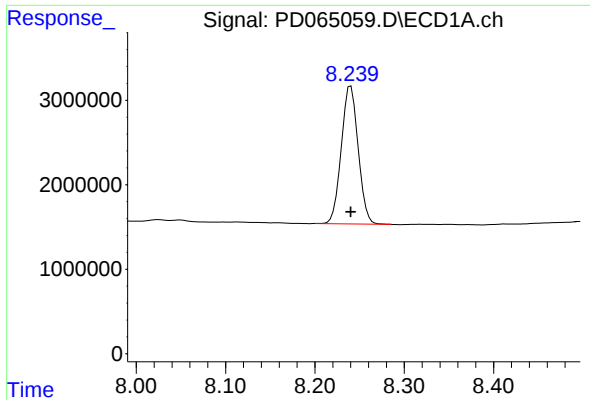

#28 Decachlorobiphenyl

R.T.: 8.240 min
Delta R.T.: 0.000 min
Response: 21365691
Conc: 18.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

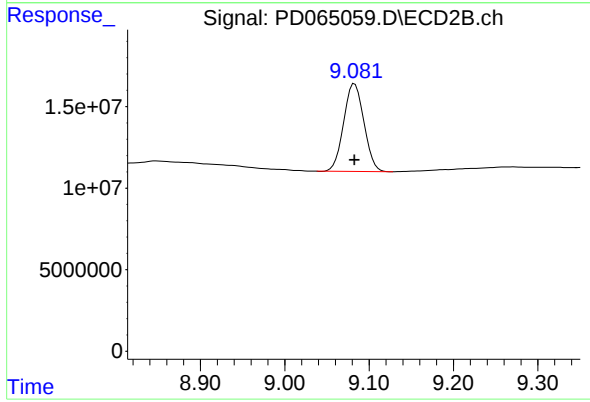

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: 0.000 min
Response: 90036215
Conc: 19.02 ng/ml