

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
 Data File : PD065065.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2021 21:11
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:41:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 01:41:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.495	4.013	116.1E6	742.8E6	96.712	94.056
28)	SA Decachlor...	8.241	9.084	106.0E6	440.9E6	93.907	92.815
Target Compounds							
23)	Chlordane-1	4.366	5.009	33790722	291.0E6	929.294	928.096
24)	Chlordane-2	4.866	5.478	38379006	268.4E6	909.564	910.627
25)	Chlordane-3	5.432	6.126	101.7E6	938.5E6	964.998	952.328
26)	Chlordane-4	5.491	6.199	83623207	1083.9E6	951.093	948.364
27)	Chlordane-5	6.328	7.009	41237206	222.2E6	957.307	954.551



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
Data File : PD065065.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2021 21:11
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:41:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 01:41:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

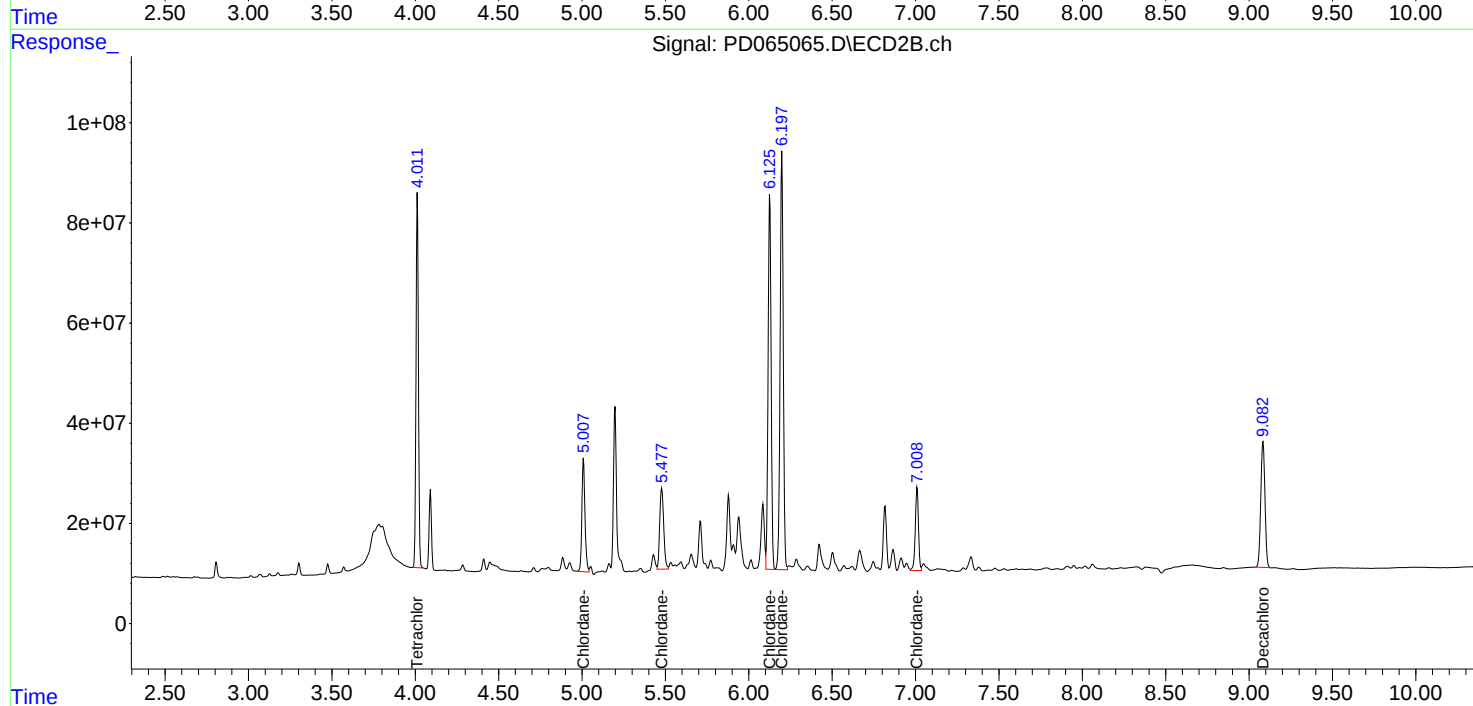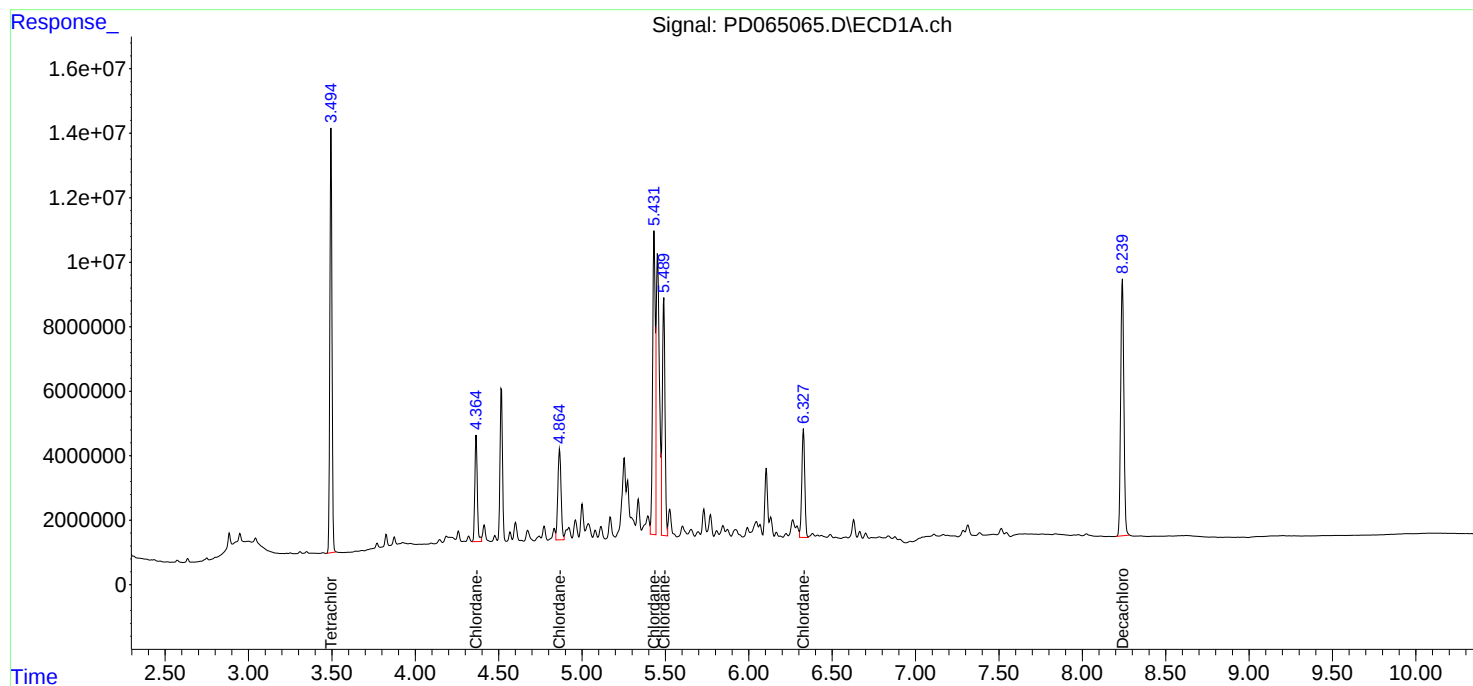


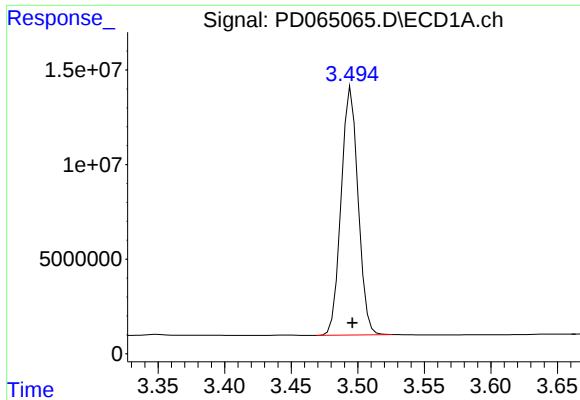

#1 Tetrachloro-m-xylene


R.T.: 3.495 min
Delta R.T.: 0.000 min
Response: 116092334
Conc: 96.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

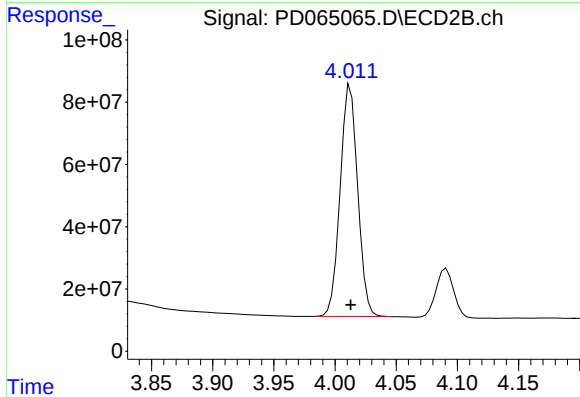


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 742781299
Conc: 94.06 ng/ml

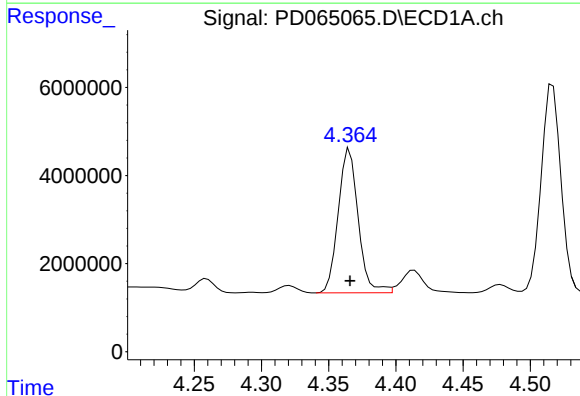


#23 Chlordane-1

R.T.: 4.366 min
Delta R.T.: 0.000 min
Response: 33790722
Conc: 929.29 ng/ml

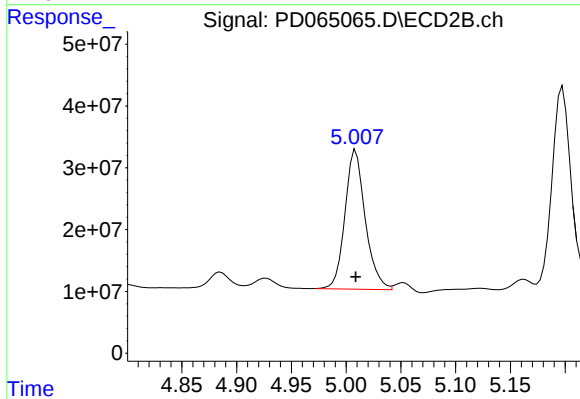

#23 Chlordane-1


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 291004070
Conc: 928.10 ng/ml

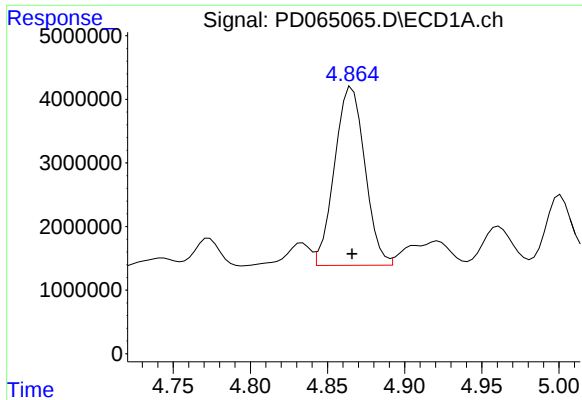

#24 Chlordane-2


R.T.: 4.866 min
Delta R.T.: 0.000 min
Response: 38379006
Conc: 909.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

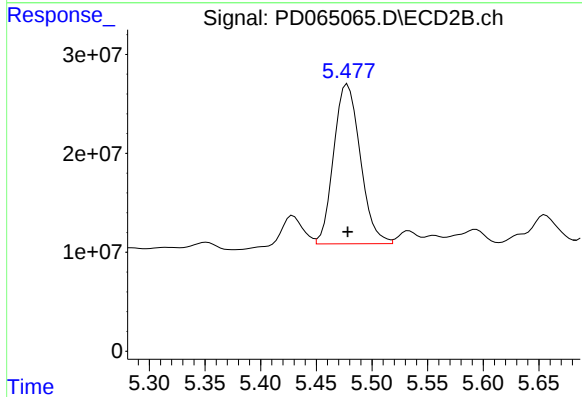


#24 Chlordane-2

R.T.: 5.478 min
Delta R.T.: 0.000 min
Response: 268425885
Conc: 910.63 ng/ml

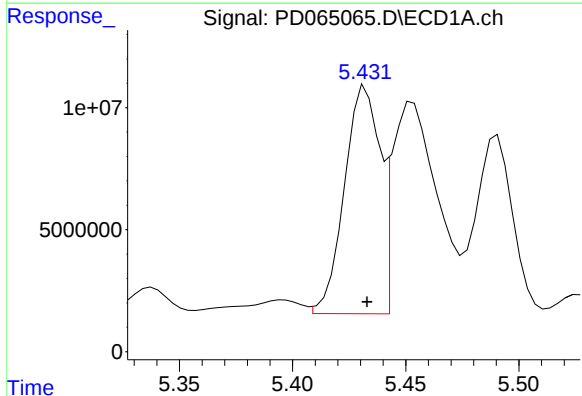


#25 Chlordane-3

R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 101657434
Conc: 965.00 ng/ml

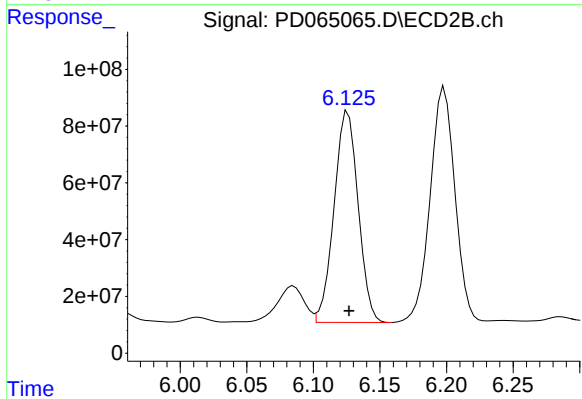

#25 Chlordane-3


R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 938539766
Conc: 952.33 ng/ml

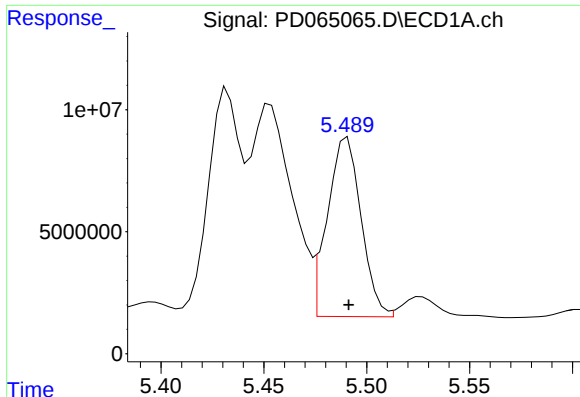

#26 Chlordane-4


R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 83623207
Conc: 951.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

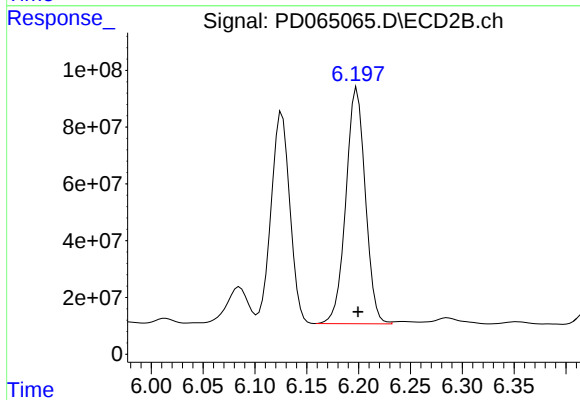


#26 Chlordane-4

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 1083889581
Conc: 948.36 ng/ml

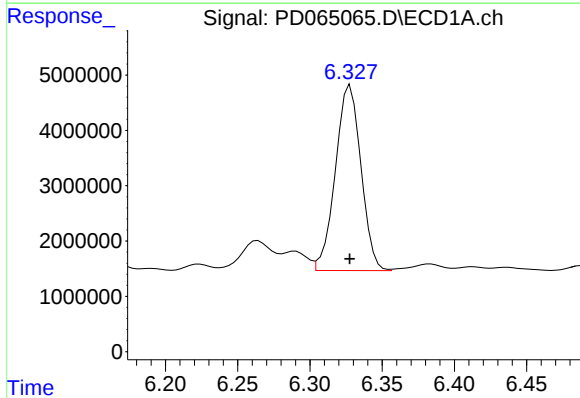


#27 Chlordane-5

R.T.: 6.328 min
Delta R.T.: 0.000 min
Response: 41237206
Conc: 957.31 ng/ml

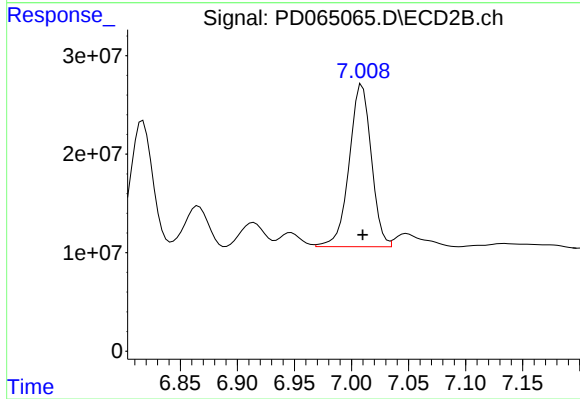

#27 Chlordane-5


R.T.: 7.009 min
Delta R.T.: 0.000 min
Response: 222176505
Conc: 954.55 ng/ml

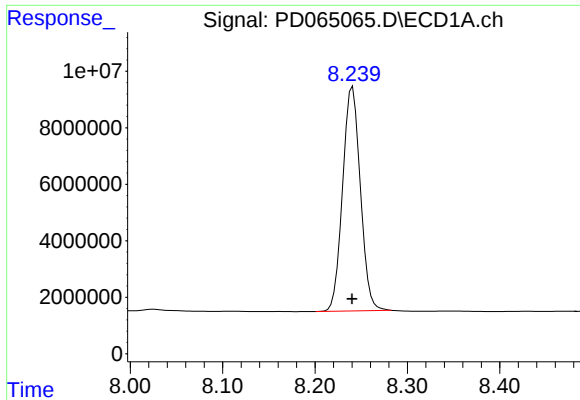

#28 Decachlorobiphenyl

R.T.: 8.241 min
Delta R.T.: 0.000 min
Response: 105990211
Conc: 93.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

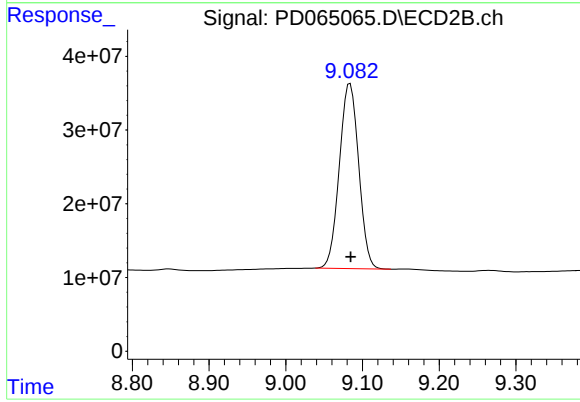

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 440876219
Conc: 92.81 ng/ml