

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
 Data File : PD065069.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2021 22:06
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:59:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 01:58:35 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	7567029	49841566	6.013	6.037
28)	SA Decachlor...	8.241	9.083	7704657	31312281	6.408	6.243
Target Compounds							
23)	Chlordane-1	4.366	5.009	2324854	16826331	61.387	54.327
24)	Chlordane-2	4.866	5.479	2564952	20535593	58.769	63.396
25)	Chlordane-3	5.432	6.126	6632507	62551115	60.093	60.503
26)	Chlordane-4	5.491	6.199	5493594	73228079	59.841	60.906
27)	Chlordane-5	6.328	7.010	2658681	13266349	58.902	55.951



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082021\
Data File : PD065069.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2021 22:06
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:59:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 01:58:35 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

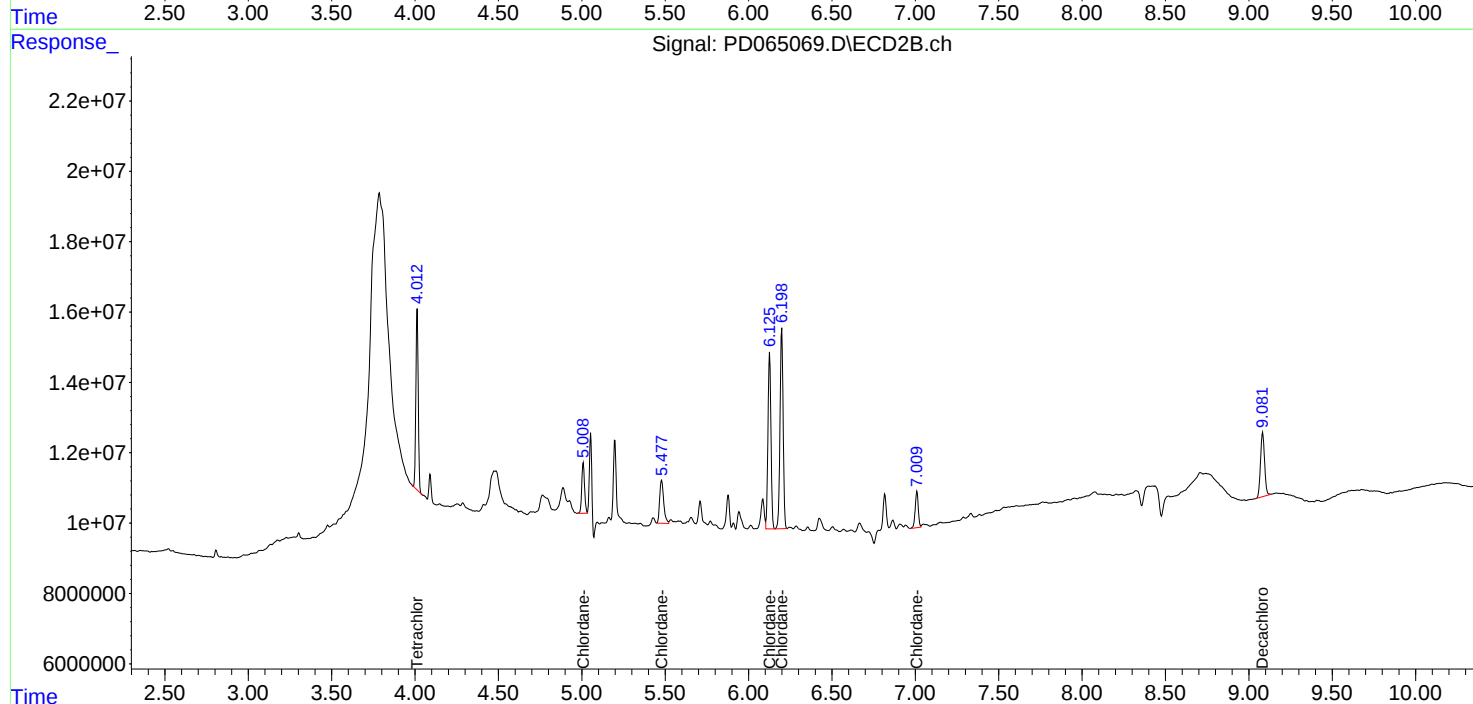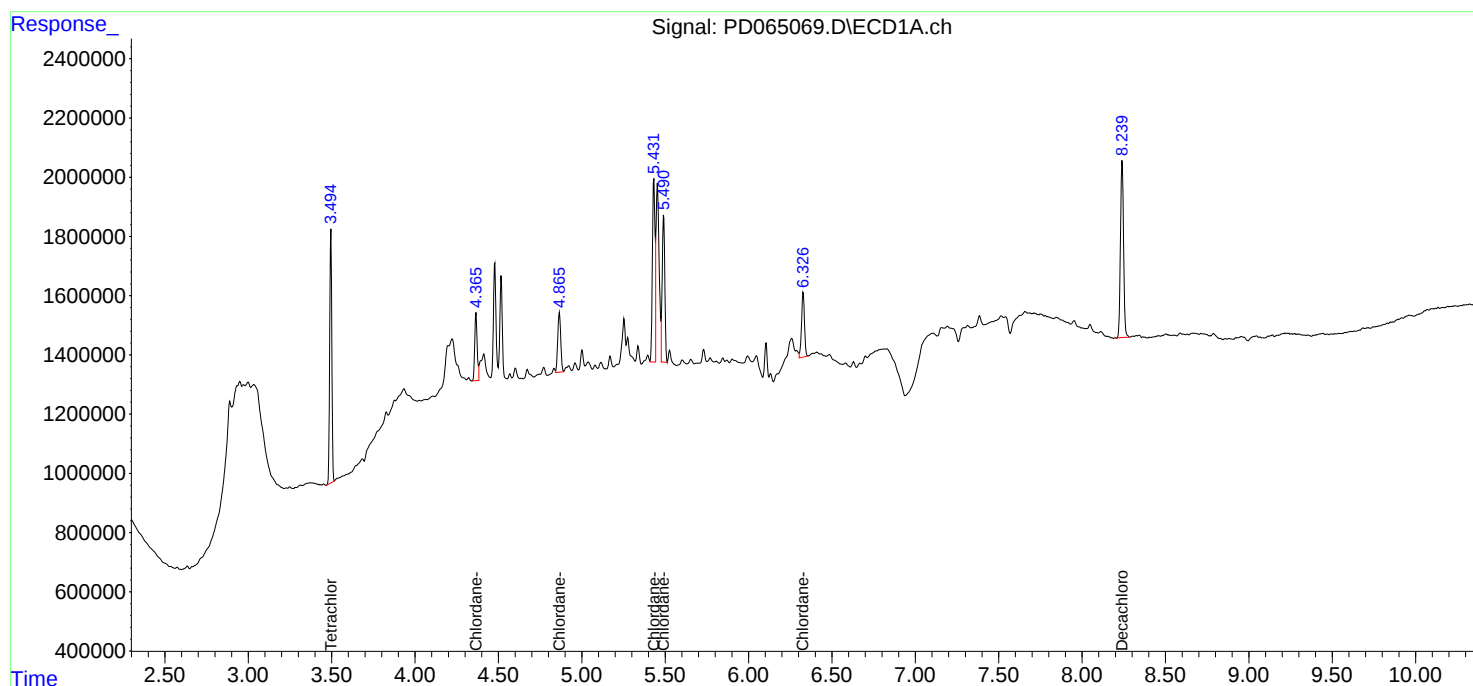


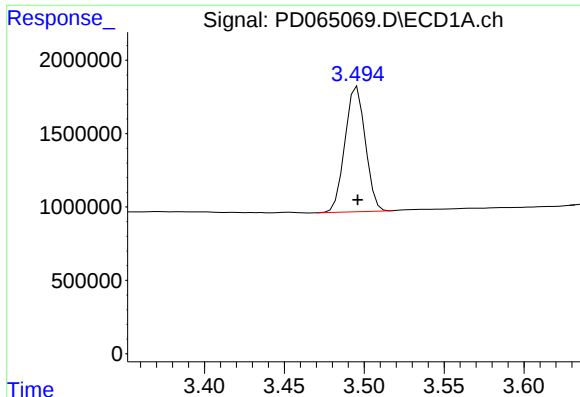

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 7567029
Conc: 6.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

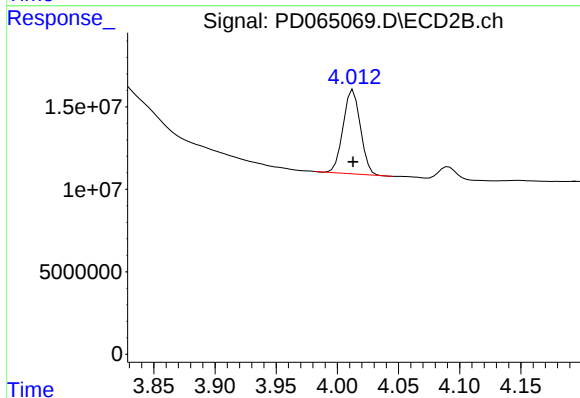


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 49841566
Conc: 6.04 ng/ml

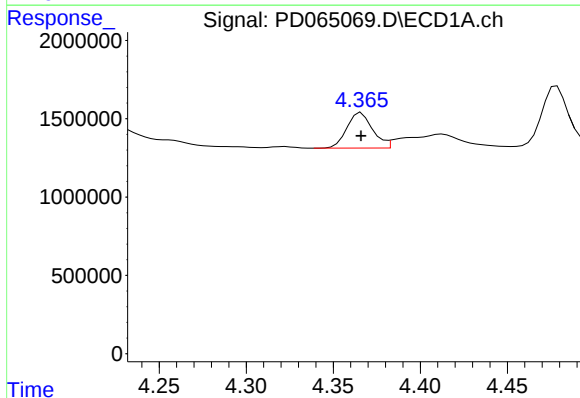


#23 Chlordane-1

R.T.: 4.366 min
Delta R.T.: 0.000 min
Response: 2324854
Conc: 61.39 ng/ml

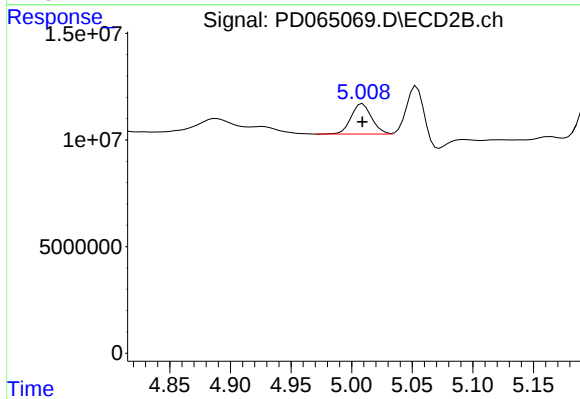

#23 Chlordane-1


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 16826331
Conc: 54.33 ng/ml

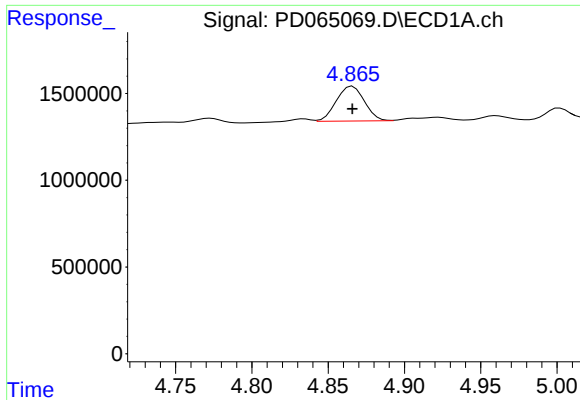

#24 Chlordane-2


R.T.: 4.866 min
Delta R.T.: 0.000 min
Response: 2564952
Conc: 58.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

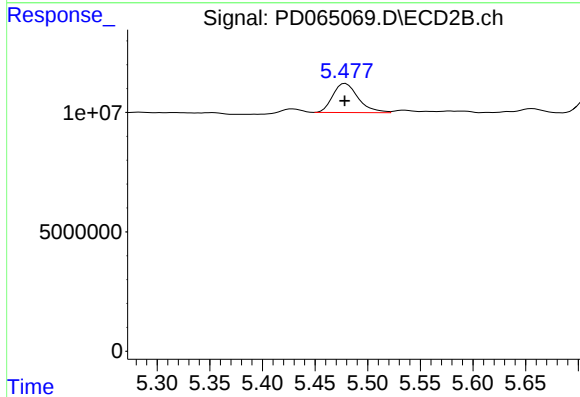


#24 Chlordane-2

R.T.: 5.479 min
Delta R.T.: 0.000 min
Response: 20535593
Conc: 63.40 ng/ml

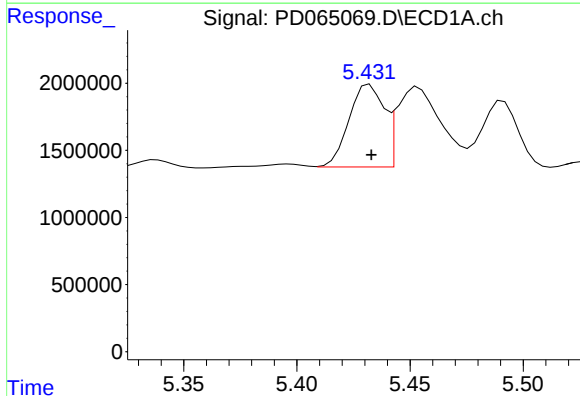


#25 Chlordane-3

R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 6632507
Conc: 60.09 ng/ml

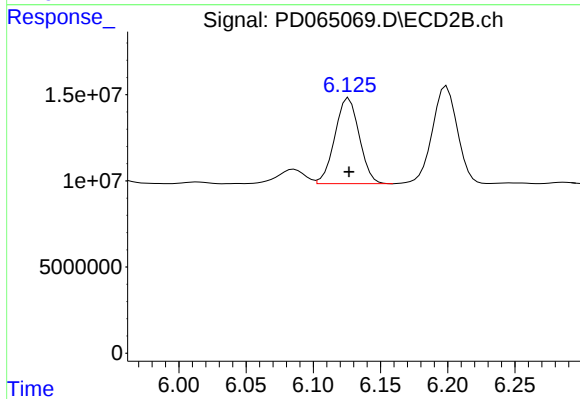

#25 Chlordane-3


R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 62551115
Conc: 60.50 ng/ml

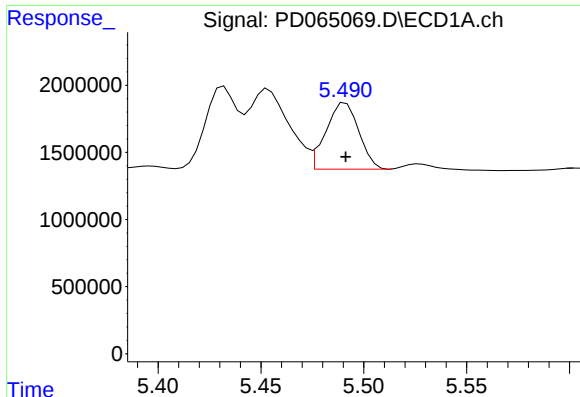

#26 Chlordane-4


R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 5493594
Conc: 59.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

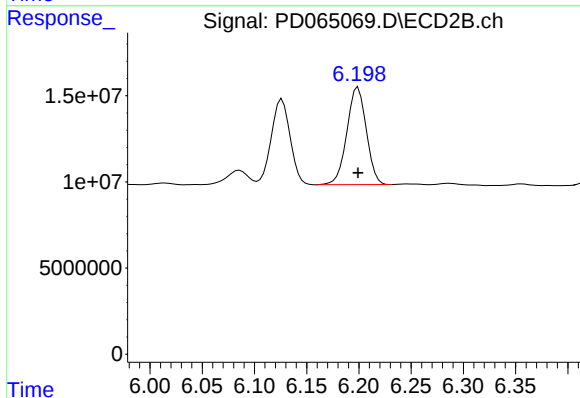


#26 Chlordane-4

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 73228079
Conc: 60.91 ng/ml

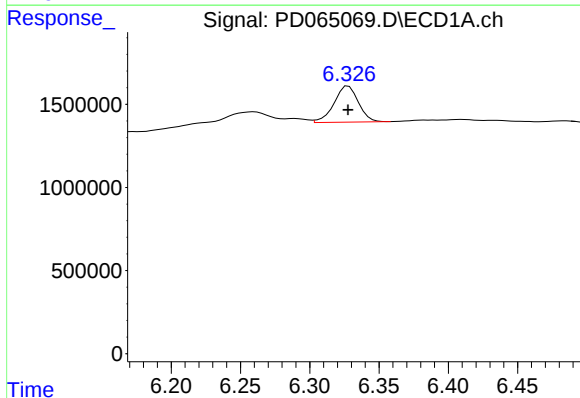


#27 Chlordane-5

R.T.: 6.328 min
Delta R.T.: 0.000 min
Response: 2658681
Conc: 58.90 ng/ml

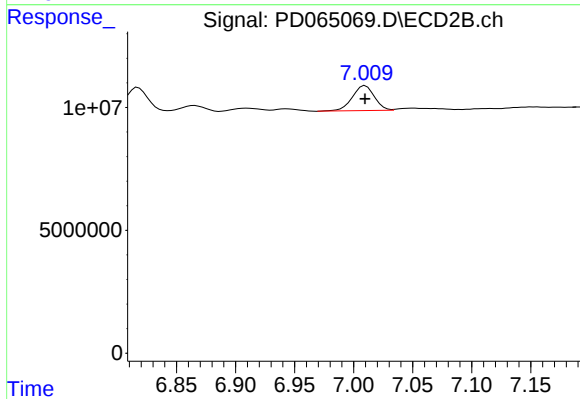

#27 Chlordane-5


R.T.: 7.010 min
Delta R.T.: 0.000 min
Response: 13266349
Conc: 55.95 ng/ml

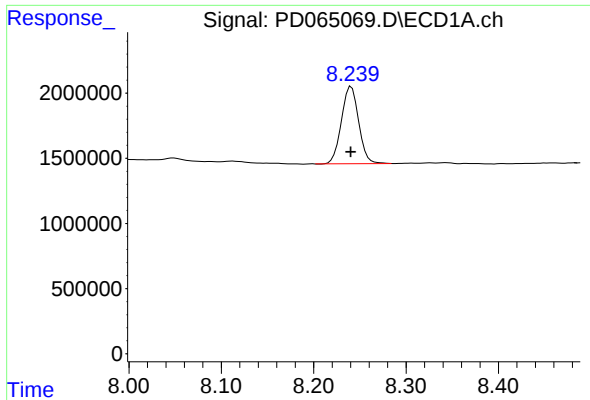

#28 Decachlorobiphenyl

R.T.: 8.241 min
Delta R.T.: 0.000 min
Response: 7704657
Conc: 6.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

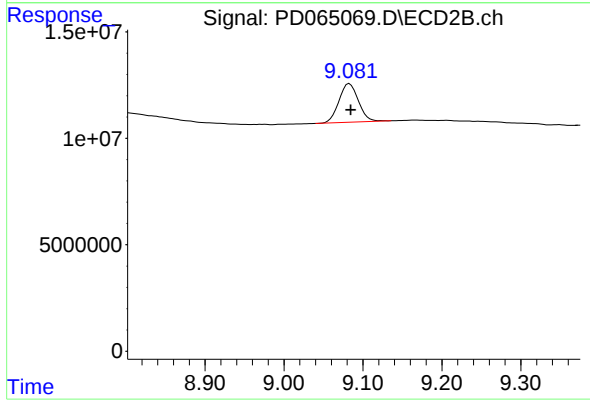

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: -0.002 min
Response: 31312281
Conc: 6.24 ng/ml