

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
 Data File : PD065123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2021 19:10
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 00:37:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	21800883	167.3E6	21.209	21.125
28)	SA Decachlor...	8.240	9.084	26204453	104.2E6	23.127	22.013
Target Compounds							
7)	B delta-BHC	0.000	5.114f	0	5703076	N.D.	0.587 #
8)	B Heptachlo...	0.000	5.889	0	49186079	N.D.	6.593 #
10)	B gamma-Chl...	0.000	6.100f	0	4284425	N.D.	0.560 #
14)	MA Endrin	6.054	0.000	868704	0	0.828	N.D. #
23)	Chlordane-1	4.394f	0.000	966296	0	25.515	N.D. #
25)	Chlordane-3	0.000	6.100f	0	4284425	N.D.	4.144 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
Data File : PD065123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2021 19:10
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 00:37:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

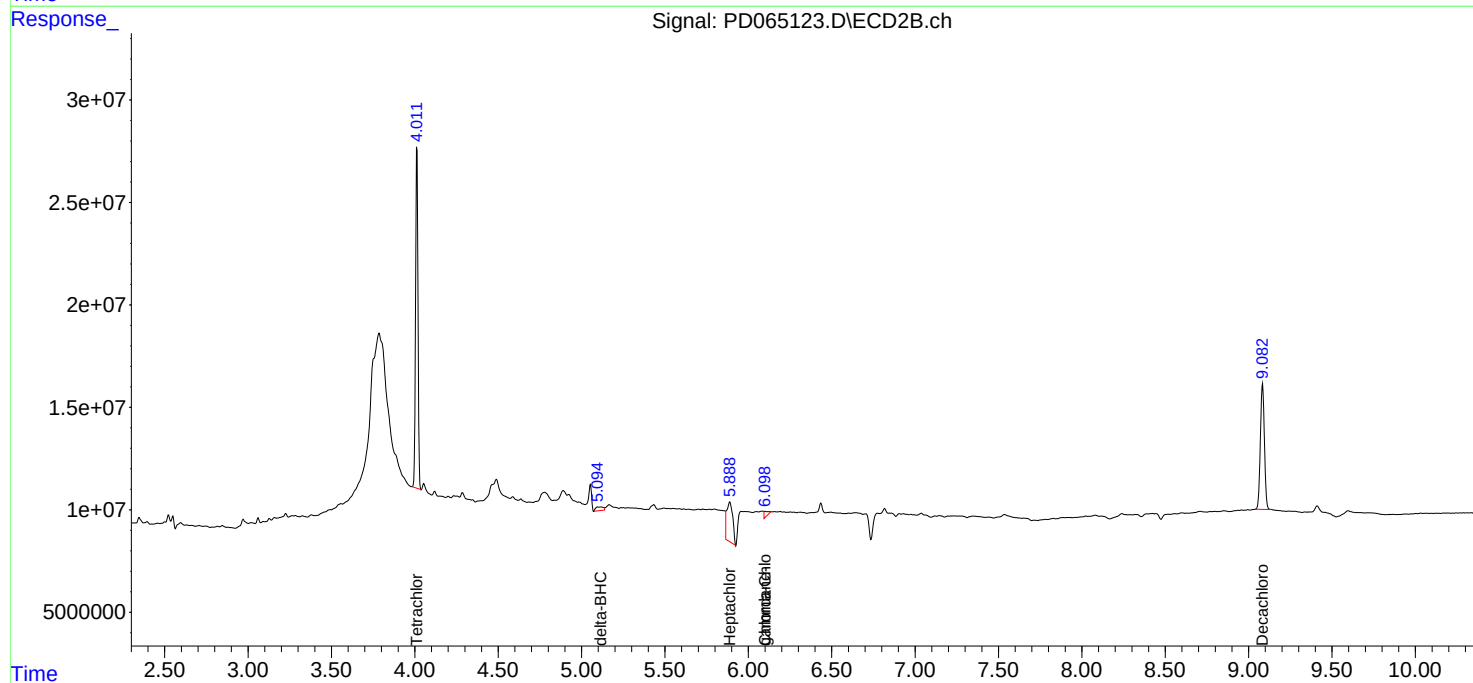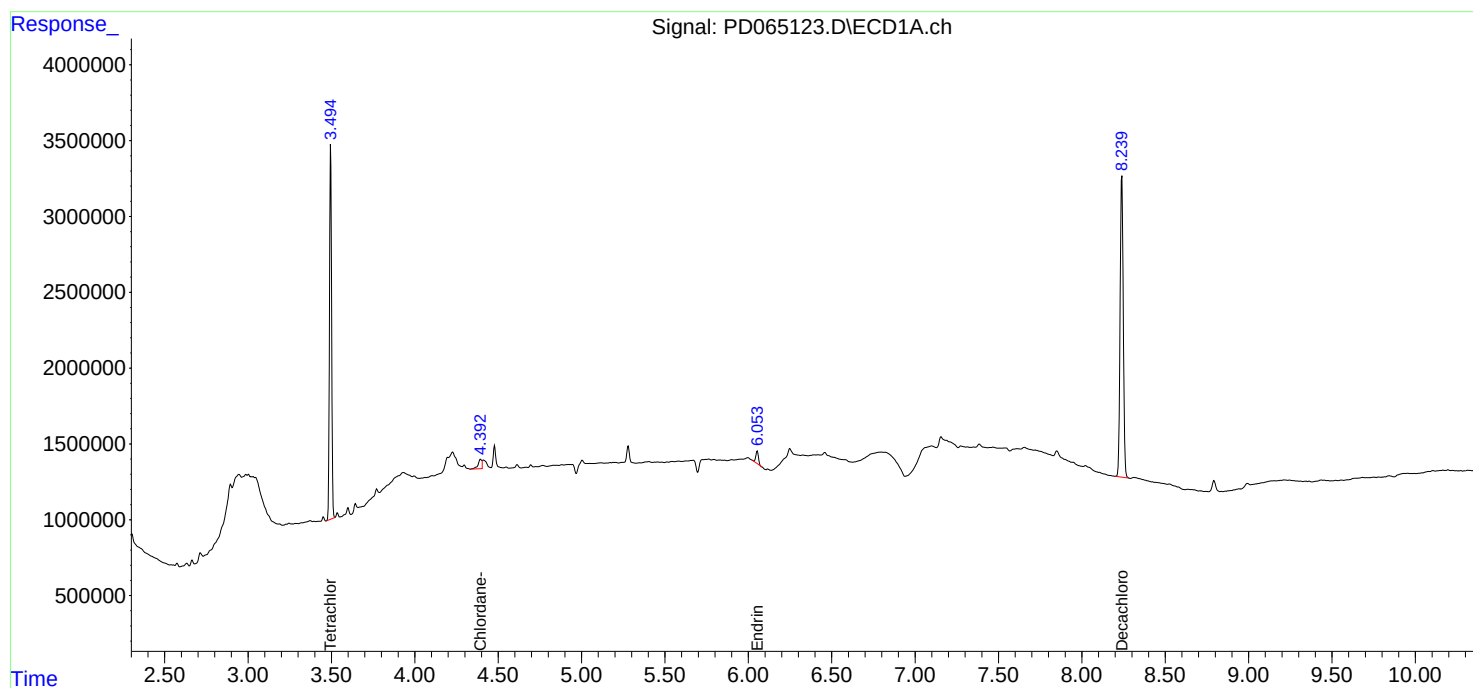


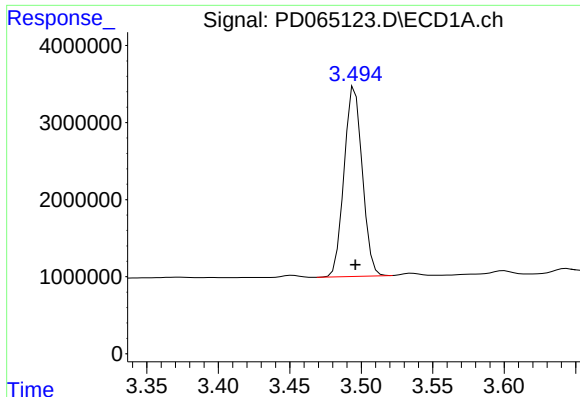

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 21800883
Conc: 21.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

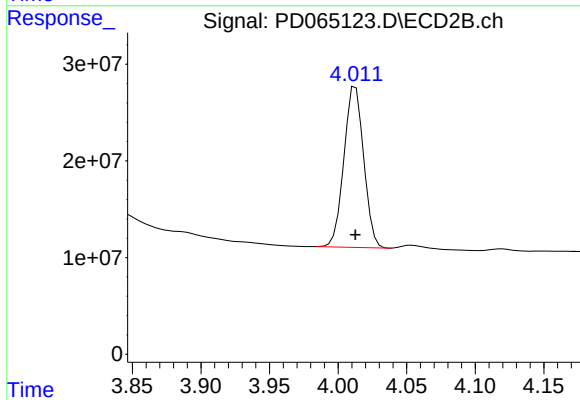


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 167323798
Conc: 21.12 ng/ml

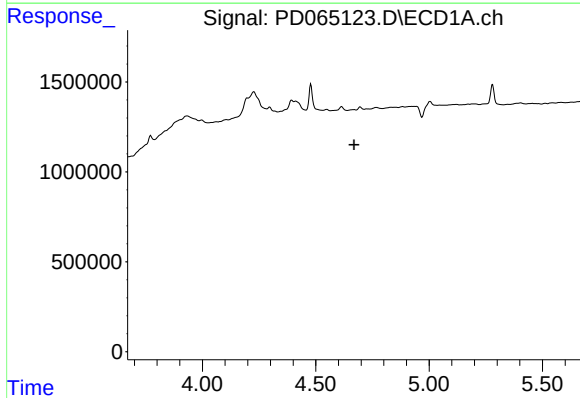


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.670 min
Response: 0
Conc: N.D.

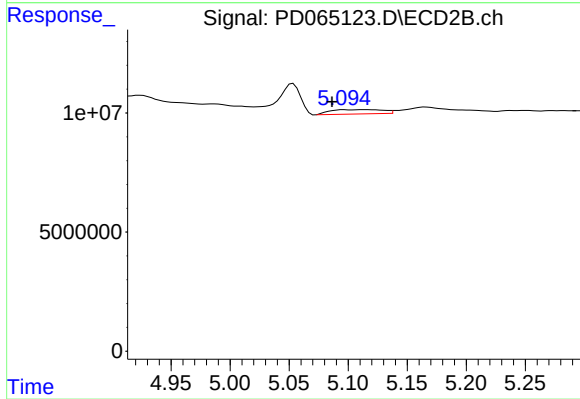

#7 delta-BHC


R.T.: 5.114 min
Delta R.T.: 0.028 min
Response: 5703076
Conc: 0.59 ng/ml

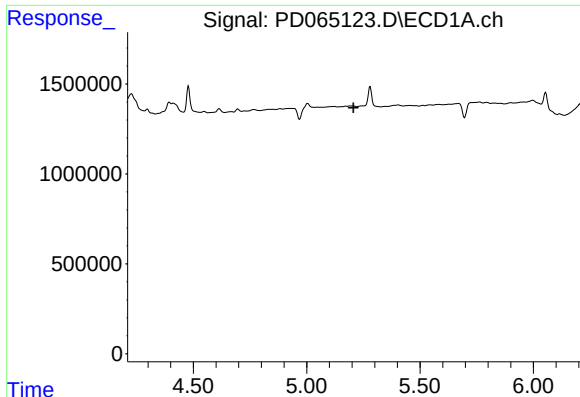

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.207 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

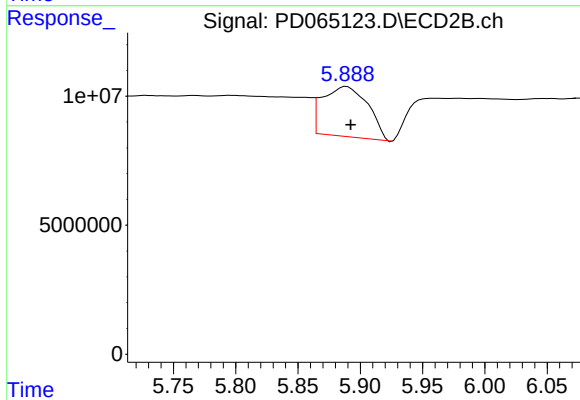


#8 Heptachlor epoxide

R.T.: 5.889 min
Delta R.T.: -0.003 min
Response: 49186079
Conc: 6.59 ng/ml

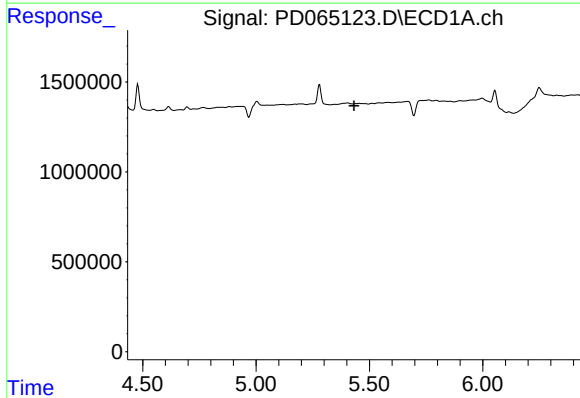


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.432 min
Response: 0
Conc: N.D.

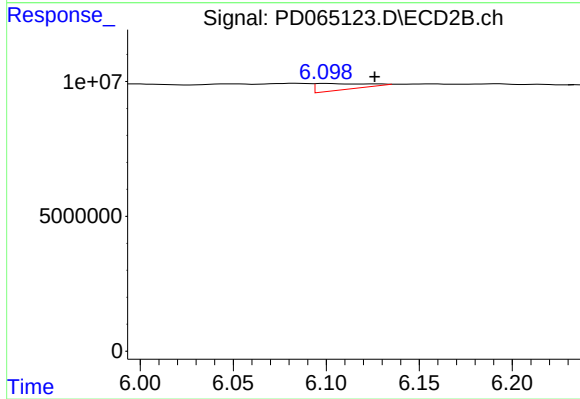

#10 gamma-Chlordane


R.T.: 6.100 min
Delta R.T.: -0.026 min
Response: 4284425
Conc: 0.56 ng/ml

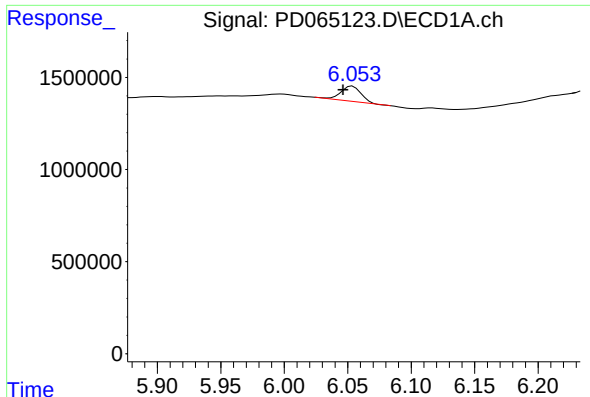

#14 Endrin


R.T.: 6.054 min
Delta R.T.: 0.007 min
Response: 868704
Conc: 0.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

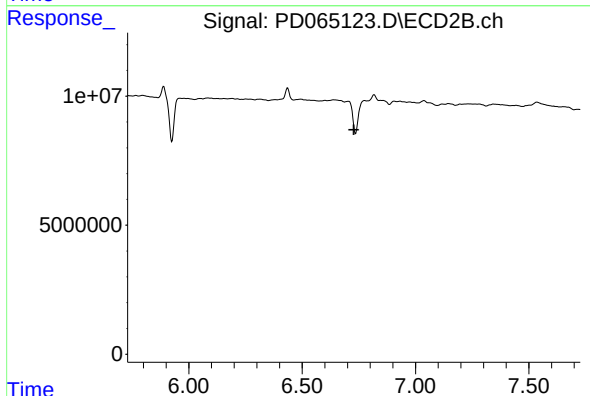


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.728 min
Response: 0
Conc: N.D.

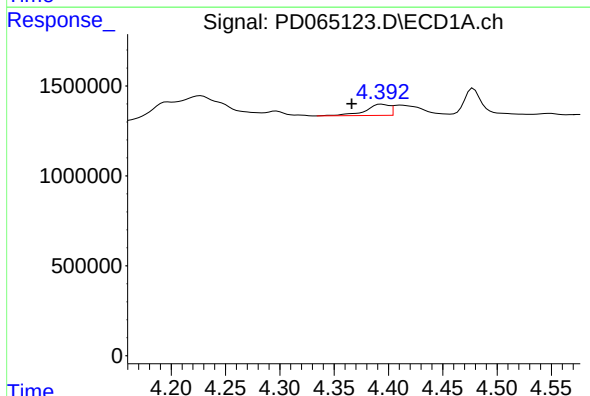


#23 Chlordane-1

R.T.: 4.394 min
Delta R.T.: 0.028 min
Response: 966296
Conc: 25.51 ng/ml

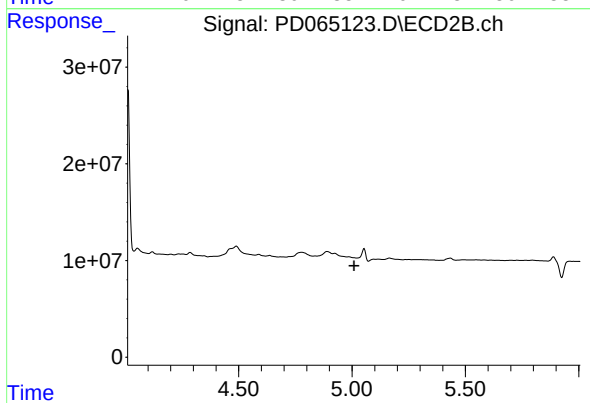

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.009 min
Response: 0
Conc: N.D.

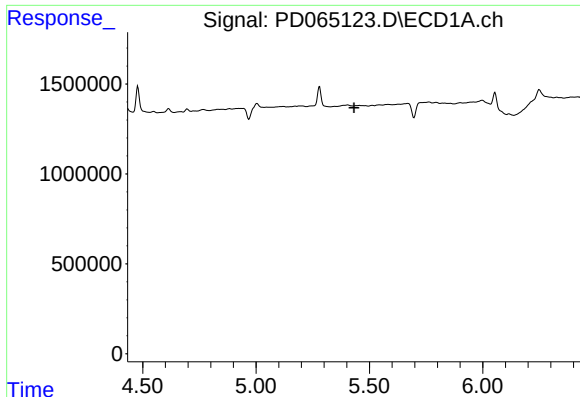

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

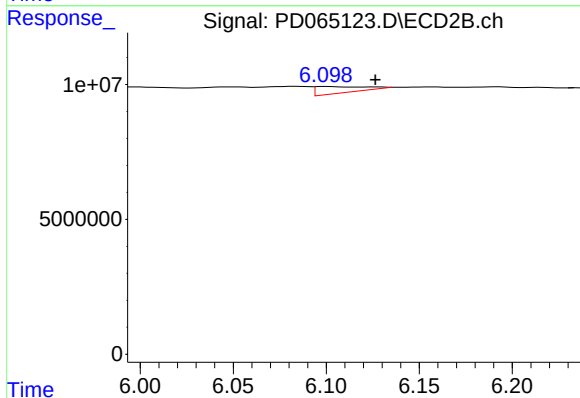


#25 Chlordane-3

R.T.: 6.100 min
Delta R.T.: -0.026 min
Response: 4284425
Conc: 4.14 ng/ml

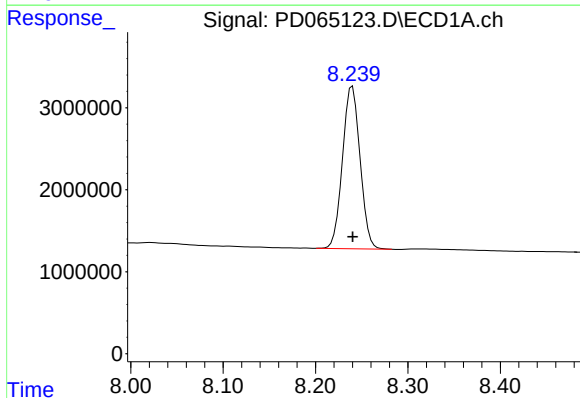

#28 Decachlorobiphenyl

R.T.: 8.240 min
Delta R.T.: 0.000 min
Response: 26204453
Conc: 23.13 ng/ml

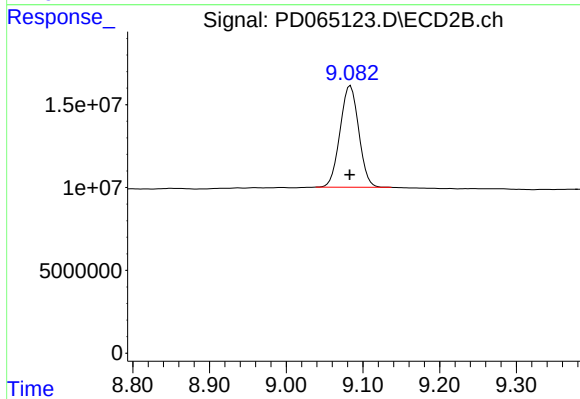

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 104179046
Conc: 22.01 ng/ml