

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
 Data File : PD065143.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2021 00:13
 Operator : AR\AJ
 Sample : M3434-15
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SWCS-12-1015

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 03:52:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	20862341	160.1E6	20.296	20.214
28)	SA Decachlor...	8.240	9.083	24036883	94614082	21.214	19.992
Target Compounds							
8)	B Heptachlo...	0.000	5.878	0	22255303	N.D.	2.983 #
10)	B gamma-Chl...	0.000	6.129	0	3470183	N.D.	0.454 #
15)	B Endosulfa...	0.000	6.932	0	1514028	N.D.	0.258 #
20)	A Methoxychlor	0.000	7.597	0	5722697	N.D.	1.891 #
21)	B Endrin ke...	0.000	7.770	0	2734220	N.D.	0.421 #
23)	Chlordane-1	4.393f	0.000	1573561	0	41.549	N.D. #
24)	Chlordane-2	4.878	0.000	682304	0	15.633	N.D. #
25)	Chlordane-3	0.000	6.129	0	3470183	N.D.	3.357 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
Data File : PD065143.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2021 00:13
Operator : AR\AJ
Sample : M3434-15
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SWCS-12-1015

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 03:52:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

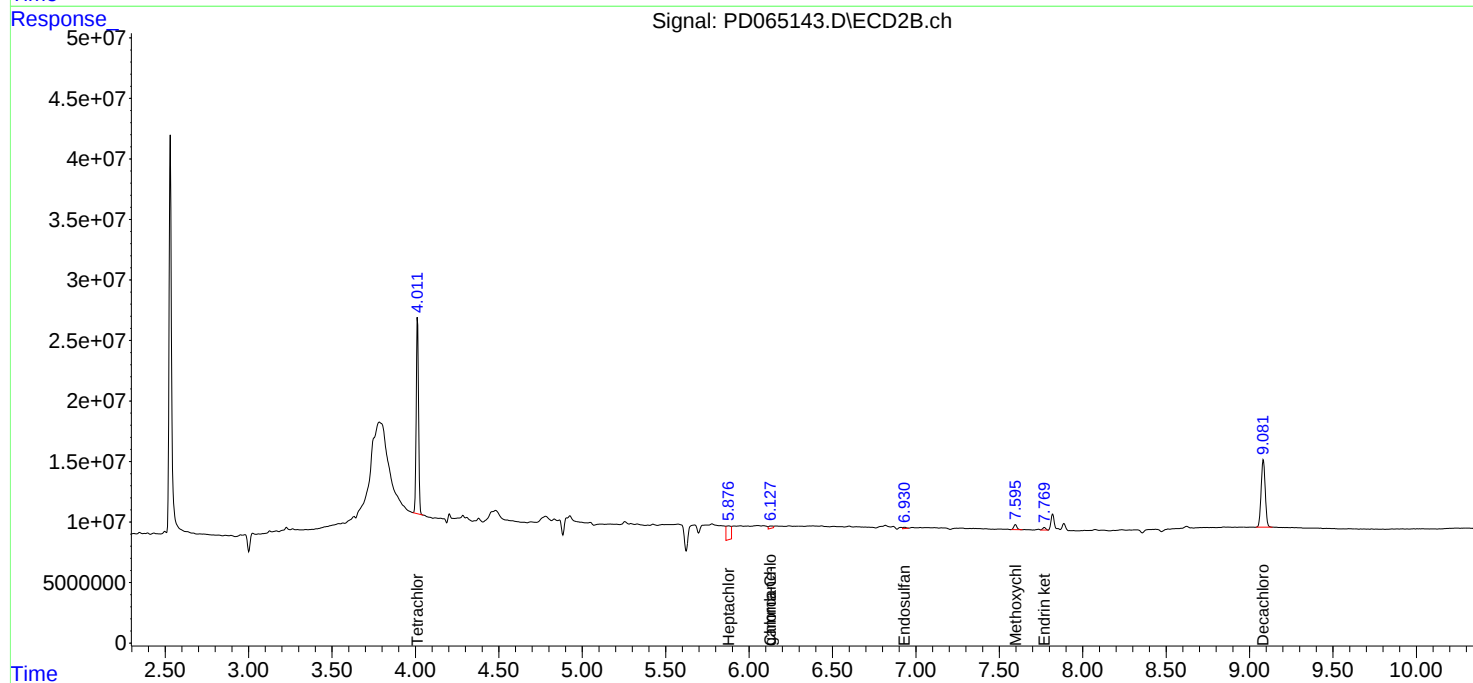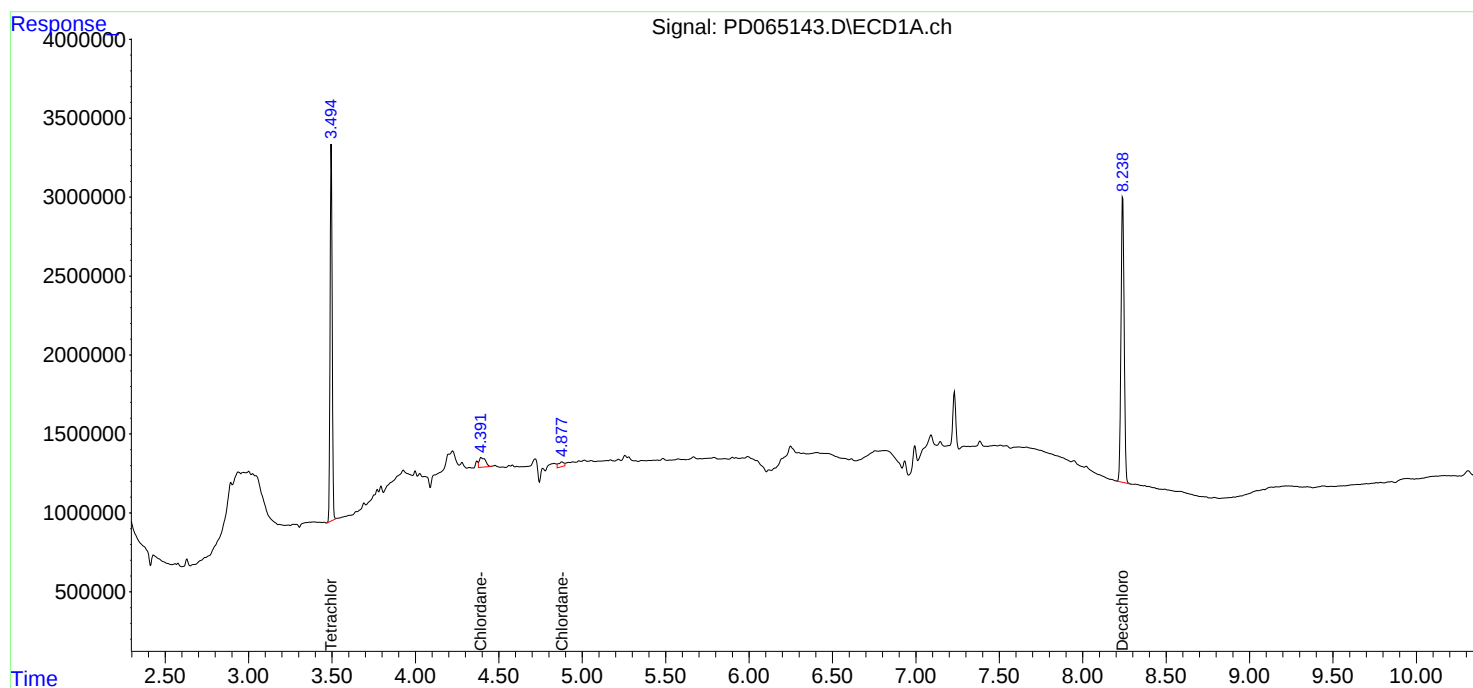


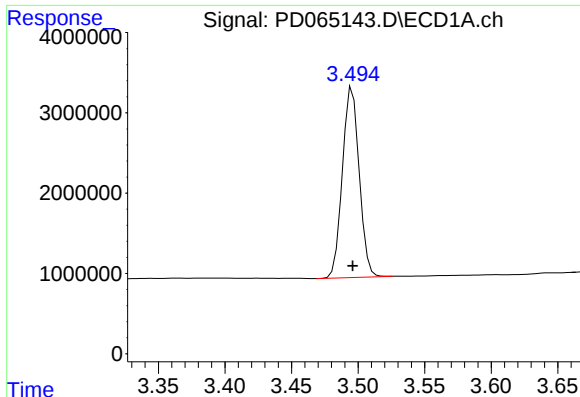

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 20862341
Conc: 20.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
SWCS-12-1015

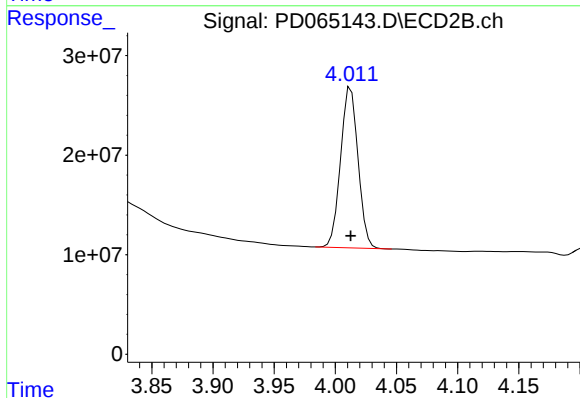


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 160106792
Conc: 20.21 ng/ml

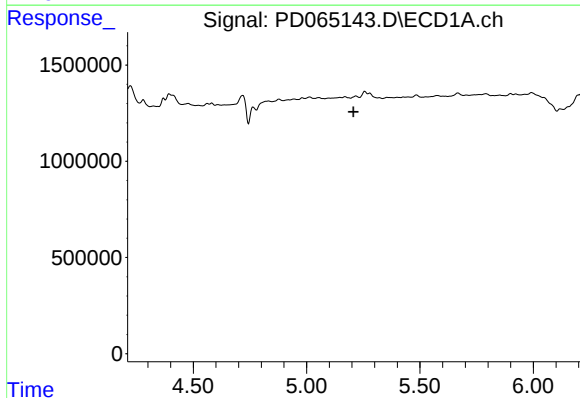


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.207 min
Response: 0
Conc: N.D.

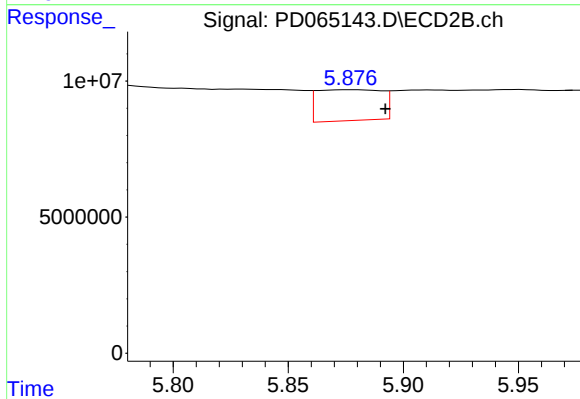

#8 Heptachlor epoxide


R.T.: 5.878 min
Delta R.T.: -0.015 min
Response: 22255303
Conc: 2.98 ng/ml

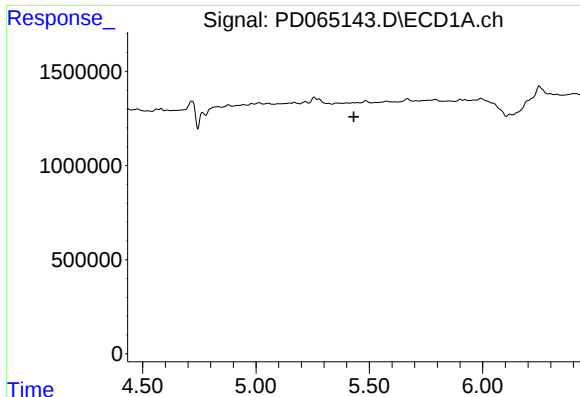

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SWCS-12-1015

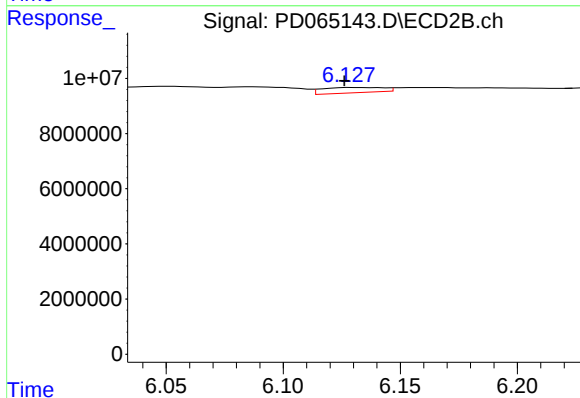


#10 gamma-Chlordane

R.T.: 6.129 min
Delta R.T.: 0.003 min
Response: 3470183
Conc: 0.45 ng/ml

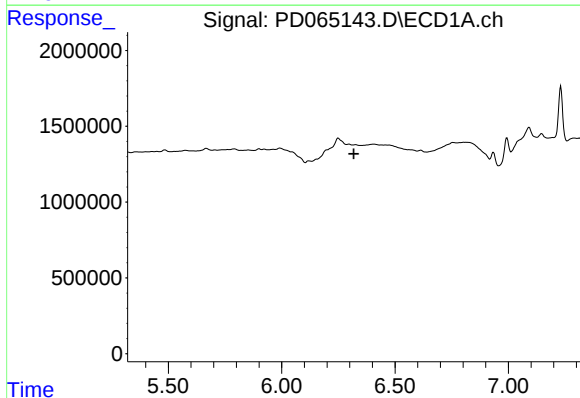


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.319 min
Response: 0
Conc: N.D.

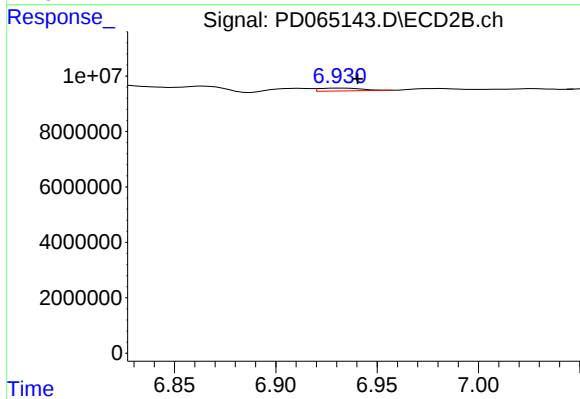

#15 Endosulfan II


R.T.: 6.932 min
Delta R.T.: -0.009 min
Response: 1514028
Conc: 0.26 ng/ml

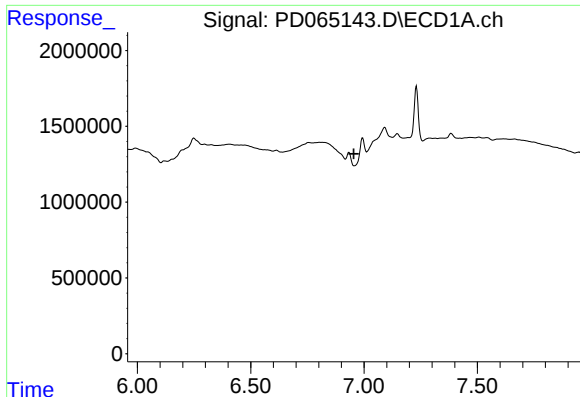

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.955 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SWCS-12-1015

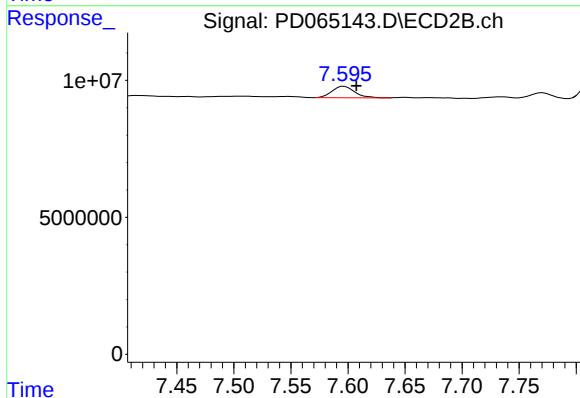


#20 Methoxychlor

R.T.: 7.597 min
Delta R.T.: -0.010 min
Response: 5722697
Conc: 1.89 ng/ml

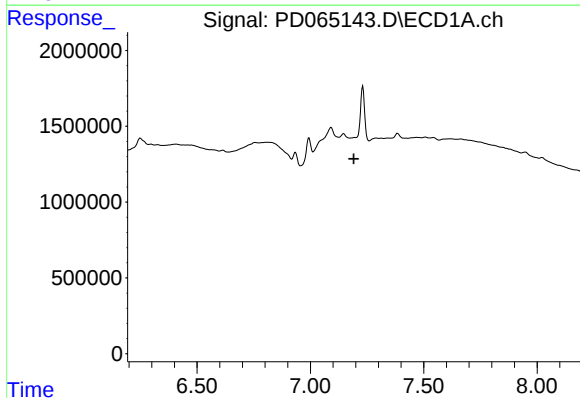


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.192 min
Response: 0
Conc: N.D.

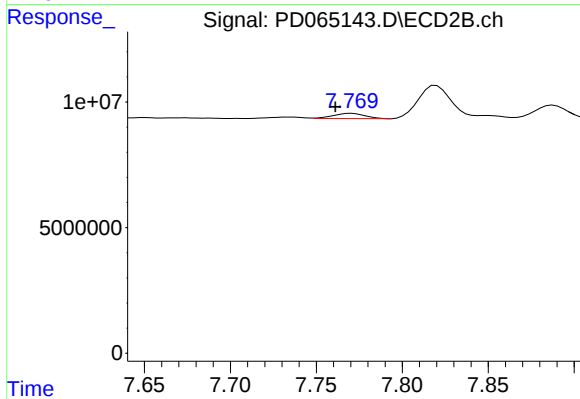

#21 Endrin ketone


R.T.: 7.770 min
Delta R.T.: 0.009 min
Response: 2734220
Conc: 0.42 ng/ml

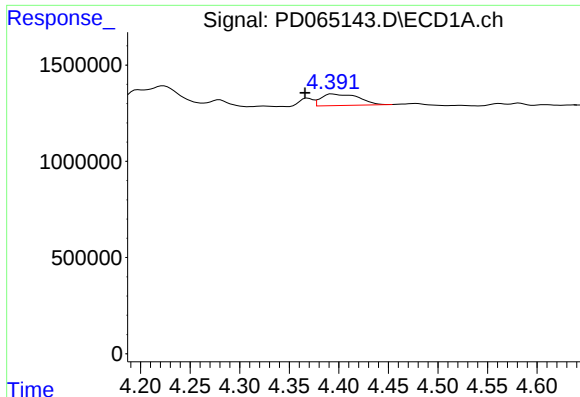

#23 Chlordane-1


R.T.: 4.393 min
Delta R.T.: 0.027 min
Response: 1573561
Conc: 41.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
SWCS-12-1015

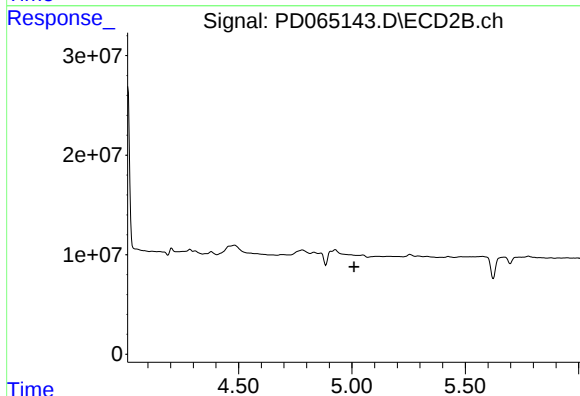


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.009 min
Response: 0
Conc: N.D.

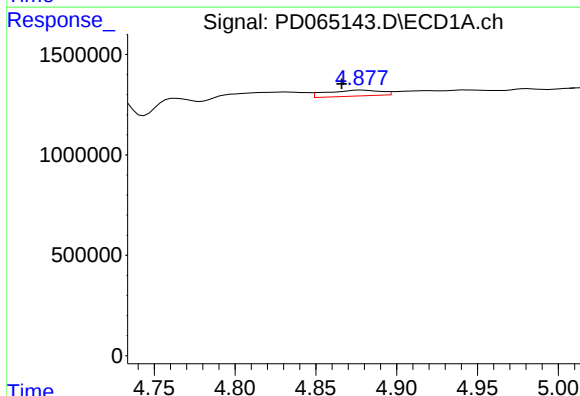


#24 Chlordane-2

R.T.: 4.878 min
Delta R.T.: 0.012 min
Response: 682304
Conc: 15.63 ng/ml

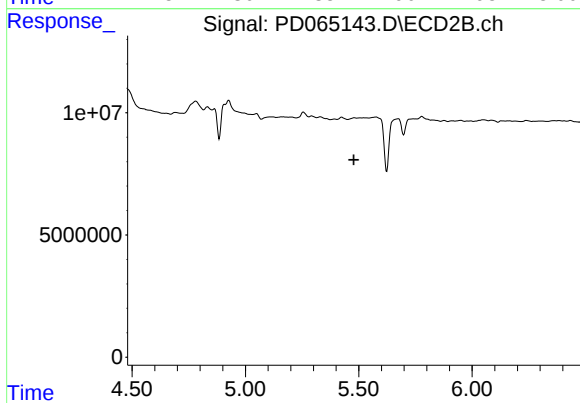

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.479 min
Response: 0
Conc: N.D.

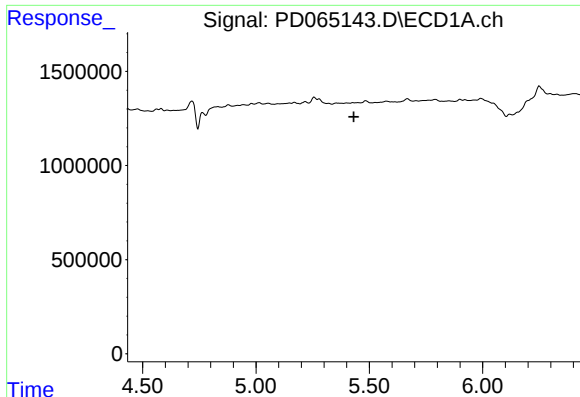

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SWCS-12-1015

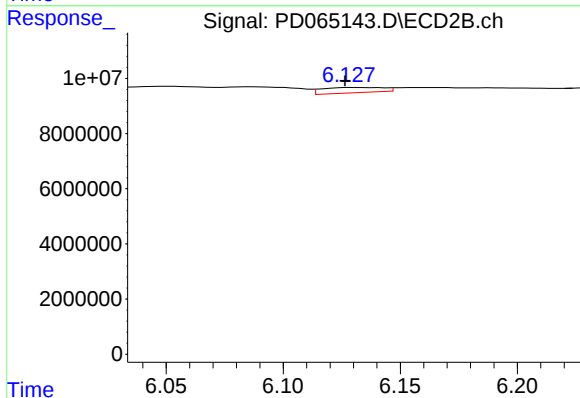


#25 Chlordane-3

R.T.: 6.129 min
Delta R.T.: 0.003 min
Response: 3470183
Conc: 3.36 ng/ml

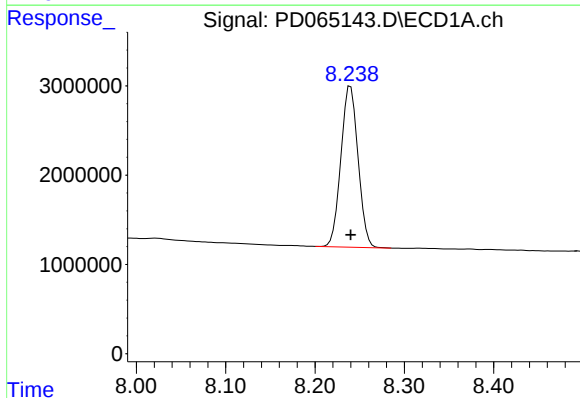

#28 Decachlorobiphenyl

R.T.: 8.240 min
Delta R.T.: 0.000 min
Response: 24036883
Conc: 21.21 ng/ml

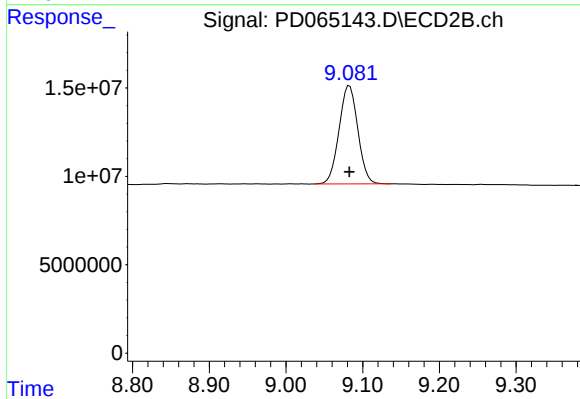

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: 0.000 min
Response: 94614082
Conc: 19.99 ng/ml