

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
 Data File : PD065147.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2021 01:08
 Operator : AR\AJ
 Sample : M3434-23
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SWCS-13-1015

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 03:53:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.012	18030549	128.2E6	17.541	16.190
28)	SA Decachlor...	8.240	9.082	12407074	48012137	10.950	10.145
Target Compounds							
4)	MA Heptachlor	0.000	5.186	0	7154234	N.D.	0.714 #
7)	B delta-BHC	0.000	5.110f	0	18626597	N.D.	1.918 #
8)	B Heptachlo...	0.000	5.916f	0	7719638	N.D.	1.035 #
10)	B gamma-Chl...	0.000	6.125	0	5115396	N.D.	0.669 #
13)	MA Dieldrin	5.763f	0.000	551545	0	0.491	N.D. #
15)	B Endosulfa...	0.000	6.928	0	4196964	N.D.	0.716 #
25)	Chlordane-3	0.000	6.125	0	5115396	N.D.	4.948 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
Data File : PD065147.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2021 01:08
Operator : AR\AJ
Sample : M3434-23
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SWCS-13-1015

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 03:53:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

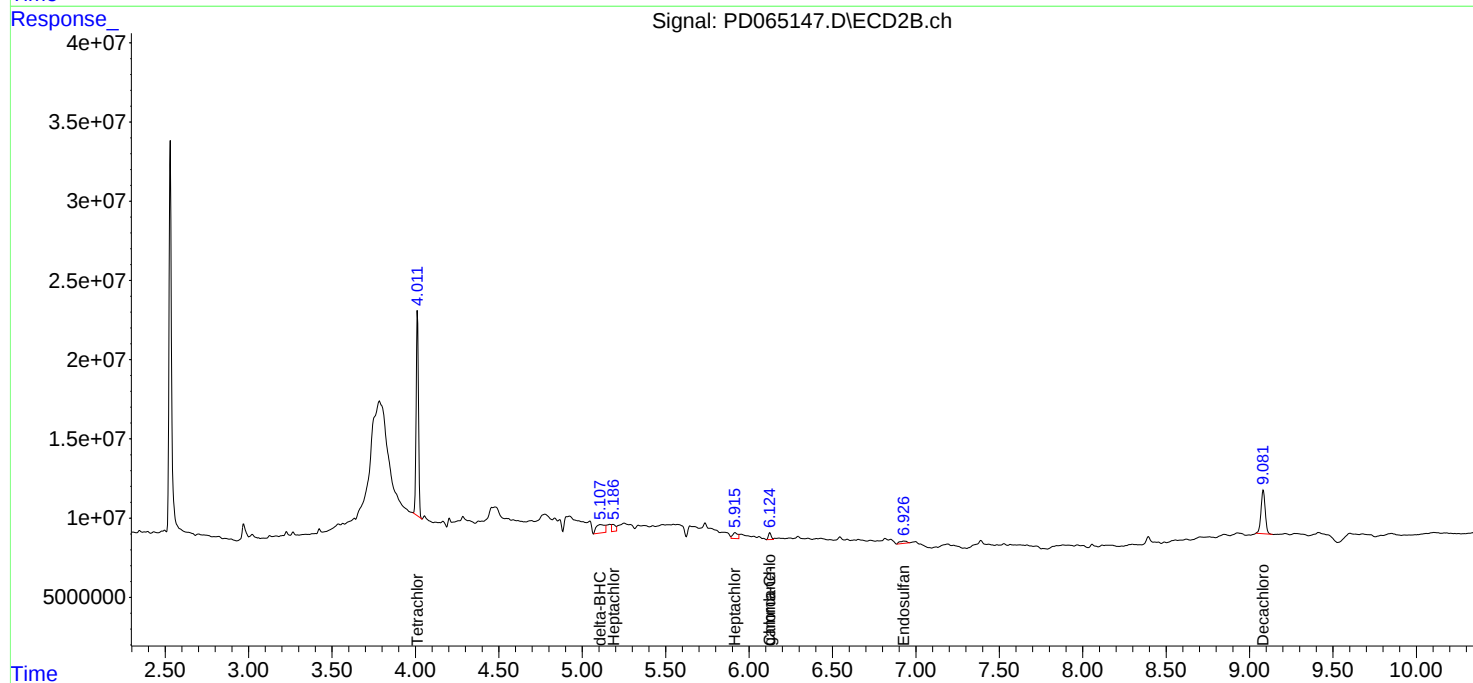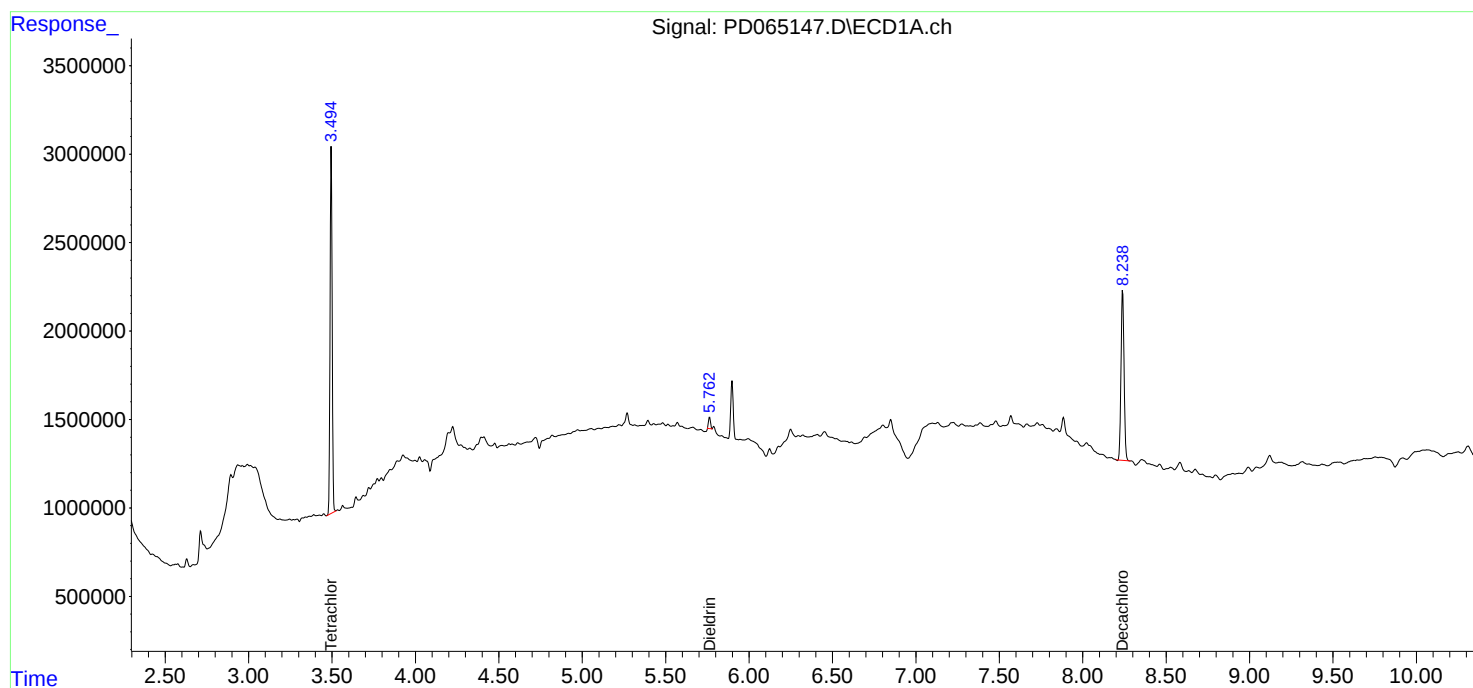


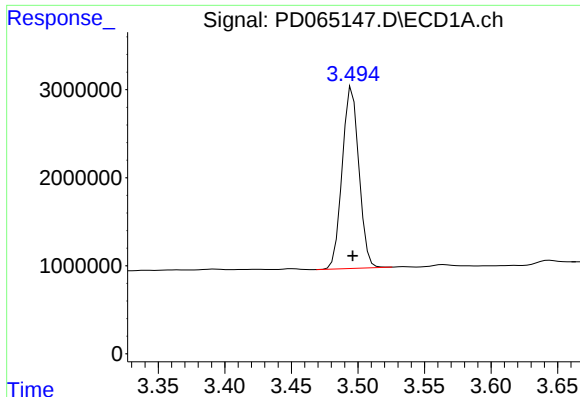

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 18030549
Conc: 17.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
SWCS-13-1015

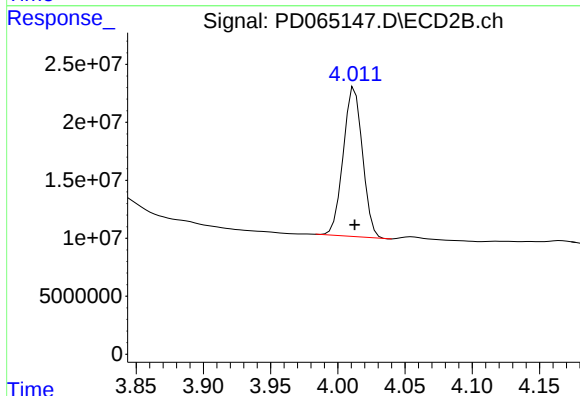


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 128233965
Conc: 16.19 ng/ml

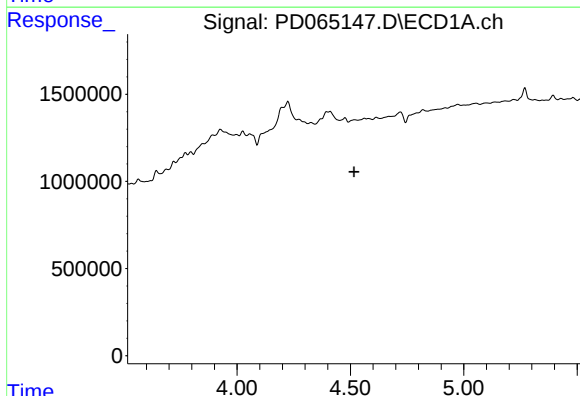


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.517 min
Response: 0
Conc: N.D.

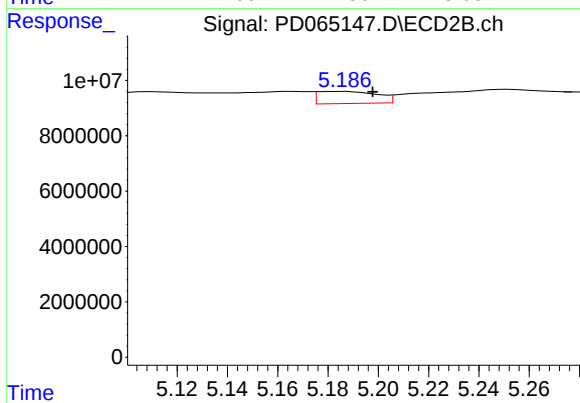

#4 Heptachlor


R.T.: 5.186 min
Delta R.T.: -0.012 min
Response: 7154234
Conc: 0.71 ng/ml

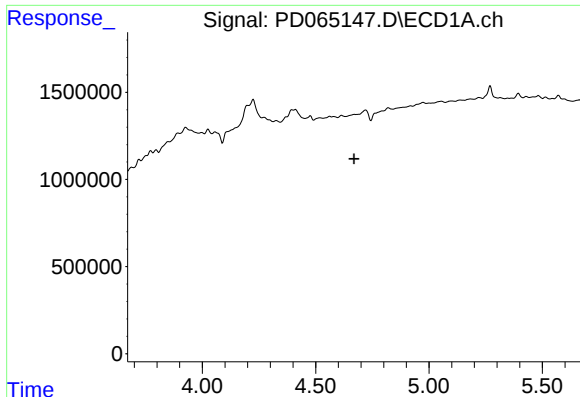

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.670 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SWCS-13-1015

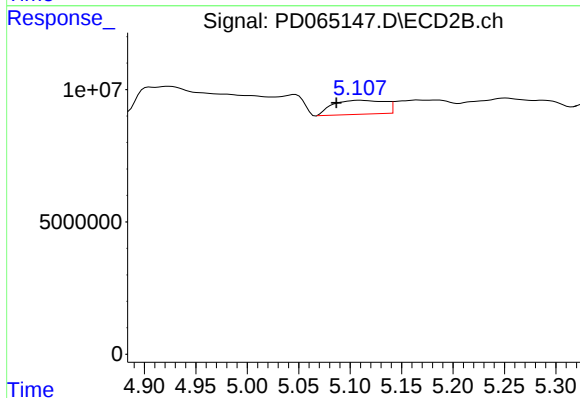


#7 delta-BHC

R.T.: 5.110 min
Delta R.T.: 0.023 min
Response: 18626597
Conc: 1.92 ng/ml

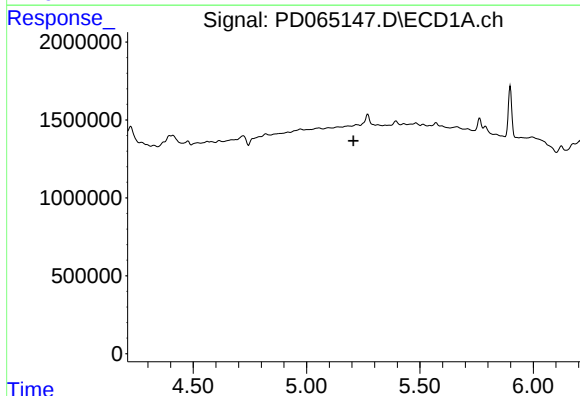


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.207 min
Response: 0
Conc: N.D.

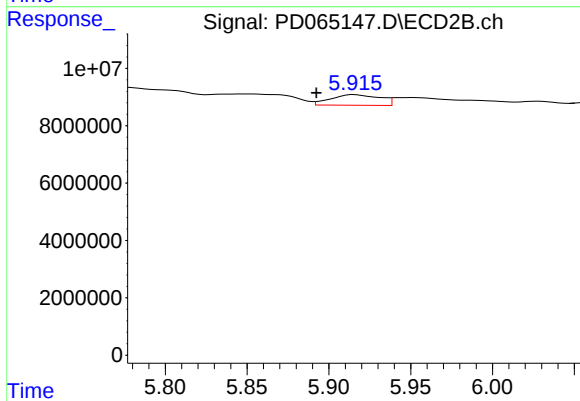

#8 Heptachlor epoxide


R.T.: 5.916 min
Delta R.T.: 0.024 min
Response: 7719638
Conc: 1.03 ng/ml

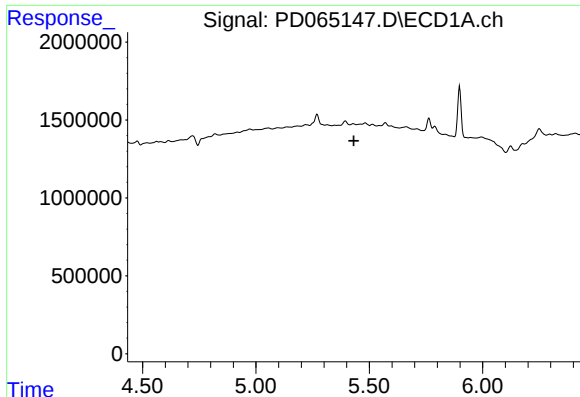

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SWCS-13-1015

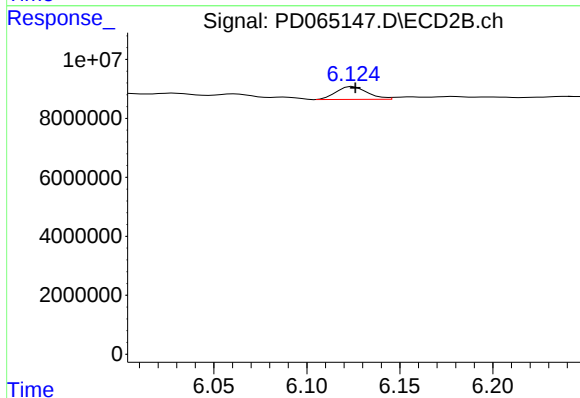


#10 gamma-Chlordane

R.T.: 6.125 min
Delta R.T.: -0.001 min
Response: 5115396
Conc: 0.67 ng/ml

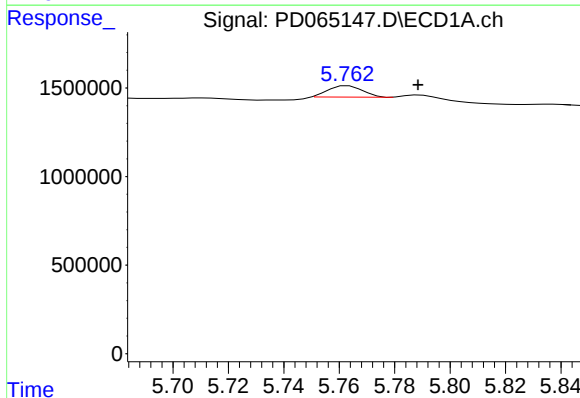


#13 Dieldrin

R.T.: 5.763 min
Delta R.T.: -0.025 min
Response: 551545
Conc: 0.49 ng/ml

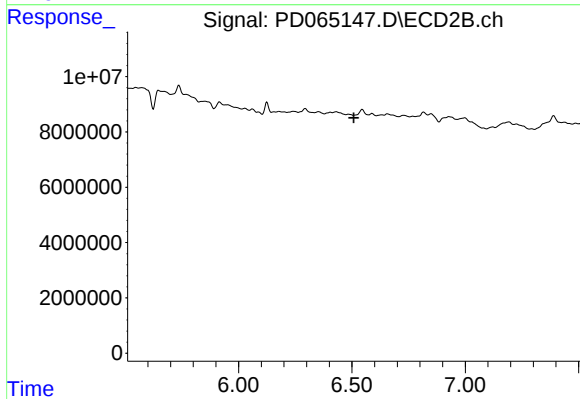

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.508 min
Response: 0
Conc: N.D.

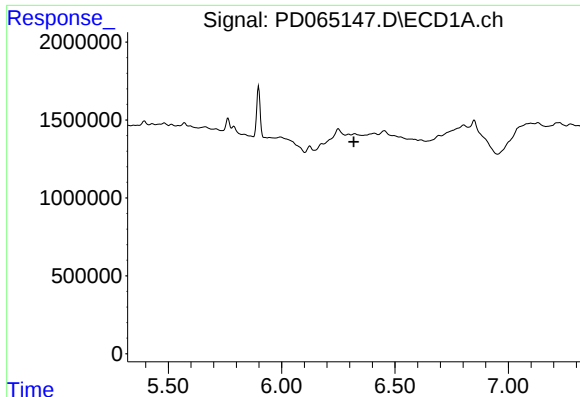

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SWCS-13-1015

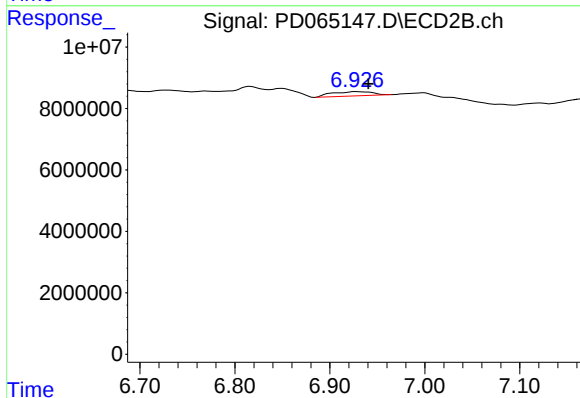


#15 Endosulfan II

R.T.: 6.928 min
Delta R.T.: -0.013 min
Response: 4196964
Conc: 0.72 ng/ml

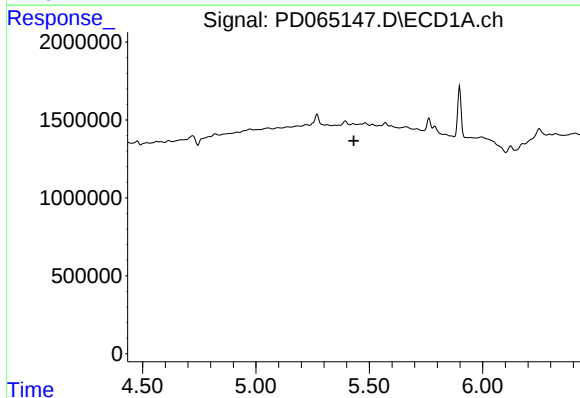


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.432 min
Response: 0
Conc: N.D.

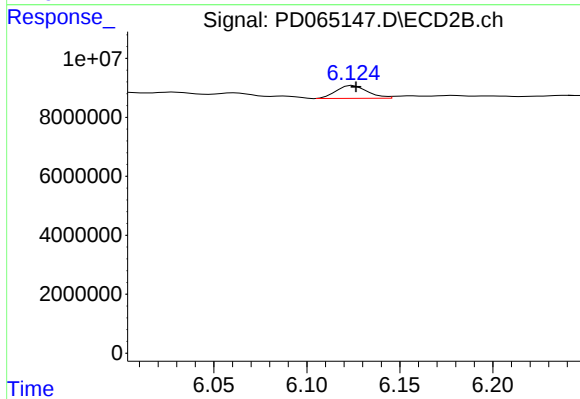

#25 Chlordane-3


R.T.: 6.125 min
Delta R.T.: -0.002 min
Response: 5115396
Conc: 4.95 ng/ml

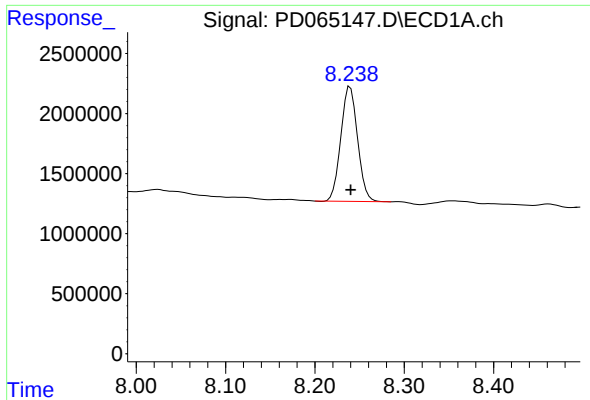

#28 Decachlorobiphenyl

R.T.: 8.240 min
Delta R.T.: 0.000 min
Response: 12407074
Conc: 10.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
SWCS-13-1015

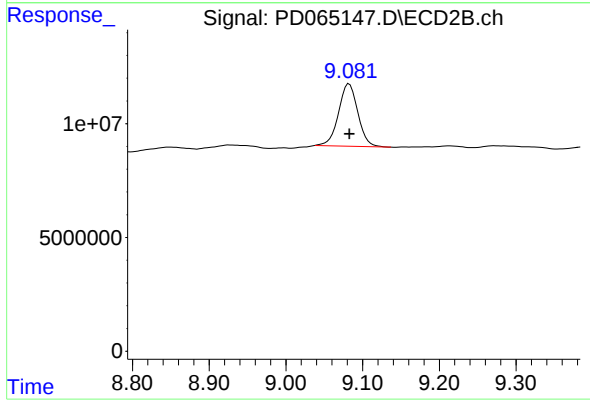

#28 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: 0.000 min
Response: 48012137
Conc: 10.15 ng/ml