

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
 Data File : PD065164.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2021 05:30
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 05:38:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	22610029	175.1E6	21.996	22.111
28)	SA Decachlor...	8.240	9.083	27535832	103.9E6	24.303	21.955
Target Compounds							
8)	B Heptachlo...	0.000	5.889	0 68920504	N.D.	9.238	#
9)	A Endosulfan I	0.000	6.259	0 16430843	N.D.	2.333	#
11)	B alpha-Chl...	0.000	6.188	0 30960085	N.D.	4.159	#
14)	MA Endrin	6.053	0.000	1070382	0	1.020	#
15)	B Endosulfa...	0.000	6.942	0 1122032	N.D.	0.191	#
22)	Mirex	0.000	8.239f	0 472380	N.D.	0.106	#
23)	Chlordane-1	4.395f	0.000	2193150	0	57.910	#
26)	Chlordane-4	0.000	6.188	0 30960085	N.D.	25.750	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
Data File : PD065164.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2021 05:30
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 05:38:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

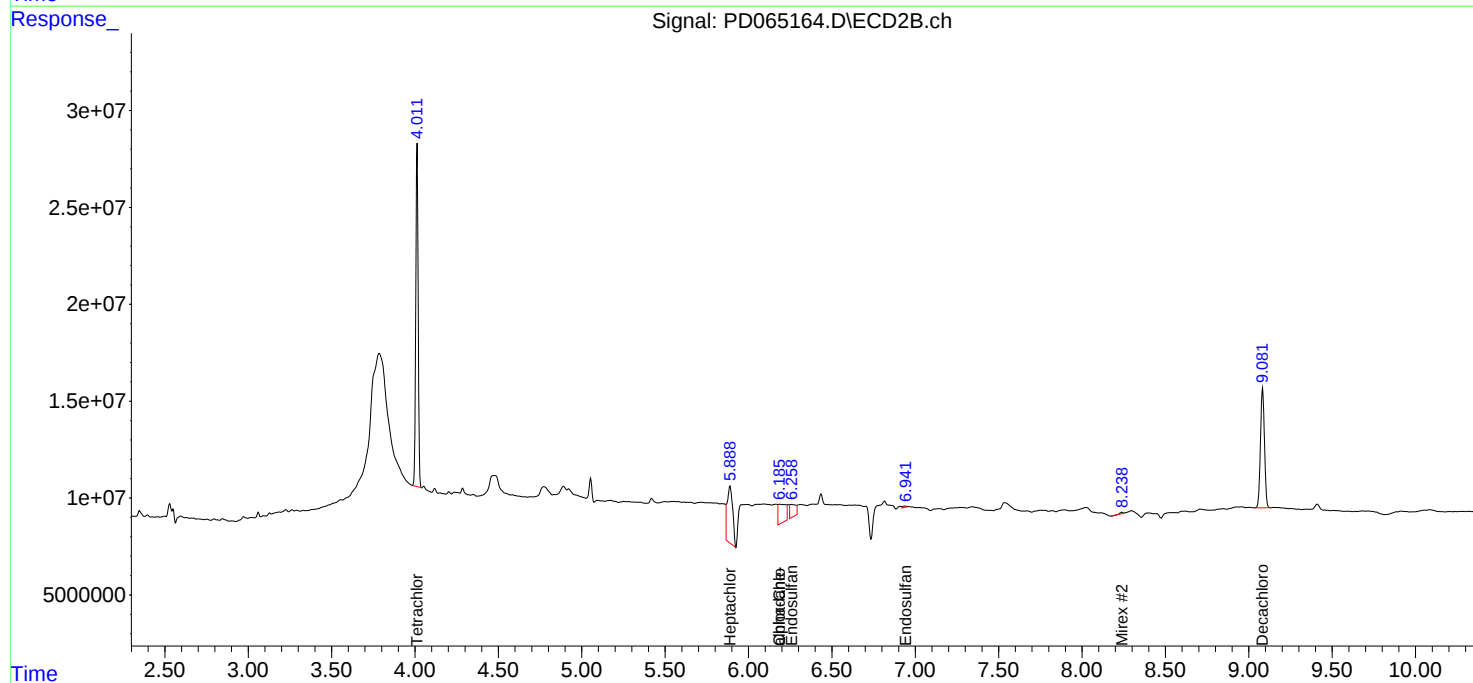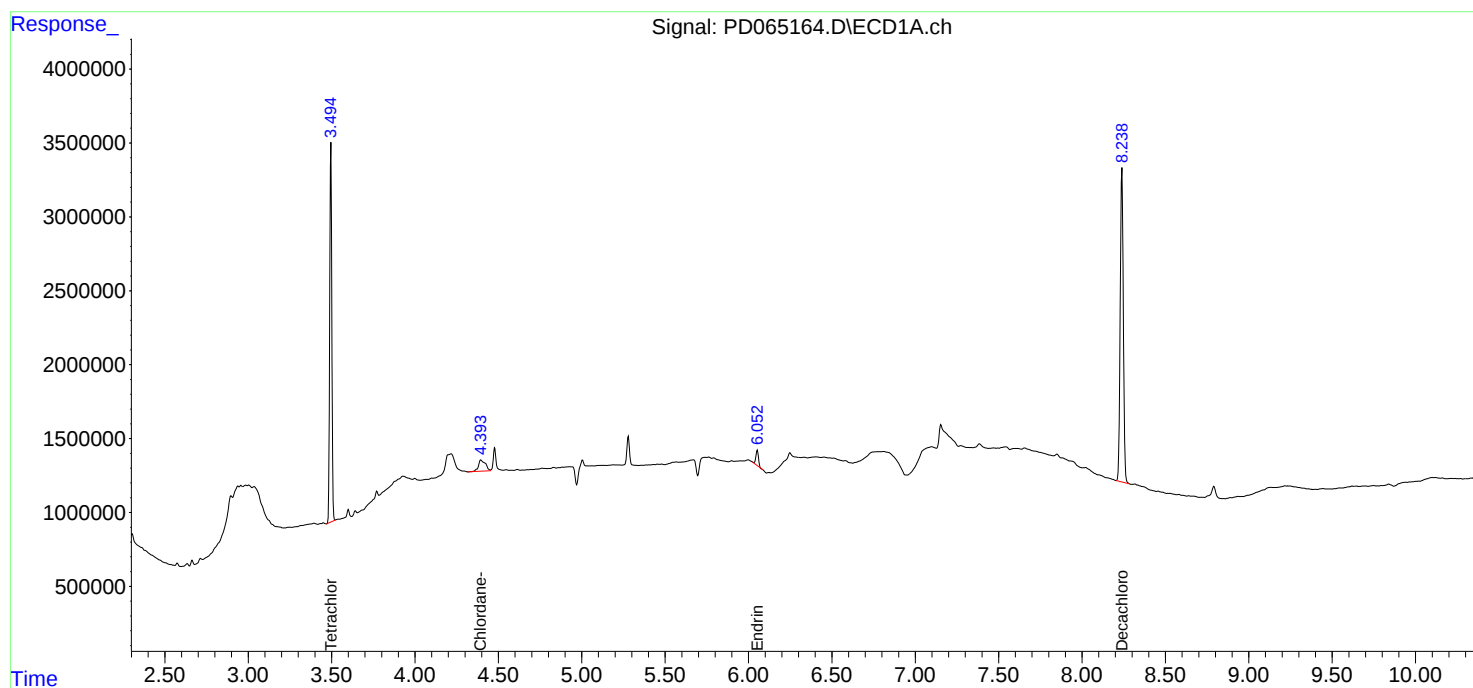


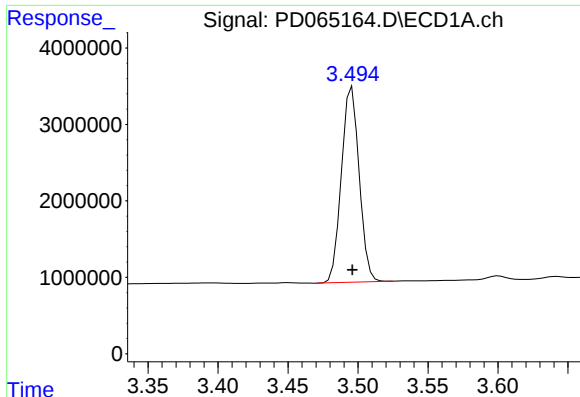

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 22610029
Conc: 22.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

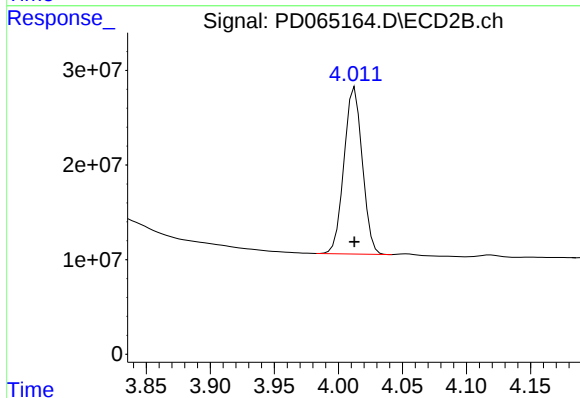


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 175135395
Conc: 22.11 ng/ml

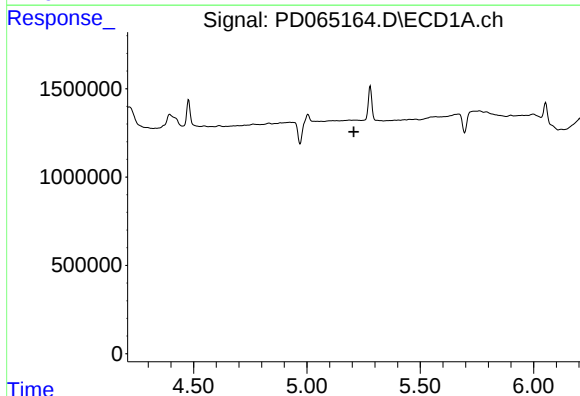


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.207 min
Response: 0
Conc: N.D.

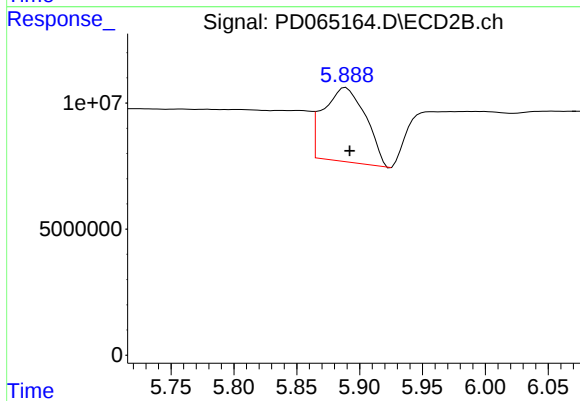

#8 Heptachlor epoxide


R.T.: 5.889 min
Delta R.T.: -0.003 min
Response: 68920504
Conc: 9.24 ng/ml

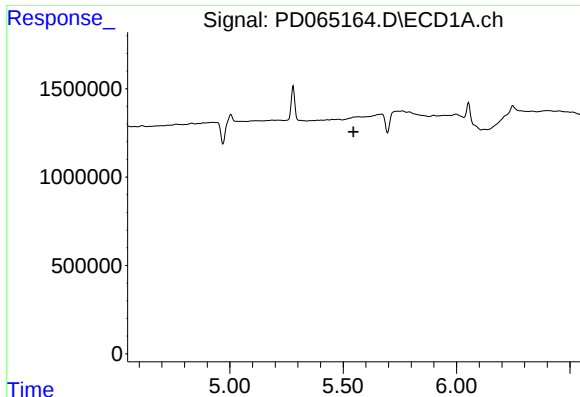

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.546 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

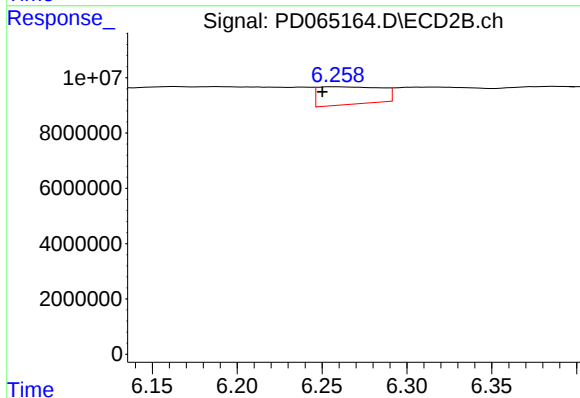


#9 Endosulfan I

R.T.: 6.259 min
Delta R.T.: 0.008 min
Response: 16430843
Conc: 2.33 ng/ml

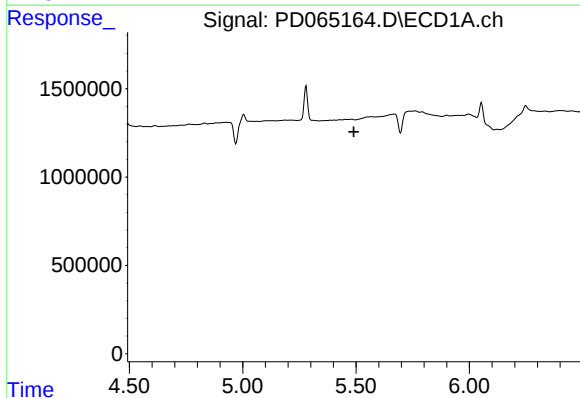


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.491 min
Response: 0
Conc: N.D.

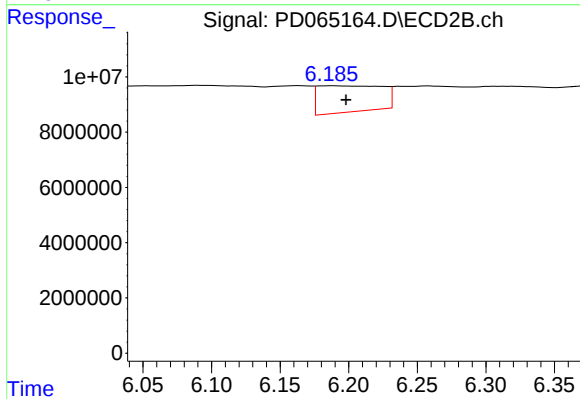

#11 alpha-Chlordane


R.T.: 6.188 min
Delta R.T.: -0.010 min
Response: 30960085
Conc: 4.16 ng/ml

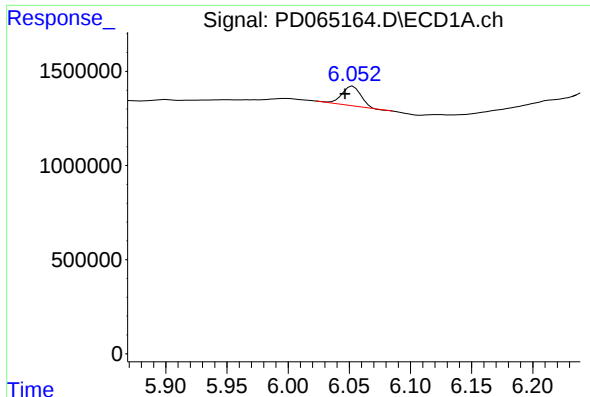

#14 Endrin


R.T.: 6.053 min
Delta R.T.: 0.007 min
Response: 1070382
Conc: 1.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

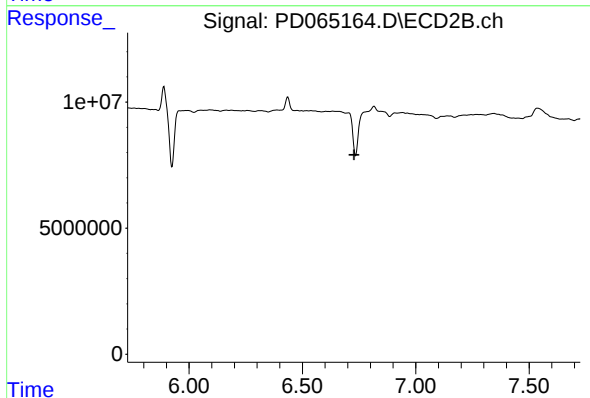


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.728 min
Response: 0
Conc: N.D.

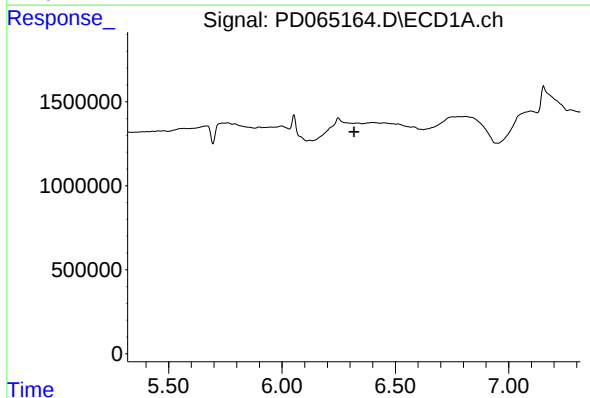


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.319 min
Response: 0
Conc: N.D.

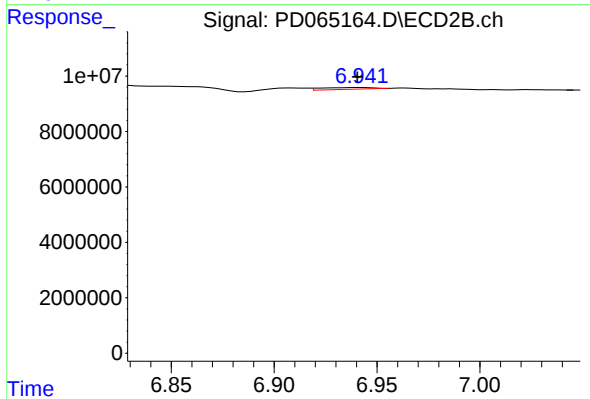

#15 Endosulfan II


R.T.: 6.942 min
Delta R.T.: 0.002 min
Response: 1122032
Conc: 0.19 ng/ml

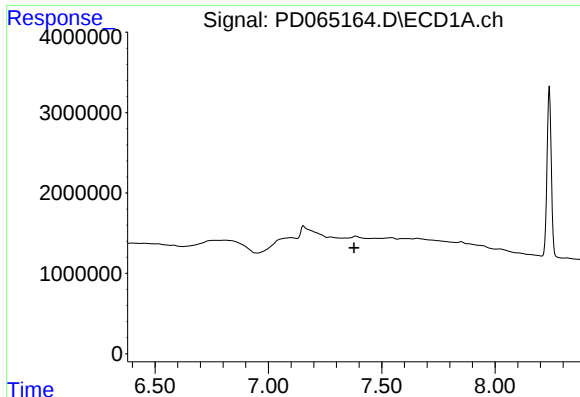

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.378 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

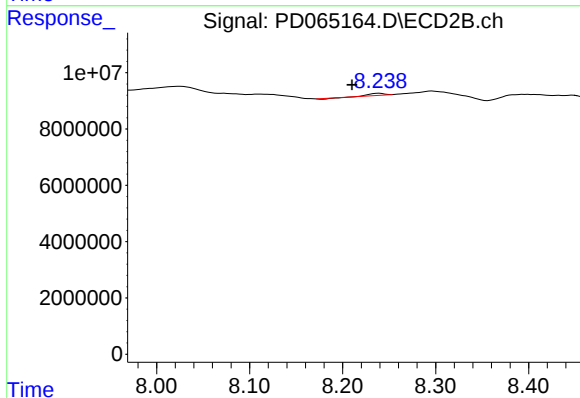


#22 Mirex

R.T.: 8.239 min
Delta R.T.: 0.029 min
Response: 472380
Conc: 0.11 ng/ml

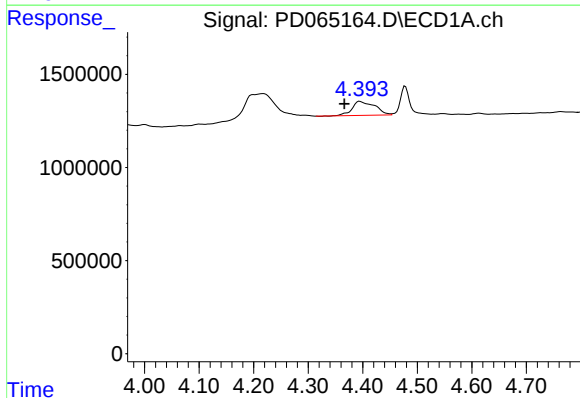


#23 Chlordane-1

R.T.: 4.395 min
Delta R.T.: 0.029 min
Response: 2193150
Conc: 57.91 ng/ml

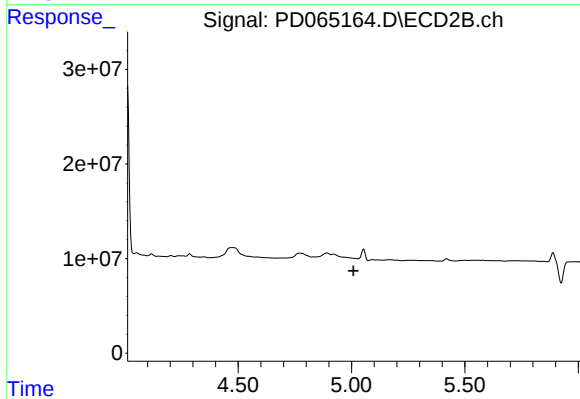

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.009 min
Response: 0
Conc: N.D.

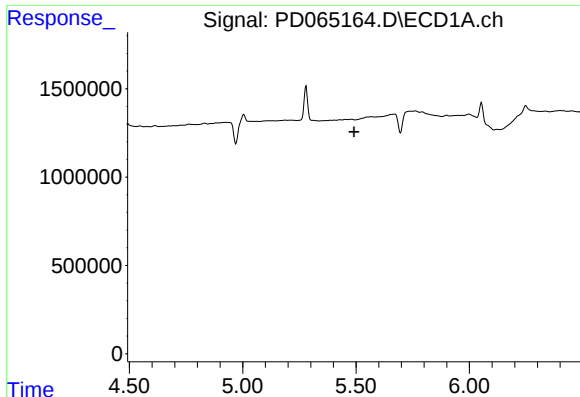

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.491 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

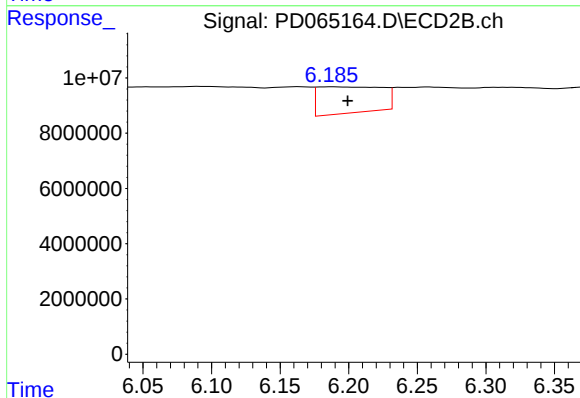


#26 Chlordane-4

R.T.: 6.188 min
Delta R.T.: -0.012 min
Response: 30960085
Conc: 25.75 ng/ml

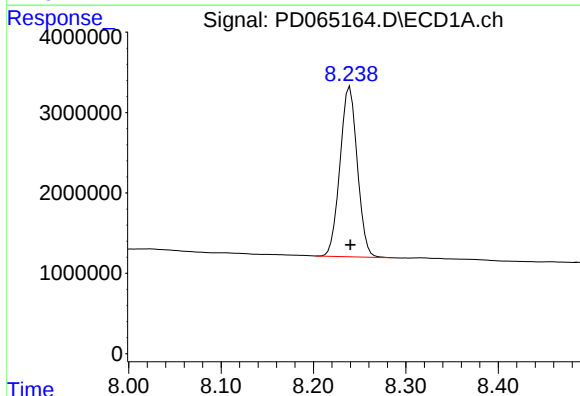

#28 Decachlorobiphenyl

R.T.: 8.240 min
Delta R.T.: 0.000 min
Response: 27535832
Conc: 24.30 ng/ml

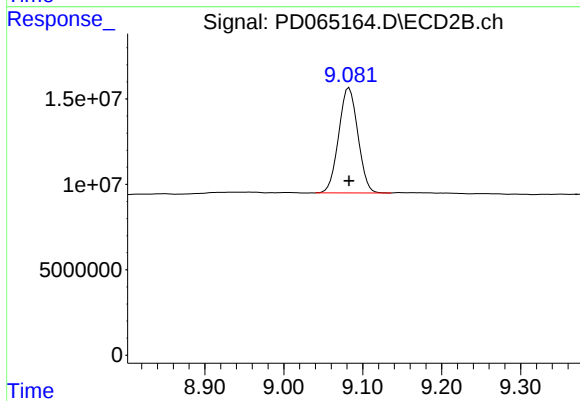

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: 0.000 min
Response: 103903124
Conc: 21.96 ng/ml