

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
 Data File : PD065186.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2021 15:47
 Operator : AR\AJ
 Sample : M3463-07
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SWCS-20-0306

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 01:52:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.012	11255163	88428623	10.950	11.164
28)	SA Decachlor...	8.243	9.085	5665115	20386359	5.000	4.308
Target Compounds							
3)	MA gamma-BHC...	0.000	4.702	0	6960797	N.D.	0.657 #
4)	MA Heptachlor	0.000	5.204	0	3329666	N.D.	0.332 #
7)	B delta-BHC	0.000	5.090	0	3681226	N.D.	0.379 #
14)	MA Endrin	6.057	0.000	1265312	0	1.206	N.D. #
15)	B Endosulfa...	0.000	6.943	0	3476827	N.D.	0.593 #
20)	A Methoxychlor	0.000	7.616	0	11868348	N.D.	3.922 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
Data File : PD065186.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2021 15:47
Operator : AR\AJ
Sample : M3463-07
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SWCS-20-0306

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 01:52:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

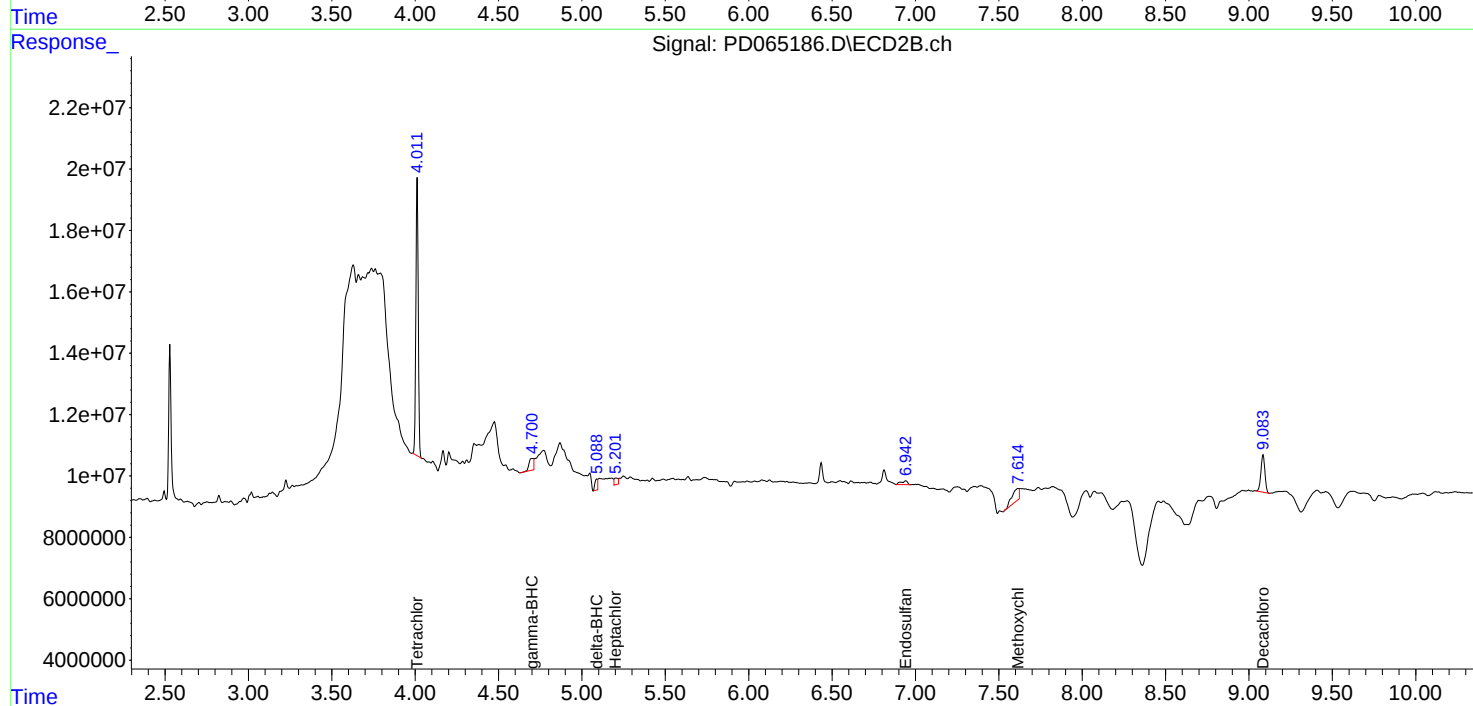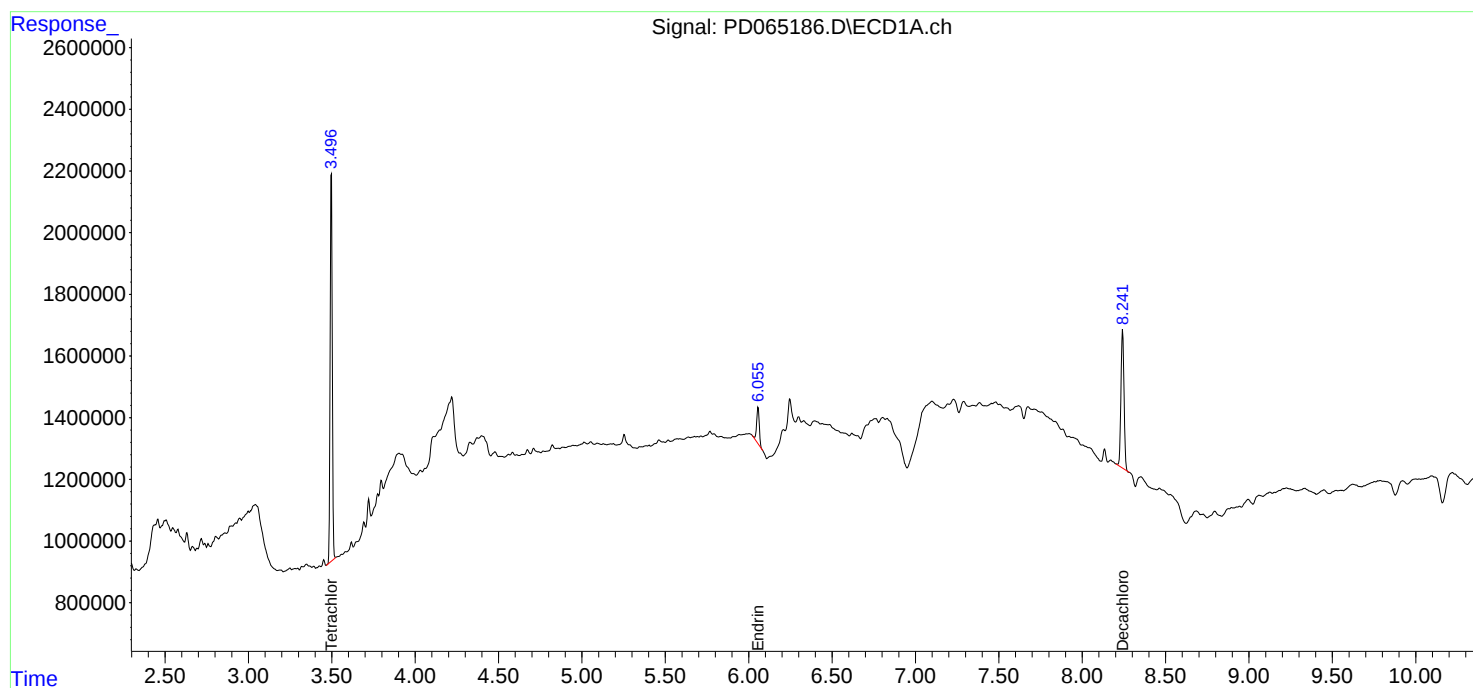


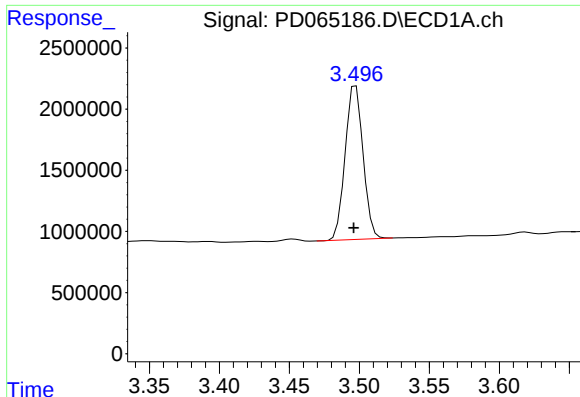

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.002 min
Response: 11255163
Conc: 10.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
SWCS-20-0306

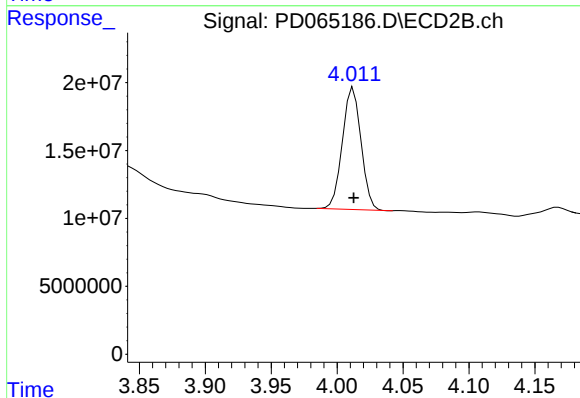


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 88428623
Conc: 11.16 ng/ml

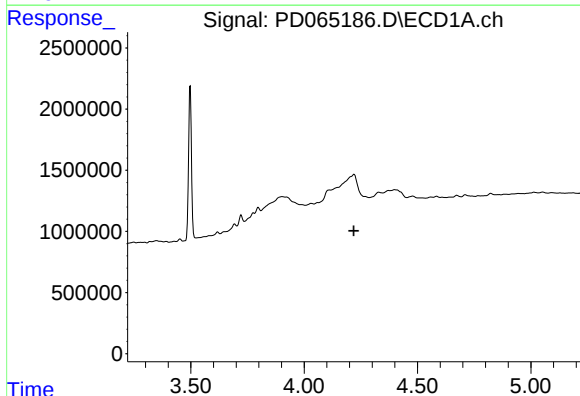


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.219 min
Response: 0
Conc: N.D.

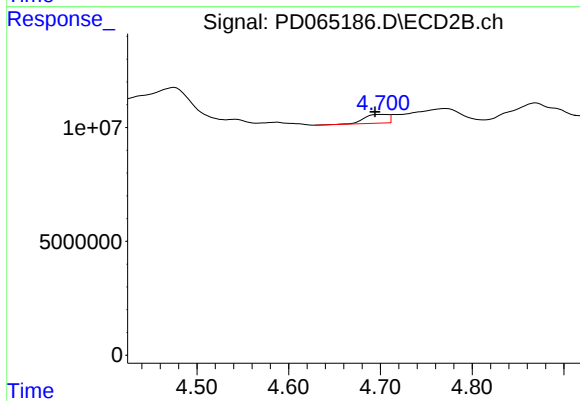

#3 gamma-BHC (Lindane)

R.T.: 4.702 min
Delta R.T.: 0.007 min
Response: 6960797
Conc: 0.66 ng/ml

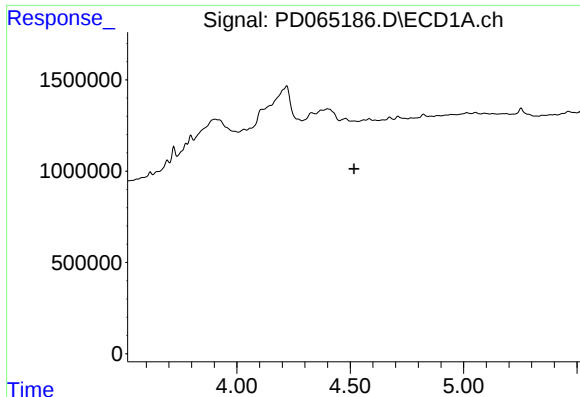

#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.517 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SWCS-20-0306

#4 Heptachlor


R.T.: 5.204 min
Delta R.T.: 0.006 min
Response: 3329666
Conc: 0.33 ng/ml

#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.670 min
Response: 0
Conc: N.D.

#7 delta-BHC


R.T.: 5.090 min
Delta R.T.: 0.003 min
Response: 3681226
Conc: 0.38 ng/ml

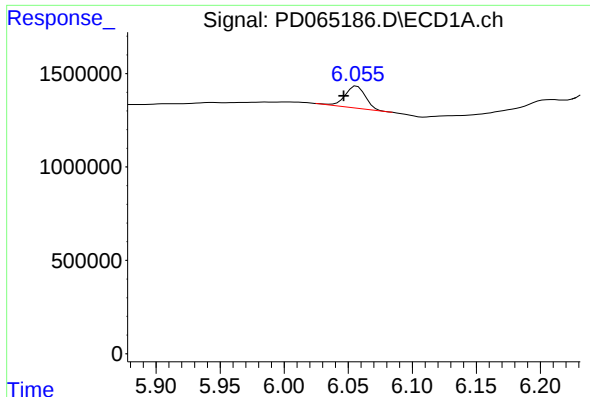

#14 Endrin


R.T.: 6.057 min
Delta R.T.: 0.010 min
Response: 1265312
Conc: 1.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
SWCS-20-0306

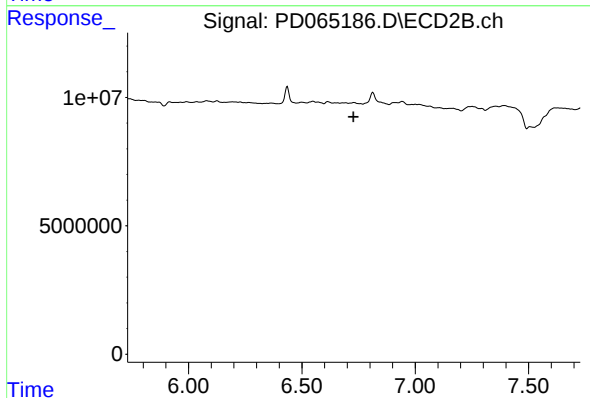


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.728 min
Response: 0
Conc: N.D.

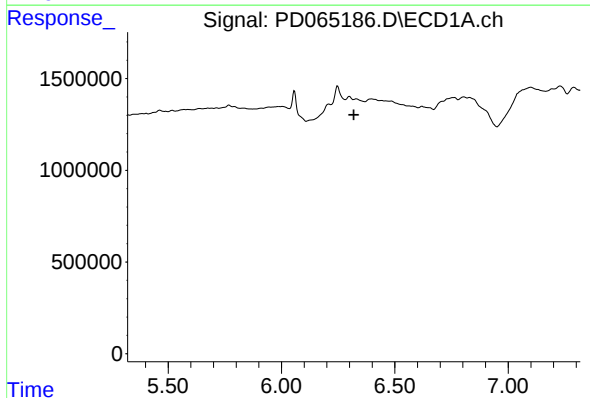


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.319 min
Response: 0
Conc: N.D.

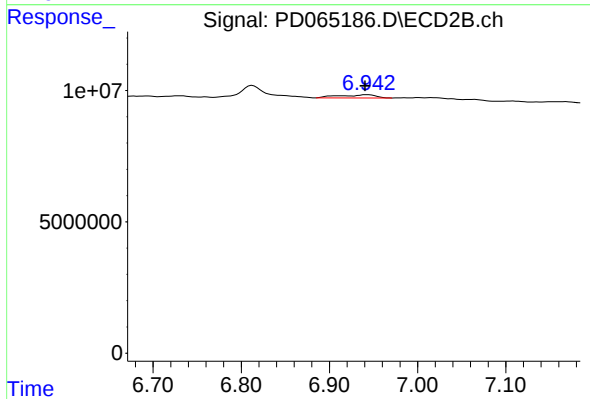

#15 Endosulfan II


R.T.: 6.943 min
Delta R.T.: 0.003 min
Response: 3476827
Conc: 0.59 ng/ml

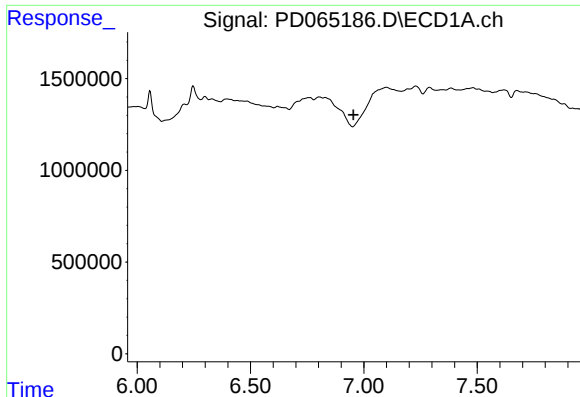

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.955 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SWCS-20-0306

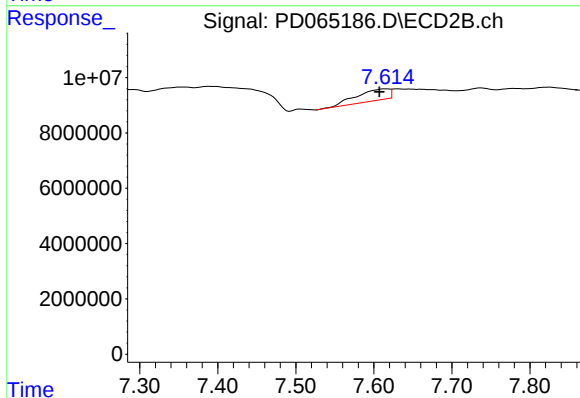


#20 Methoxychlor

R.T.: 7.616 min
Delta R.T.: 0.009 min
Response: 11868348
Conc: 3.92 ng/ml

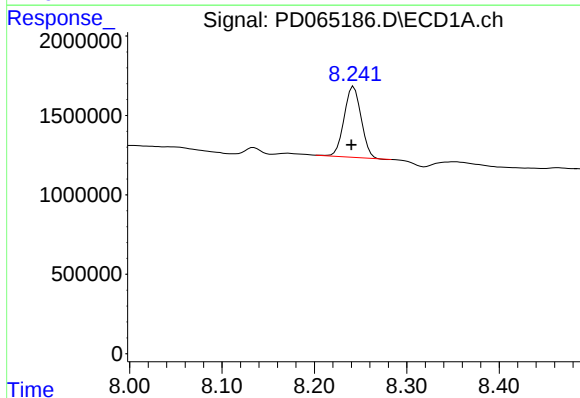

#28 Decachlorobiphenyl

R.T.: 8.243 min
Delta R.T.: 0.003 min
Response: 5665115
Conc: 5.00 ng/ml

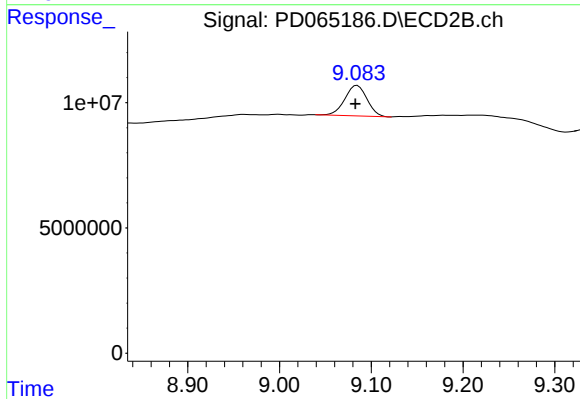

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.002 min
Response: 20386359
Conc: 4.31 ng/ml