

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
 Data File : PD065191.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2021 16:56
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 01:54:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	22828844	175.6E6	22.209	22.174
28)	SA Decachlor...	8.240	9.084	28115003	109.1E6	24.814	23.043
Target Compounds							
8)	B Heptachlo...	0.000	5.889	0	45568395	N.D.	6.108 #
14)	MA Endrin	6.054	0.000	2099248	0	2.000	N.D. #
15)	B Endosulfa...	0.000	6.944	0	654290	N.D.	0.112 #
20)	A Methoxychlor	0.000	7.634f	0	393523	N.D.	0.130 #
23)	Chlordane-1	4.394f	0.000	1181738	0	31.203	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
Data File : PD065191.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2021 16:56
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 01:54:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

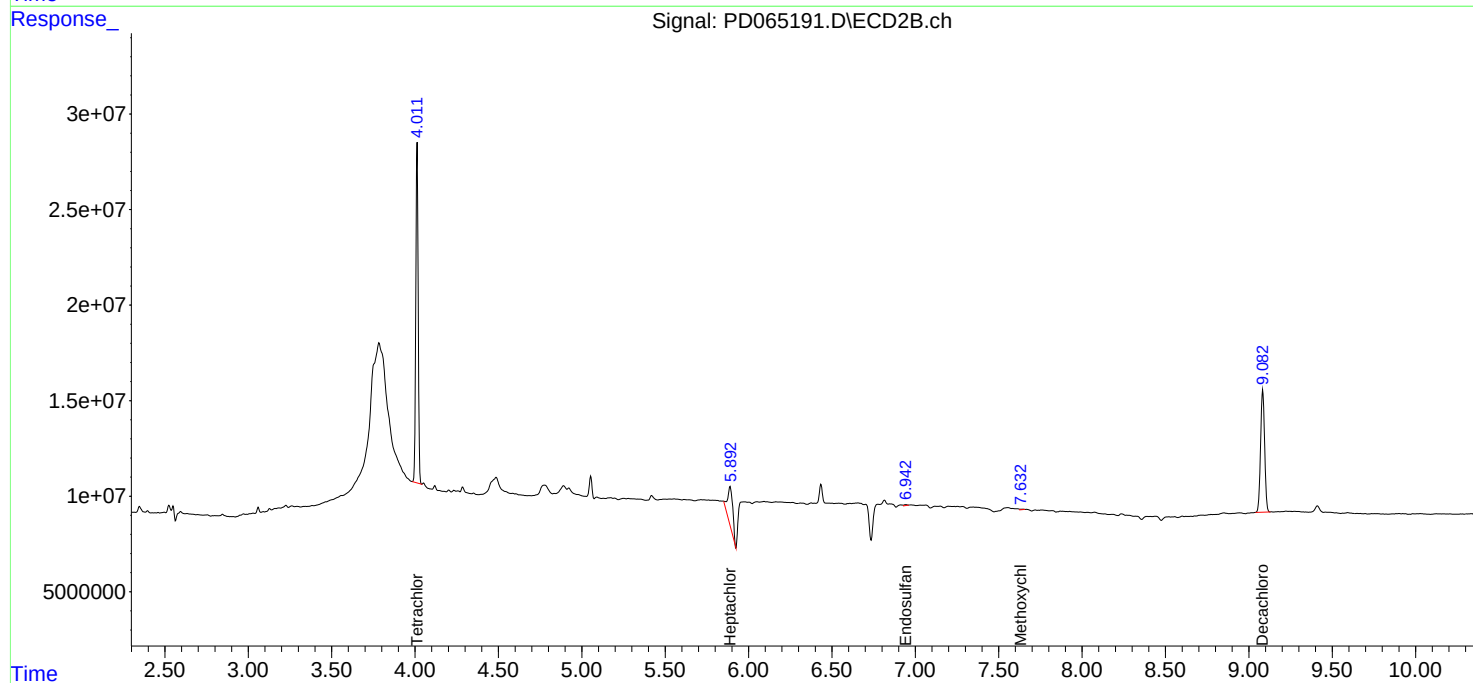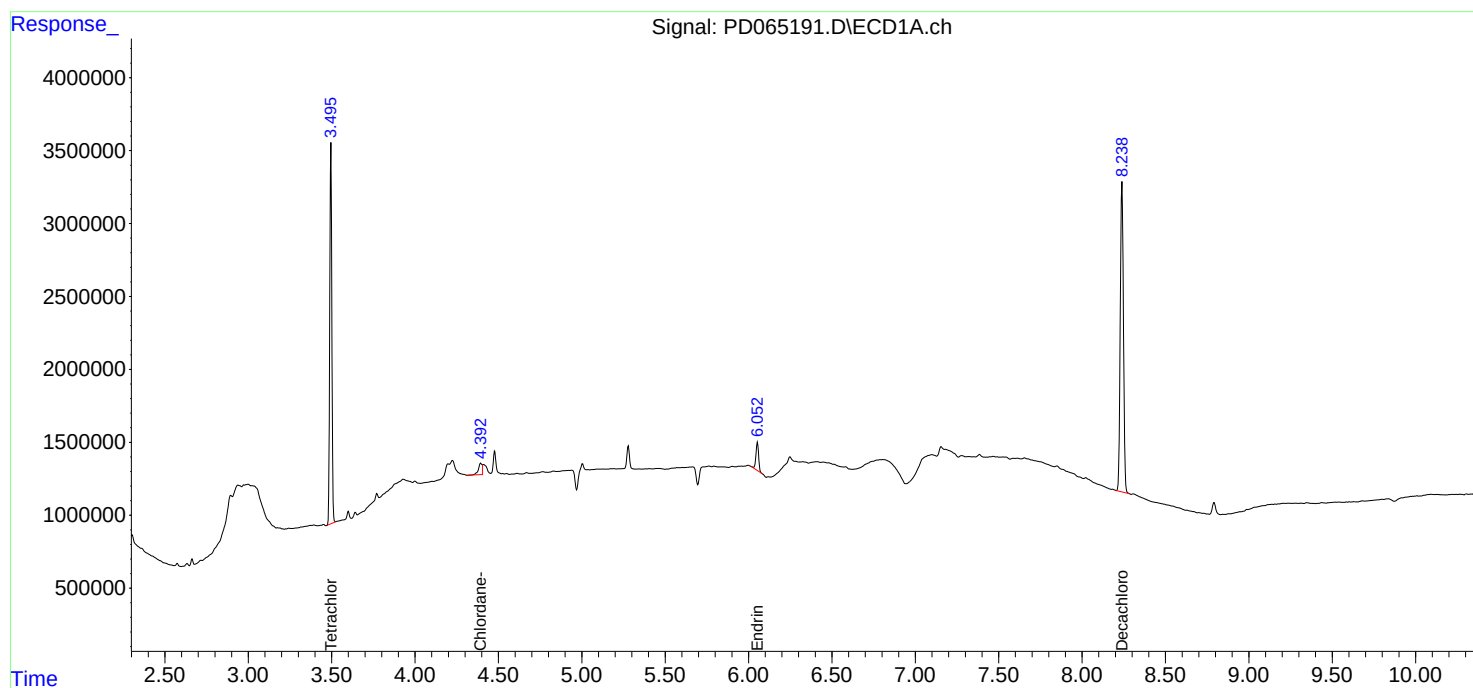


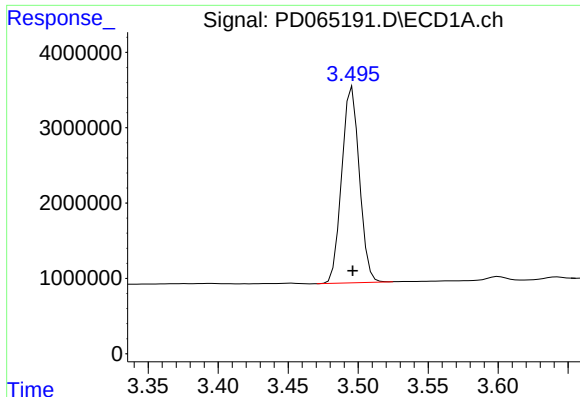

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 22828844
Conc: 22.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

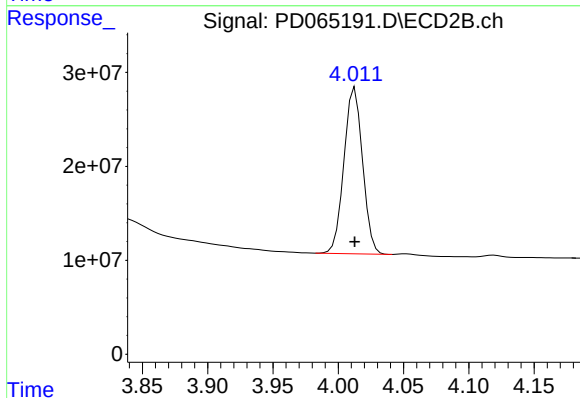


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 175630624
Conc: 22.17 ng/ml

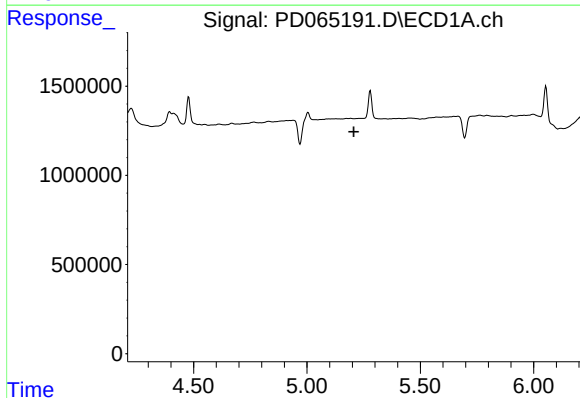


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.207 min
Response: 0
Conc: N.D.

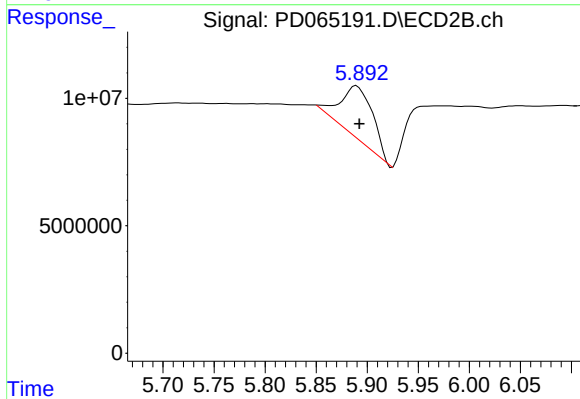

#8 Heptachlor epoxide


R.T.: 5.889 min
Delta R.T.: -0.003 min
Response: 45568395
Conc: 6.11 ng/ml

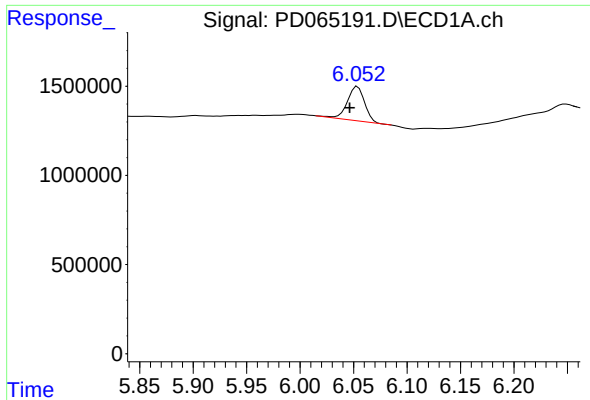

#14 Endrin


R.T.: 6.054 min
Delta R.T.: 0.007 min
Response: 2099248
Conc: 2.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

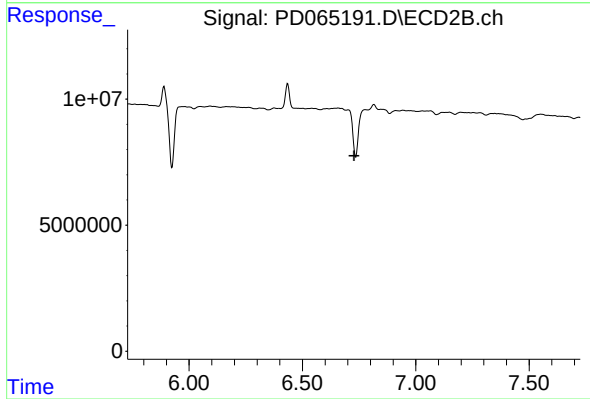


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.728 min
Response: 0
Conc: N.D.

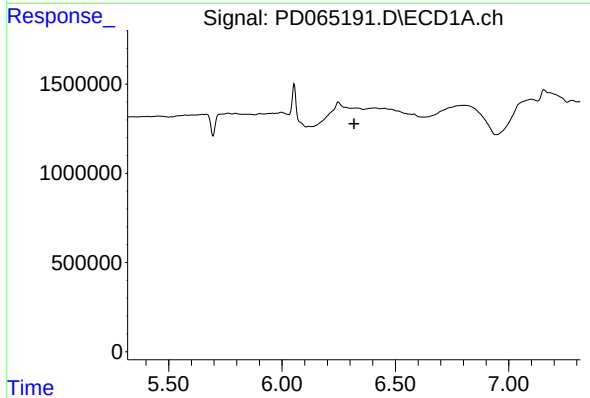


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.319 min
Response: 0
Conc: N.D.

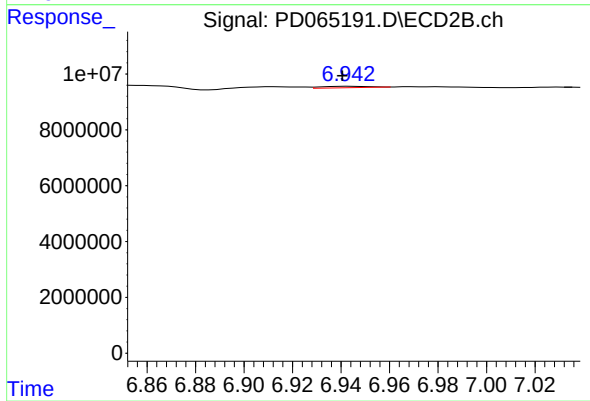

#15 Endosulfan II


R.T.: 6.944 min
Delta R.T.: 0.004 min
Response: 654290
Conc: 0.11 ng/ml

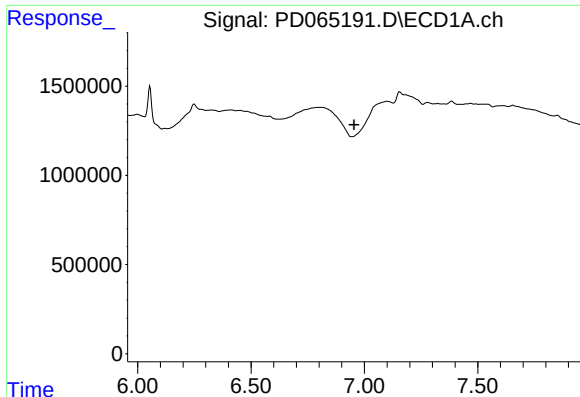

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.955 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

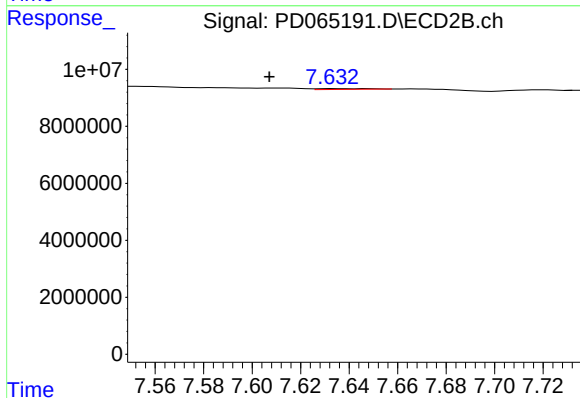


#20 Methoxychlor

R.T.: 7.634 min
Delta R.T.: 0.026 min
Response: 393523
Conc: 0.13 ng/ml

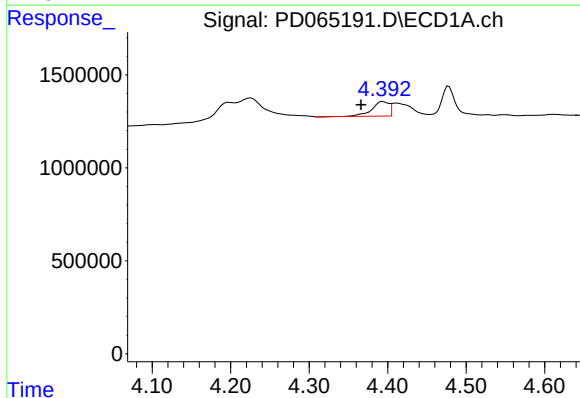


#23 Chlordane-1

R.T.: 4.394 min
Delta R.T.: 0.028 min
Response: 1181738
Conc: 31.20 ng/ml

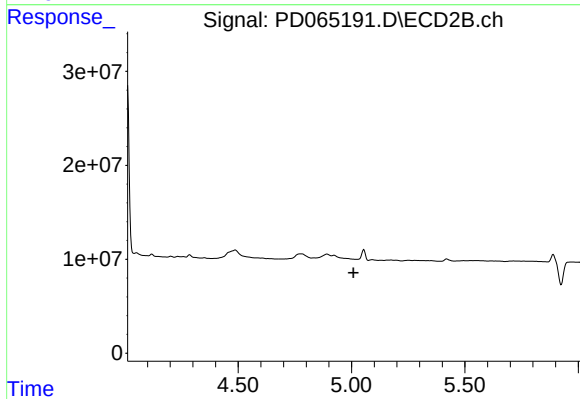

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.009 min
Response: 0
Conc: N.D.

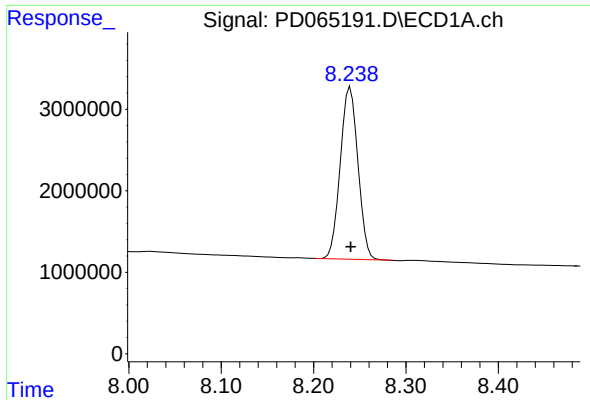

#28 Decachlorobiphenyl

R.T.: 8.240 min
Delta R.T.: 0.000 min
Response: 28115003
Conc: 24.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

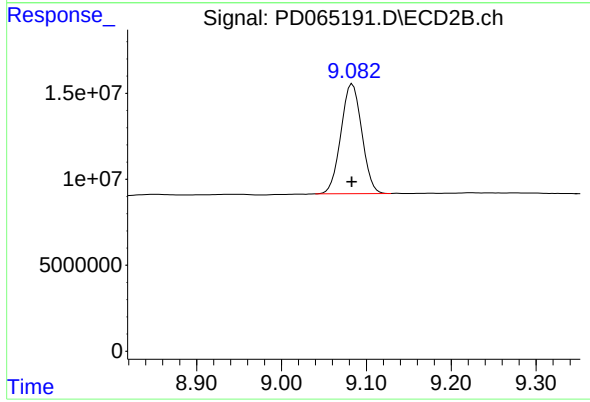

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 109053961
Conc: 23.04 ng/ml