

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
 Data File : PD065197.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2021 18:59
 Operator : AR\AJ
 Sample : M3463-27
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SWCS-23-0204

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 01:55:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	15526141	117.9E6	15.105	14.890
28)	SA Decachlor...	8.240	9.084	12463035	46952193	11.000	9.921
Target Compounds							
3)	MA gamma-BHC...	4.222	0.000	1539688	0	1.122	N.D. #
4)	MA Heptachlor	0.000	5.207	0	10268173	N.D.	1.024 #
10)	B gamma-Chl...	0.000	6.127	0	225574	N.D.	0.030 #
15)	B Endosulfa...	0.000	6.917f	0	776553	N.D.	0.132 #
25)	Chlordane-3	0.000	6.127	0	225574	N.D.	0.218 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
Data File : PD065197.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2021 18:59
Operator : AR\AJ
Sample : M3463-27
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SWCS-23-0204

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 01:55:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

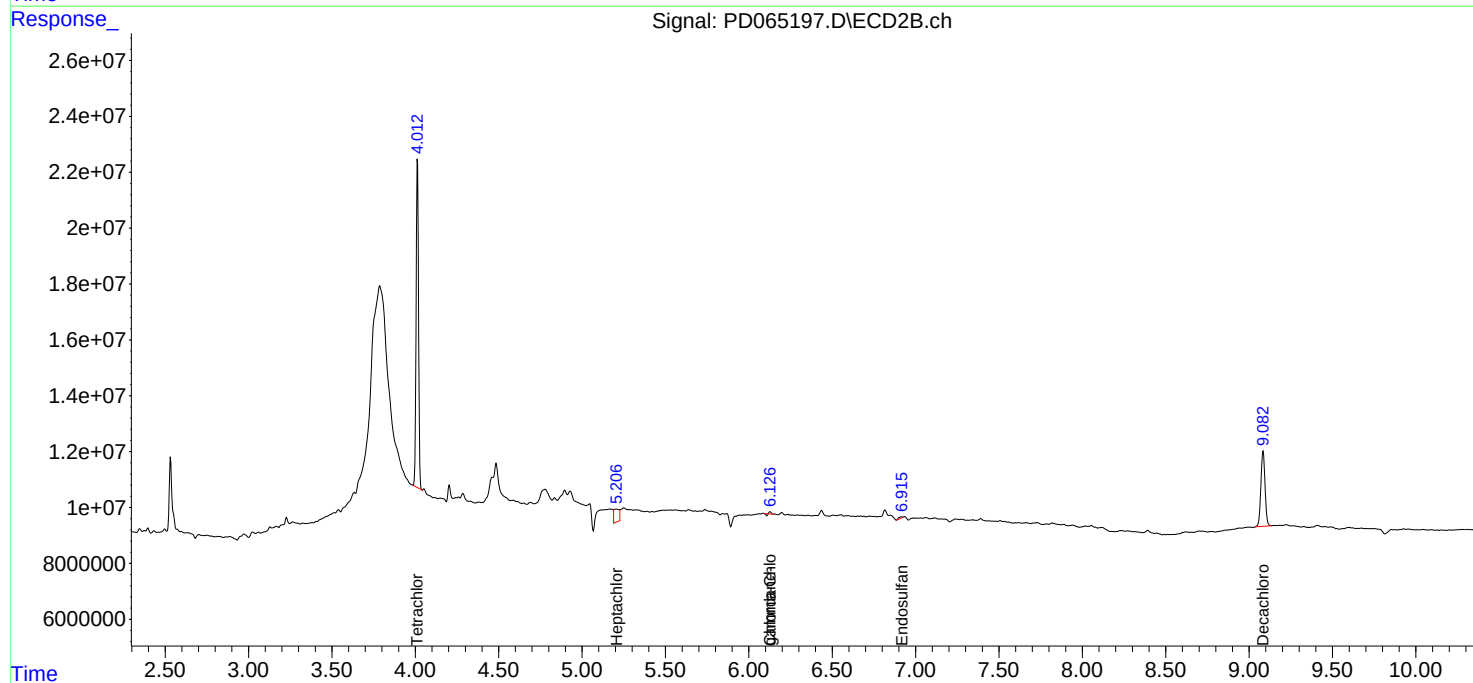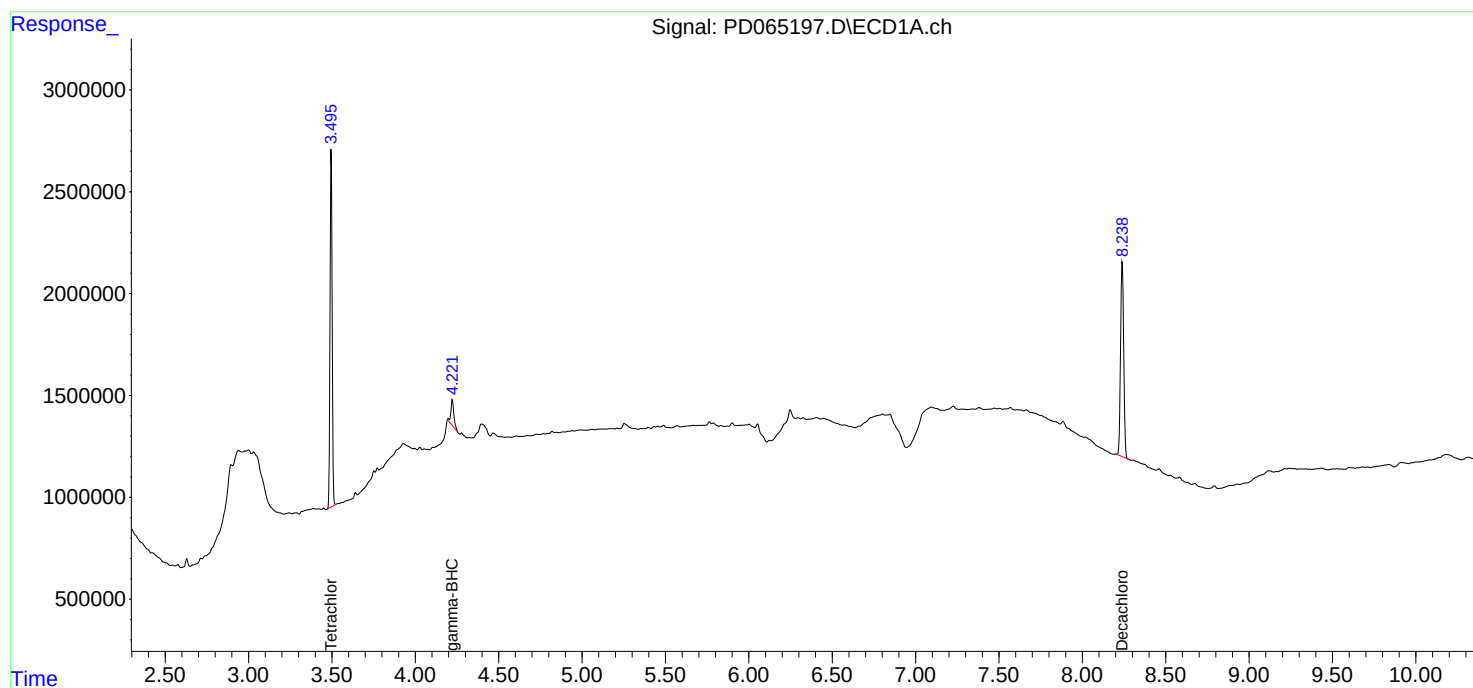


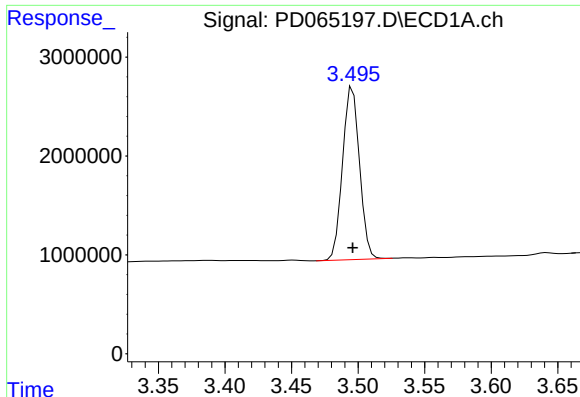

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 15526141
Conc: 15.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
SWCS-23-0204

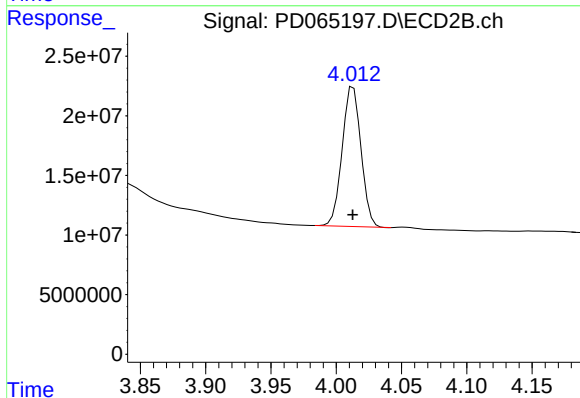


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 117935936
Conc: 14.89 ng/ml

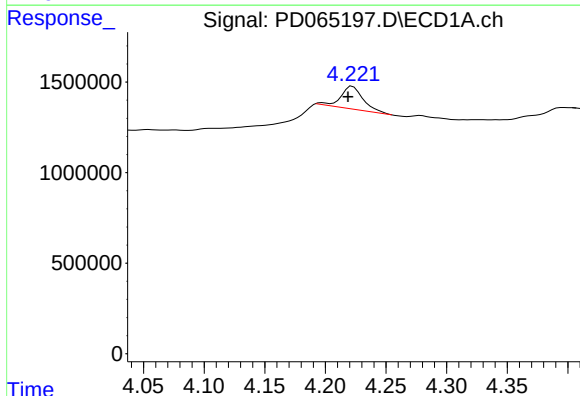


#3 gamma-BHC (Lindane)

R.T.: 4.222 min
Delta R.T.: 0.004 min
Response: 1539688
Conc: 1.12 ng/ml

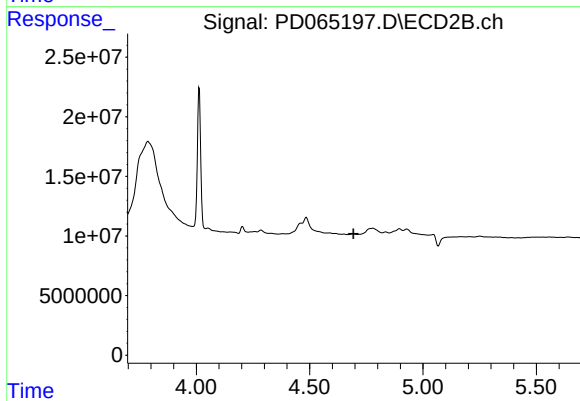

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.694 min
Response: 0
Conc: N.D.

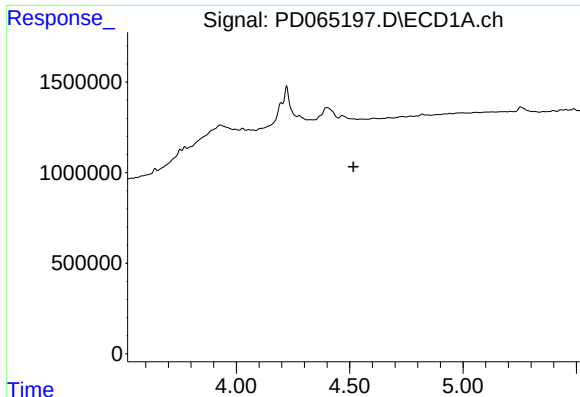

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.517 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SWCS-23-0204

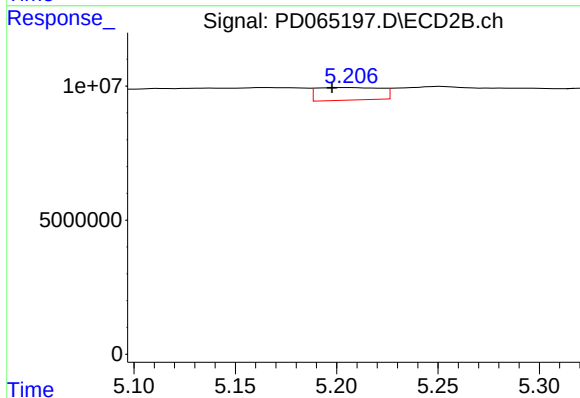


#4 Heptachlor

R.T.: 5.207 min
Delta R.T.: 0.009 min
Response: 10268173
Conc: 1.02 ng/ml

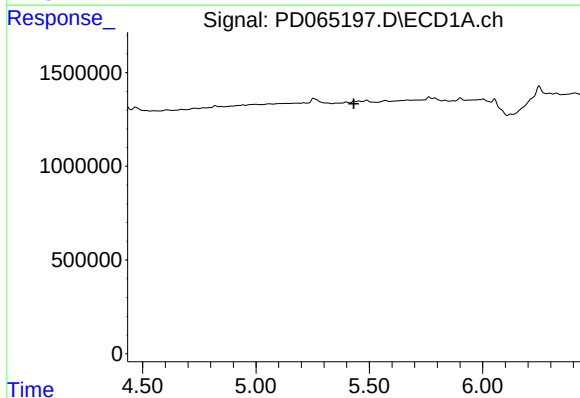


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.432 min
Response: 0
Conc: N.D.

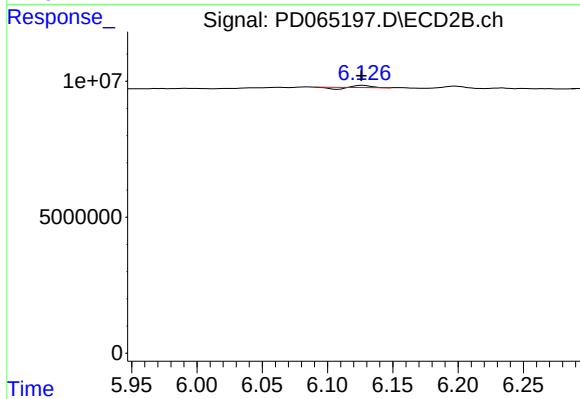

#10 gamma-Chlordane


R.T.: 6.127 min
Delta R.T.: 0.001 min
Response: 225574
Conc: 0.03 ng/ml

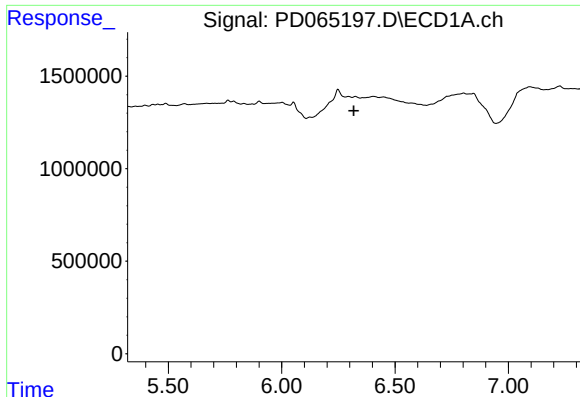

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SWCS-23-0204

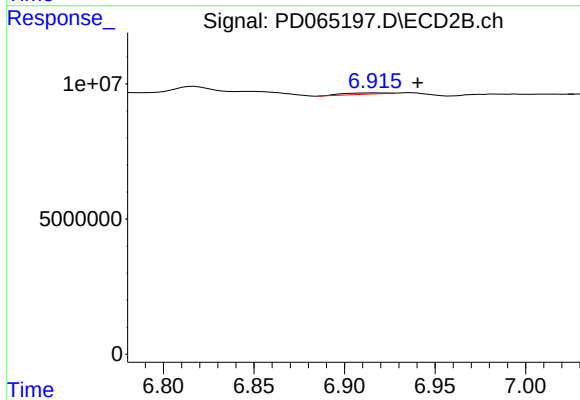


#15 Endosulfan II

R.T.: 6.917 min
Delta R.T.: -0.024 min
Response: 776553
Conc: 0.13 ng/ml

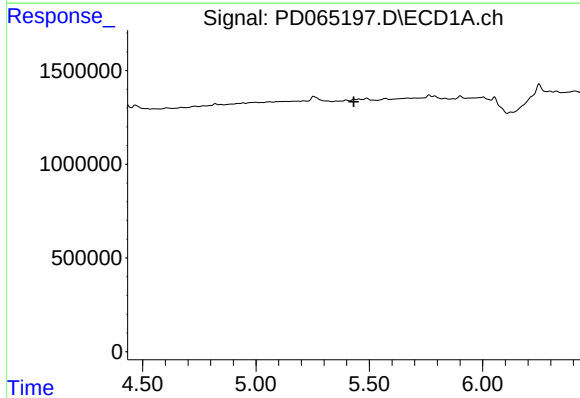


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.432 min
Response: 0
Conc: N.D.

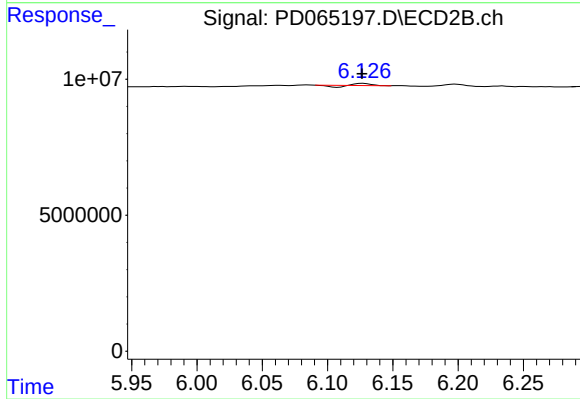

#25 Chlordane-3


R.T.: 6.127 min
Delta R.T.: 0.001 min
Response: 225574
Conc: 0.22 ng/ml

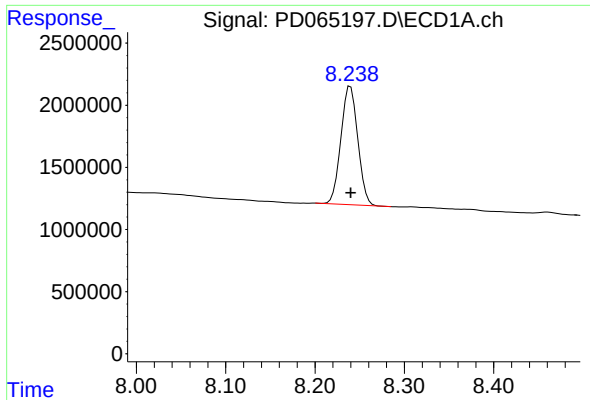

#28 Decachlorobiphenyl

R.T.: 8.240 min
Delta R.T.: 0.000 min
Response: 12463035
Conc: 11.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
SWCS-23-0204

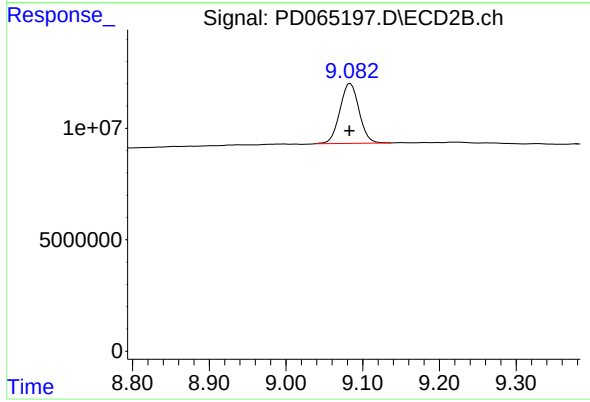

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.001 min
Response: 46952193
Conc: 9.92 ng/ml