

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
 Data File : PD065201.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2021 19:54
 Operator : AR\AJ
 Sample : M3463-35
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SWCS-27-0204

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 01:56:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	19546333	148.4E6	19.016	18.737
28)	SA Decachlor...	8.239	9.083	17772095	66338262	15.685	14.018
Target Compounds							
2)	A alpha-BHC	0.000	4.431f	0	14742884	N.D.	1.269 #
10)	B gamma-Chl...	0.000	6.126	0	345767	N.D.	0.045 #
11)	B alpha-Chl...	0.000	6.198	0	2875557	N.D.	0.386 #
13)	MA Dieldrin	5.788	6.507	824717	2088961	0.735	0.288 #
20)	A Methoxychlor	0.000	7.597	0	4094213	N.D.	1.353 #
23)	Chlordane-1	4.395f	0.000	1919979	0	50.697	N.D. #
25)	Chlordane-3	0.000	6.126	0	345767	N.D.	0.334 #
26)	Chlordane-4	0.000	6.198	0	2875557	N.D.	2.392 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
Data File : PD065201.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2021 19:54
Operator : AR\AJ
Sample : M3463-35
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SWCS-27-0204

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 01:56:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

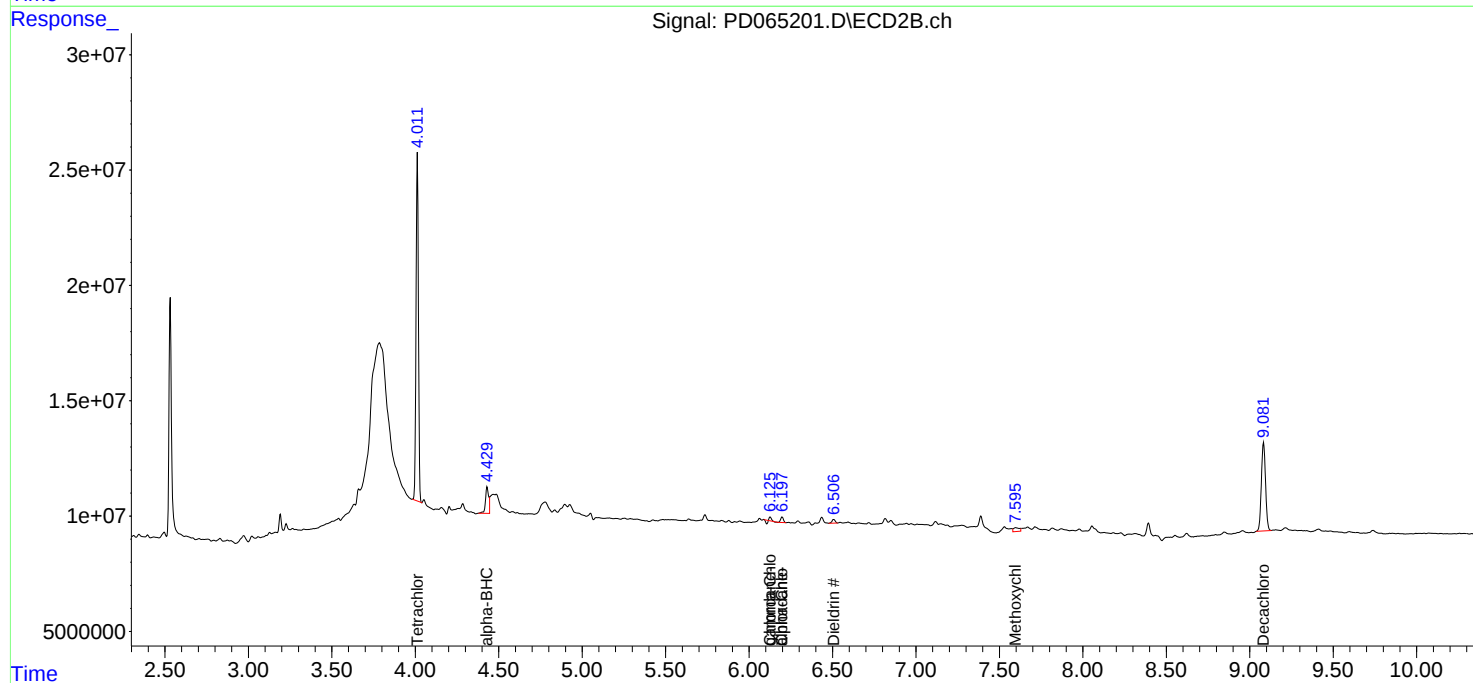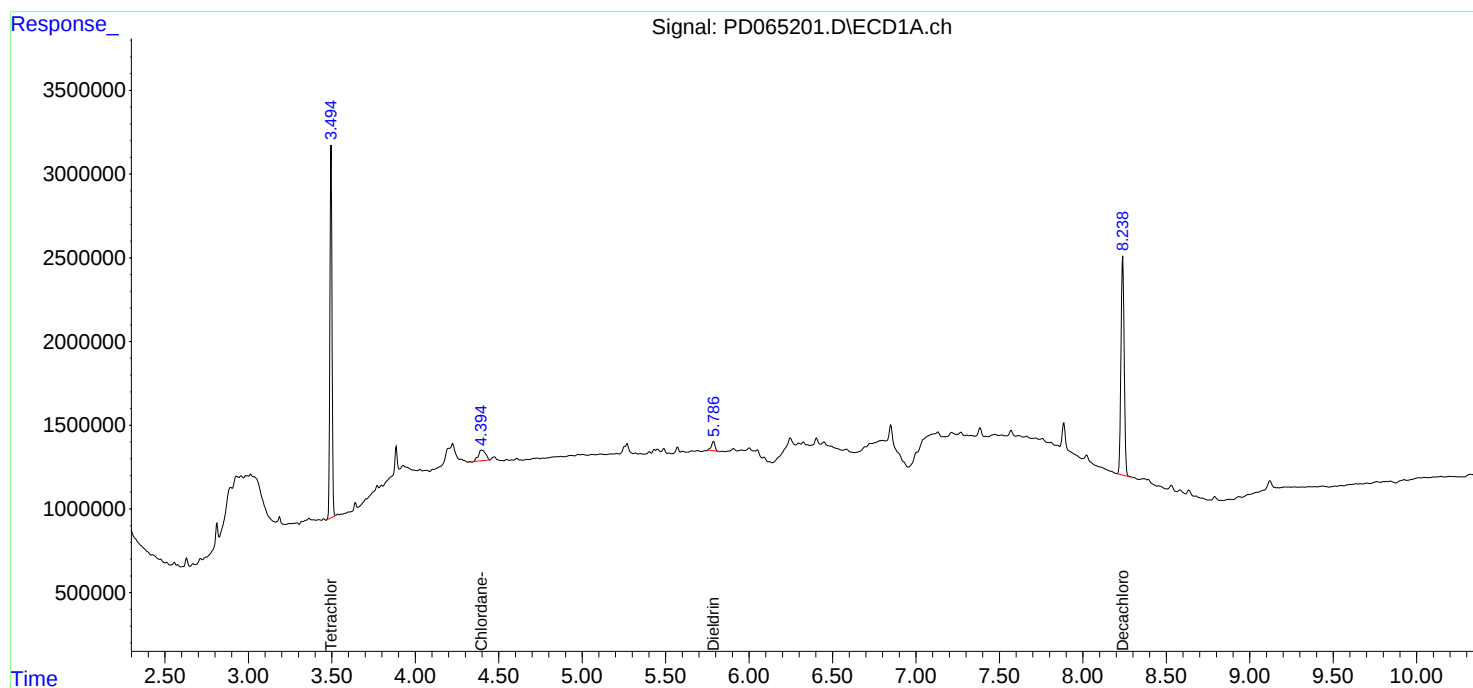


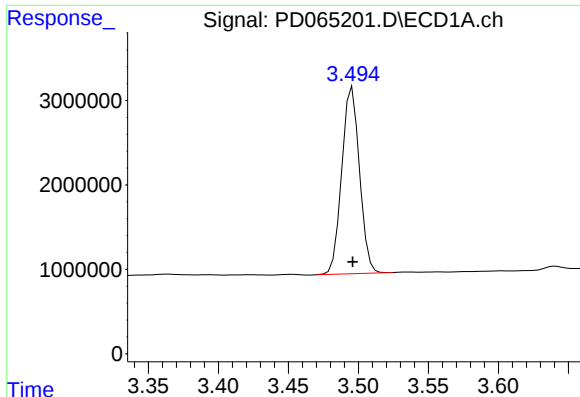

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 19546333
Conc: 19.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
SWCS-27-0204

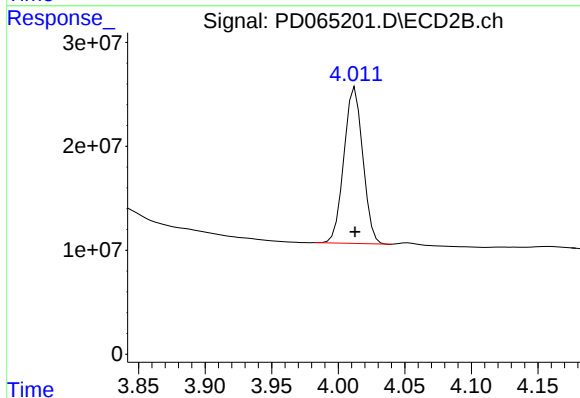


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 148409627
Conc: 18.74 ng/ml

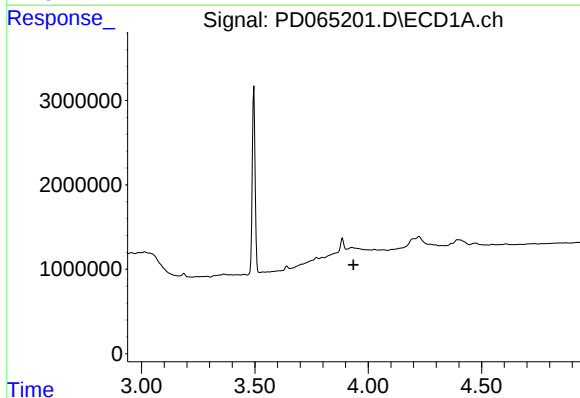


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.935 min
Response: 0
Conc: N.D.

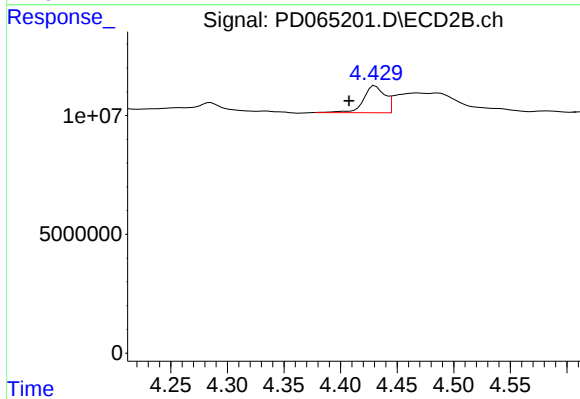

#2 alpha-BHC


R.T.: 4.431 min
Delta R.T.: 0.023 min
Response: 14742884
Conc: 1.27 ng/ml

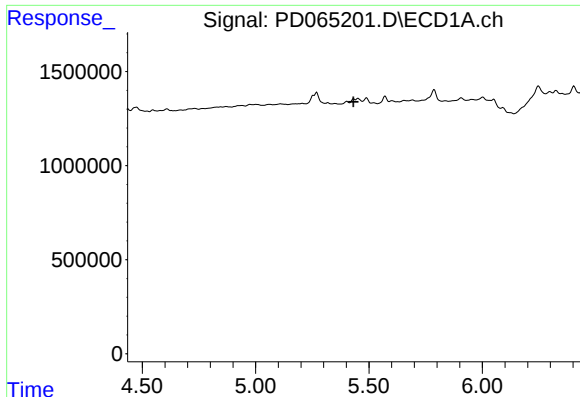

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SWCS-27-0204

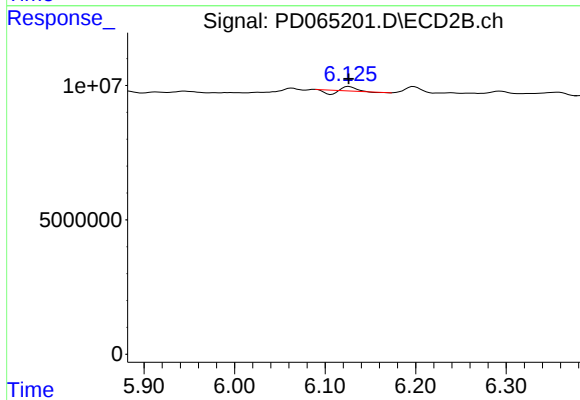


#10 gamma-Chlordane

R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 345767
Conc: 0.05 ng/ml

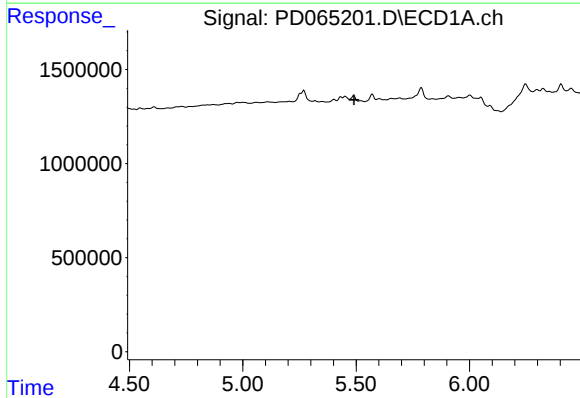


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.491 min
Response: 0
Conc: N.D.

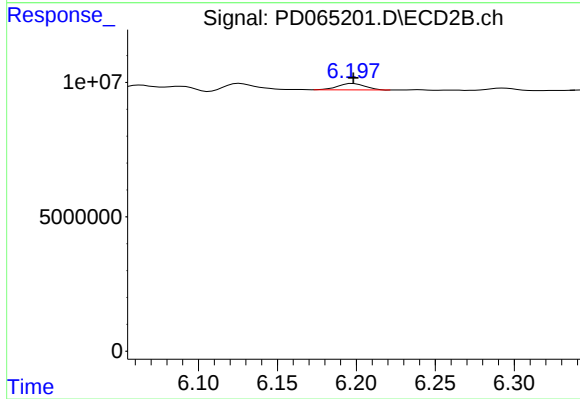

#11 alpha-Chlordane


R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 2875557
Conc: 0.39 ng/ml

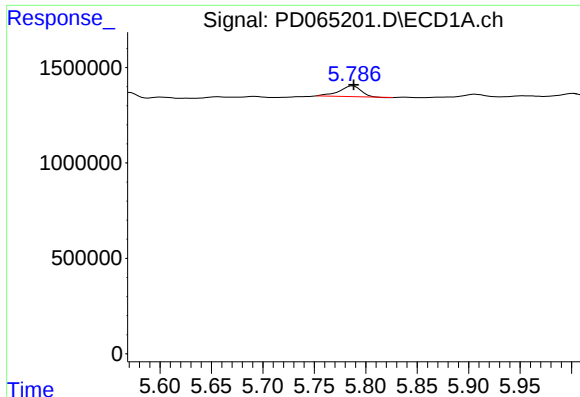

#13 Dieldrin


R.T.: 5.788 min
Delta R.T.: 0.000 min
Response: 824717
Conc: 0.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
SWCS-27-0204

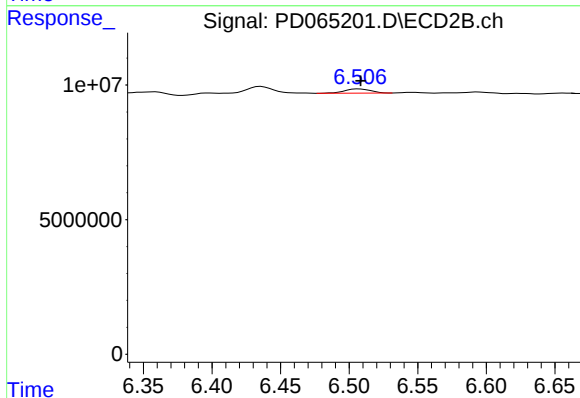


#13 Dieldrin

R.T.: 6.507 min
Delta R.T.: -0.001 min
Response: 2088961
Conc: 0.29 ng/ml

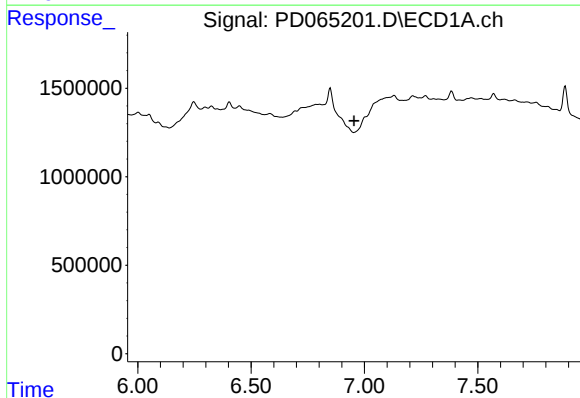


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.955 min
Response: 0
Conc: N.D.

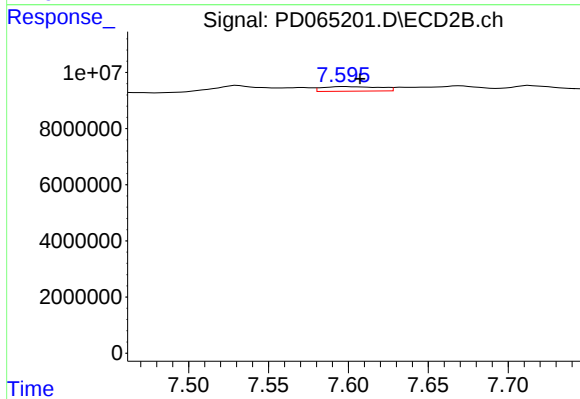

#20 Methoxychlor


R.T.: 7.597 min
Delta R.T.: -0.010 min
Response: 4094213
Conc: 1.35 ng/ml

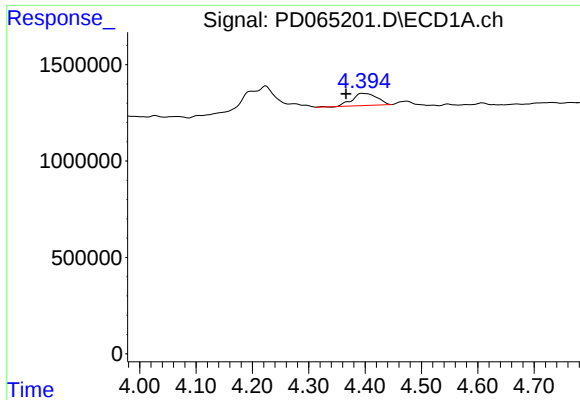

#23 Chlordane-1


R.T.: 4.395 min
Delta R.T.: 0.029 min
Response: 1919979
Conc: 50.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
SWCS-27-0204

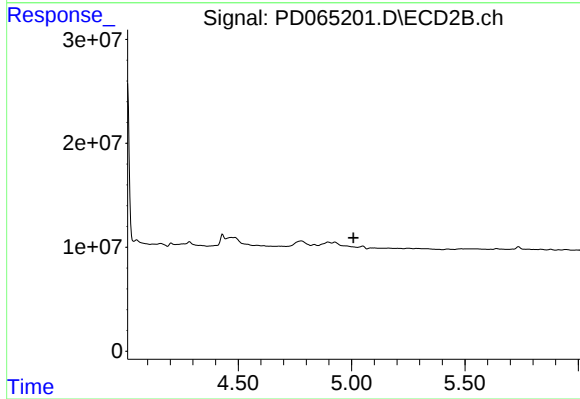


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.009 min
Response: 0
Conc: N.D.

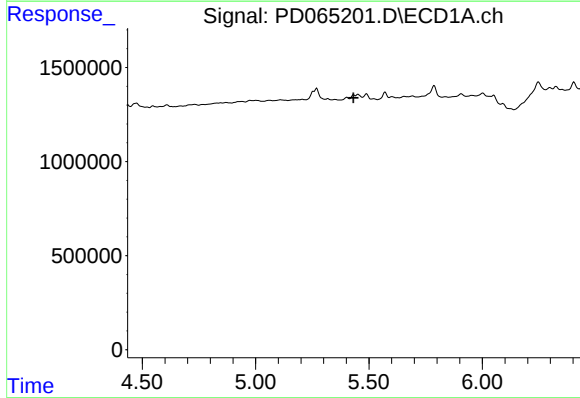


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.432 min
Response: 0
Conc: N.D.

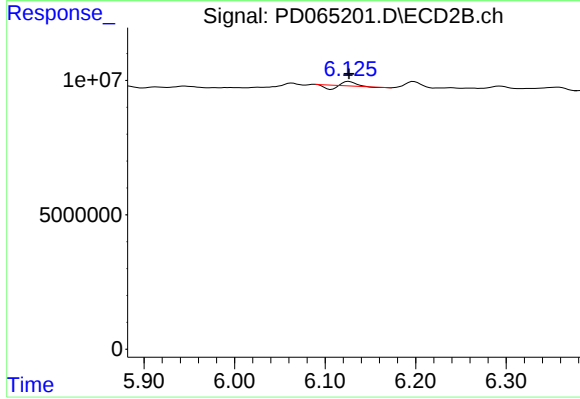

#25 Chlordane-3


R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 345767
Conc: 0.33 ng/ml

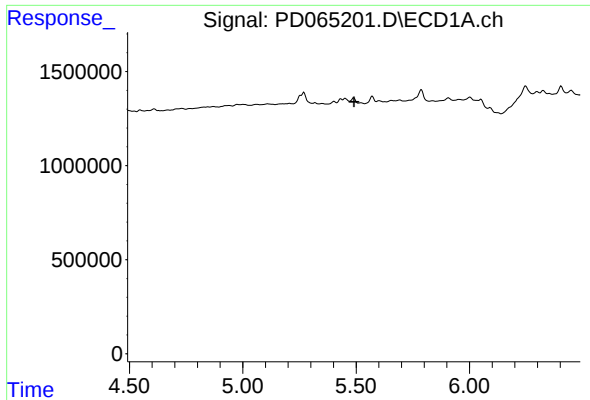

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.491 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SWCS-27-0204

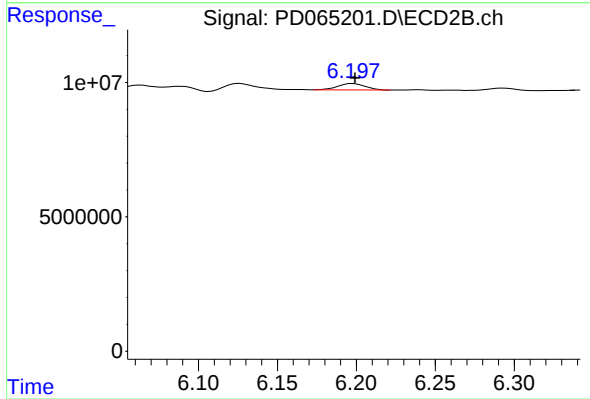


#26 Chlordane-4

R.T.: 6.198 min
Delta R.T.: -0.001 min
Response: 2875557
Conc: 2.39 ng/ml

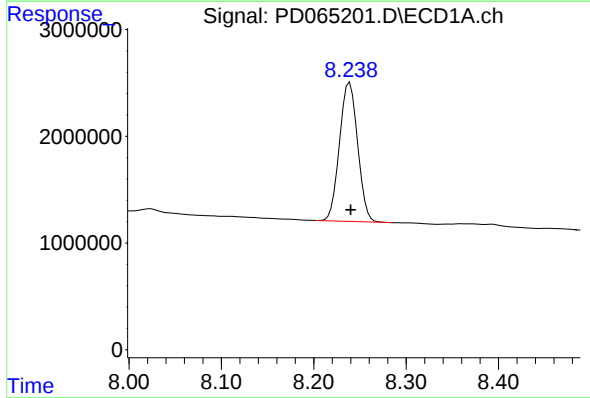

#28 Decachlorobiphenyl

R.T.: 8.239 min
Delta R.T.: -0.001 min
Response: 17772095
Conc: 15.69 ng/ml

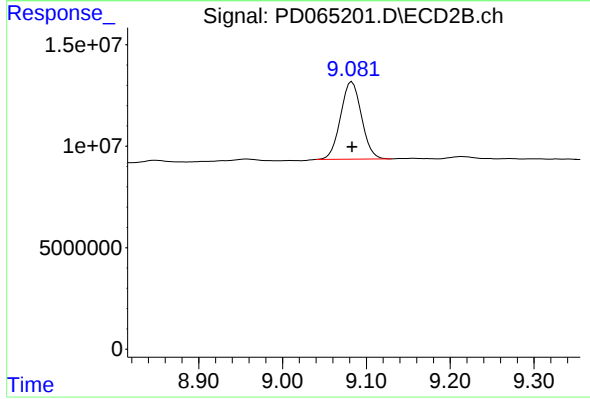

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: 0.000 min
Response: 66338262
Conc: 14.02 ng/ml