

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
 Data File : PD065100.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2021 12:18
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 02:03:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:56:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.496	4.012	50974938	393.6E6	49.375	49.350
7) SA Decachlor...	8.240	9.082	59460964	245.9E6	49.001	50.607
Target Compounds						
2) Toxaphene-1	5.748	6.406	4367642	18215680	493.706	496.840
3) Toxaphene-2	5.909	6.598	4562229	29740349	494.938	489.734
4) Toxaphene-3	6.351	7.181	10318357	53989359	494.391	503.176
5) Toxaphene-4	6.597	7.267	11065004	53899776	491.657	515.410
6) Toxaphene-5	7.082	7.685	12742312	43206435	486.094	511.407

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
Data File : PD065100.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2021 12:18
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 02:03:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:56:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

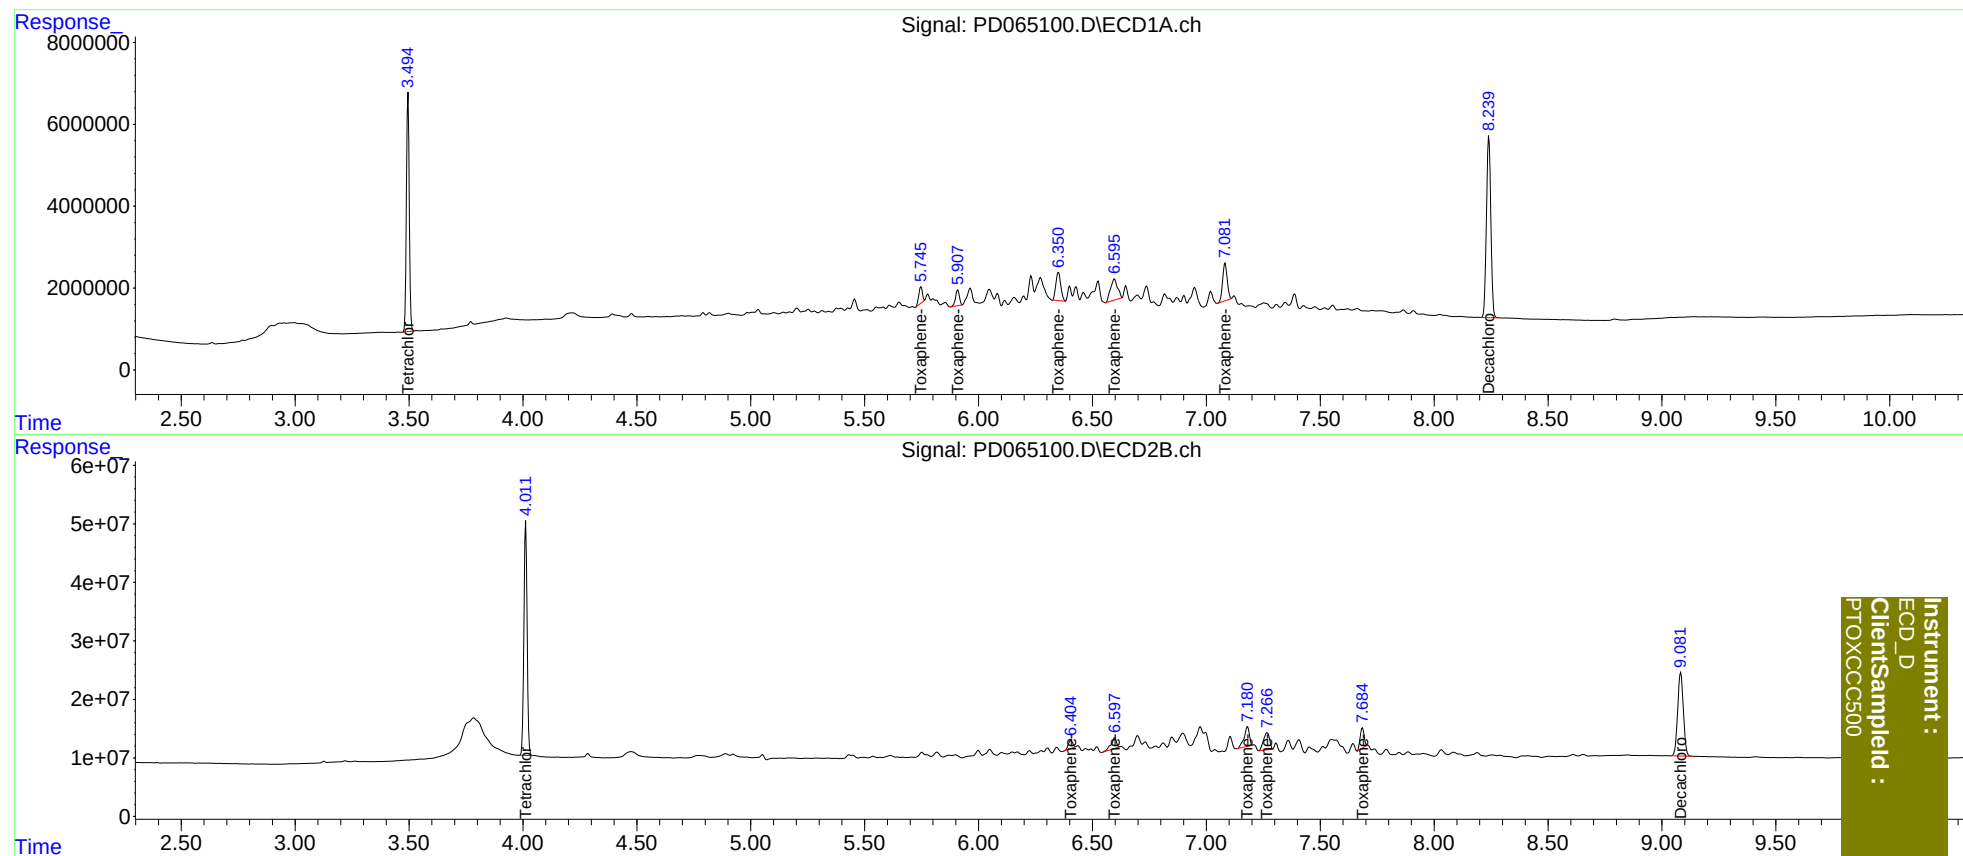

Instrument :
ECD_D
ClientSampled :
PTOXC500