

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
 Data File : PD065112.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2021 16:38
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Manual Integrations
 APPROVED

mohammad
 8/23/2021 2:23:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 02:05:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:56:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.496	4.013	50956742	373.8E6	49.358	46.879
7) SA Decachlor...	8.240	9.084	61041946	247.2E6	50.304	50.877
Target Compounds						
2) Toxaphene-1	5.748	6.404	4279622	15309714	483.756	417.579m
3) Toxaphene-2	5.909	6.599	4637407	24730587	503.094	407.239
4) Toxaphene-3	6.351	7.183	10239037	51162854	490.590	476.834
5) Toxaphene-4	6.597	7.268	11329452	54571200	503.407	521.830
6) Toxaphene-5	7.083	7.686	12564909	42549743	479.327	503.635

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
Data File : PD065112.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2021 16:38
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 02:05:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:56:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

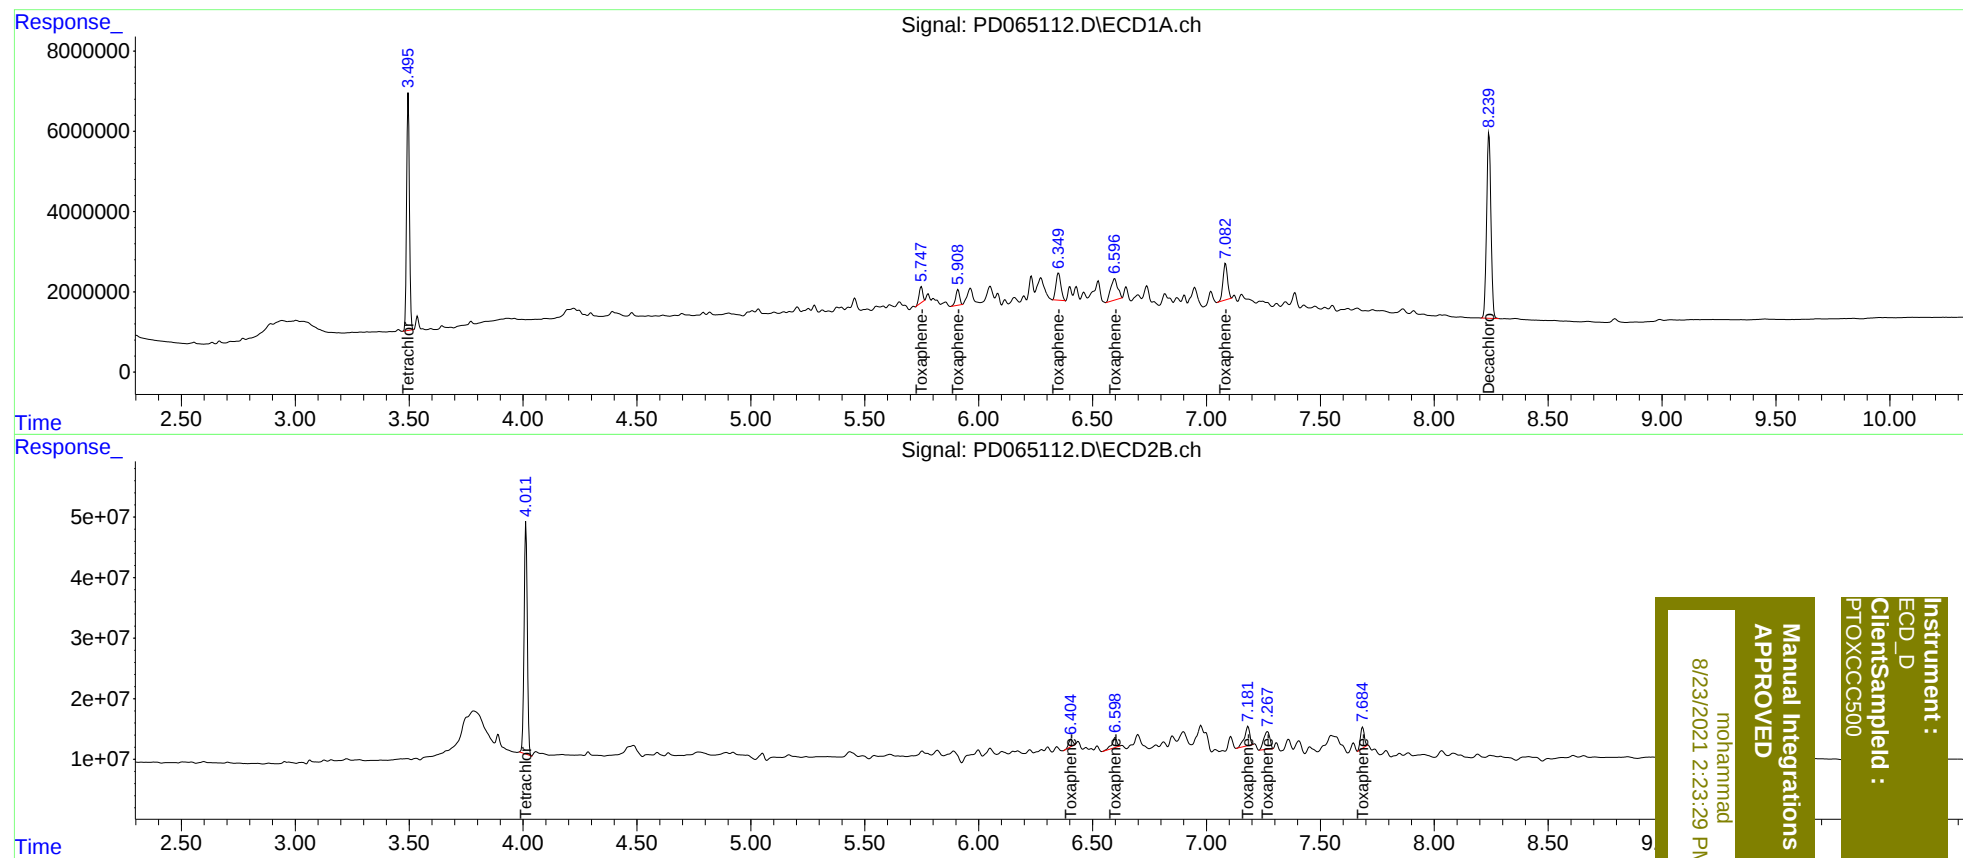

Manual Integrations
APPROVED

mohammad
8/23/2021 2:23:29 PM

Instrument :
ECD_D
Client Sampled :
PTOXCCC500