

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
 Data File : PD065167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2021 06:52
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 96 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 06:56:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:56:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.496	4.013	50728562	392.3E6	49.137	49.198
7) SA Decachlor...	8.239	9.084	61153726	242.3E6	50.396	49.867
Target Compounds						
2) Toxaphene-1	5.748	6.406	4483211	16834582	506.770	459.170
3) Toxaphene-2	5.909	6.598	4713496	30719473	511.348	505.857
4) Toxaphene-3	6.350	7.181	10658014	52548741	510.665	489.750
5) Toxaphene-4	6.596	7.267	11443021	53691326	508.454	513.417
6) Toxaphene-5	7.083	7.686	12923601	43839982	493.010	518.906

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
Data File : PD065167.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2021 06:52
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 96 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 06:56:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:56:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

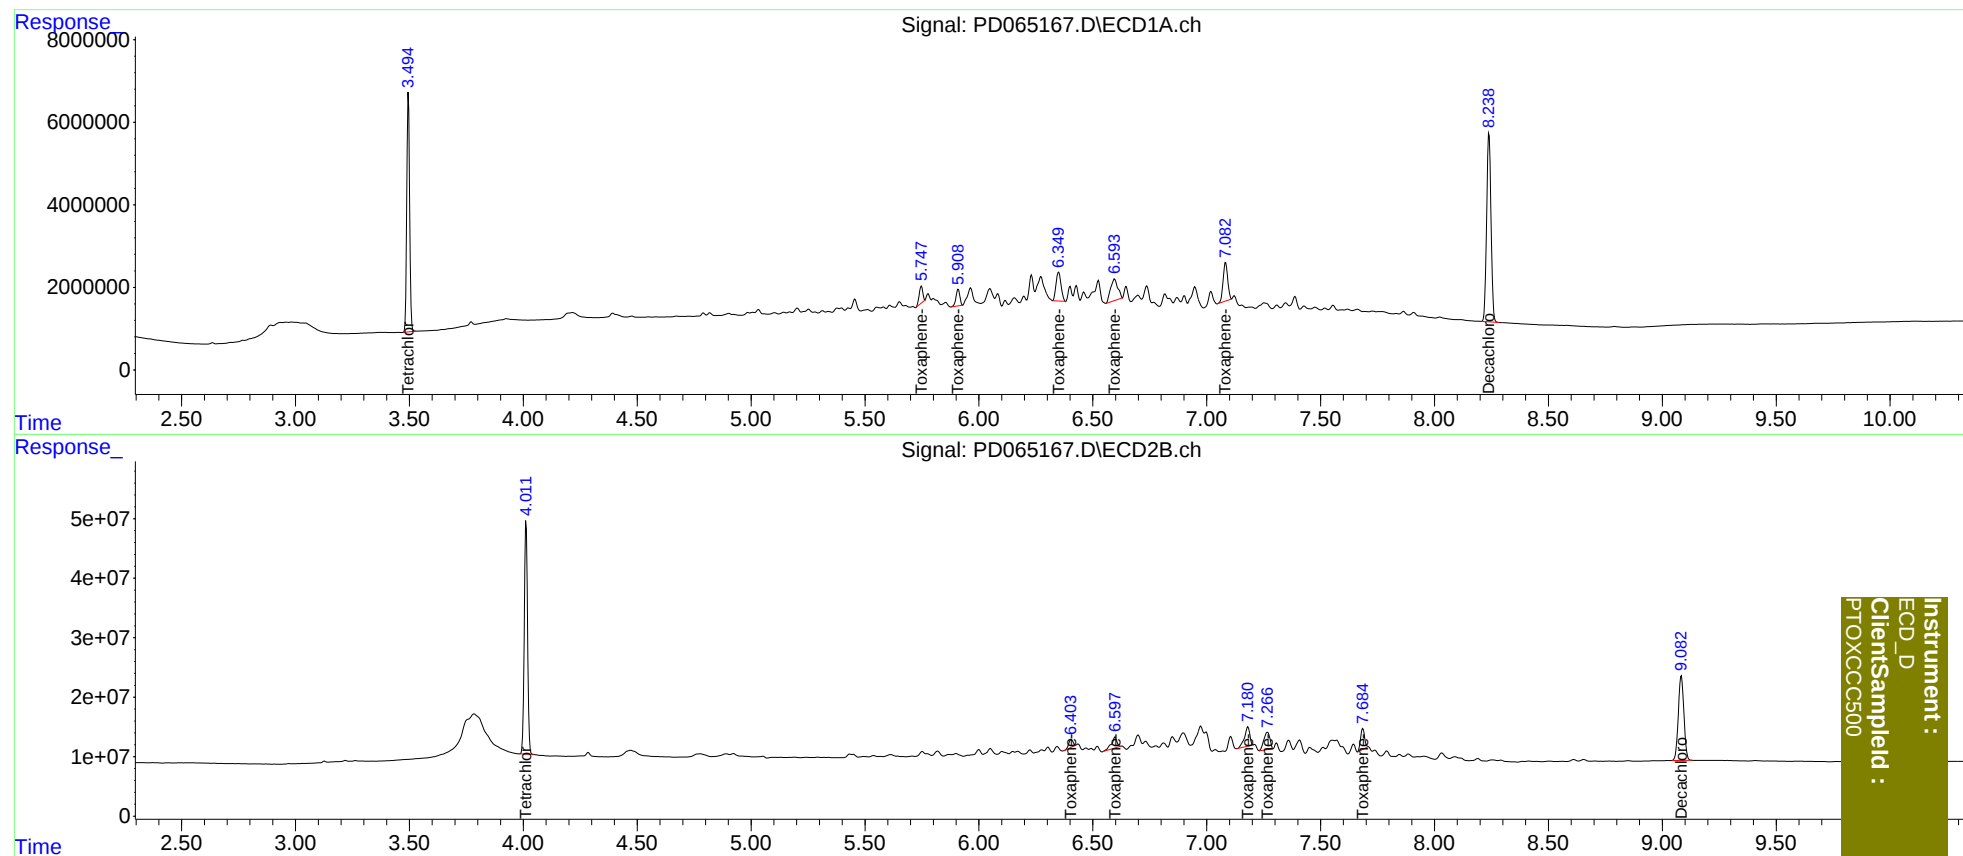

Instrument :
ECD_D
ClientSampled :
PTOXCCC500