

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
 Data File : PD065135.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2021 21:55
 Operator : AR\AJ
 Sample : M3434-11
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SWCS-12-0205

Manual Integrations
 APPROVED

mohammad
 8/23/2021 2:30:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 00:40:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.012	19783288	153.5E6	19.246	19.376
28)	SA Decachlor...	8.240	9.083	22536662	89800467	19.890	18.975
Target Compounds							
17)	MA 4,4'-DDT	6.405	7.145	2355892	5486741	2.369	0.915m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
Data File : PD065135.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2021 21:55
Operator : AR\AJ
Sample : M3434-11
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SWCS-12-0205


Manual Integrations
APPROVED

mohammad
8/23/2021 2:30:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 00:40:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

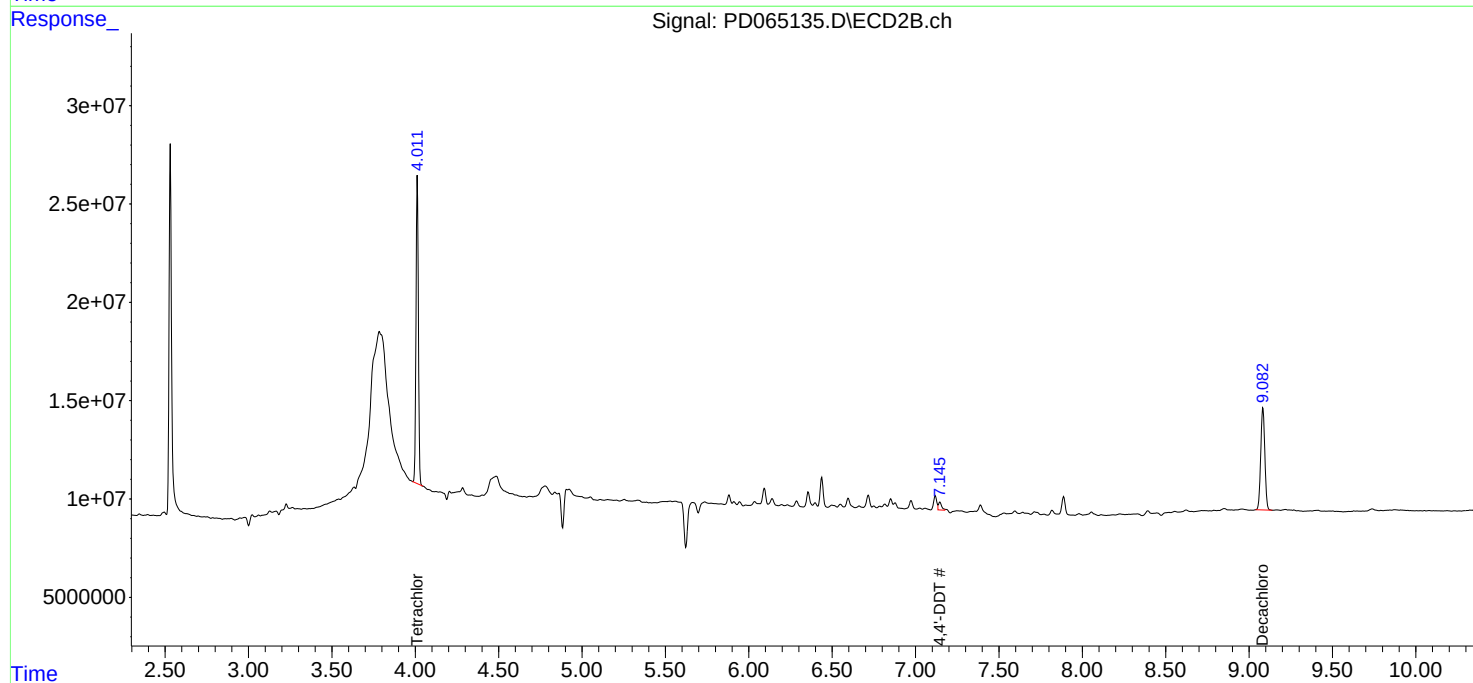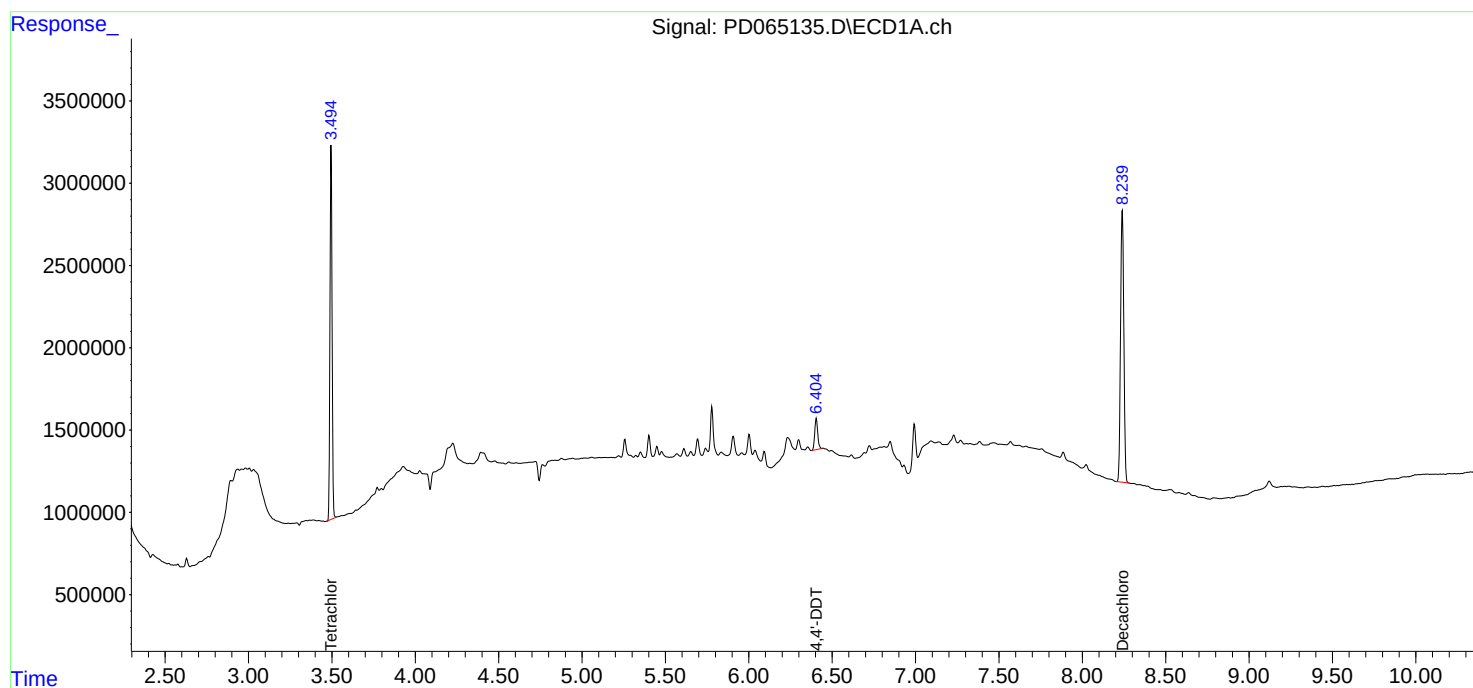

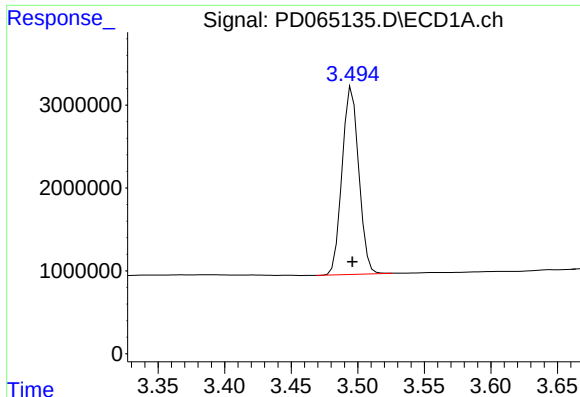


#1 Tetrachloro-m-xylene

R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 19783288
Conc: 19.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
SWCS-12-0205


Manual Integrations
APPROVED

mohammad
8/23/2021 2:30:26 PM

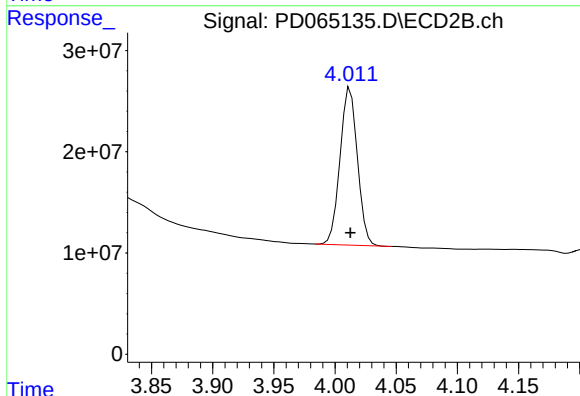


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 153470615
Conc: 19.38 ng/ml

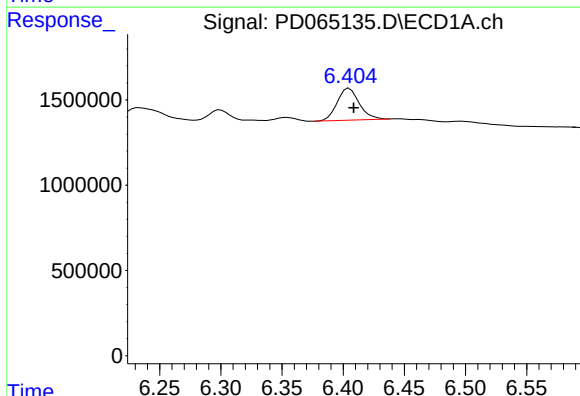


#17 4,4'-DDT

R.T.: 6.405 min
Delta R.T.: -0.004 min
Response: 2355892
Conc: 2.37 ng/ml

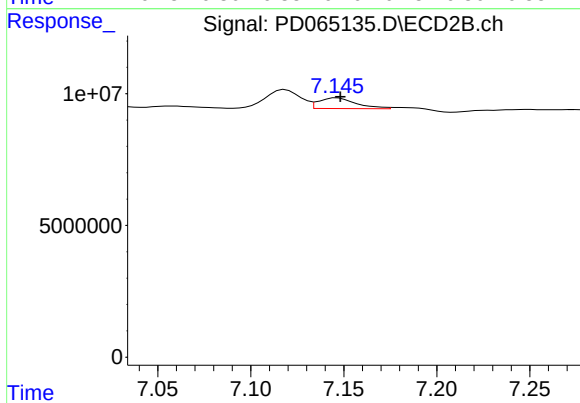

#17 4,4'-DDT

R.T.: 7.145 min
Delta R.T.: -0.003 min
Response: 5486741
Conc: 0.91 ng/ml m

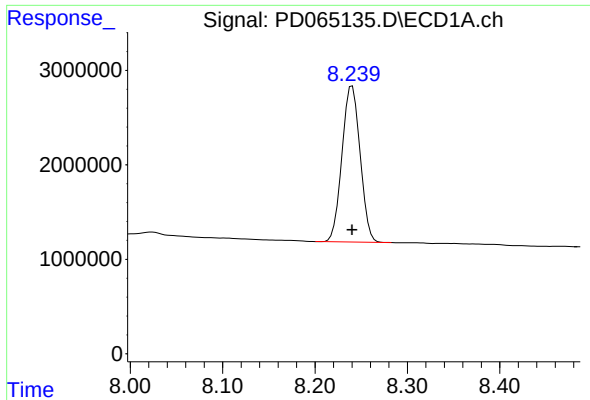


#28 Decachlorobiphenyl

R.T.: 8.240 min
Delta R.T.: 0.000 min
Response: 22536662
Conc: 19.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
SWCS-12-0205

Manual Integrations
APPROVED

mohammad
8/23/2021 2:30:26 PM

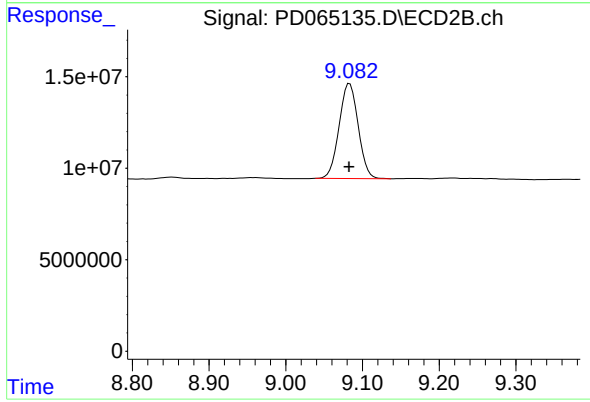

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: 0.000 min
Response: 89800467
Conc: 18.98 ng/ml