

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
 Data File : PD065162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2021 05:02
 Operator : AR\AJ
 Sample : M3449-07
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 05:38:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	20347022	157.4E6	19.795	19.876
28)	SA Decachlor...	8.240	9.084	21637116	85393511	19.096	18.044
Target Compounds							
17)	MA 4,4'-DDT	6.406	7.147	560338	2110516	0.563	0.352 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
Data File : PD065162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2021 05:02
Operator : AR\AJ
Sample : M3449-07
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 05:38:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

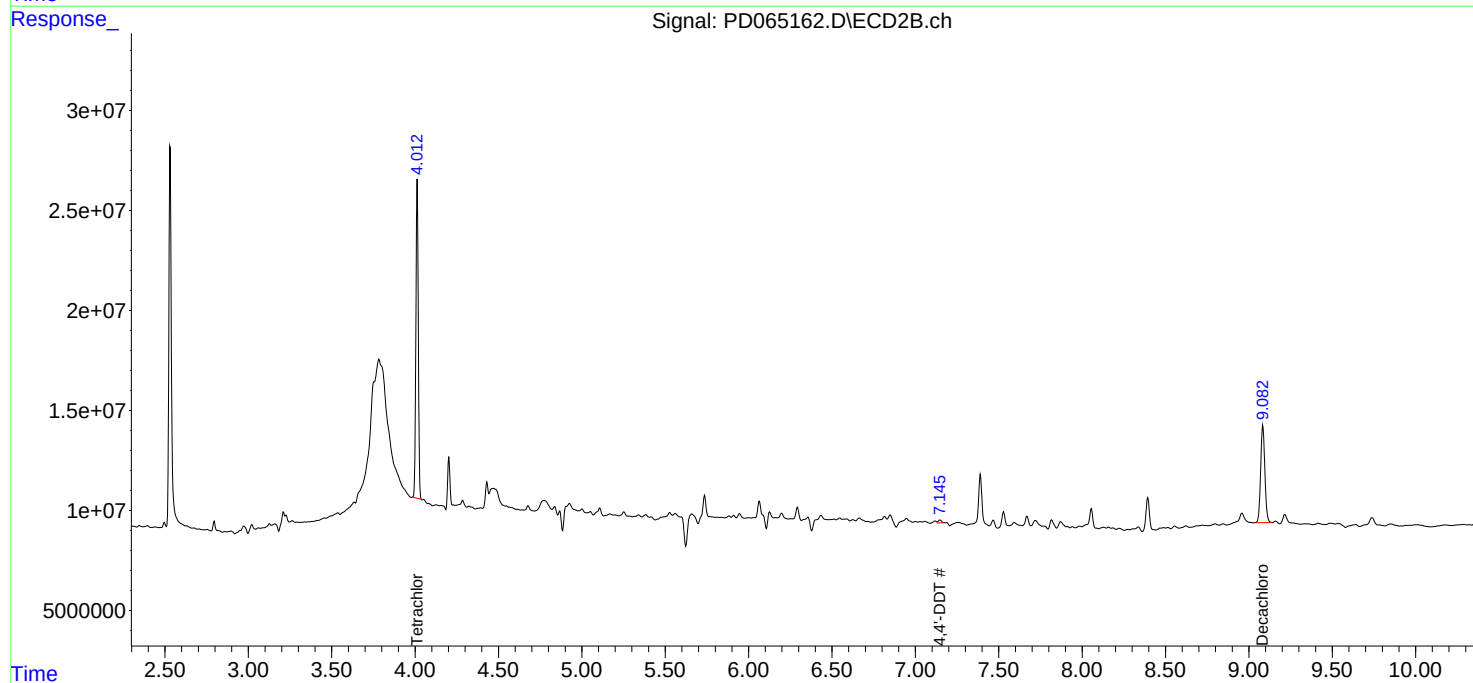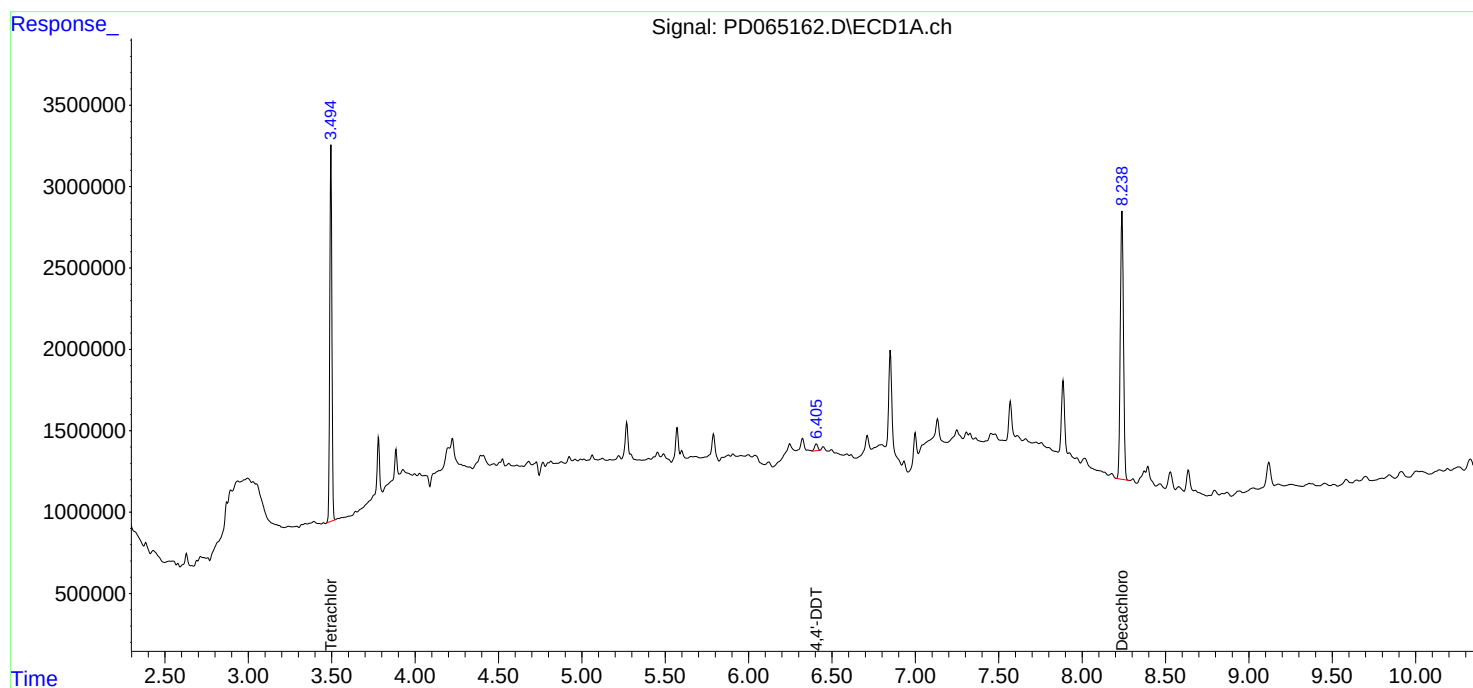


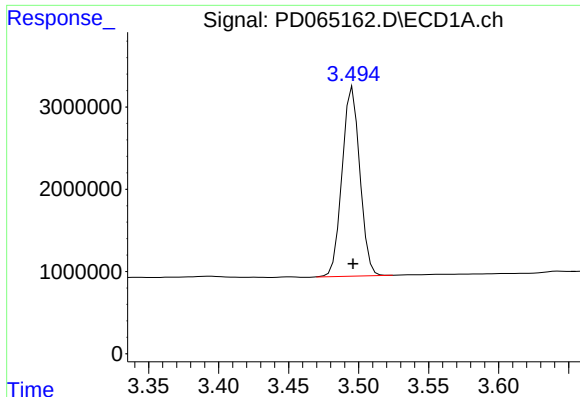

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 20347022
Conc: 19.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP3

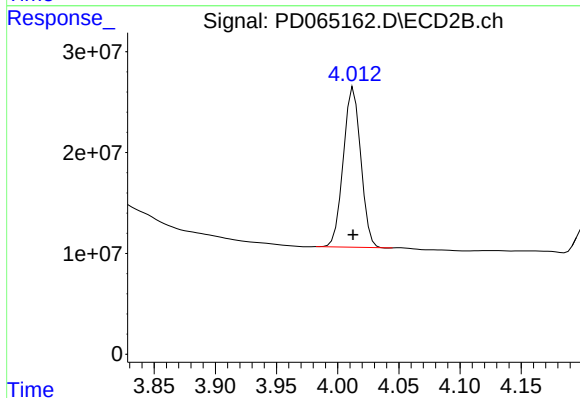


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 157433077
Conc: 19.88 ng/ml

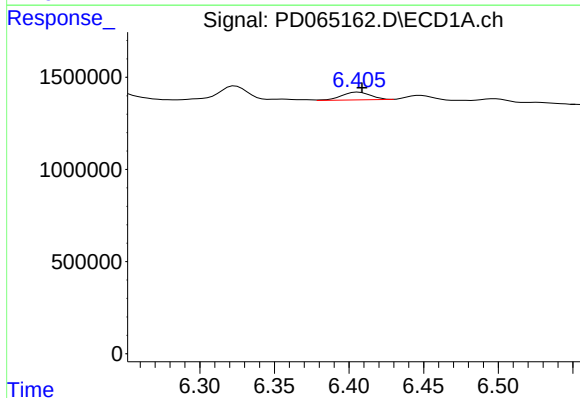


#17 4,4'-DDT

R.T.: 6.406 min
Delta R.T.: -0.002 min
Response: 560338
Conc: 0.56 ng/ml

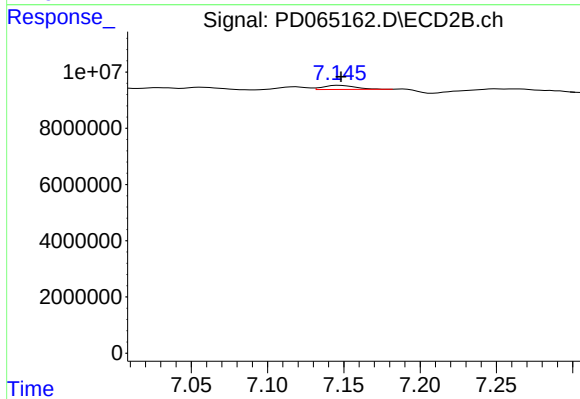

#17 4,4'-DDT


R.T.: 7.147 min
Delta R.T.: -0.001 min
Response: 2110516
Conc: 0.35 ng/ml

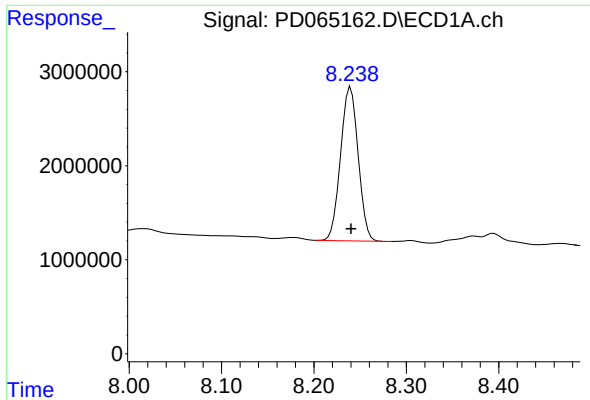

#28 Decachlorobiphenyl

R.T.: 8.240 min
Delta R.T.: 0.000 min
Response: 21637116
Conc: 19.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP3

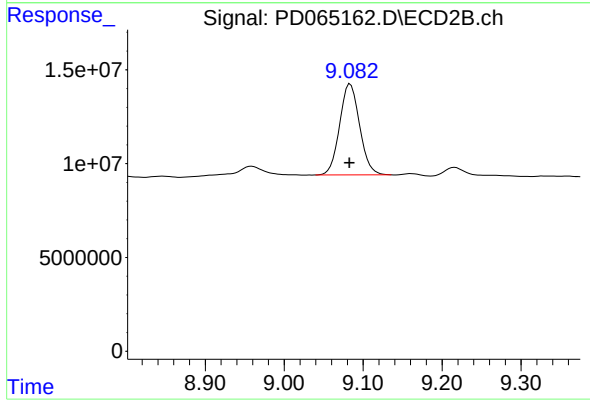

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 85393511
Conc: 18.04 ng/ml