

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
 Data File : PD065200.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2021 19:40
 Operator : AR\AJ
 Sample : M3463-33
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SWCS-27-0002

Manual Integrations
 APPROVED

mohammad
 8/23/2021 2:41:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 01:56:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.496	4.013	11913171	91648941	11.590	11.571
28) SA Decachlor...	8.239	9.083	10316162	36677258	9.105	7.750
Target Compounds						
11) B alpha-Chl...	5.489	6.198	402601	3713460	0.360m	0.499 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
Data File : PD065200.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2021 19:40
Operator : AR\AJ
Sample : M3463-33
Misc :
ALS Vial : 79 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SWCS-27-0002


Manual Integrations
APPROVED

mohammad
8/23/2021 2:41:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 01:56:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

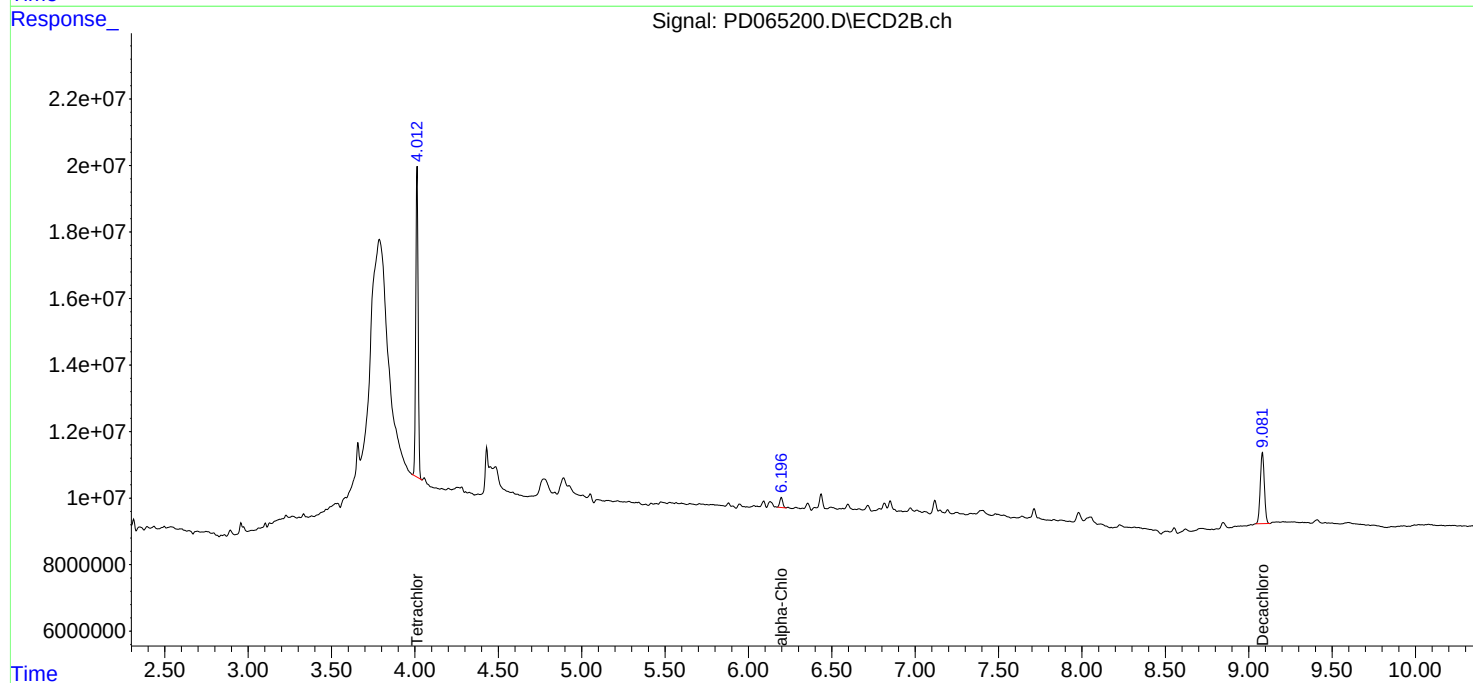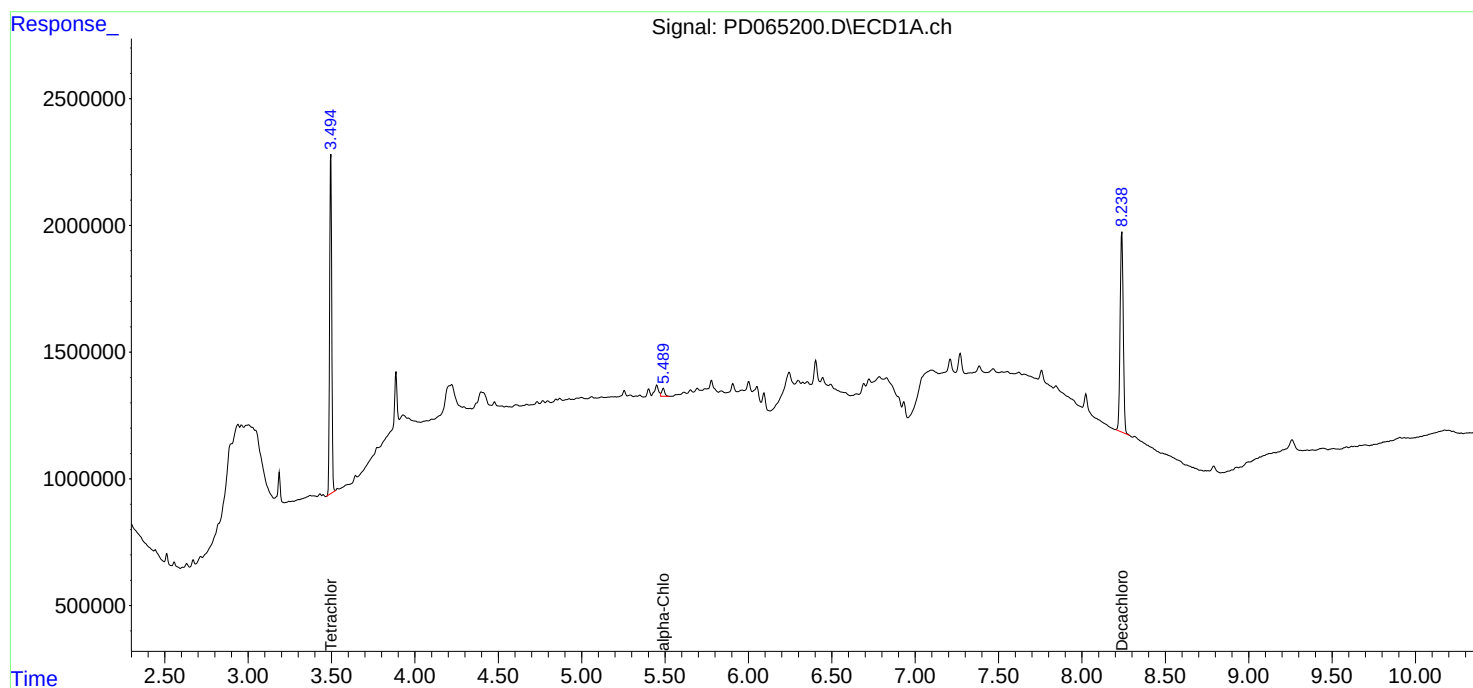

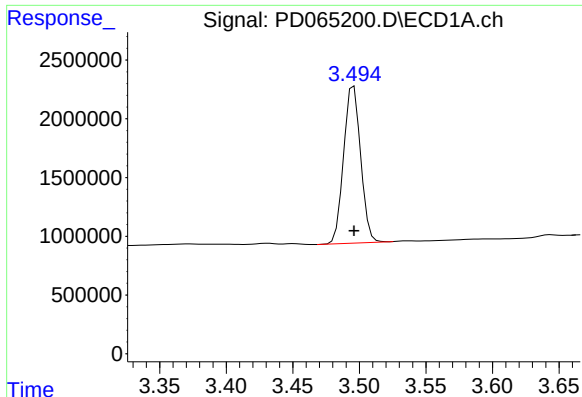


#1 Tetrachloro-m-xylene

R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 11913171
Conc: 11.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
SWCS-27-0002


Manual Integrations
APPROVED

mohammad
8/23/2021 2:41:42 PM

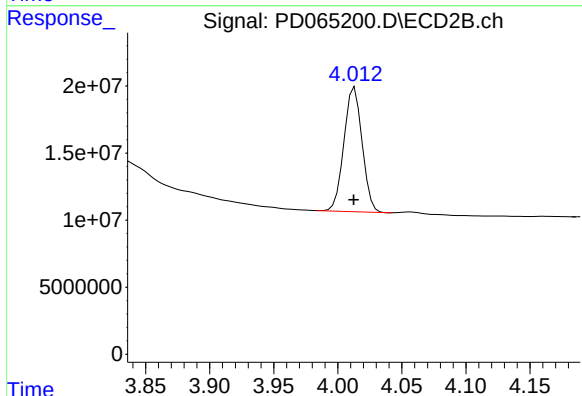


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 91648941
Conc: 11.57 ng/ml

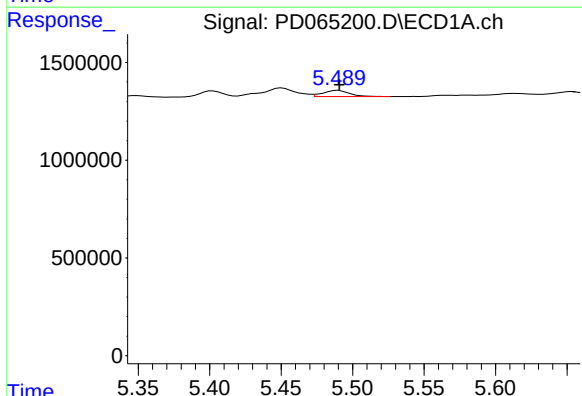


#11 alpha-Chlordane

R.T.: 5.489 min
Delta R.T.: -0.002 min
Response: 402601
Conc: 0.36 ng/ml m

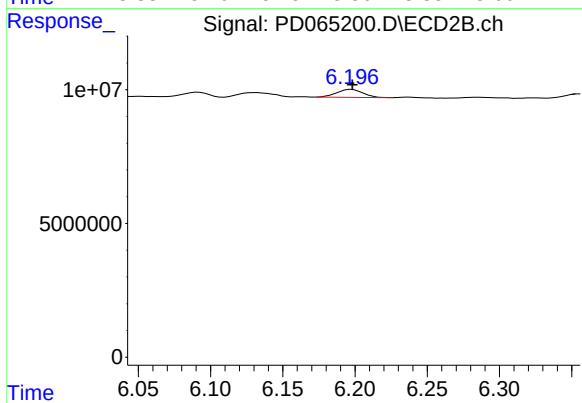

#11 alpha-Chlordane

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 3713460
Conc: 0.50 ng/ml

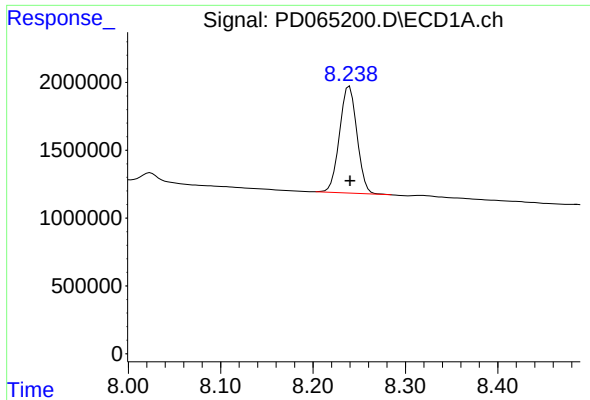


#28 Decachlorobiphenyl

R.T.: 8.239 min
Delta R.T.: 0.000 min
Response: 10316162
Conc: 9.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
SWCS-27-0002

Manual Integrations
APPROVED

mohammad
8/23/2021 2:41:42 PM

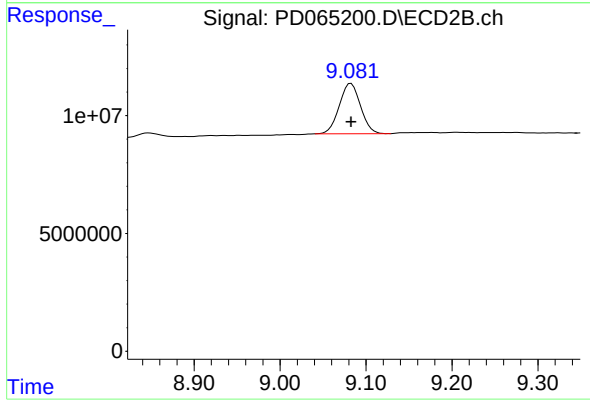

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: 0.000 min
Response: 36677258
Conc: 7.75 ng/ml