

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
 Data File : PD065224.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2021 02:06
 Operator : AR\AJ
 Sample : M3514-01
 Misc :
 ALS Vial : 96 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 NB-8-082021

Manual Integrations
 APPROVED

mohammad
 8/23/2021 2:42:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 02:02:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	13188088	94230532	12.830	11.897
28)	SA Decachlor...	8.239	9.084	13577644	48956699	11.983	10.345
Target Compounds							
10)	B gamma-Chl...	5.431	6.125	1030653	8856409	0.912m	1.158m#
11)	B alpha-Chl...	5.489	6.197	2009722	21944425	1.795m	2.948m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082121\
Data File : PD065224.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2021 02:06
Operator : AR\AJ
Sample : M3514-01
Misc :
ALS Vial : 96 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
NB-8-082021


Manual Integrations
APPROVED

mohammad
8/23/2021 2:42:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 02:02:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

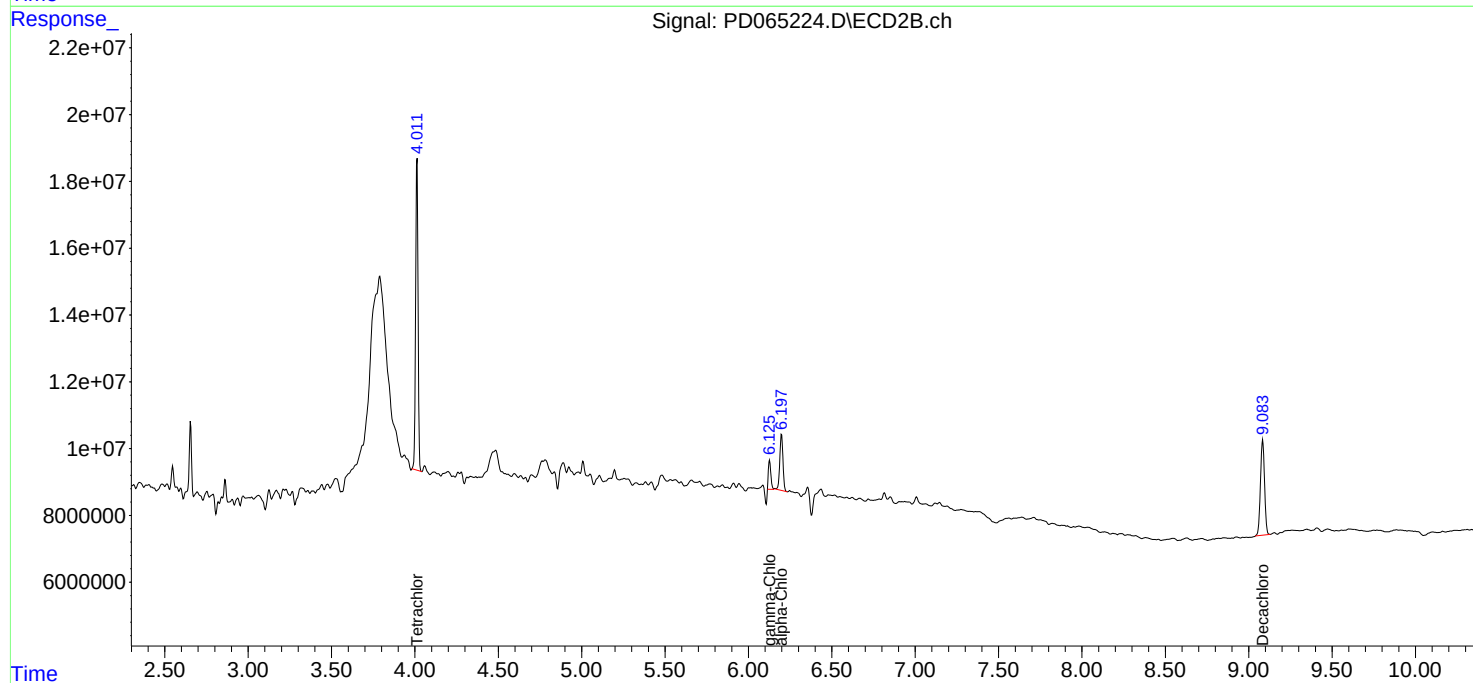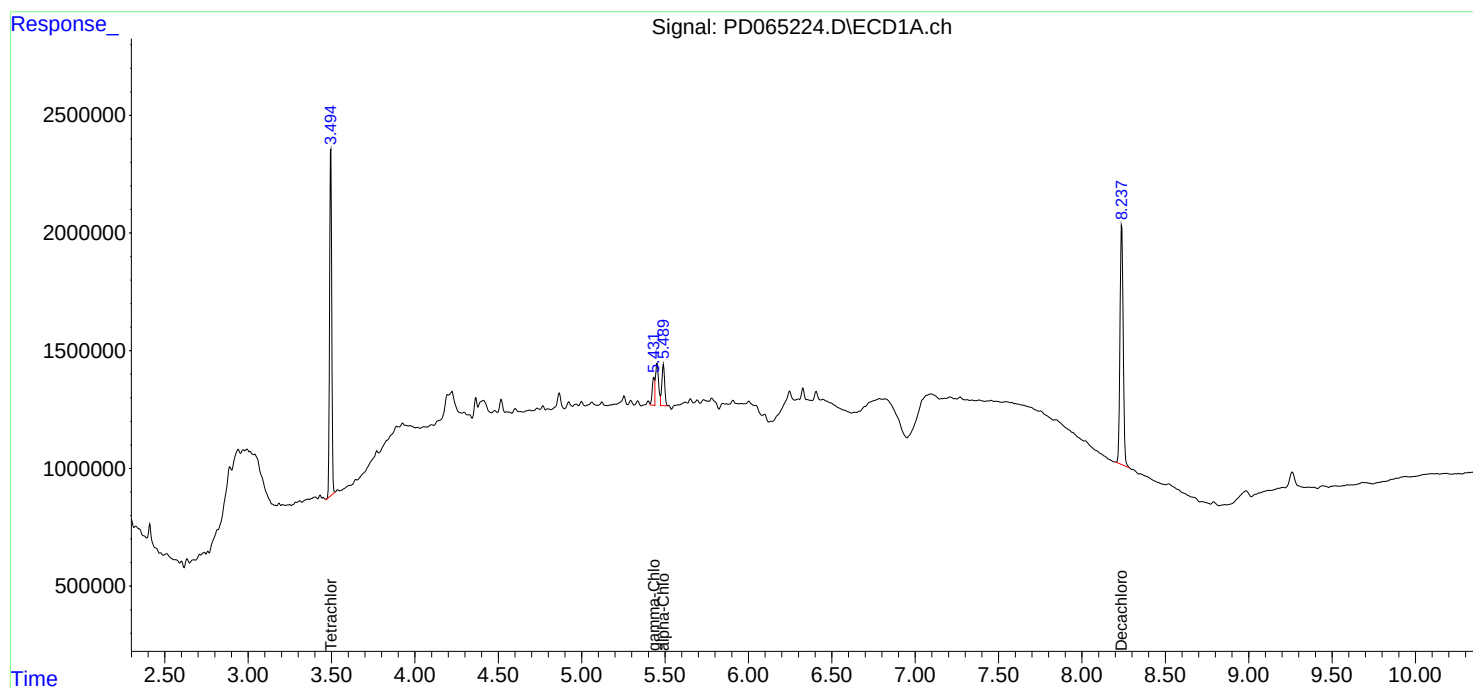

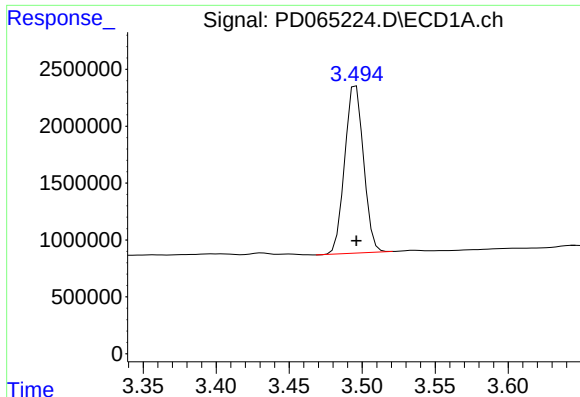


#1 Tetrachloro-m-xylene

R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 13188088
Conc: 12.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
NB-8-082021


Manual Integrations
APPROVED

mohammad
8/23/2021 2:42:54 PM

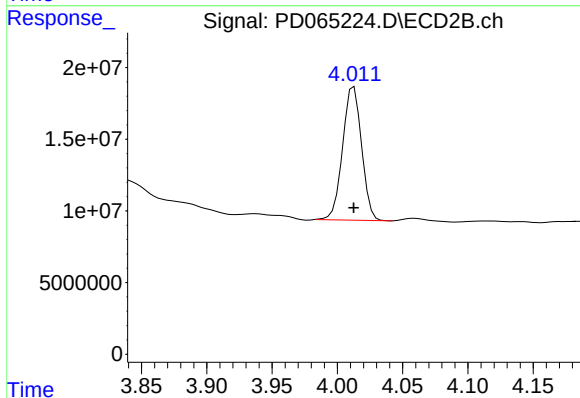


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 94230532
Conc: 11.90 ng/ml

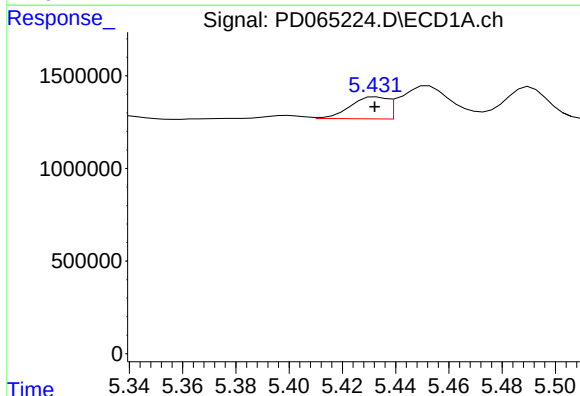


#10 gamma-Chlordane

R.T.: 5.431 min
Delta R.T.: 0.000 min
Response: 1030653
Conc: 0.91 ng/ml m

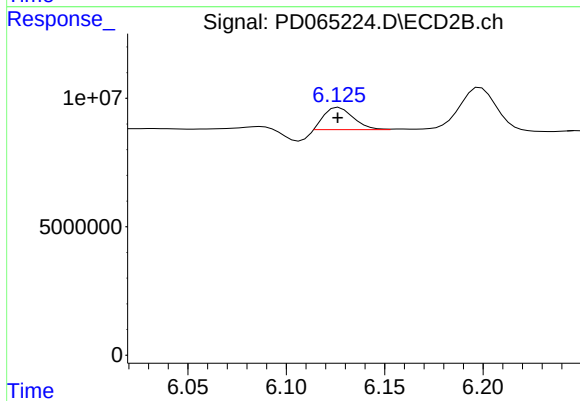

#10 gamma-Chlordane

R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 8856409
Conc: 1.16 ng/ml m

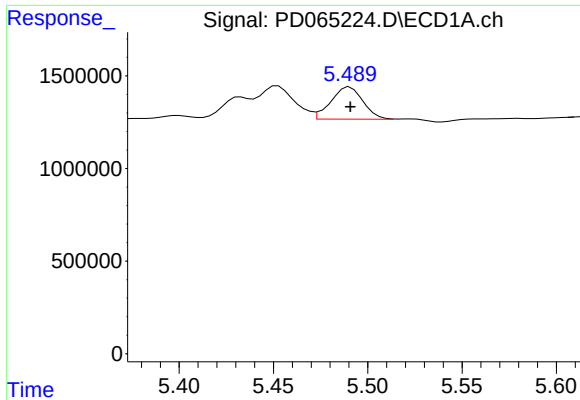


#11 alpha-Chlordane

R.T.: 5.489 min
Delta R.T.: -0.002 min
Response: 2009722
Conc: 1.79 ng/ml m

Instrument :
ECD_D
ClientSampleId :
NB-8-082021


Manual Integrations
APPROVED

mohammad
8/23/2021 2:42:54 PM

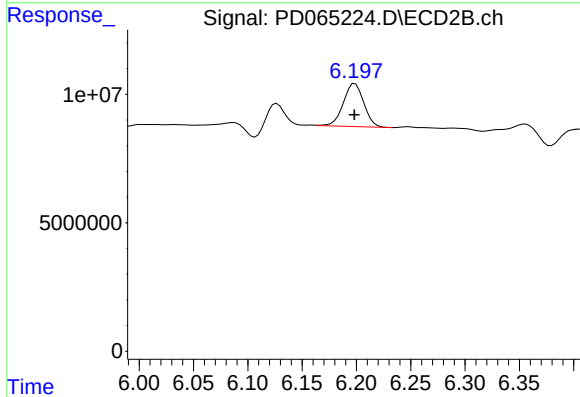


#11 alpha-Chlordane

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 21944425
Conc: 2.95 ng/ml m

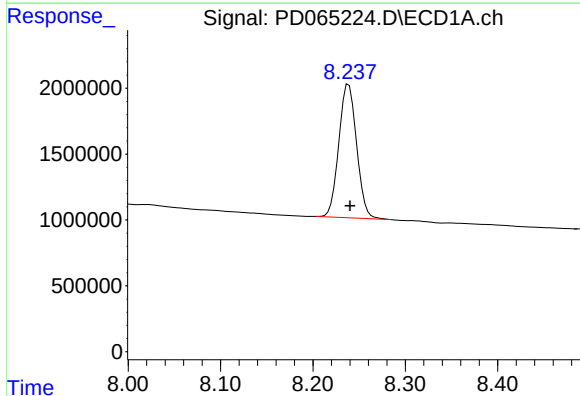

#28 Decachlorobiphenyl

R.T.: 8.239 min
Delta R.T.: -0.001 min
Response: 13577644
Conc: 11.98 ng/ml

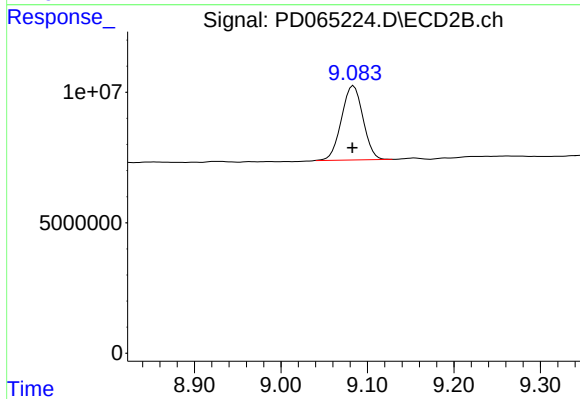

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.001 min
Response: 48956699
Conc: 10.34 ng/ml