

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082123\
 Data File : PD077268.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2023 15:23
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 22:22:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.762	49596804	29323459	20.958	21.528
28)	SA Decachlor...	9.083	7.901	60176735	30123097	21.961	21.049
Target Compounds							
4)	MA Heptachlor	4.911	0.000	315797	0	0.088	N.D. #
6)	B beta-BHC	4.557f	0.000	79091	0	0.053	N.D. #
7)	B delta-BHC	4.767	0.000	1948421	0	0.559	N.D. #
8)	B Heptachlo...	5.688	0.000	1381236	0	0.417	N.D. #
14)	MA Endrin	0.000	5.642f	0	210162	N.D.	0.144 #
15)	B Endosulfa...	6.782f	0.000	794680	0	0.250	N.D. #
21)	B Endrin ke...	7.689f	0.000	246646	0	0.082	N.D. #
22)	Mirex	8.166f	0.000	309861	0	0.136	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082123\
Data File : PD077268.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 15:23
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:22:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

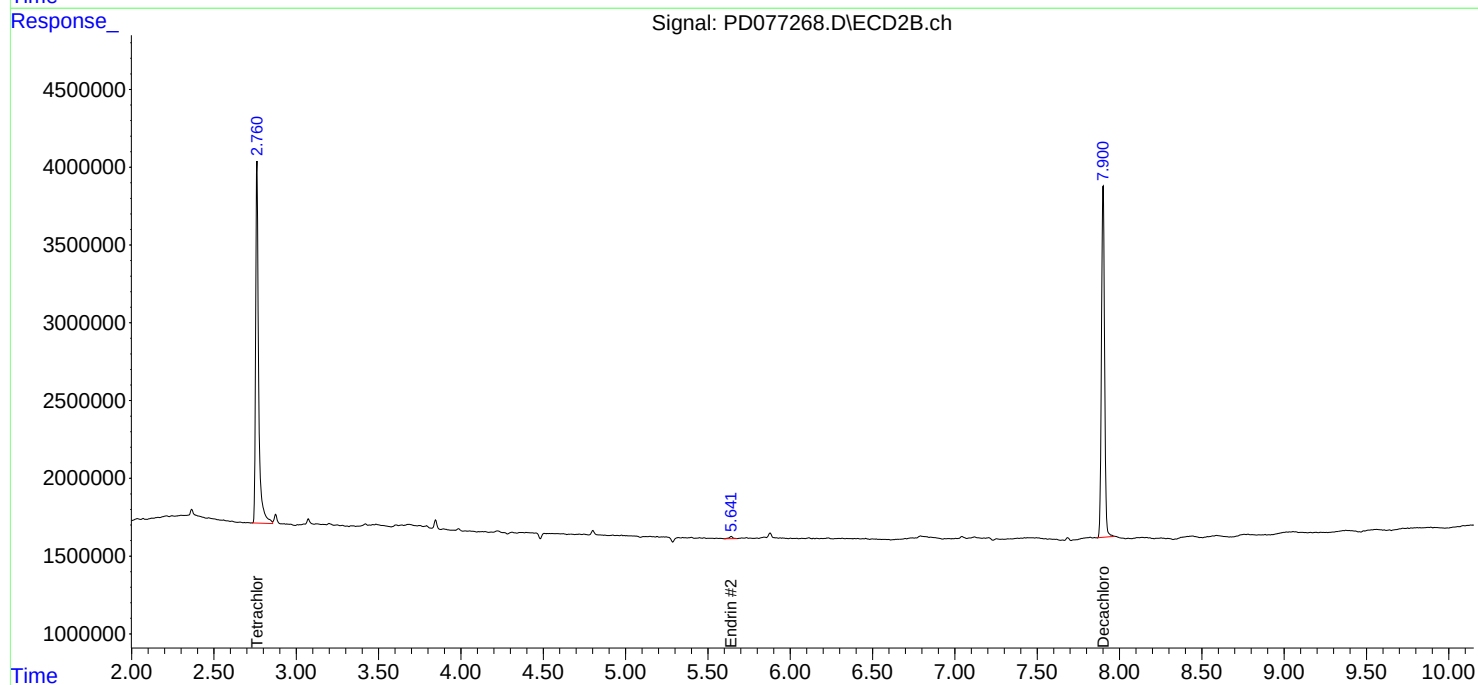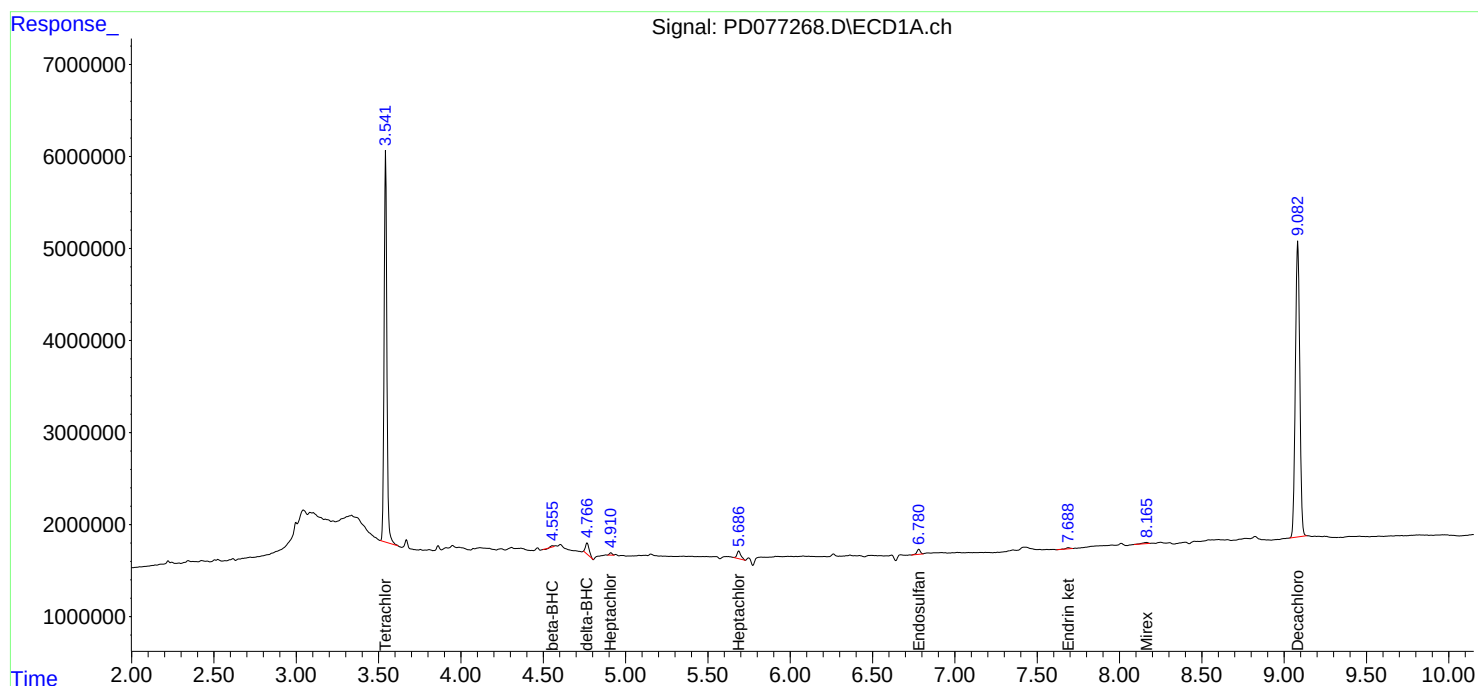


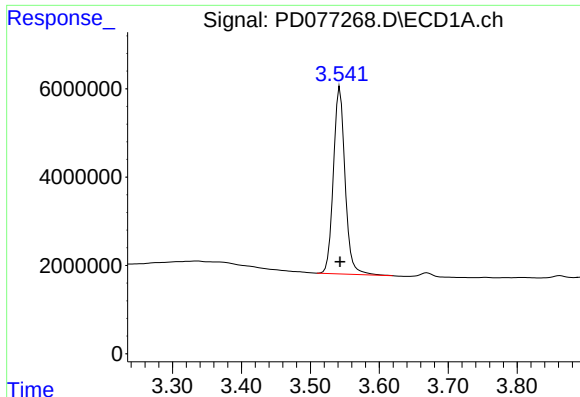

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 49596804
Conc: 20.96 ng/ml

Instrument :
ECD_D
ClientSampleId :

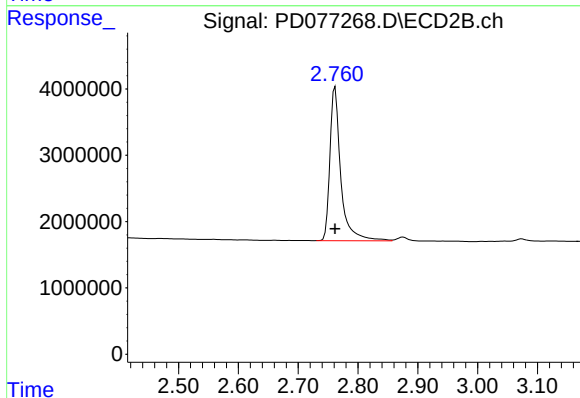


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 29323459
Conc: 21.53 ng/ml

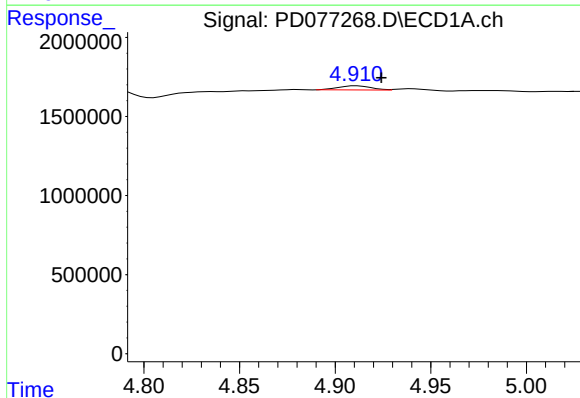


#4 Heptachlor

R.T.: 4.911 min
Delta R.T.: -0.013 min
Response: 315797
Conc: 0.09 ng/ml

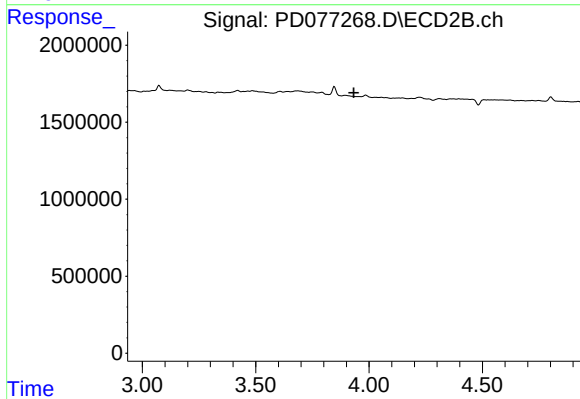

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.933 min
Response: 0
Conc: N.D.

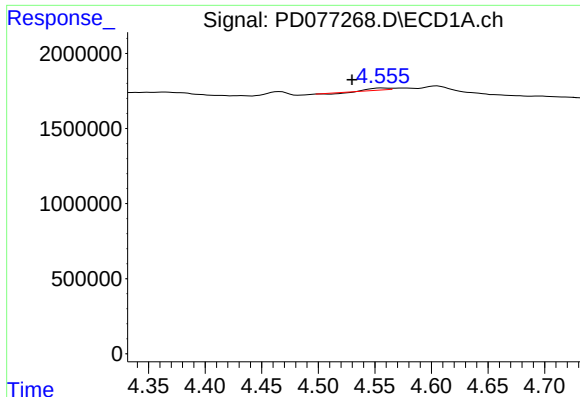

#6 beta-BHC


R.T.: 4.557 min
Delta R.T.: 0.027 min
Response: 79091
Conc: 0.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

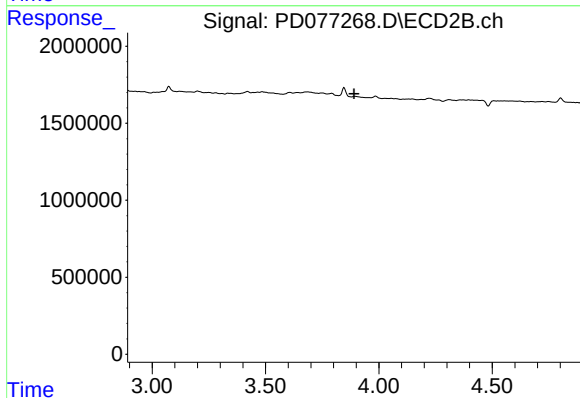


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 3.890 min
Response: 0
Conc: N.D.

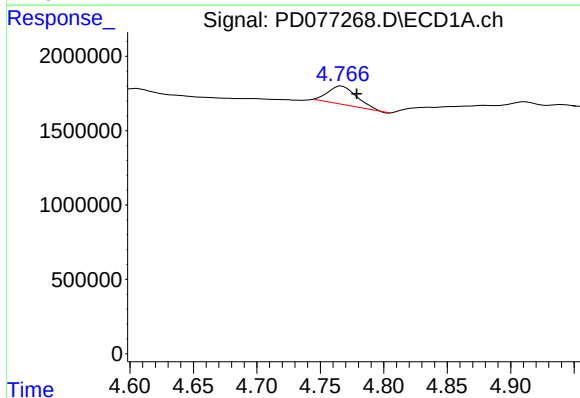


#7 delta-BHC

R.T.: 4.767 min
Delta R.T.: -0.012 min
Response: 1948421
Conc: 0.56 ng/ml

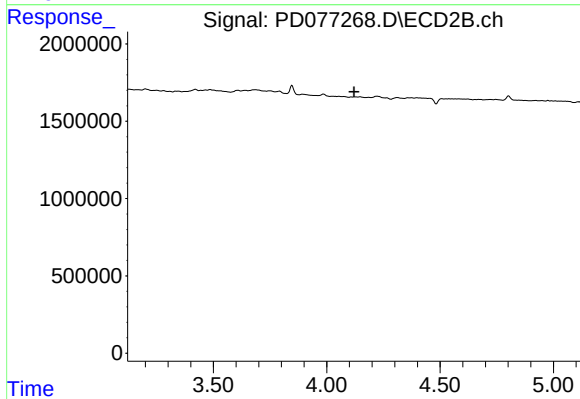

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.120 min
Response: 0
Conc: N.D.

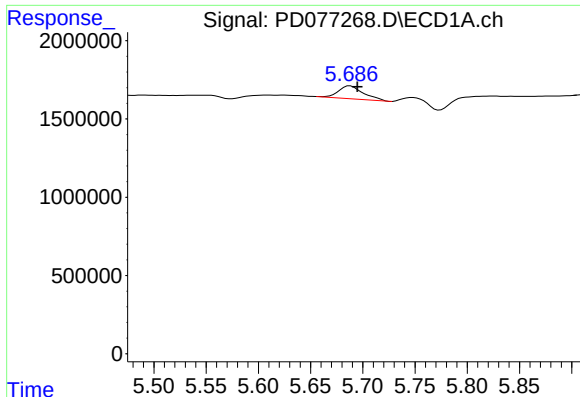

#8 Heptachlor epoxide


R.T.: 5.688 min
Delta R.T.: -0.007 min
Response: 1381236
Conc: 0.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

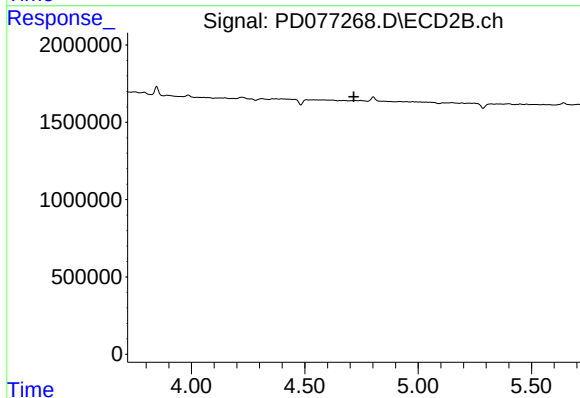


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.716 min
Response: 0
Conc: N.D.

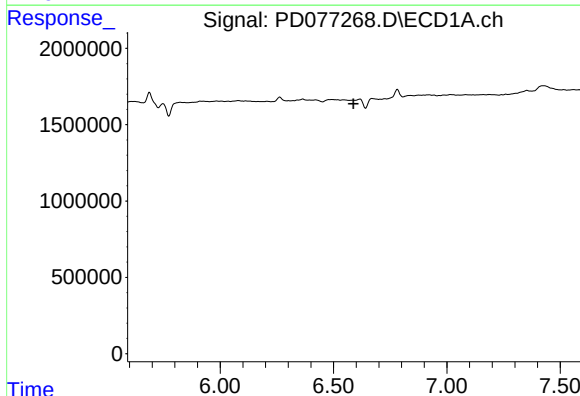


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.588 min
Response: 0
Conc: N.D.

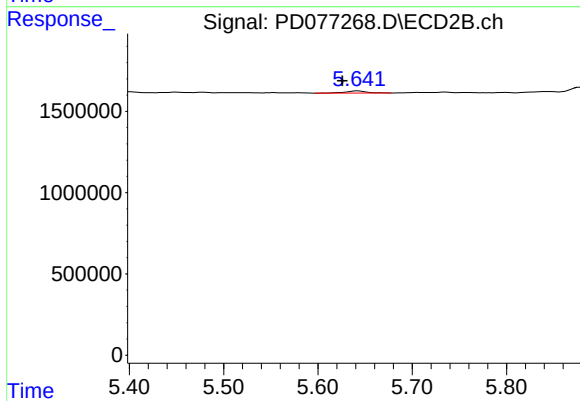

#14 Endrin


R.T.: 5.642 min
Delta R.T.: 0.016 min
Response: 210162
Conc: 0.14 ng/ml

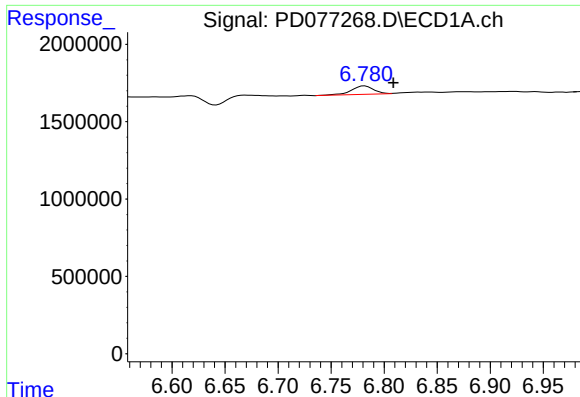

#15 Endosulfan II


R.T.: 6.782 min
Delta R.T.: -0.027 min
Response: 794680
Conc: 0.25 ng/ml

Instrument :
ECD_D
ClientSampleId :

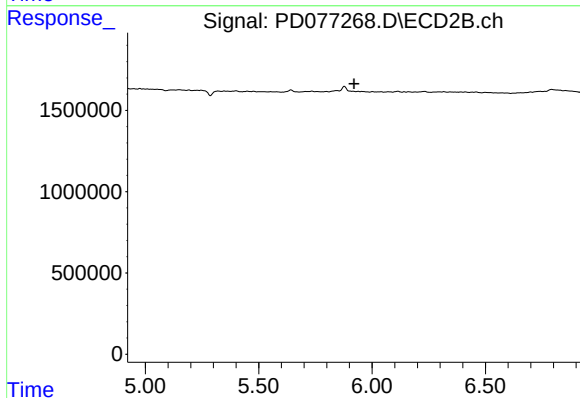


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.920 min
Response: 0
Conc: N.D.

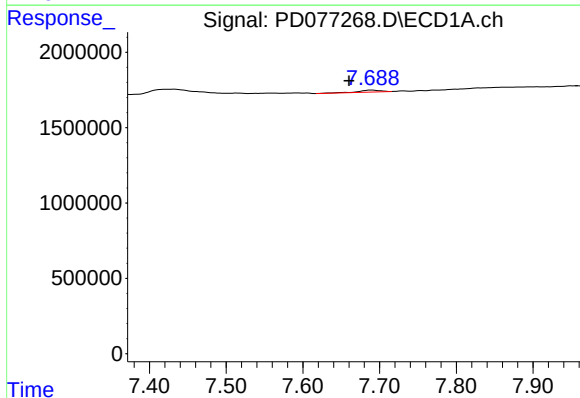


#21 Endrin ketone

R.T.: 7.689 min
Delta R.T.: 0.029 min
Response: 246646
Conc: 0.08 ng/ml

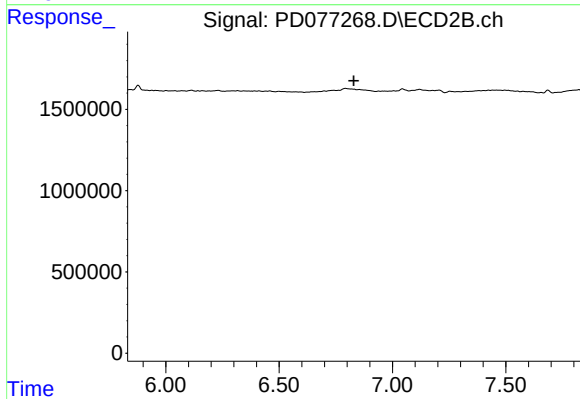

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.830 min
Response: 0
Conc: N.D.

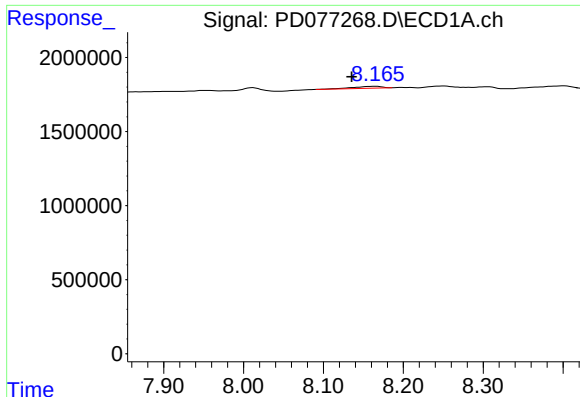

#22 Mirex


R.T.: 8.166 min
Delta R.T.: 0.031 min
Response: 309861
Conc: 0.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

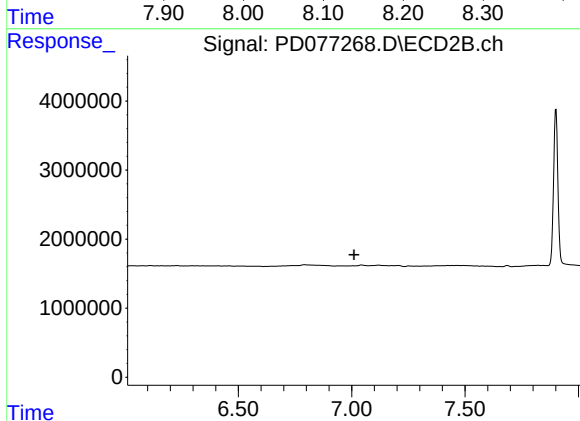


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.011 min
Response: 0
Conc: N.D.

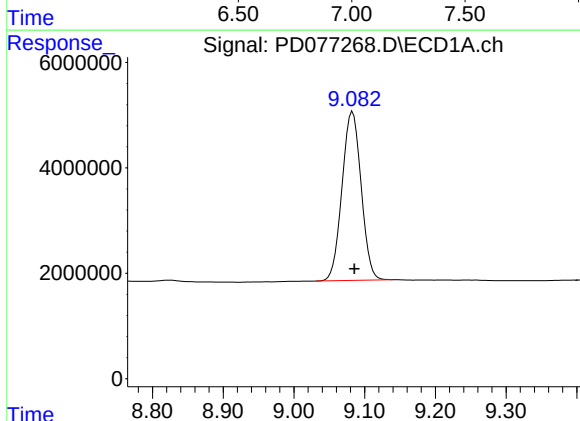

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: -0.003 min
Response: 60176735
Conc: 21.96 ng/ml

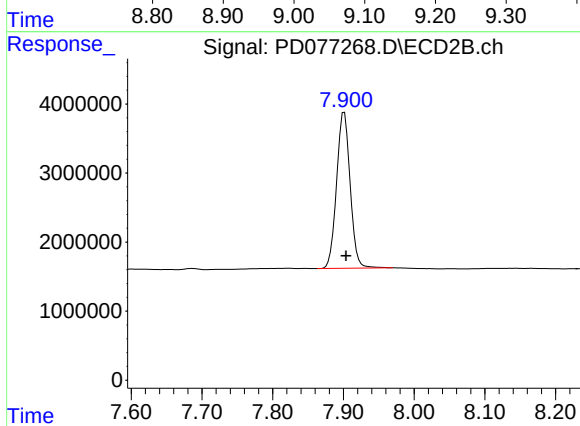

#28 Decachlorobiphenyl

R.T.: 7.901 min
Delta R.T.: -0.003 min
Response: 30123097
Conc: 21.05 ng/ml