

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082123\
 Data File : PD077280.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2023 18:10
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 22:25:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.762	50352368	29670266	21.277	21.782
28)	SA Decachlor...	9.082	7.901	63618575	30865191	23.217	21.568
Target Compounds							
3)	MA gamma-BHC...	0.000	3.605	0	223617	N.D.	0.120 #
4)	MA Heptachlor	4.909f	0.000	230278	0	0.064	N.D. #
6)	B beta-BHC	4.555f	0.000	119870	0	0.080	N.D. #
7)	B delta-BHC	4.767	0.000	2089170	0	0.599	N.D. #
8)	B Heptachlo...	5.688	0.000	2276149	0	0.687	N.D. #
14)	MA Endrin	0.000	5.643f	0	432644	N.D.	0.296 #
15)	B Endosulfa...	6.781f	0.000	835358	0	0.263	N.D. #
21)	B Endrin ke...	7.678f	0.000	2702181	0	0.897	N.D. #
24)	Chlordane-2	0.000	4.343	0	944445	N.D.	16.794 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082123\
Data File : PD077280.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 18:10
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:25:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

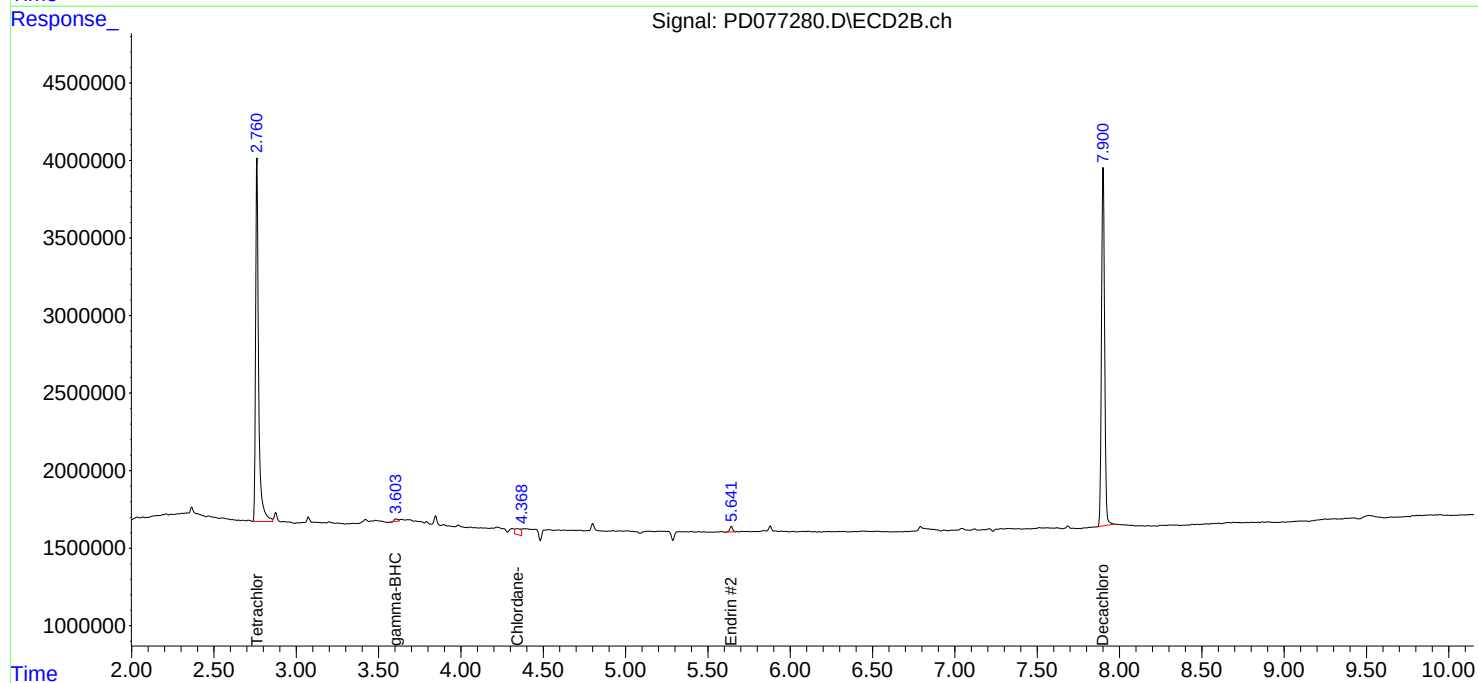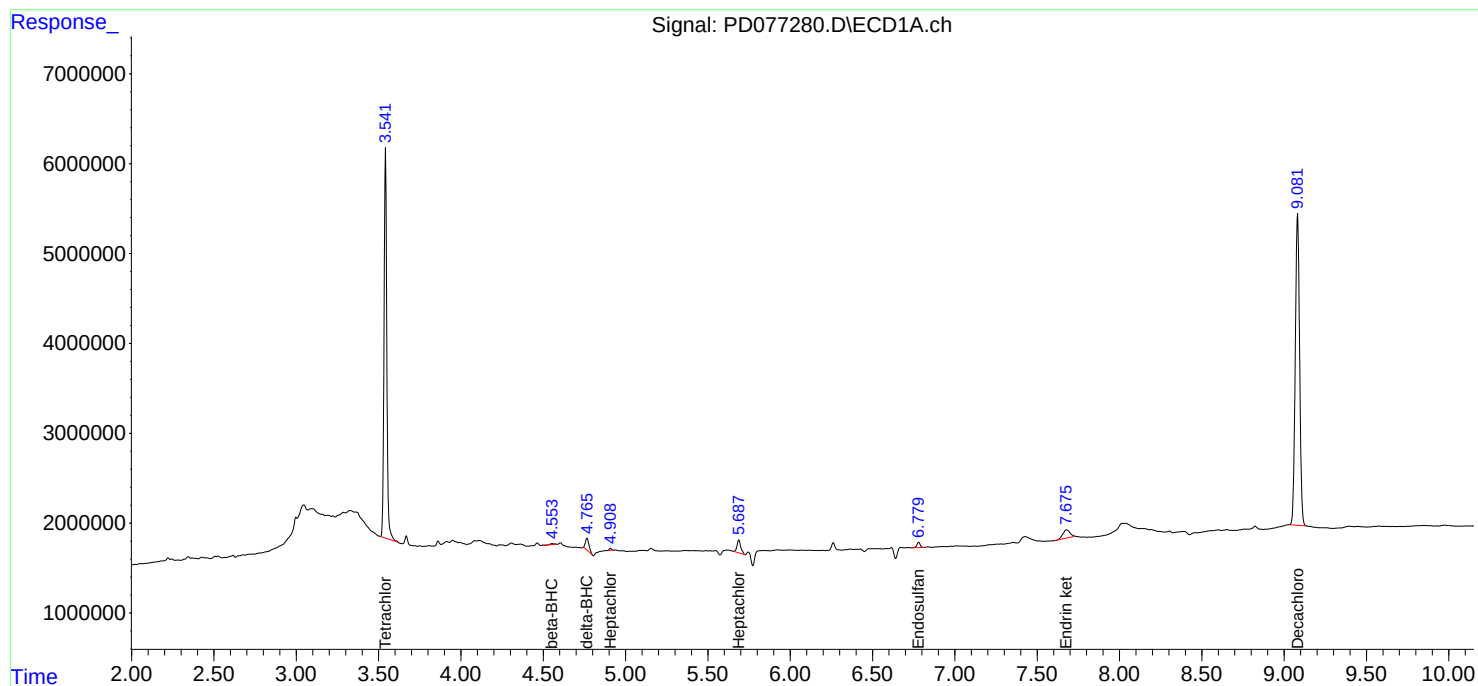


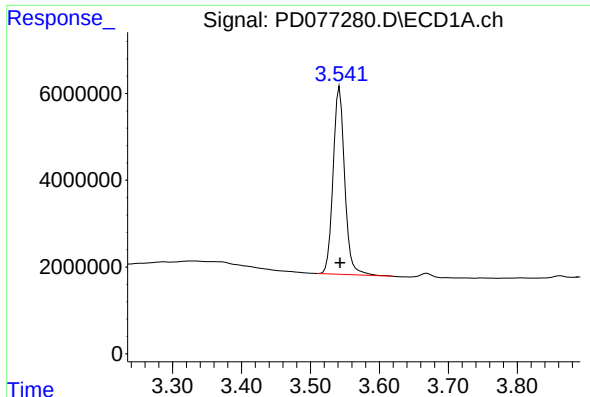

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 50352368
Conc: 21.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

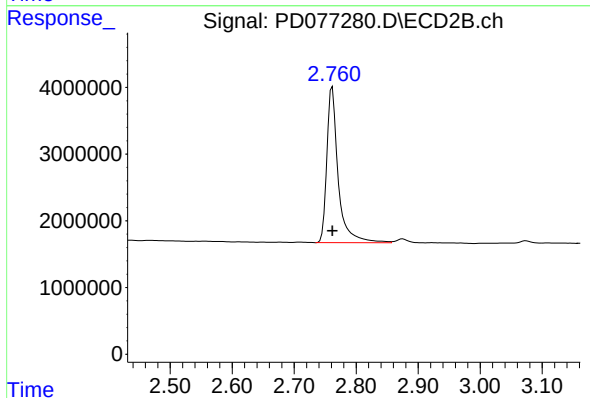


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 29670266
Conc: 21.78 ng/ml

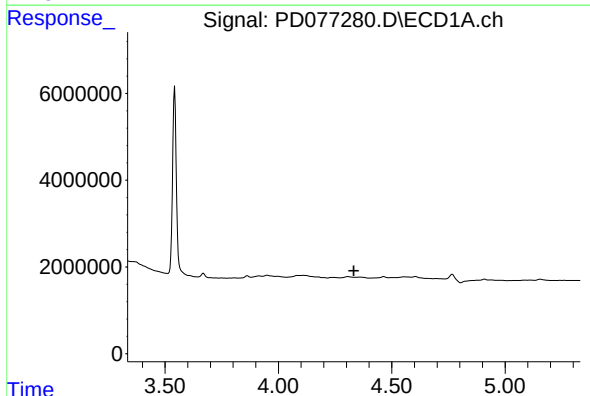


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.333 min
Response: 0
Conc: N.D.

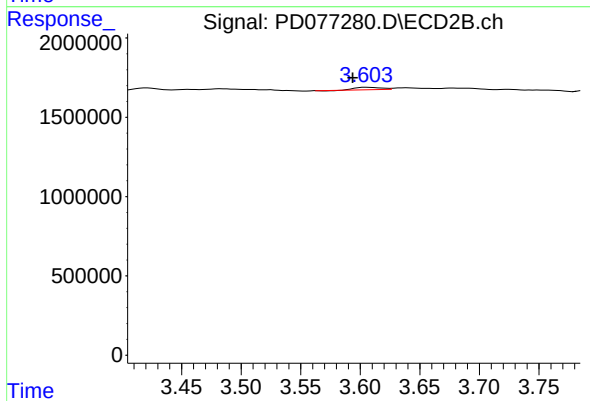

#3 gamma-BHC (Lindane)


R.T.: 3.605 min
Delta R.T.: 0.011 min
Response: 223617
Conc: 0.12 ng/ml

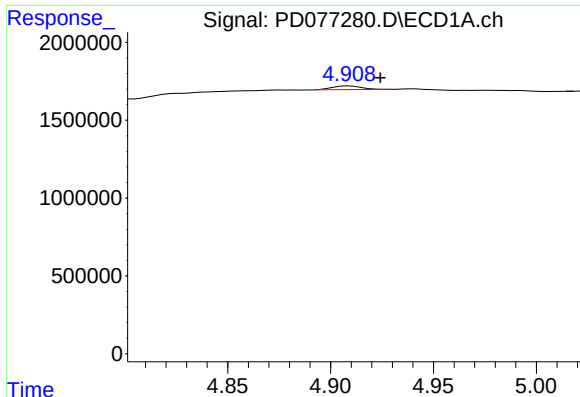

#4 Heptachlor


R.T.: 4.909 min
Delta R.T.: -0.015 min
Response: 230278
Conc: 0.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

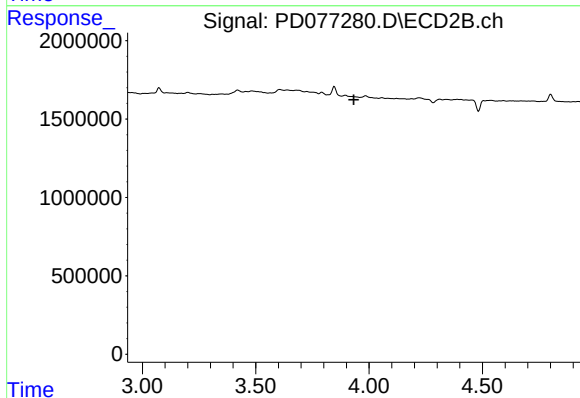


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 3.933 min
Response: 0
Conc: N.D.

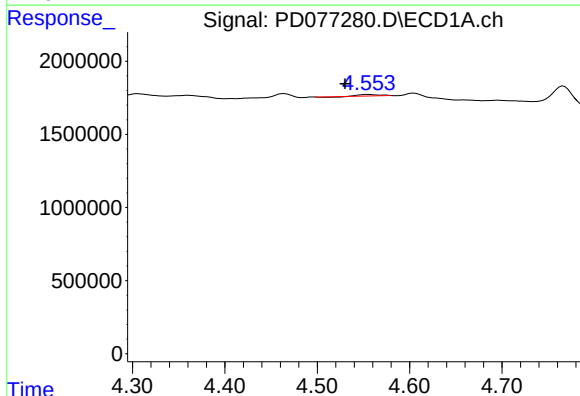


#6 beta-BHC

R.T.: 4.555 min
Delta R.T.: 0.025 min
Response: 119870
Conc: 0.08 ng/ml

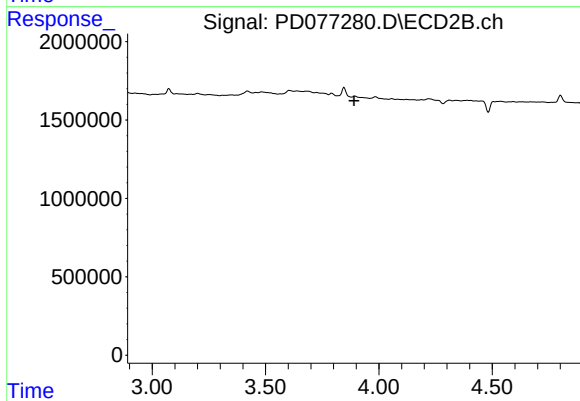

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 3.890 min
Response: 0
Conc: N.D.

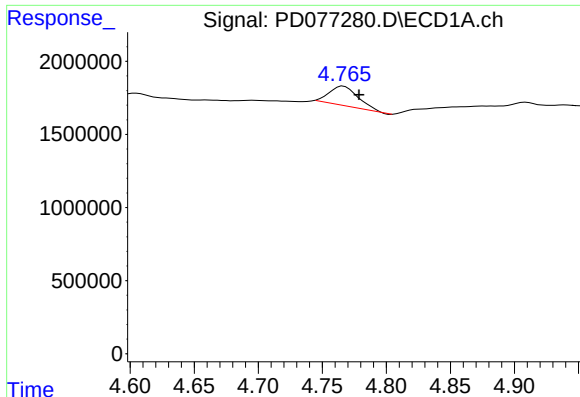

#7 delta-BHC


R.T.: 4.767 min
Delta R.T.: -0.012 min
Response: 2089170
Conc: 0.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

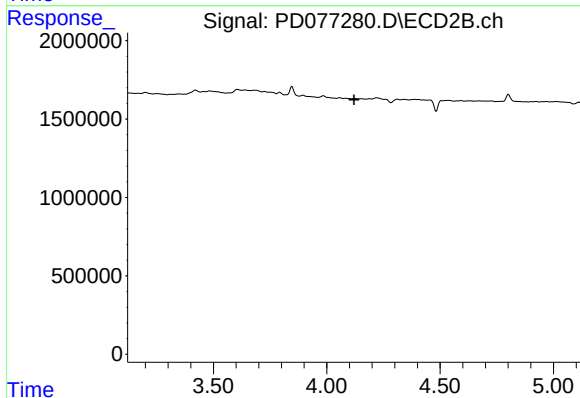


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.120 min
Response: 0
Conc: N.D.

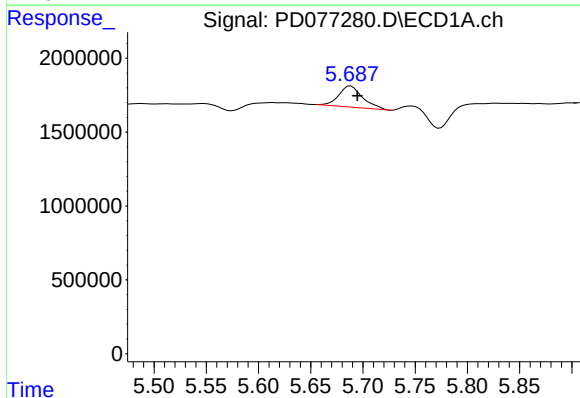


#8 Heptachlor epoxide

R.T.: 5.688 min
Delta R.T.: -0.006 min
Response: 2276149
Conc: 0.69 ng/ml

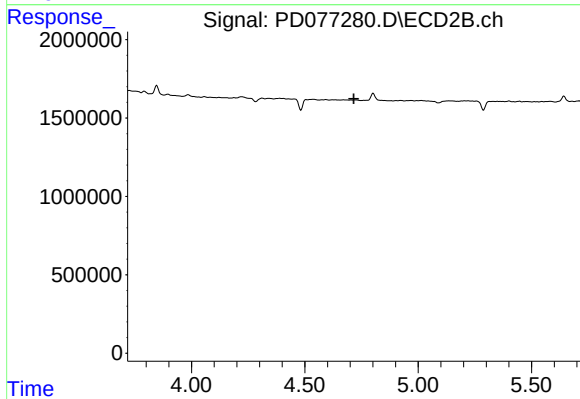

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.716 min
Response: 0
Conc: N.D.

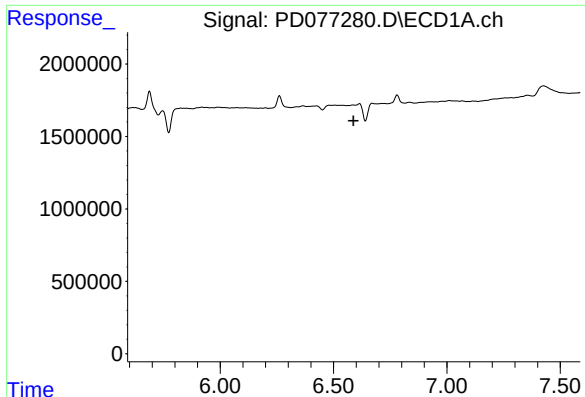

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.588 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

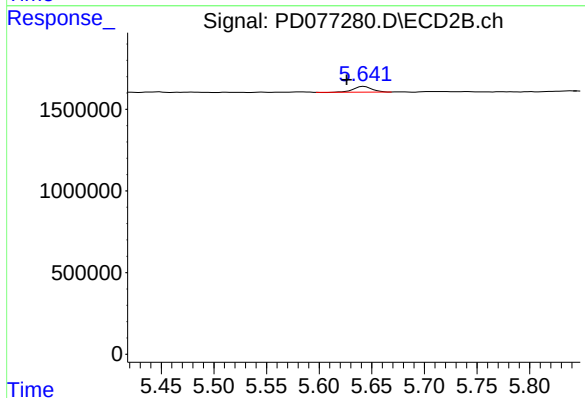


#14 Endrin

R.T.: 5.643 min
Delta R.T.: 0.017 min
Response: 432644
Conc: 0.30 ng/ml

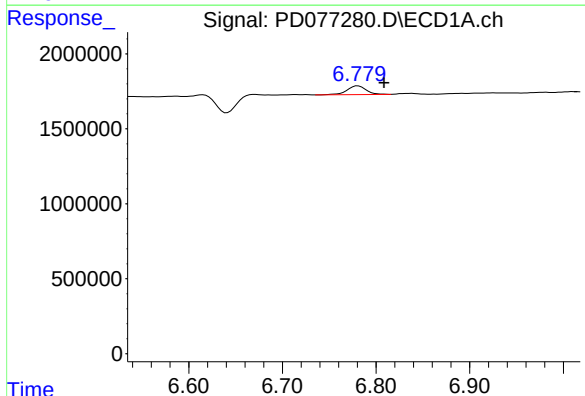


#15 Endosulfan II

R.T.: 6.781 min
Delta R.T.: -0.028 min
Response: 835358
Conc: 0.26 ng/ml

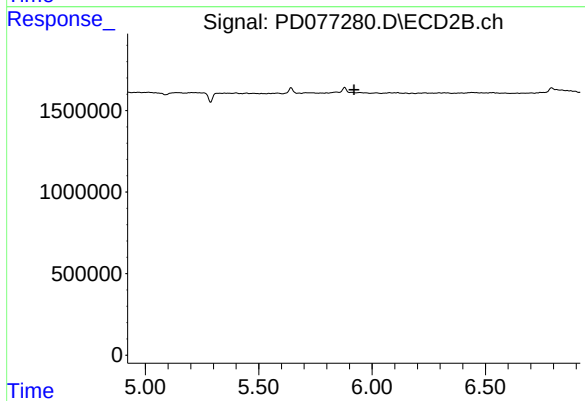

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.920 min
Response: 0
Conc: N.D.

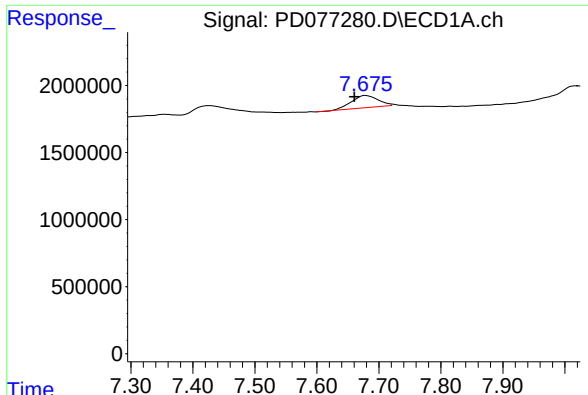

#21 Endrin ketone


R.T.: 7.678 min
Delta R.T.: 0.017 min
Response: 2702181
Conc: 0.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

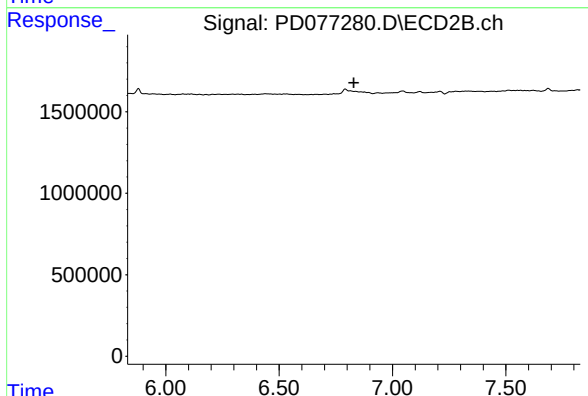


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.830 min
Response: 0
Conc: N.D.

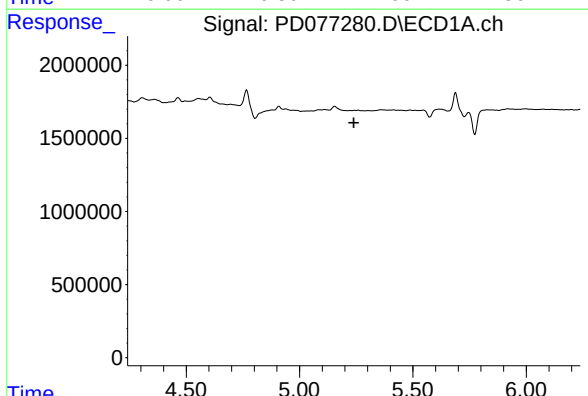


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.240 min
Response: 0
Conc: N.D.

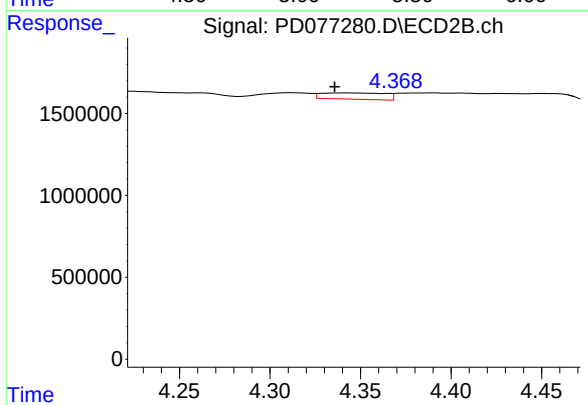

#24 Chlordane-2


R.T.: 4.343 min
Delta R.T.: 0.007 min
Response: 944445
Conc: 16.79 ng/ml

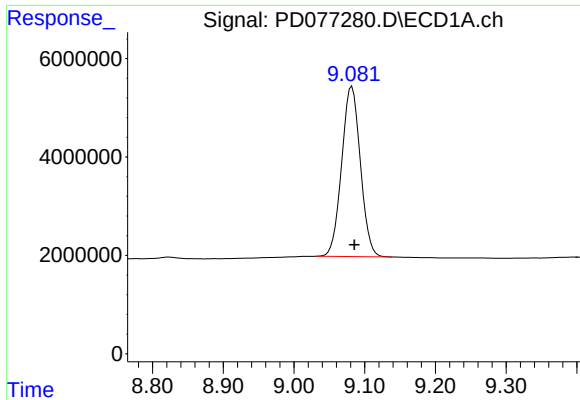

#28 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: -0.004 min
Response: 63618575
Conc: 23.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

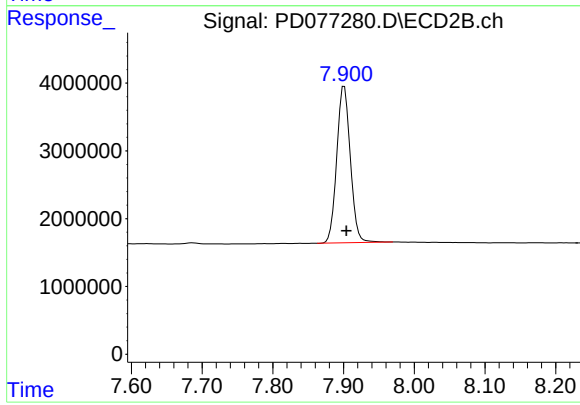

#28 Decachlorobiphenyl

R.T.: 7.901 min
Delta R.T.: -0.003 min
Response: 30865191
Conc: 21.57 ng/ml