

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082123\
 Data File : PD077293.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2023 21:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 22:29:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.761	49140749	29172526	20.765	21.417
28)	SA Decachlor...	9.082	7.902	60942599	31005791	22.240	21.666
Target Compounds							
3)	MA gamma-BHC...	0.000	3.608	0	58117	N.D.	0.031 #
4)	MA Heptachlor	4.910	0.000	294492	0	0.082	N.D. #
7)	B delta-BHC	4.767	0.000	1953004	0	0.560	N.D. #
8)	B Heptachlo...	5.688	0.000	2153481	0	0.650	N.D. #
14)	MA Endrin	0.000	5.643f	0	597109	N.D.	0.408 #
15)	B Endosulfa...	6.781f	0.000	747210	0	0.235	N.D. #
21)	B Endrin ke...	7.689f	0.000	107629	0	0.036	N.D. #
24)	Chlordane-2	0.000	4.337	0	510482	N.D.	9.078 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082123\
Data File : PD077293.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 21:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:29:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

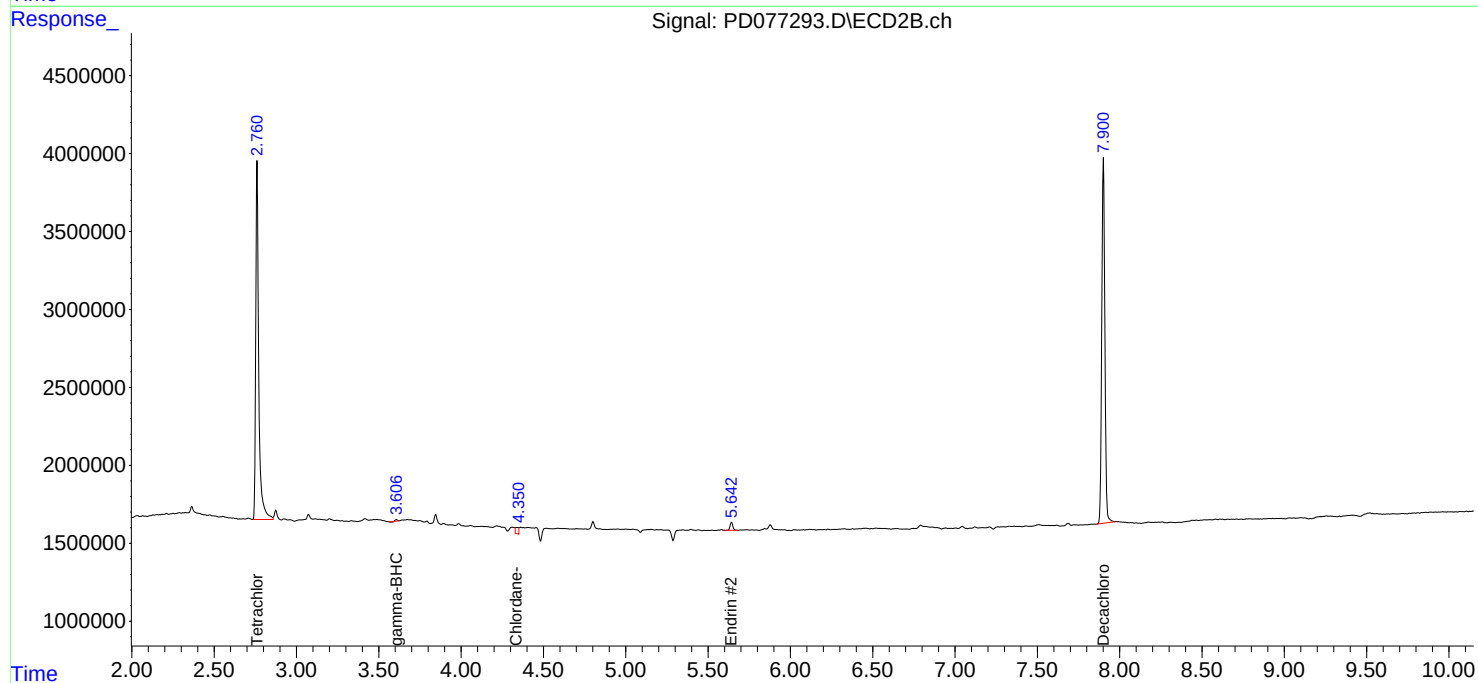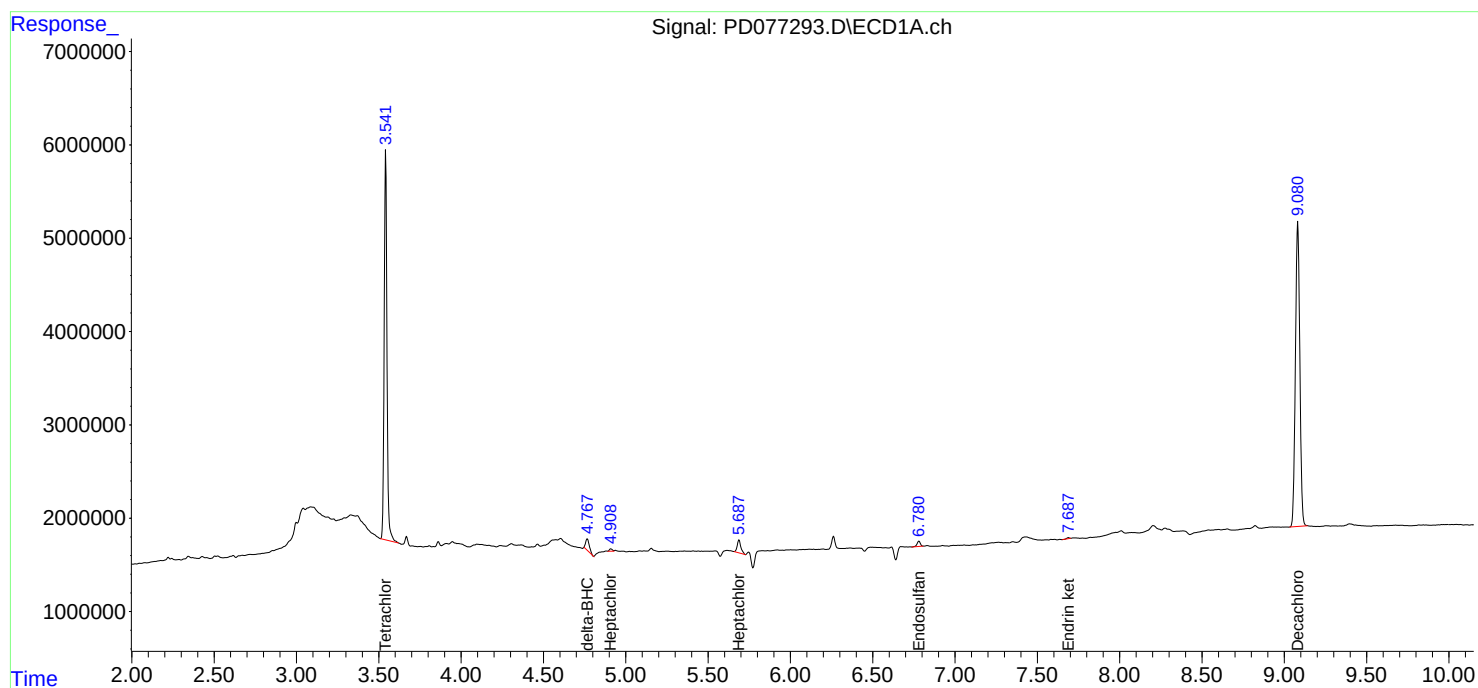


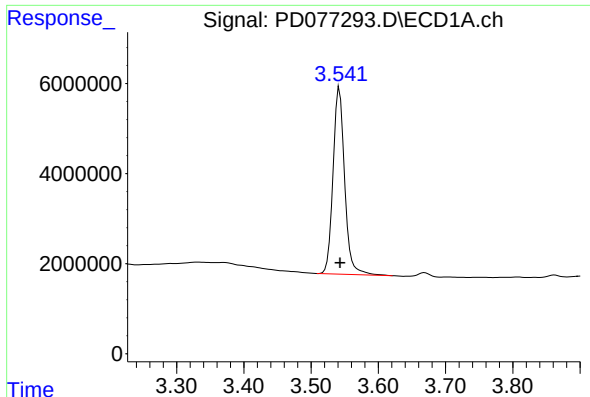

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 49140749
Conc: 20.77 ng/ml

Instrument :
ECD_D
ClientSampleId :

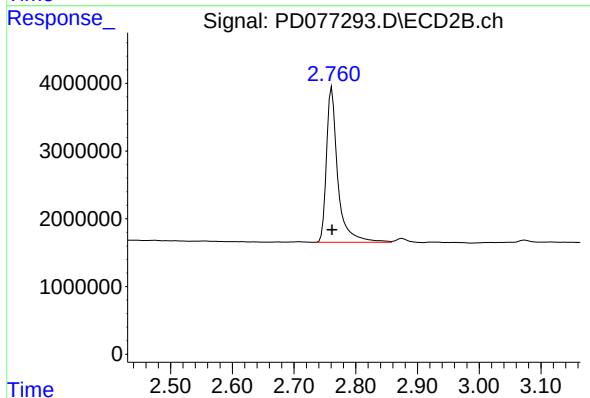


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 29172526
Conc: 21.42 ng/ml

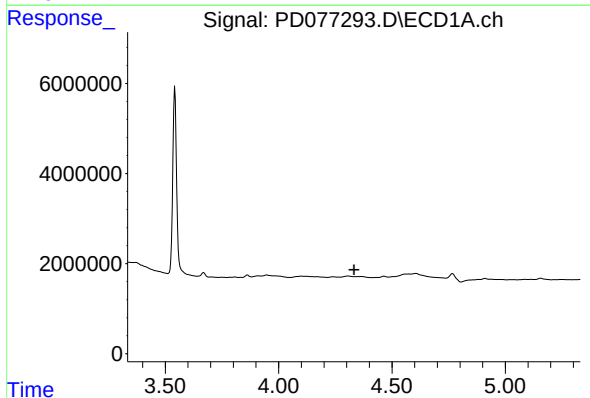


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.333 min
Response: 0
Conc: N.D.

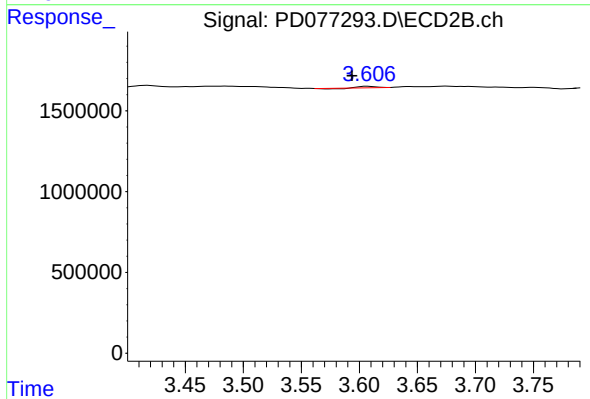

#3 gamma-BHC (Lindane)


R.T.: 3.608 min
Delta R.T.: 0.014 min
Response: 58117
Conc: 0.03 ng/ml

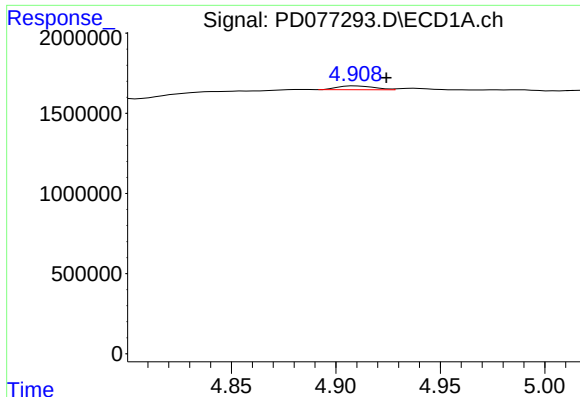

#4 Heptachlor


R.T.: 4.910 min
Delta R.T.: -0.015 min
Response: 294492
Conc: 0.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

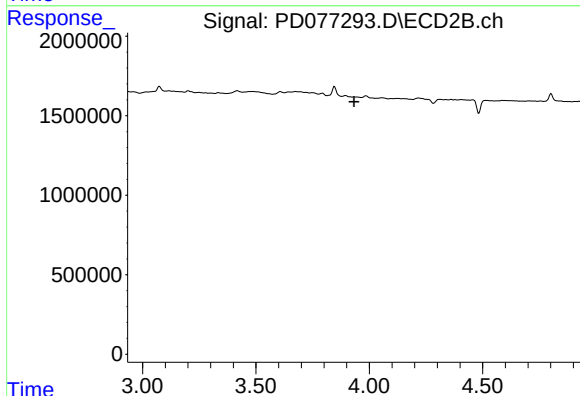


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 3.933 min
Response: 0
Conc: N.D.

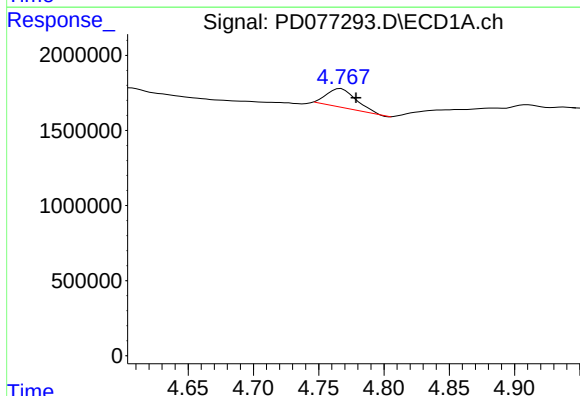


#7 delta-BHC

R.T.: 4.767 min
Delta R.T.: -0.012 min
Response: 1953004
Conc: 0.56 ng/ml

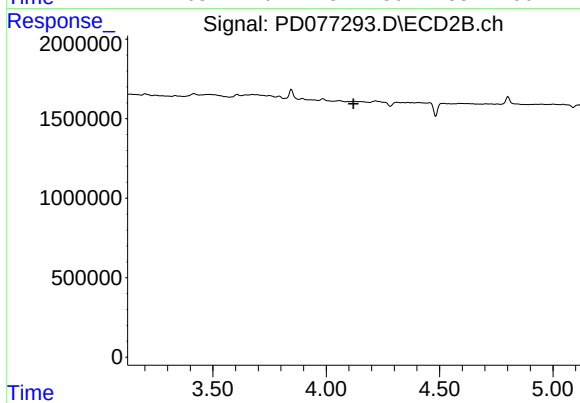

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.120 min
Response: 0
Conc: N.D.

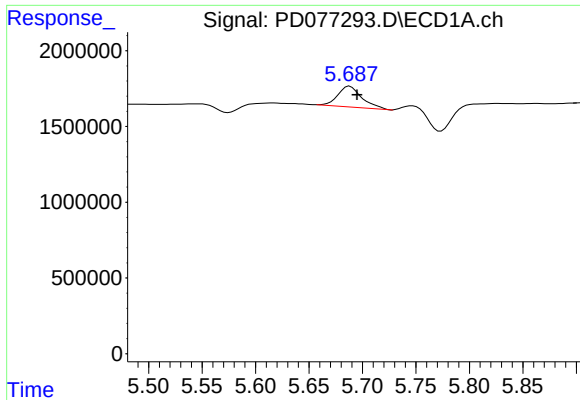

#8 Heptachlor epoxide


R.T.: 5.688 min
Delta R.T.: -0.007 min
Response: 2153481
Conc: 0.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

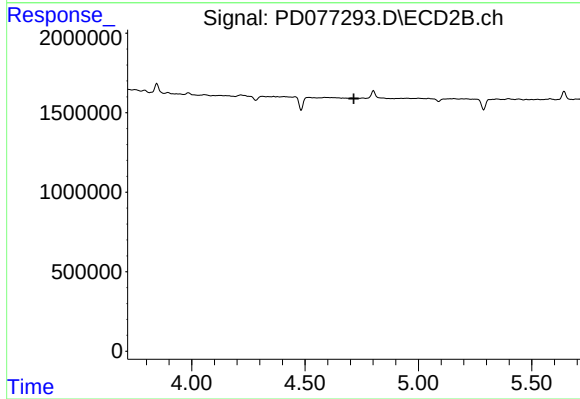


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.716 min
Response: 0
Conc: N.D.

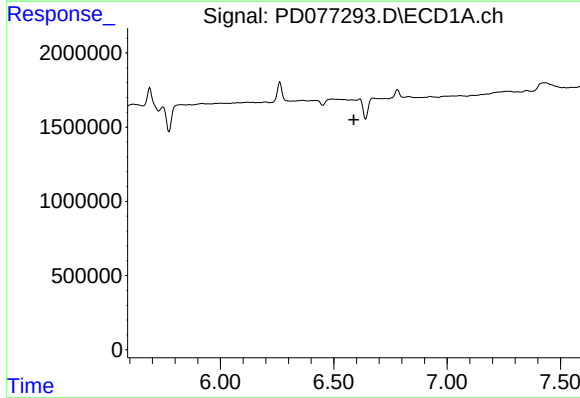


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.588 min
Response: 0
Conc: N.D.

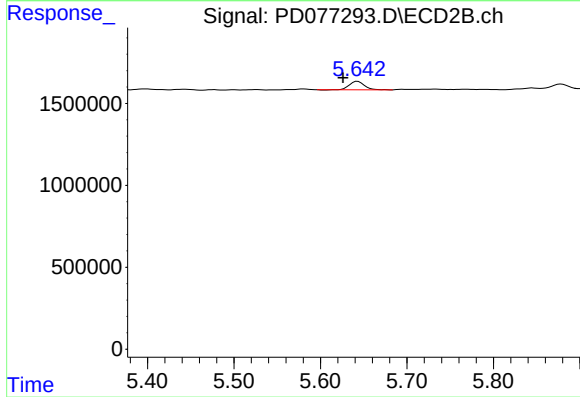

#14 Endrin


R.T.: 5.643 min
Delta R.T.: 0.017 min
Response: 597109
Conc: 0.41 ng/ml

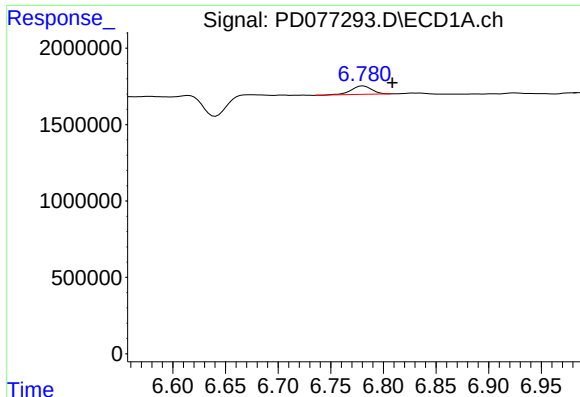

#15 Endosulfan II


R.T.: 6.781 min
Delta R.T.: -0.028 min
Response: 747210
Conc: 0.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

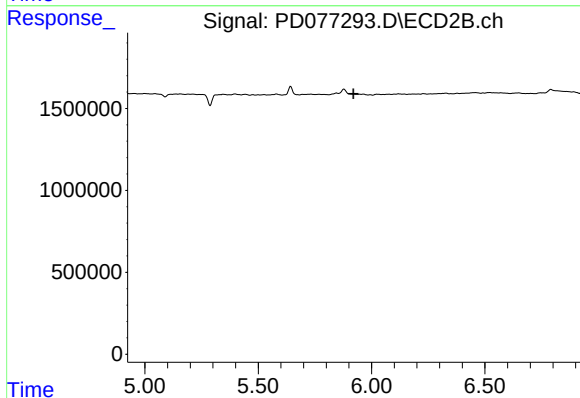


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.920 min
Response: 0
Conc: N.D.

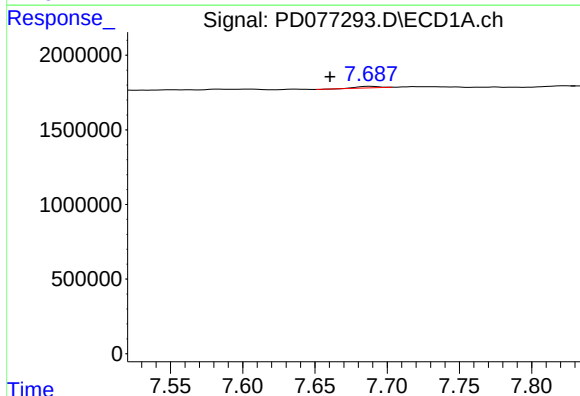


#21 Endrin ketone

R.T.: 7.689 min
Delta R.T.: 0.028 min
Response: 107629
Conc: 0.04 ng/ml

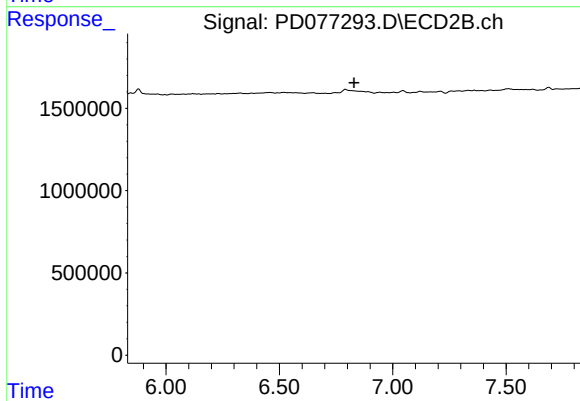

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.830 min
Response: 0
Conc: N.D.

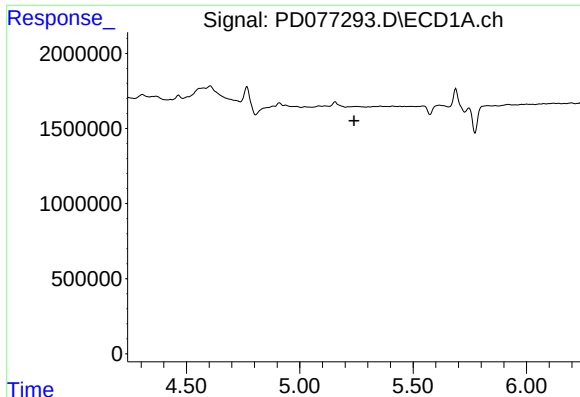

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.240 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

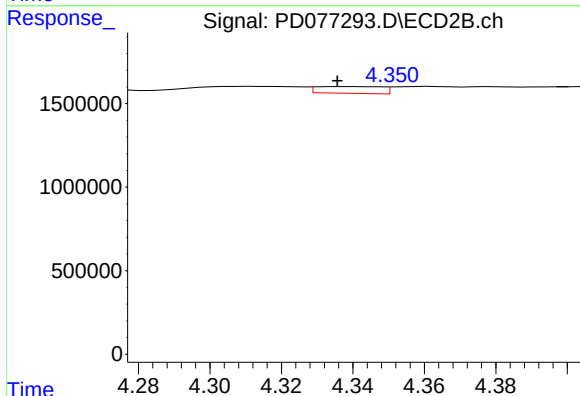


#24 Chlordane-2

R.T.: 4.337 min
Delta R.T.: 0.001 min
Response: 510482
Conc: 9.08 ng/ml

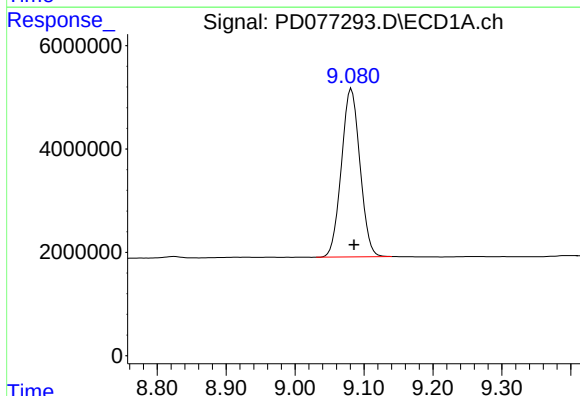

#28 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: -0.004 min
Response: 60942599
Conc: 22.24 ng/ml

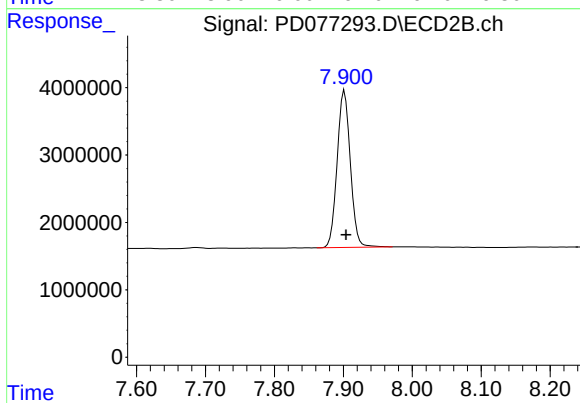

#28 Decachlorobiphenyl

R.T.: 7.902 min
Delta R.T.: -0.002 min
Response: 31005791
Conc: 21.67 ng/ml