

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082123\
 Data File : PD077306.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2023 00:24
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 05:53:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.761	45450142	26955903	19.206	19.790
28)	SA Decachlor...	9.081	7.901	57874594	29318477	21.121	20.487
Target Compounds							
2)	A alpha-BHC	3.998	3.263	35289139	18717030	9.191	9.676
3)	MA gamma-BHC...	4.332	3.592	34415079	17557796	9.350	9.438
6)	B beta-BHC	4.529	3.889	16257096	8538808	10.803	11.193
7)	B delta-BHC	4.766	0.000	1027516	0	0.295	N.D. #
8)	B Heptachlo...	5.687	0.000	1705845	0	0.515	N.D. #
9)	A Endosulfan I	6.109f	0.000	221435	0	0.073	N.D. #
12)	B 4,4'-DDE	6.201	5.218	542044	1220952	0.183	0.842 #
13)	MA Dieldrin	6.378f	0.000	619556	0	0.189	N.D. #
14)	MA Endrin	6.586	5.624	121.2E6	66339770	43.612	45.338
15)	B Endosulfa...	6.823	5.933	1928156	662980	0.606	0.450 #
16)	A 4,4'-DDD	6.720	5.772	5627775	3015254	2.392	2.711
17)	MA 4,4'-DDT	7.035	6.022	248.0E6	130.9E6	102.008	117.791
18)	B Endrin al...	6.936	6.098	4685496	3431040	2.145	3.014 #
20)	A Methoxychlor	7.511	6.597	332.7E6	164.1E6	234.797	274.404
21)	B Endrin ke...	7.657	6.826	9773967	6060663	3.245	3.823
22)	Mirex	8.148	0.000	234399	0	0.103	N.D. #
27)	Chlordane-5	0.000	5.933	0	662980	N.D.	11.097 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082123\
Data File : PD077306.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2023 00:24
Operator : AR\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 05:53:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

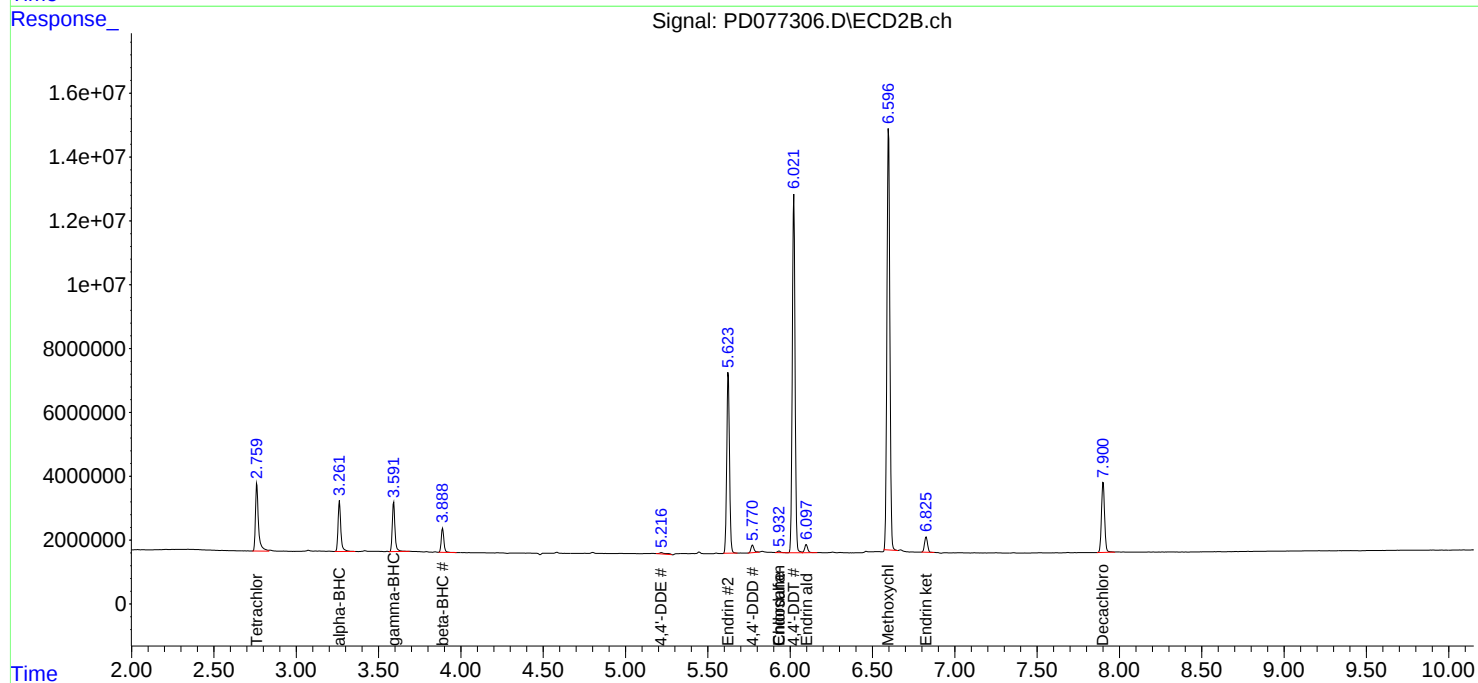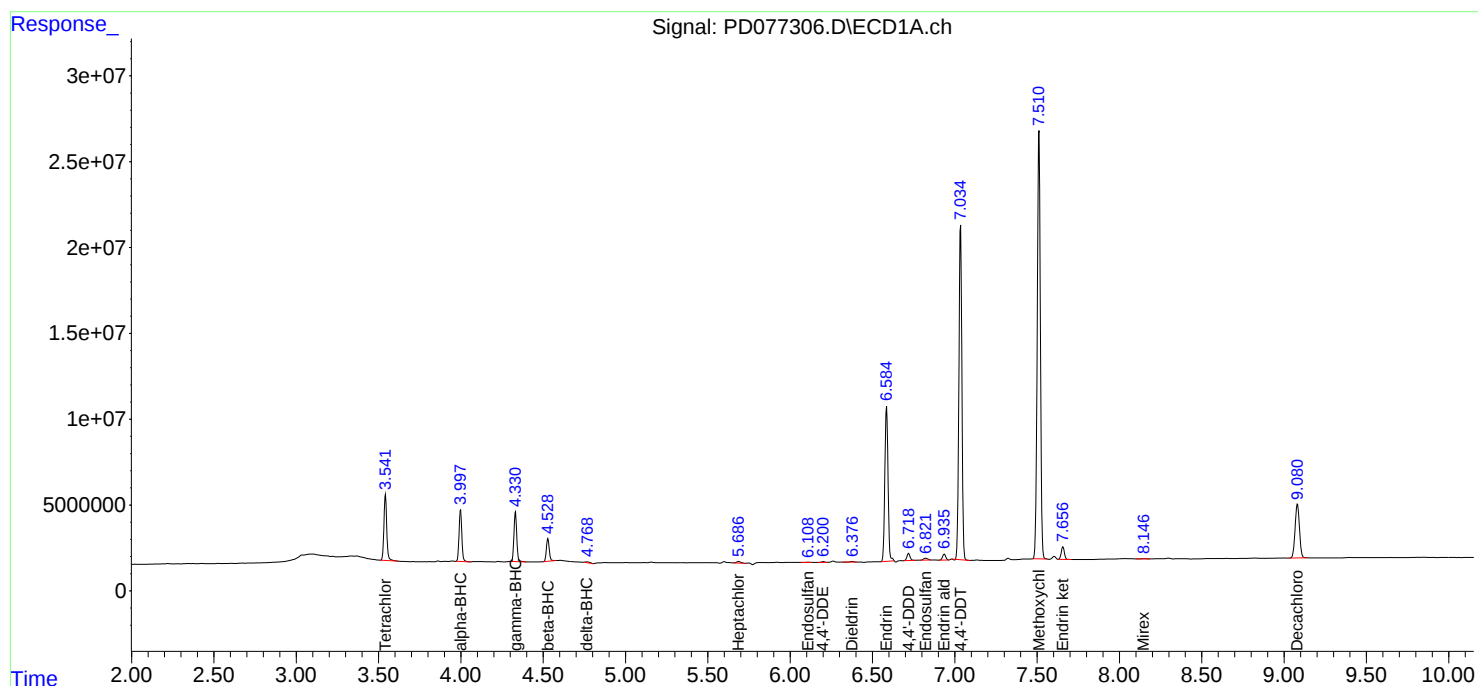


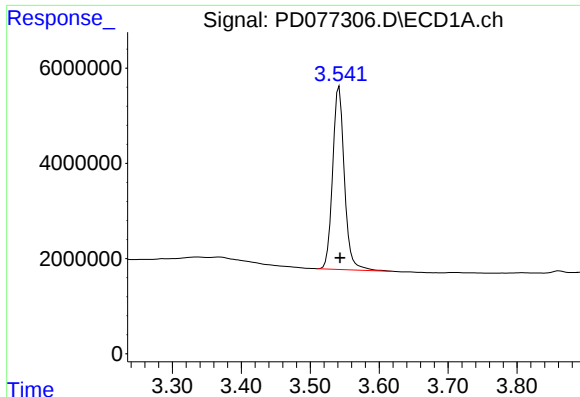

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: -0.001 min
Response: 45450142
Conc: 19.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

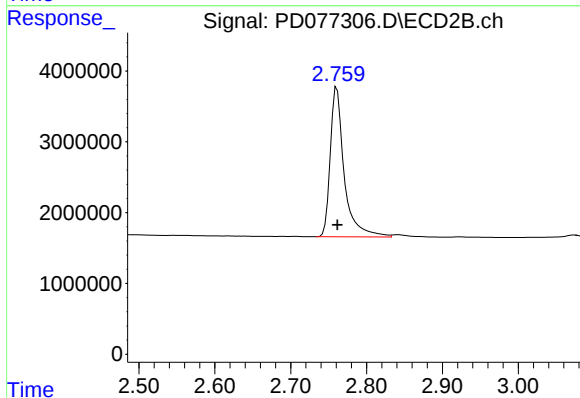


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 26955903
Conc: 19.79 ng/ml

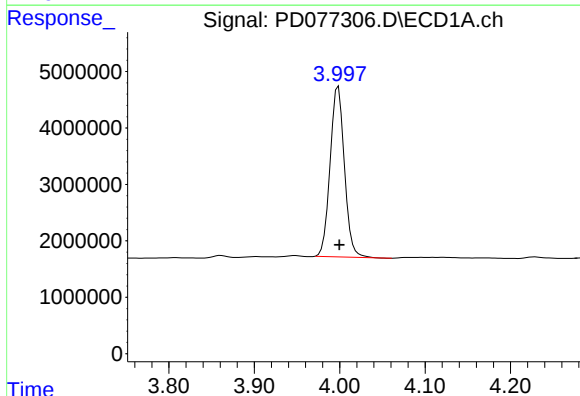


#2 alpha-BHC

R.T.: 3.998 min
Delta R.T.: -0.001 min
Response: 35289139
Conc: 9.19 ng/ml

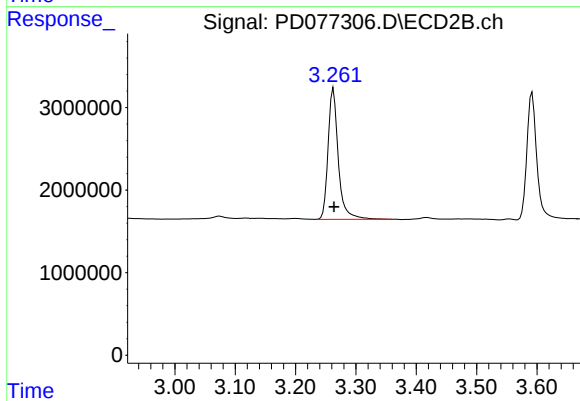

#2 alpha-BHC


R.T.: 3.263 min
Delta R.T.: -0.001 min
Response: 18717030
Conc: 9.68 ng/ml

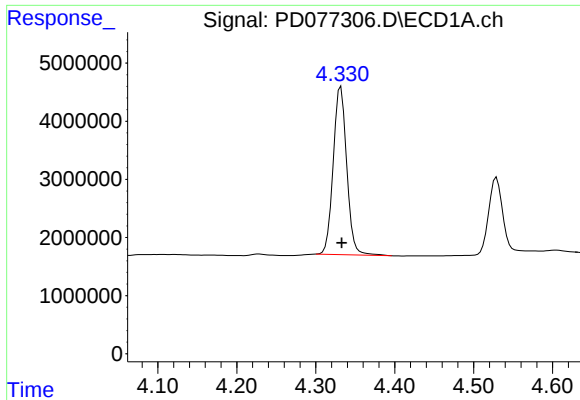

#3 gamma-BHC (Lindane)


R.T.: 4.332 min
Delta R.T.: -0.001 min
Response: 34415079
Conc: 9.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

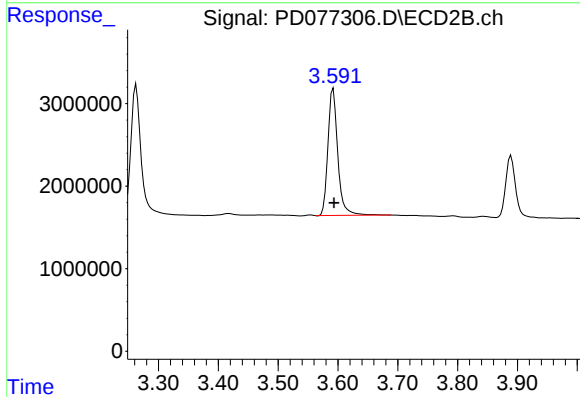


#3 gamma-BHC (Lindane)

R.T.: 3.592 min
Delta R.T.: -0.002 min
Response: 17557796
Conc: 9.44 ng/ml

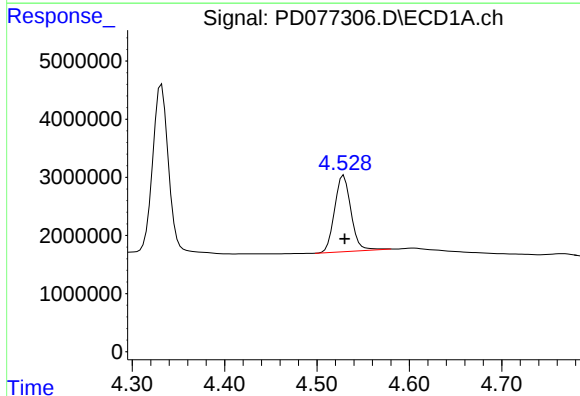


#6 beta-BHC

R.T.: 4.529 min
Delta R.T.: 0.000 min
Response: 16257096
Conc: 10.80 ng/ml

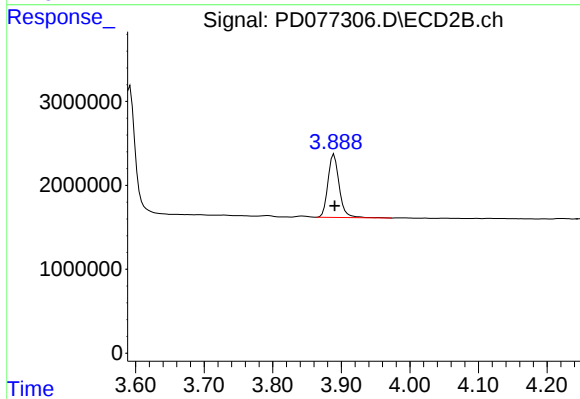

#6 beta-BHC


R.T.: 3.889 min
Delta R.T.: -0.001 min
Response: 8538808
Conc: 11.19 ng/ml

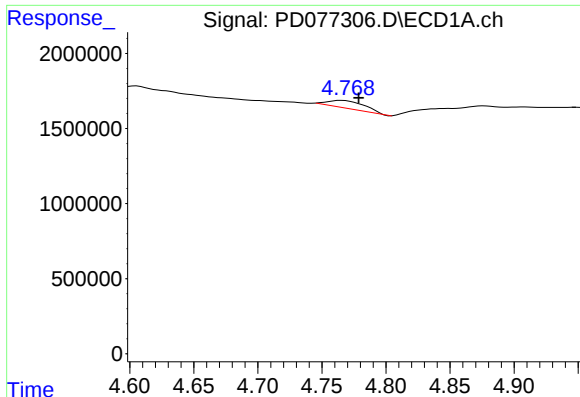

#7 delta-BHC


R.T.: 4.766 min
Delta R.T.: -0.012 min
Response: 1027516
Conc: 0.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

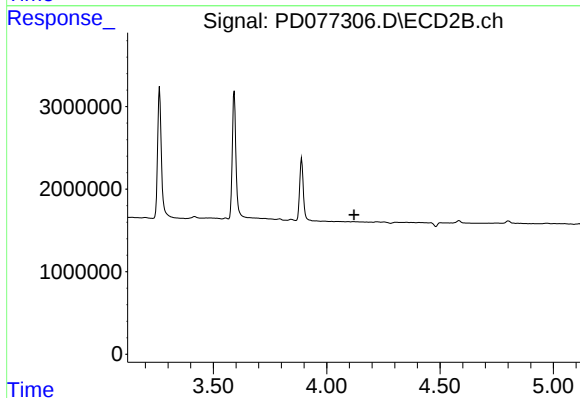


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.120 min
Response: 0
Conc: N.D.

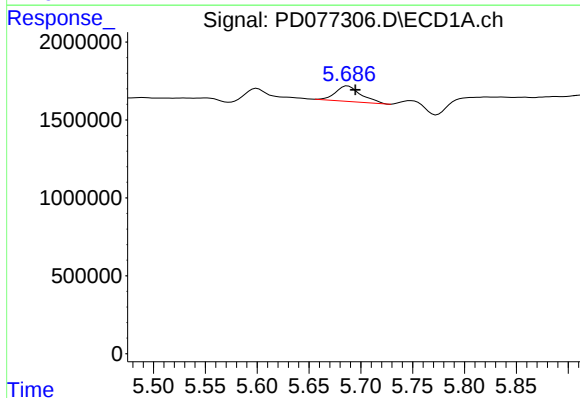


#8 Heptachlor epoxide

R.T.: 5.687 min
Delta R.T.: -0.007 min
Response: 1705845
Conc: 0.52 ng/ml

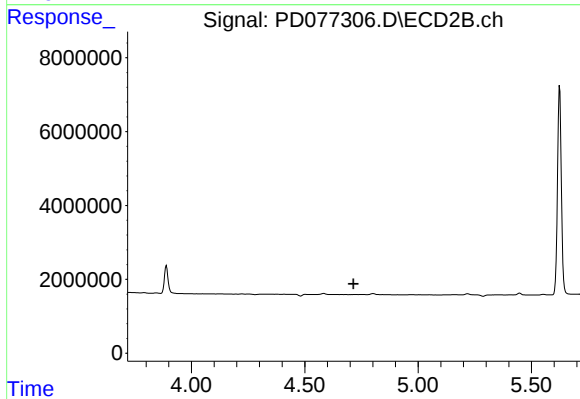

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.716 min
Response: 0
Conc: N.D.

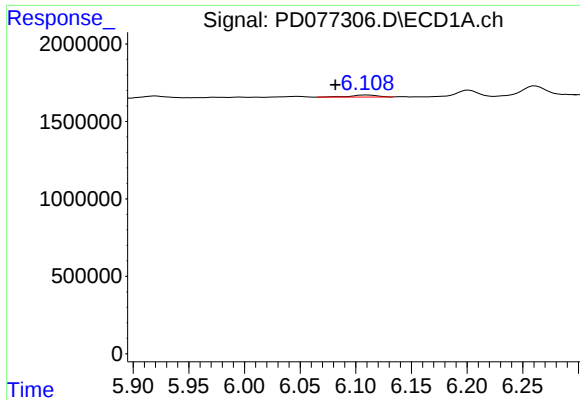

#9 Endosulfan I


R.T.: 6.109 min
Delta R.T.: 0.028 min
Response: 221435
Conc: 0.07 ng/ml

Instrument :
ECD_D
ClientSampleId :

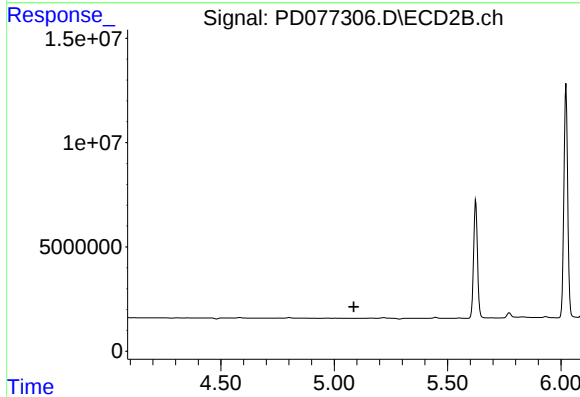


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.086 min
Response: 0
Conc: N.D.

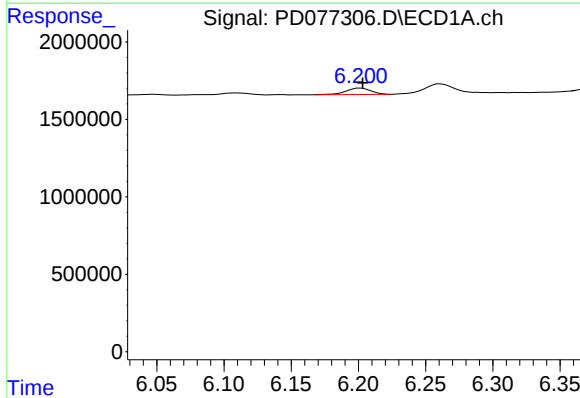


#12 4,4'-DDE

R.T.: 6.201 min
Delta R.T.: -0.002 min
Response: 542044
Conc: 0.18 ng/ml

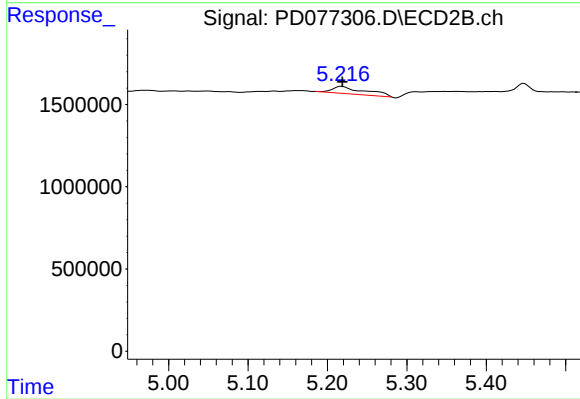

#12 4,4'-DDE


R.T.: 5.218 min
Delta R.T.: 0.000 min
Response: 1220952
Conc: 0.84 ng/ml

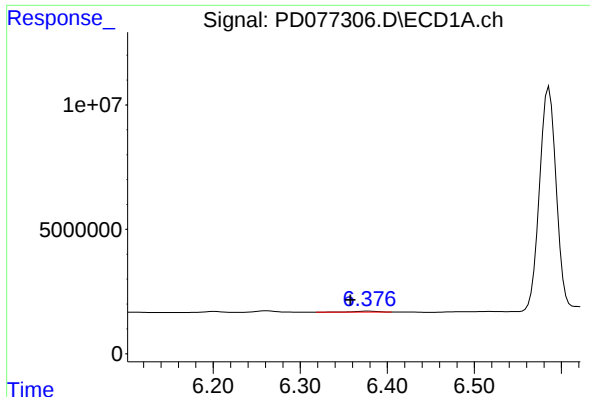

#13 Dieldrin


R.T.: 6.378 min
Delta R.T.: 0.020 min
Response: 619556
Conc: 0.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

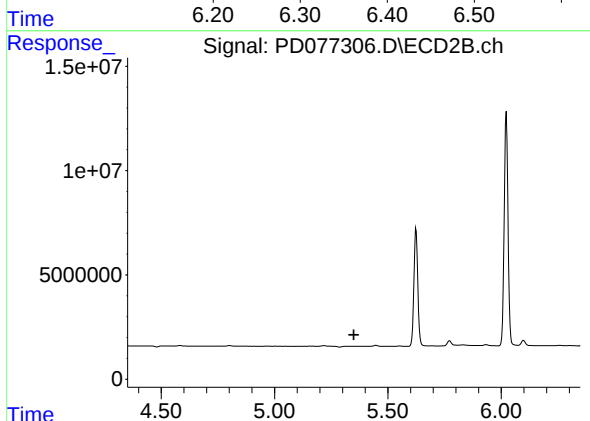


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.350 min
Response: 0
Conc: N.D.

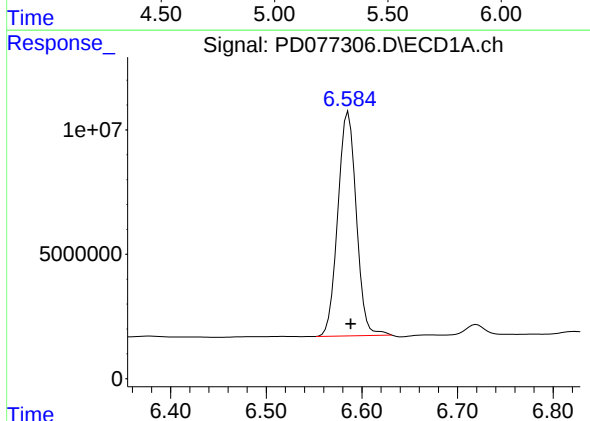


#14 Endrin

R.T.: 6.586 min
Delta R.T.: -0.003 min
Response: 121183179
Conc: 43.61 ng/ml

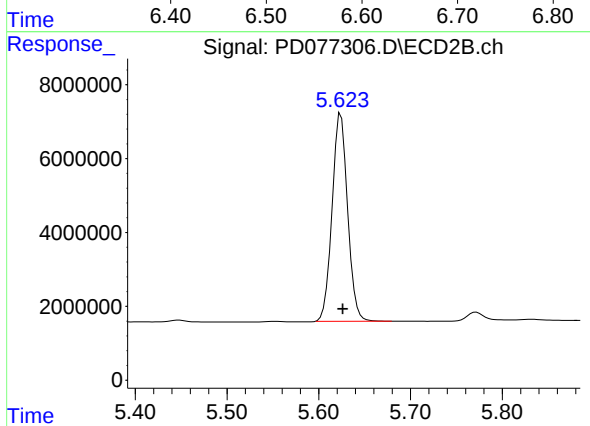

#14 Endrin


R.T.: 5.624 min
Delta R.T.: -0.002 min
Response: 66339770
Conc: 45.34 ng/ml

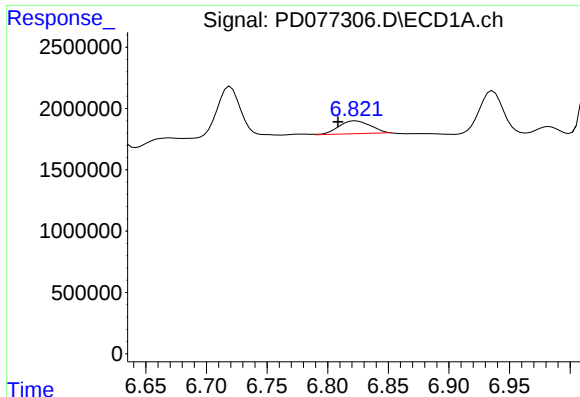

#15 Endosulfan II


R.T.: 6.823 min
Delta R.T.: 0.014 min
Response: 1928156
Conc: 0.61 ng/ml

Instrument :
ECD_D
ClientSampleId :

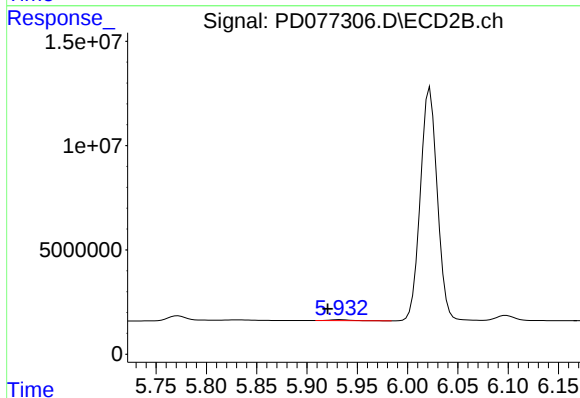


#15 Endosulfan II

R.T.: 5.933 min
Delta R.T.: 0.012 min
Response: 662980
Conc: 0.45 ng/ml

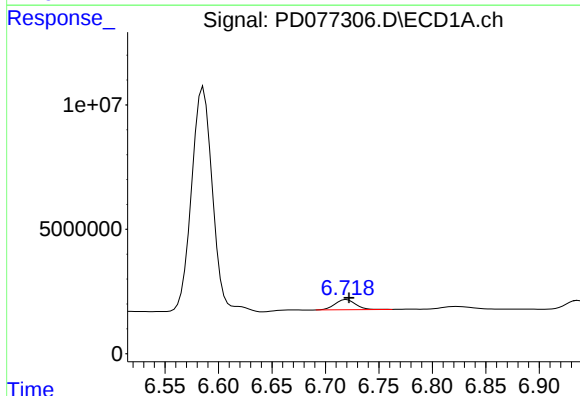


#16 4,4'-DDD

R.T.: 6.720 min
Delta R.T.: -0.003 min
Response: 5627775
Conc: 2.39 ng/ml

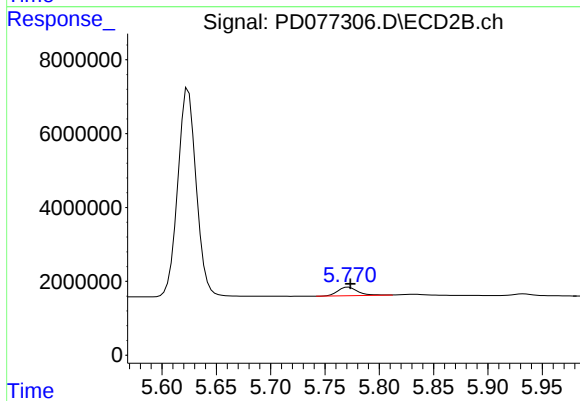

#16 4,4'-DDD


R.T.: 5.772 min
Delta R.T.: -0.002 min
Response: 3015254
Conc: 2.71 ng/ml

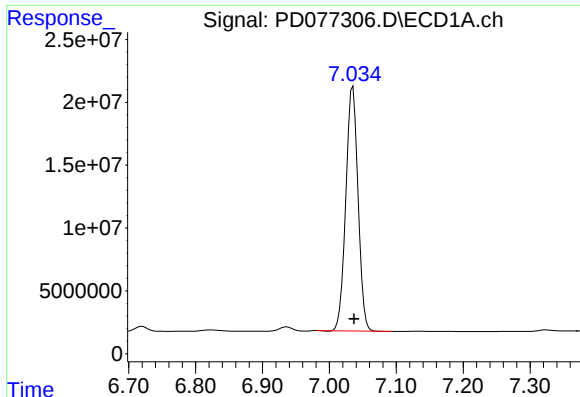

#17 4,4'-DDT


R.T.: 7.035 min
Delta R.T.: -0.002 min
Response: 248045812
Conc: 102.01 ng/ml

Instrument :
ECD_D
ClientSampleId :

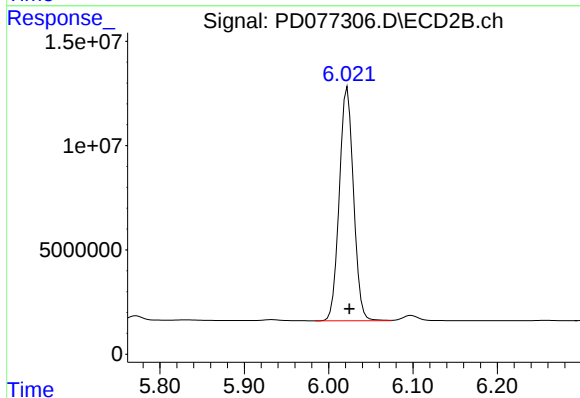


#17 4,4'-DDT

R.T.: 6.022 min
Delta R.T.: -0.002 min
Response: 130933883
Conc: 117.79 ng/ml

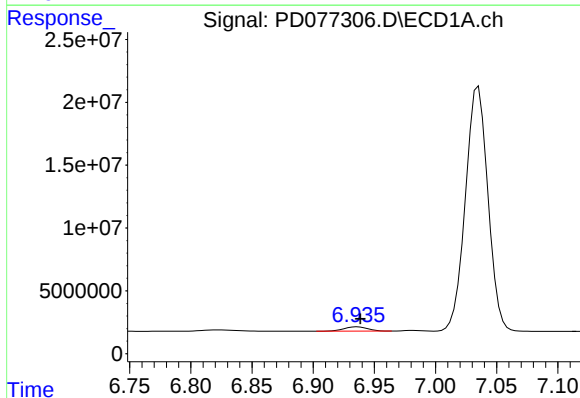


#18 Endrin aldehyde

R.T.: 6.936 min
Delta R.T.: -0.003 min
Response: 4685496
Conc: 2.14 ng/ml

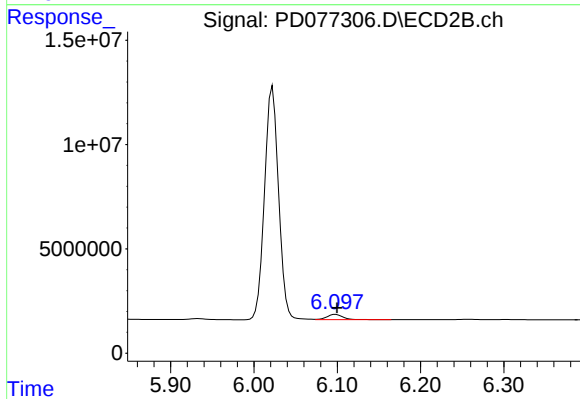

#18 Endrin aldehyde


R.T.: 6.098 min
Delta R.T.: -0.002 min
Response: 3431040
Conc: 3.01 ng/ml

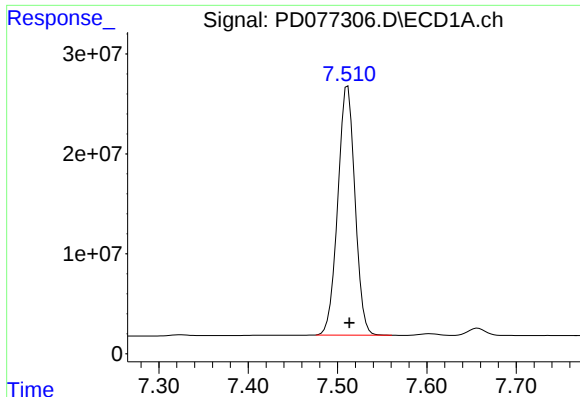

#20 Methoxychlor


R.T.: 7.511 min
Delta R.T.: -0.002 min
Response: 332676294
Conc: 234.80 ng/ml

Instrument :
ECD_D
ClientSampleId :

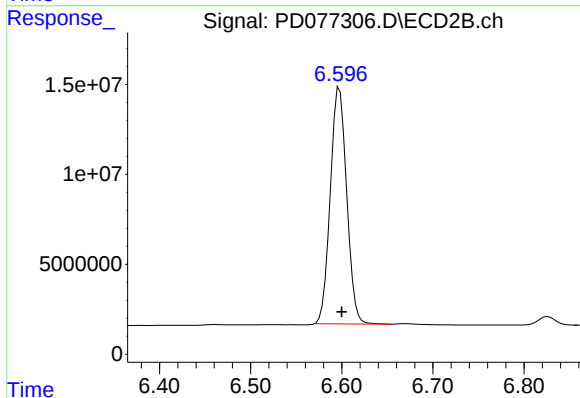


#20 Methoxychlor

R.T.: 6.597 min
Delta R.T.: -0.003 min
Response: 164076486
Conc: 274.40 ng/ml

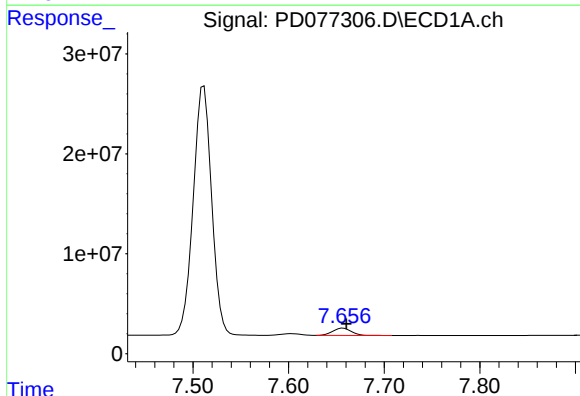


#21 Endrin ketone

R.T.: 7.657 min
Delta R.T.: -0.003 min
Response: 9773967
Conc: 3.25 ng/ml

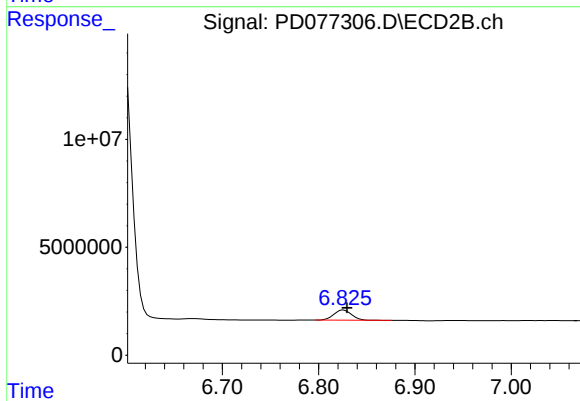

#21 Endrin ketone


R.T.: 6.826 min
Delta R.T.: -0.003 min
Response: 6060663
Conc: 3.82 ng/ml

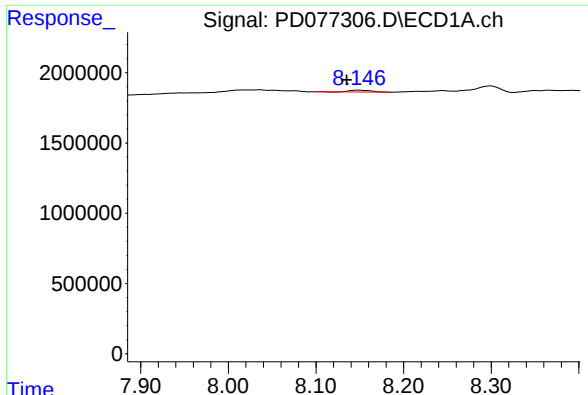

#22 Mirex


R.T.: 8.148 min
Delta R.T.: 0.013 min
Response: 234399
Conc: 0.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

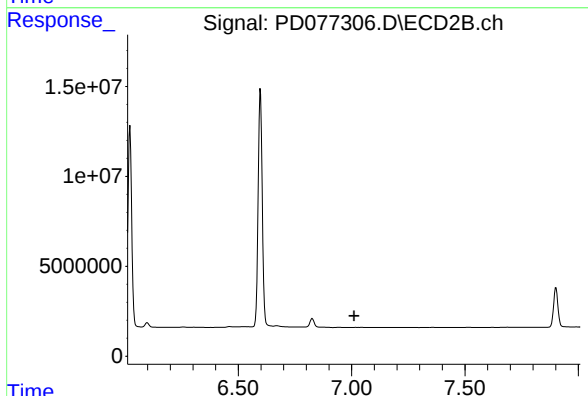


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.011 min
Response: 0
Conc: N.D.

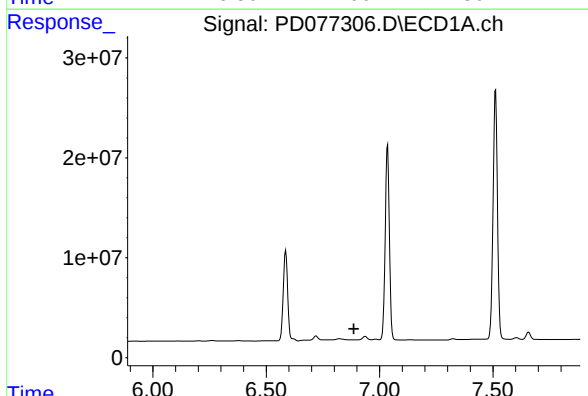


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.886 min
Response: 0
Conc: N.D.

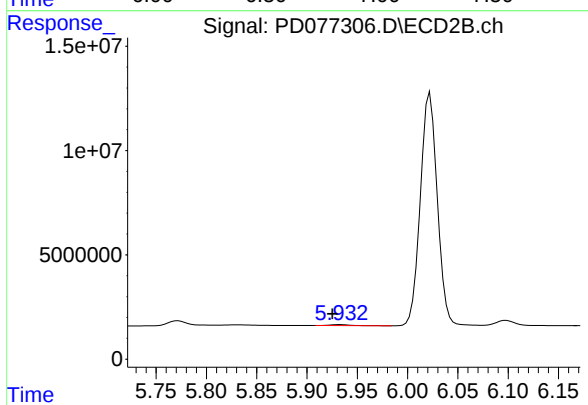

#27 Chlordane-5


R.T.: 5.933 min
Delta R.T.: 0.007 min
Response: 662980
Conc: 11.10 ng/ml

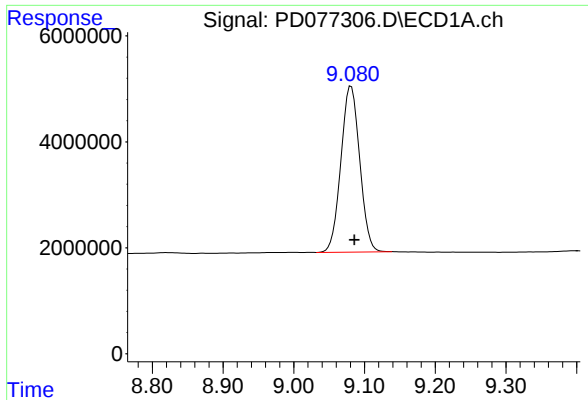

#28 Decachlorobiphenyl

R.T.: 9.081 min
Delta R.T.: -0.005 min
Response: 57874594
Conc: 21.12 ng/ml

Instrument :
ECD_D
ClientSampleId :

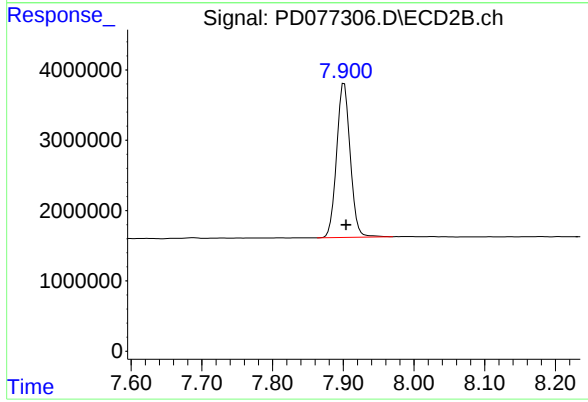

#28 Decachlorobiphenyl

R.T.: 7.901 min
Delta R.T.: -0.003 min
Response: 29318477
Conc: 20.49 ng/ml