

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082123\
 Data File : PD077251.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2023 11:06
 Operator : AR\AJ
 Sample : 04087-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EO-03-081823

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 22:17:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.762	20794965	12866033	8.787	9.446
28) SA Decachlor...	9.084	7.902	29939712	13545563	10.926	9.465
Target Compounds						
12) B 4,4'-DDE	6.201	5.217	1390588	750126	0.469	0.517



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082123\
Data File : PD077251.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:06
Operator : AR\AJ
Sample : 04087-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
EO-03-081823

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:17:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

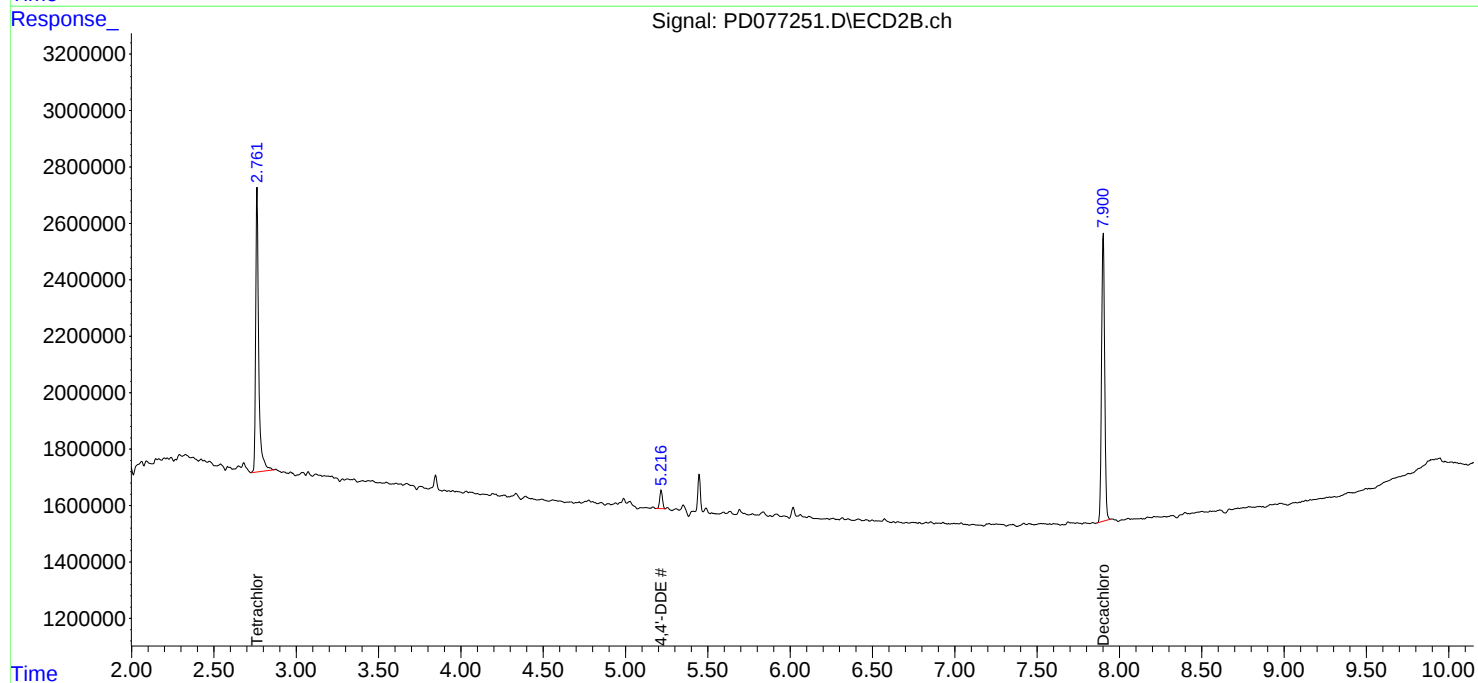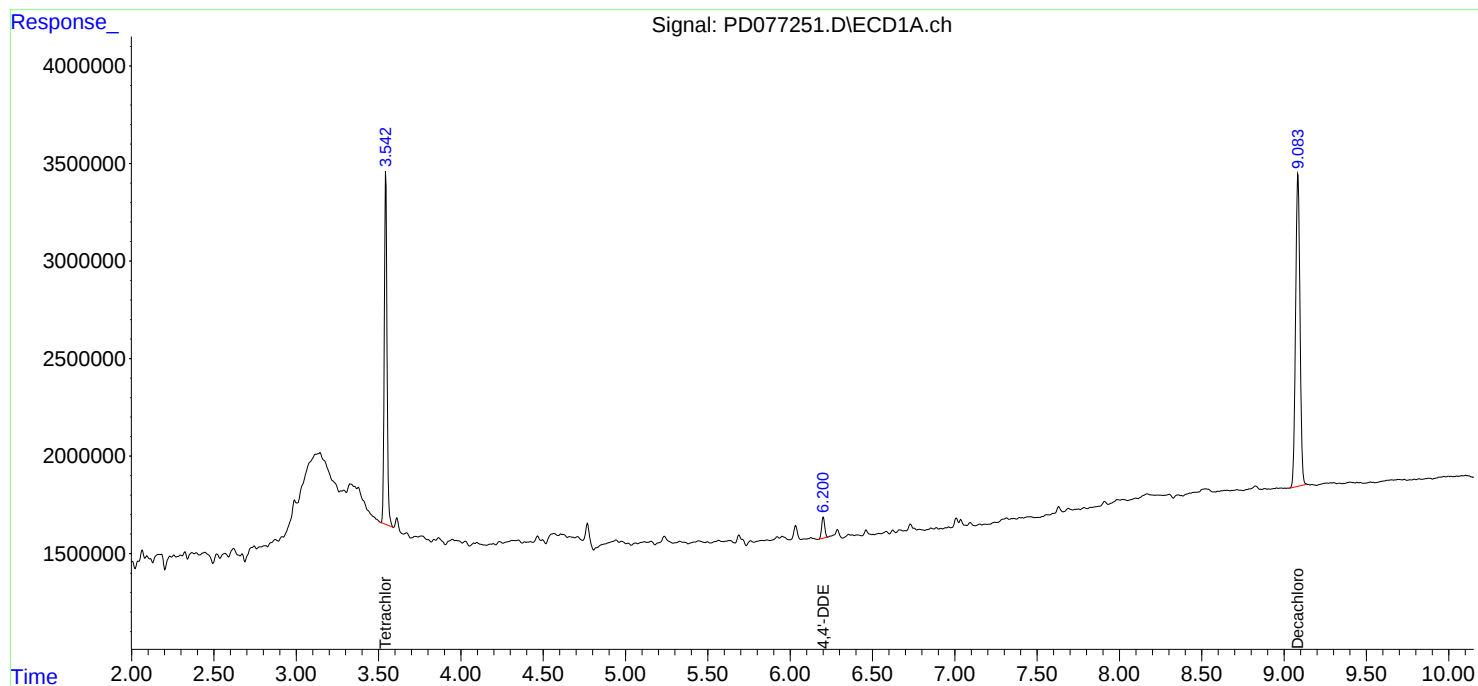


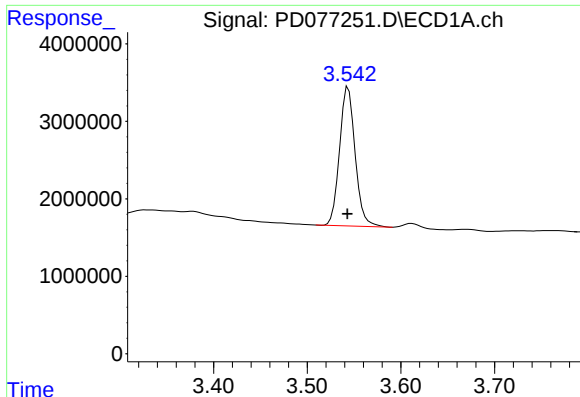

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 20794965
Conc: 8.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
EO-03-081823

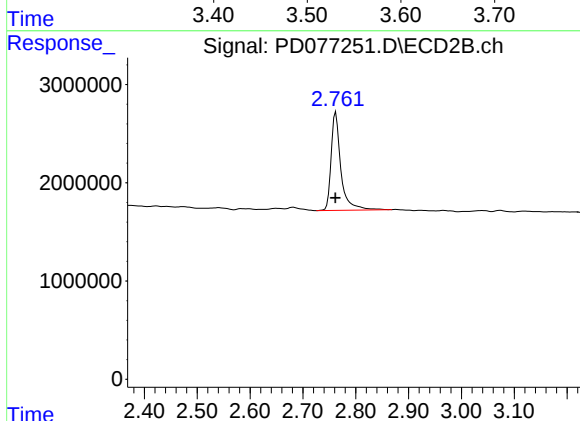


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 12866033
Conc: 9.45 ng/ml

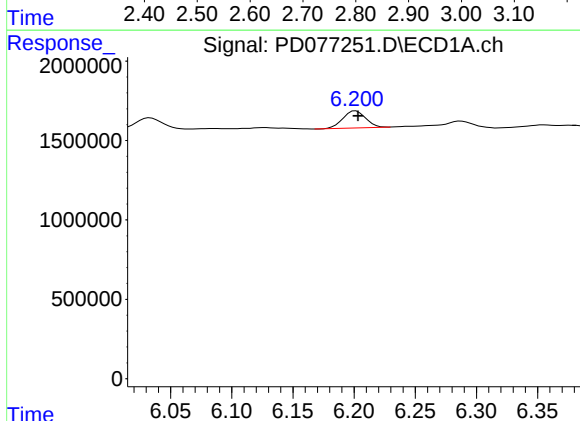


#12 4,4'-DDE

R.T.: 6.201 min
Delta R.T.: -0.002 min
Response: 1390588
Conc: 0.47 ng/ml

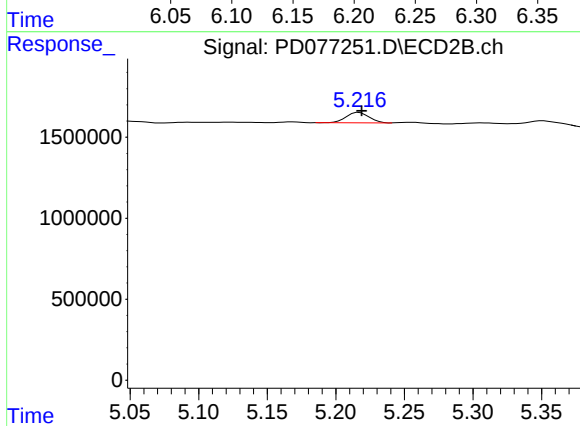

#12 4,4'-DDE


R.T.: 5.217 min
Delta R.T.: -0.002 min
Response: 750126
Conc: 0.52 ng/ml

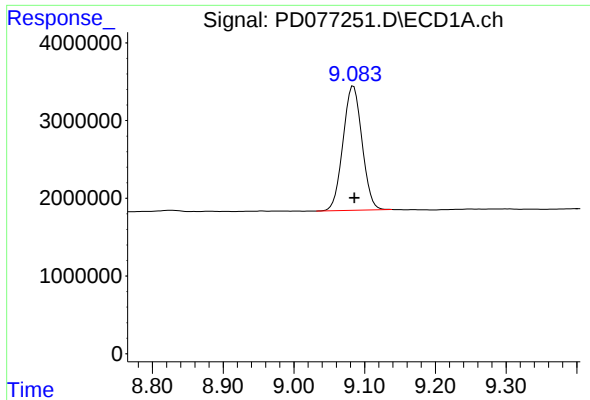

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: -0.001 min
Response: 29939712
Conc: 10.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
EO-03-081823

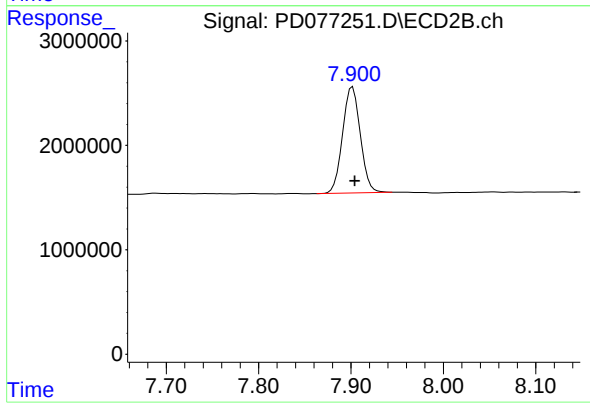

#28 Decachlorobiphenyl

R.T.: 7.902 min
Delta R.T.: -0.002 min
Response: 13545563
Conc: 9.47 ng/ml