

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082123\
 Data File : PD077261.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2023 13:26
 Operator : AR\AJ
 Sample : 04082-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 217

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 22:20:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.761	23874585	15019481	10.089	11.027
28)	SA Decachlor...	9.082	7.900	28057263	12226010	10.239	8.543
Target Compounds							
12)	B 4,4'-DDE	6.200	5.216	3550622	2084017	1.197	1.437



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082123\
Data File : PD077261.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 13:26
Operator : AR\AJ
Sample : 04082-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
217

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:20:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

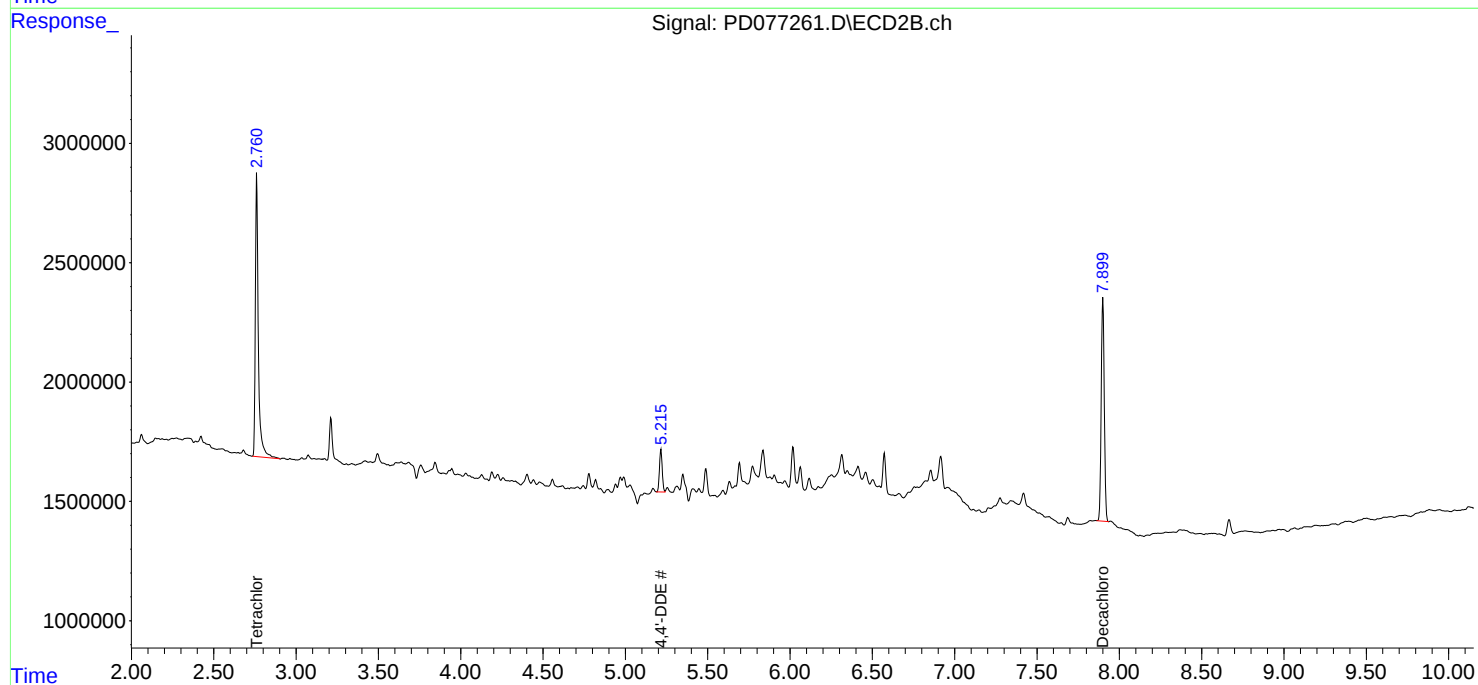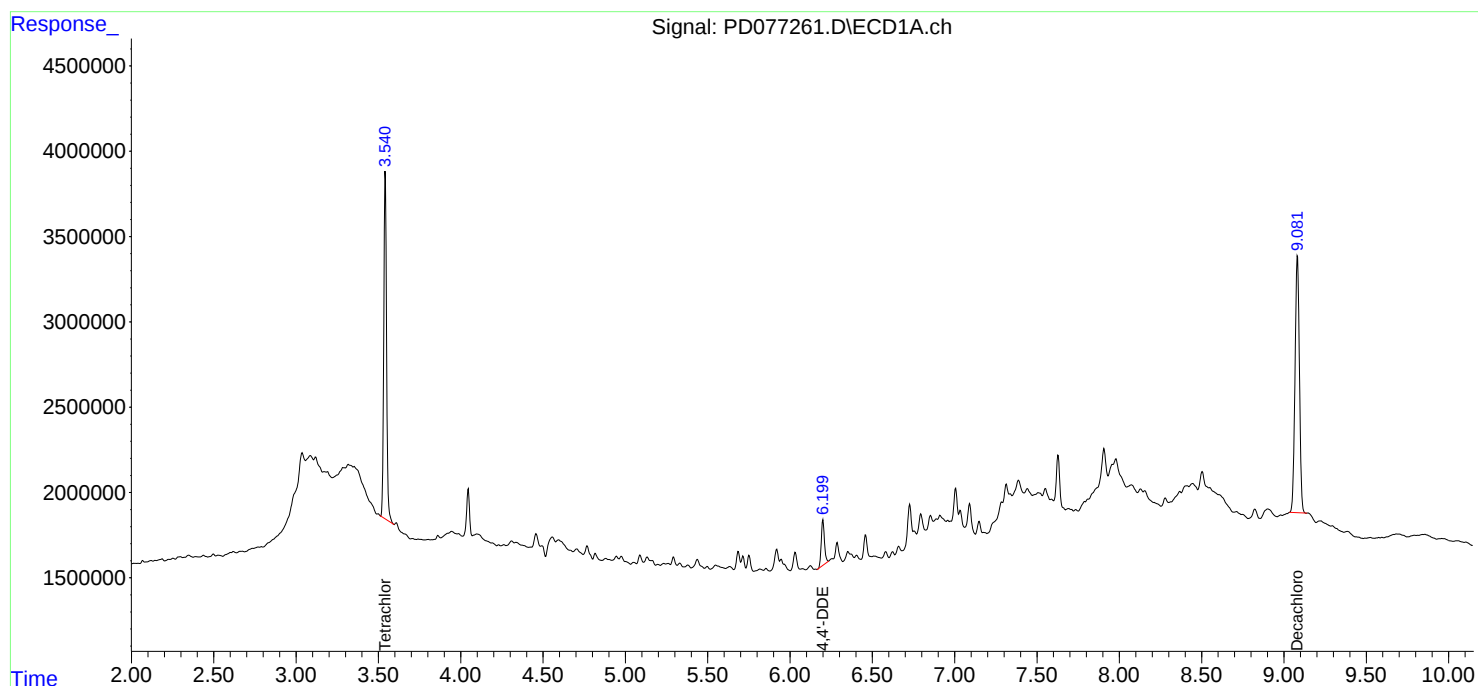


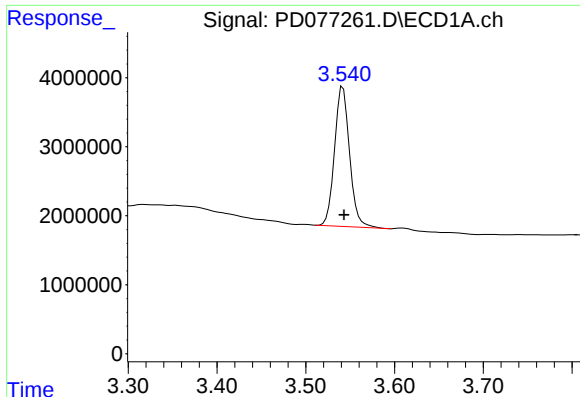

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: -0.001 min
Response: 23874585
Conc: 10.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
217

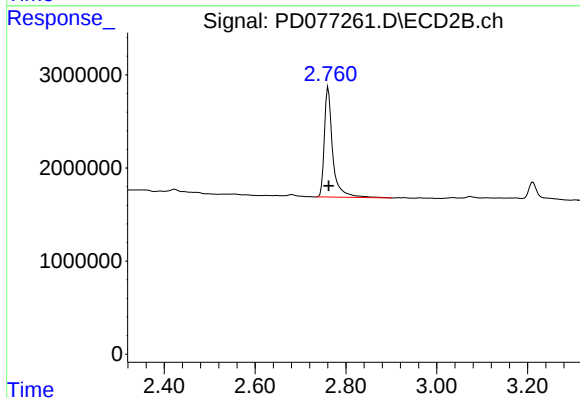


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 15019481
Conc: 11.03 ng/ml

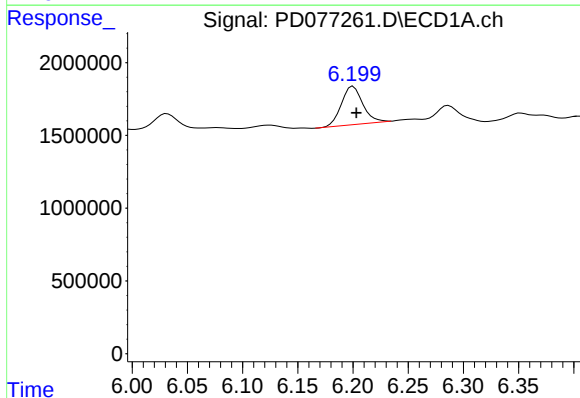


#12 4,4'-DDE

R.T.: 6.200 min
Delta R.T.: -0.003 min
Response: 3550622
Conc: 1.20 ng/ml

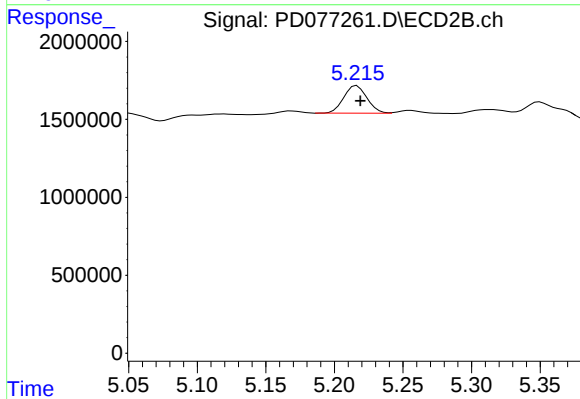

#12 4,4'-DDE

R.T.: 5.216 min
Delta R.T.: -0.002 min
Response: 2084017
Conc: 1.44 ng/ml

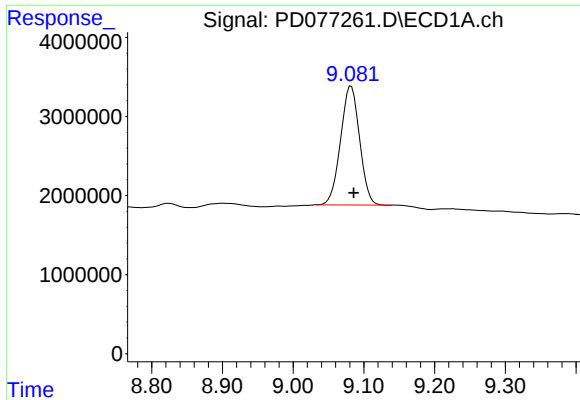

#28 Decachlorobiphenyl


R.T.: 9.082 min

Delta R.T.: -0.004 min

Response: 28057263

Conc: 10.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
217

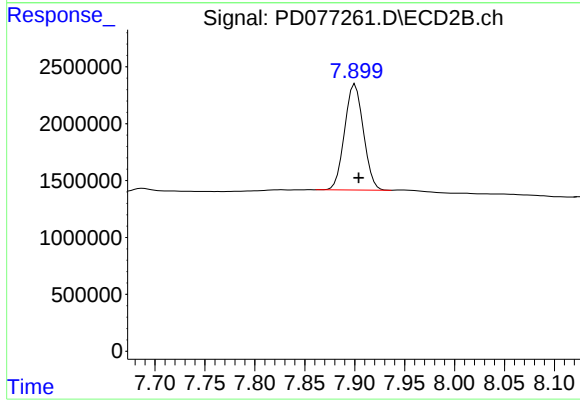

#28 Decachlorobiphenyl

R.T.: 7.900 min

Delta R.T.: -0.004 min

Response: 12226010

Conc: 8.54 ng/ml