

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082123\
 Data File : PD077279.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2023 17:57
 Operator : AR\AJ
 Sample : 04086-06
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 B-PP09B

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/22/2023
 Supervised By : Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 22:25:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.760	40444080	22504163	17.090	16.521m
28)	SA Decachlor...	9.081	7.901	42029899	20336446	15.338	14.210

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082123\
Data File : PD077279.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 17:57
Operator : AR\AJ
Sample : 04086-06
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
B-PP09B


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/22/2023
Supervised By : Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:25:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

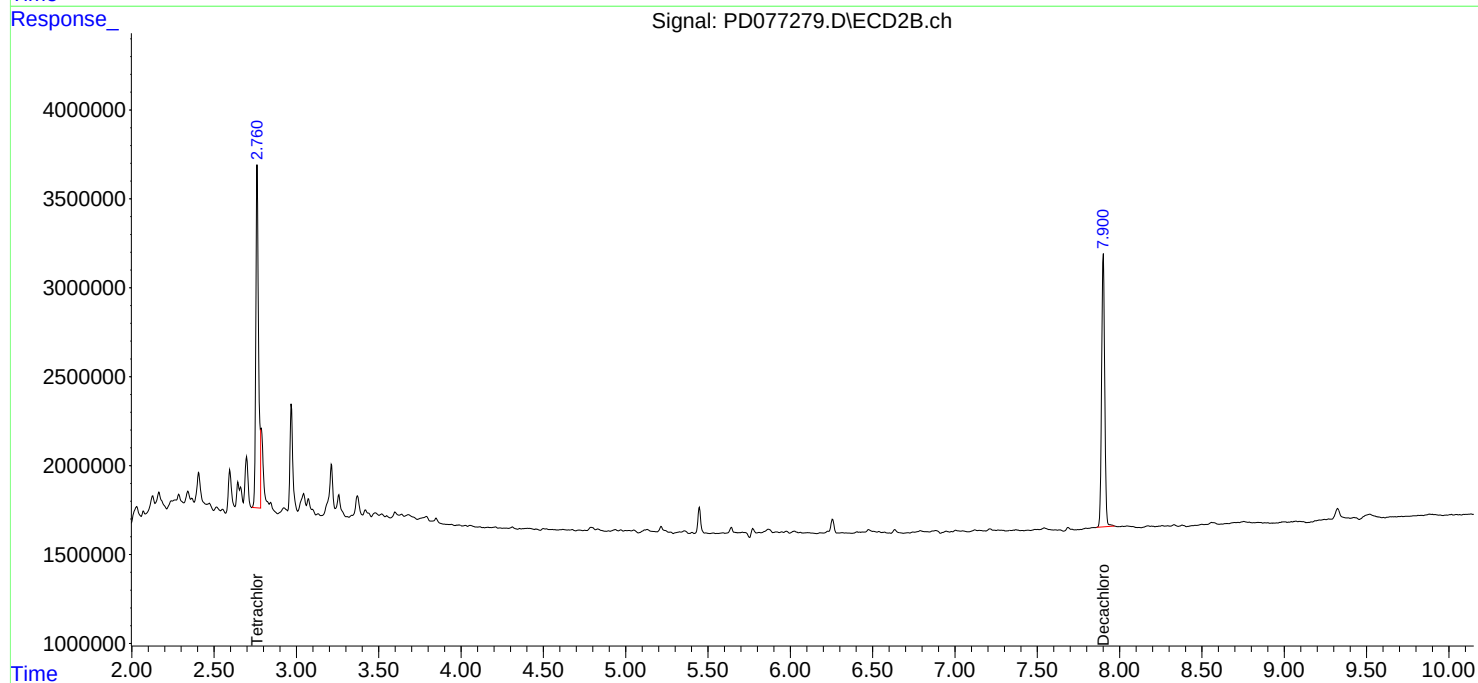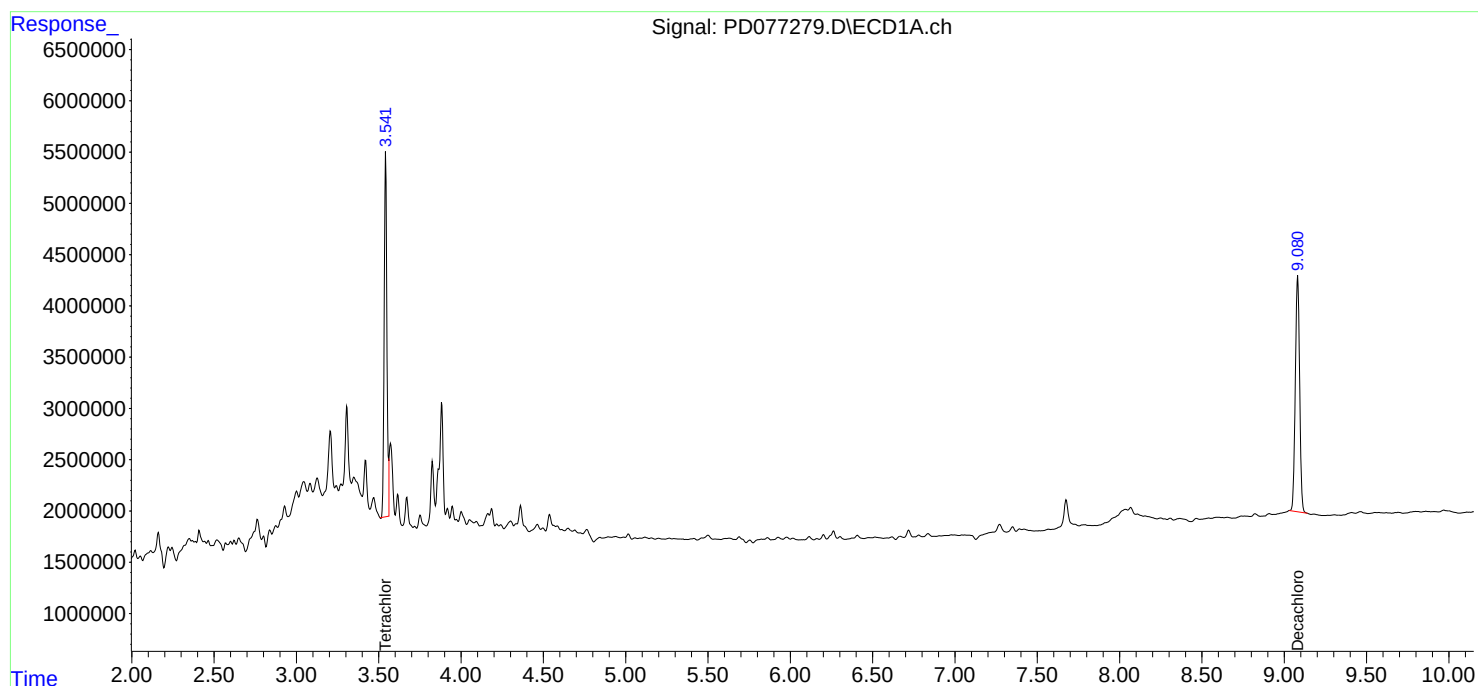

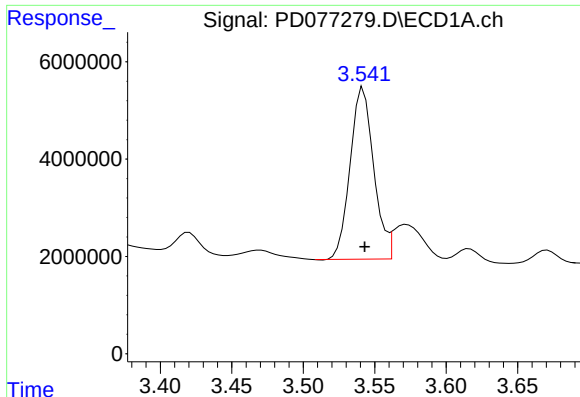


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 40444080
Conc: 17.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
B-PP09B


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

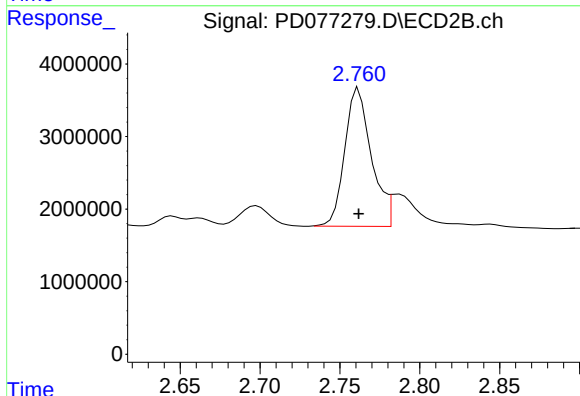


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: -0.001 min
Response: 22504163
Conc: 16.52 ng/ml m

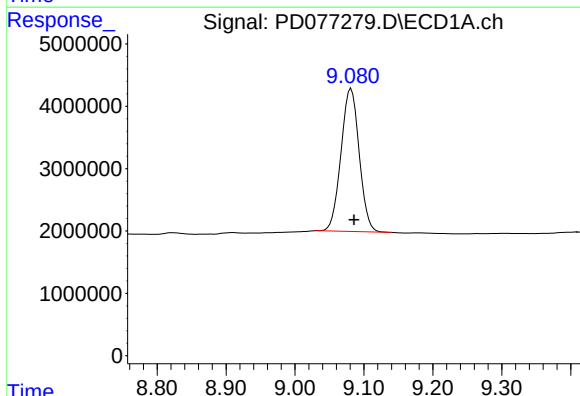

#28 Decachlorobiphenyl

R.T.: 9.081 min
Delta R.T.: -0.004 min
Response: 42029899
Conc: 15.34 ng/ml

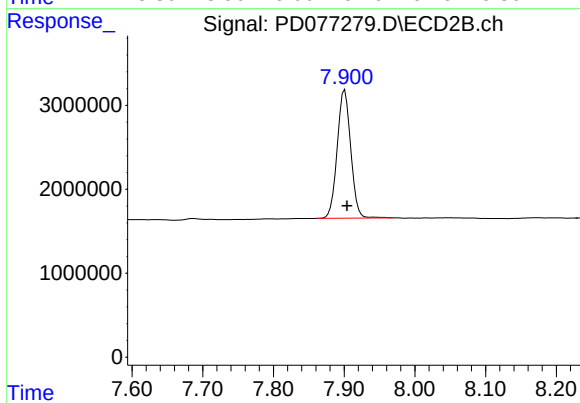

#28 Decachlorobiphenyl

R.T.: 7.901 min
Delta R.T.: -0.003 min
Response: 20336446
Conc: 14.21 ng/ml