

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082123\
 Data File : PD077300.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2023 23:04
 Operator : AR\AJ
 Sample : 04090-04
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-K

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 05:50:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.762	45381230	26527021	19.177	19.475
28)	SA Decachlor...	9.081	7.901	43190020	20793255	15.762	14.530
Target Compounds							
12)	B 4,4'-DDE	6.201	5.216	5928986	3418461	1.999	2.357
17)	MA 4,4'-DDT	7.035	6.023	3705561	1814531	1.524	1.632



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082123\
Data File : PD077300.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 23:04
Operator : AR\AJ
Sample : 04090-04
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP-K

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 05:50:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

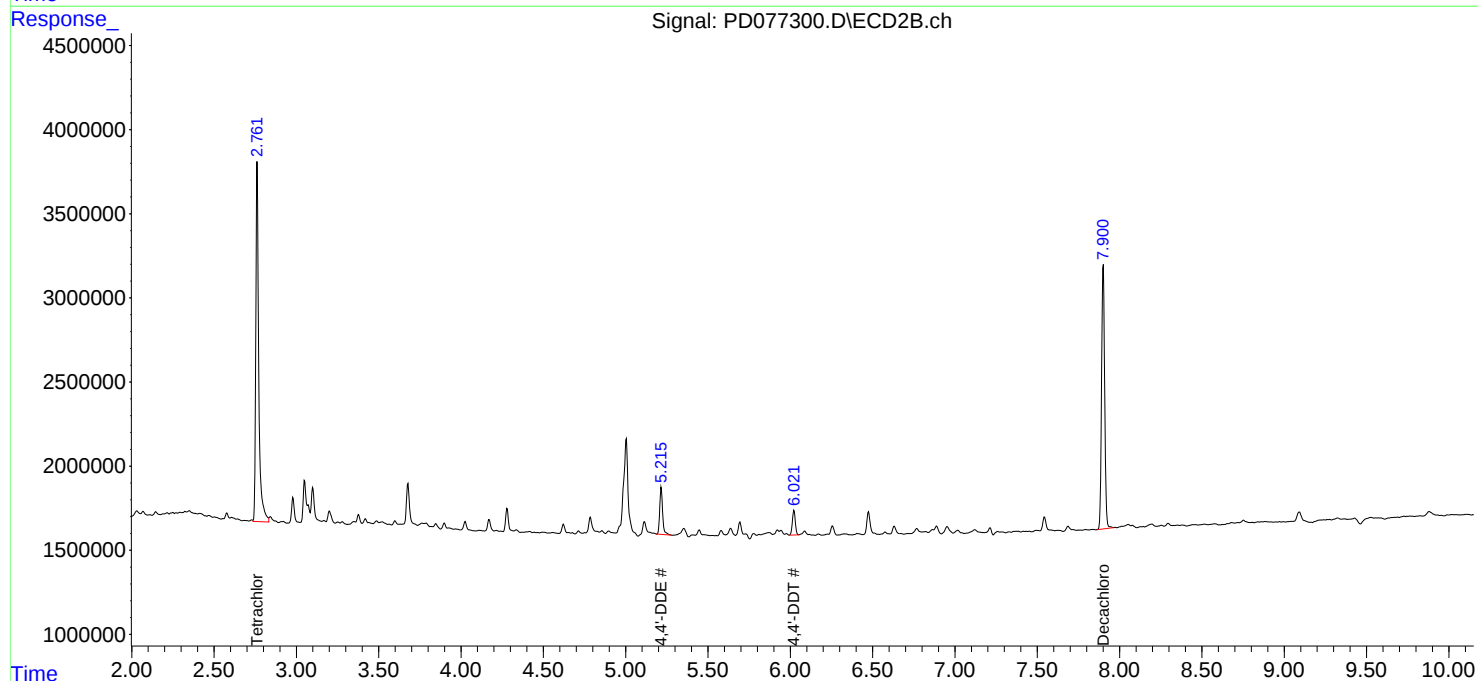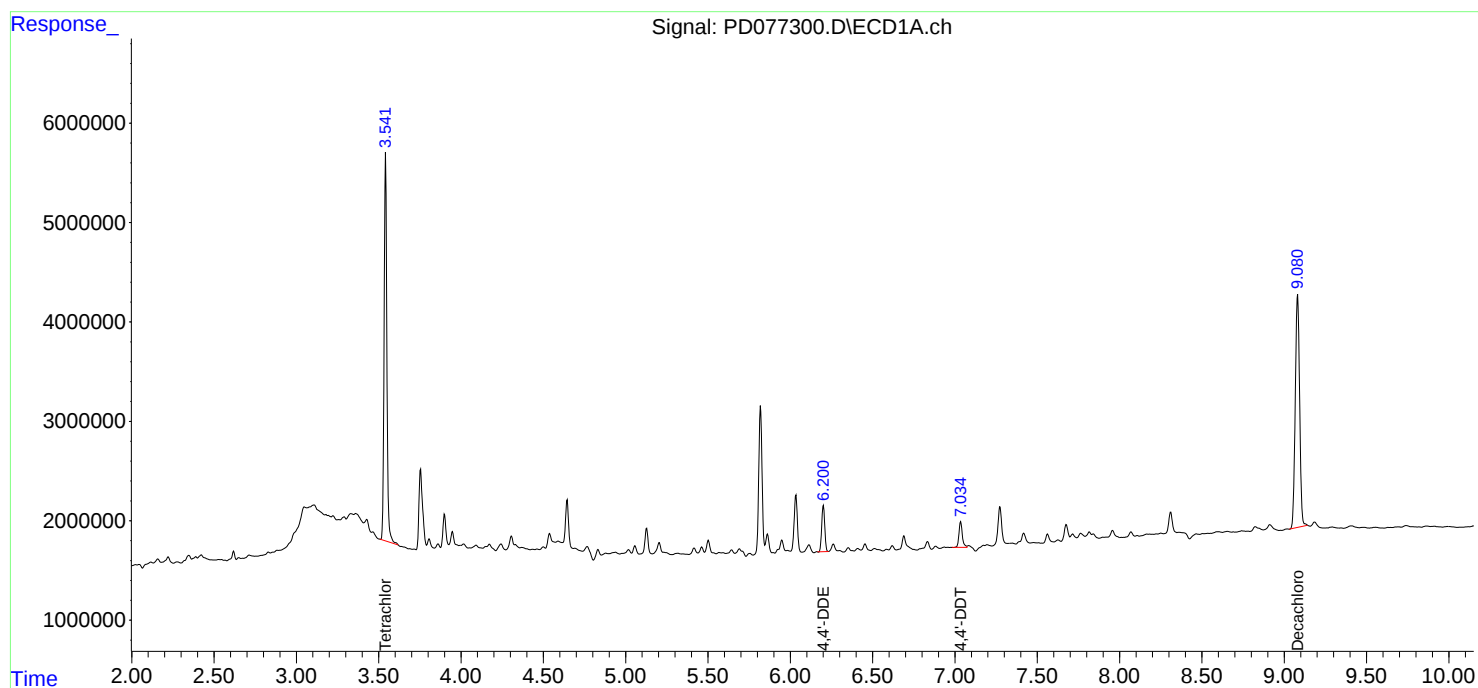


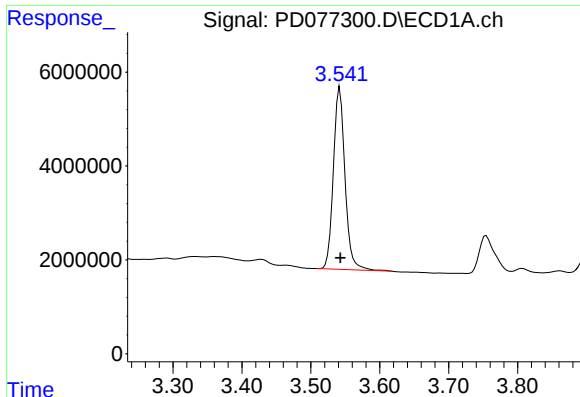

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 45381230
Conc: 19.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-K

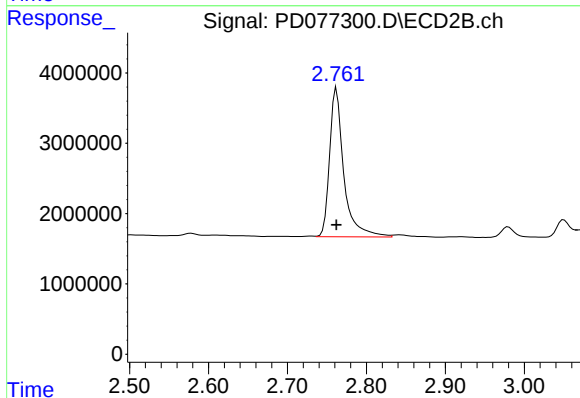


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 26527021
Conc: 19.47 ng/ml

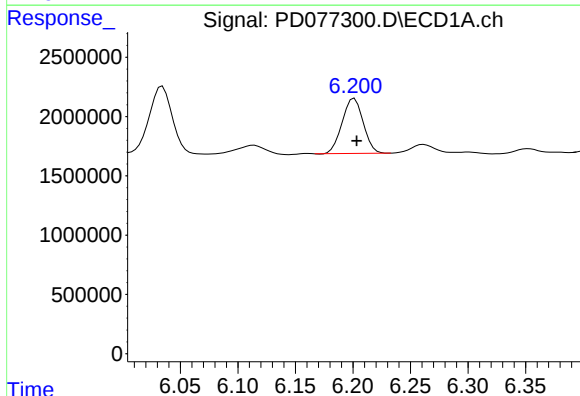


#12 4,4'-DDE

R.T.: 6.201 min
Delta R.T.: -0.002 min
Response: 5928986
Conc: 2.00 ng/ml

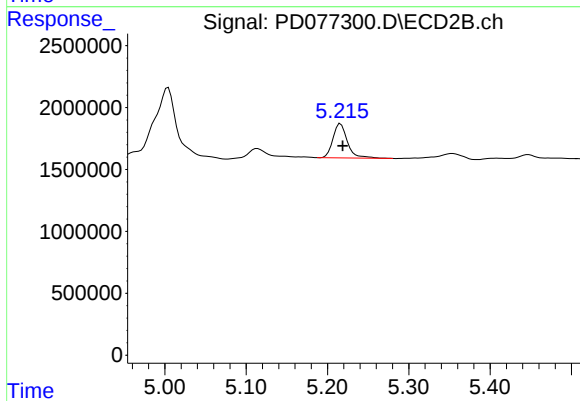

#12 4,4'-DDE


R.T.: 5.216 min
Delta R.T.: -0.003 min
Response: 3418461
Conc: 2.36 ng/ml

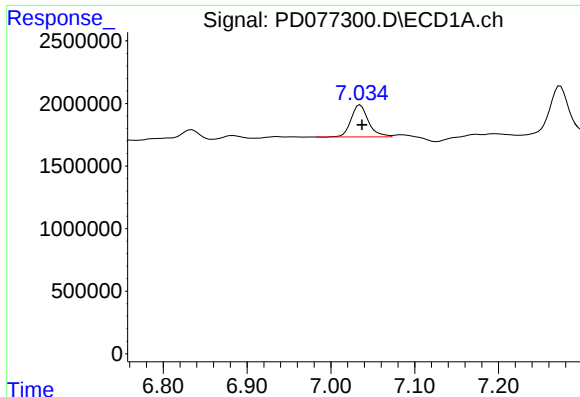

#17 4,4'-DDT


R.T.: 7.035 min
Delta R.T.: -0.002 min
Response: 3705561
Conc: 1.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-K

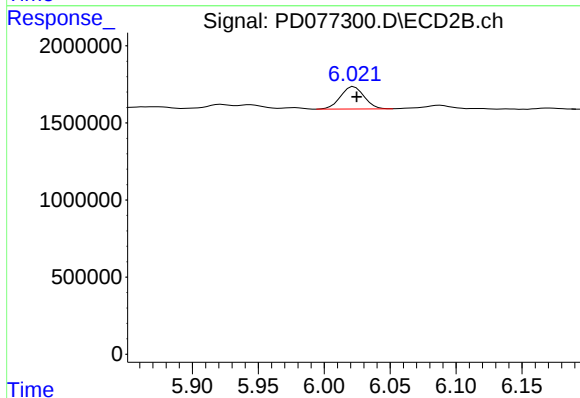


#17 4,4'-DDT

R.T.: 6.023 min
Delta R.T.: -0.002 min
Response: 1814531
Conc: 1.63 ng/ml

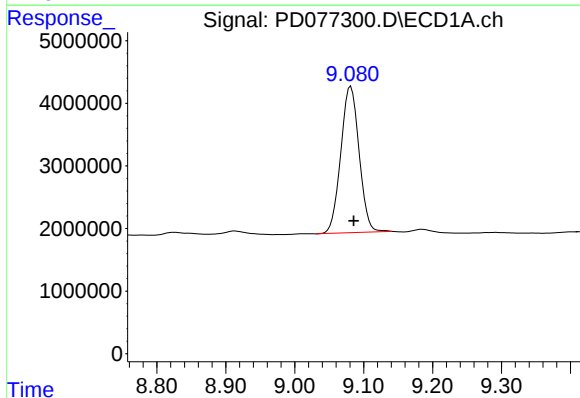

#28 Decachlorobiphenyl

R.T.: 9.081 min
Delta R.T.: -0.004 min
Response: 43190020
Conc: 15.76 ng/ml

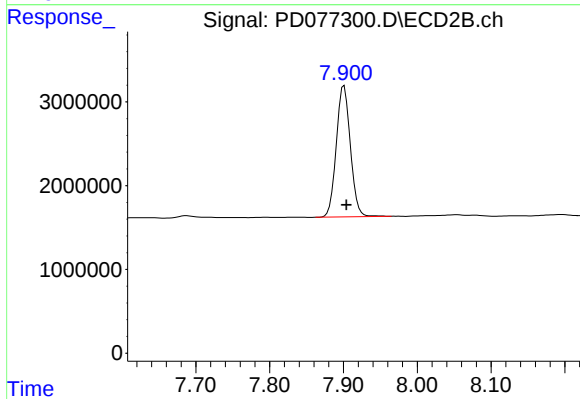

#28 Decachlorobiphenyl

R.T.: 7.901 min
Delta R.T.: -0.003 min
Response: 20793255
Conc: 14.53 ng/ml