

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082123\
 Data File : PD077308.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2023 01:04
 Operator : AR\AJ
 Sample : 04091-01
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 06:09:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.761	37846755	22955218	15.993	16.853
28)	SA Decachlor...	9.082	7.902	35637708	17923799	13.006	12.525
Target Compounds							
12)	B 4,4'-DDE	6.200	5.216	3525837	2462130	1.189	1.698 #
17)	MA 4,4'-DDT	7.035	6.023	5049405	2767466	2.077	2.490



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082123\
Data File : PD077308.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2023 01:04
Operator : AR\AJ
Sample : 04091-01
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 06:09:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

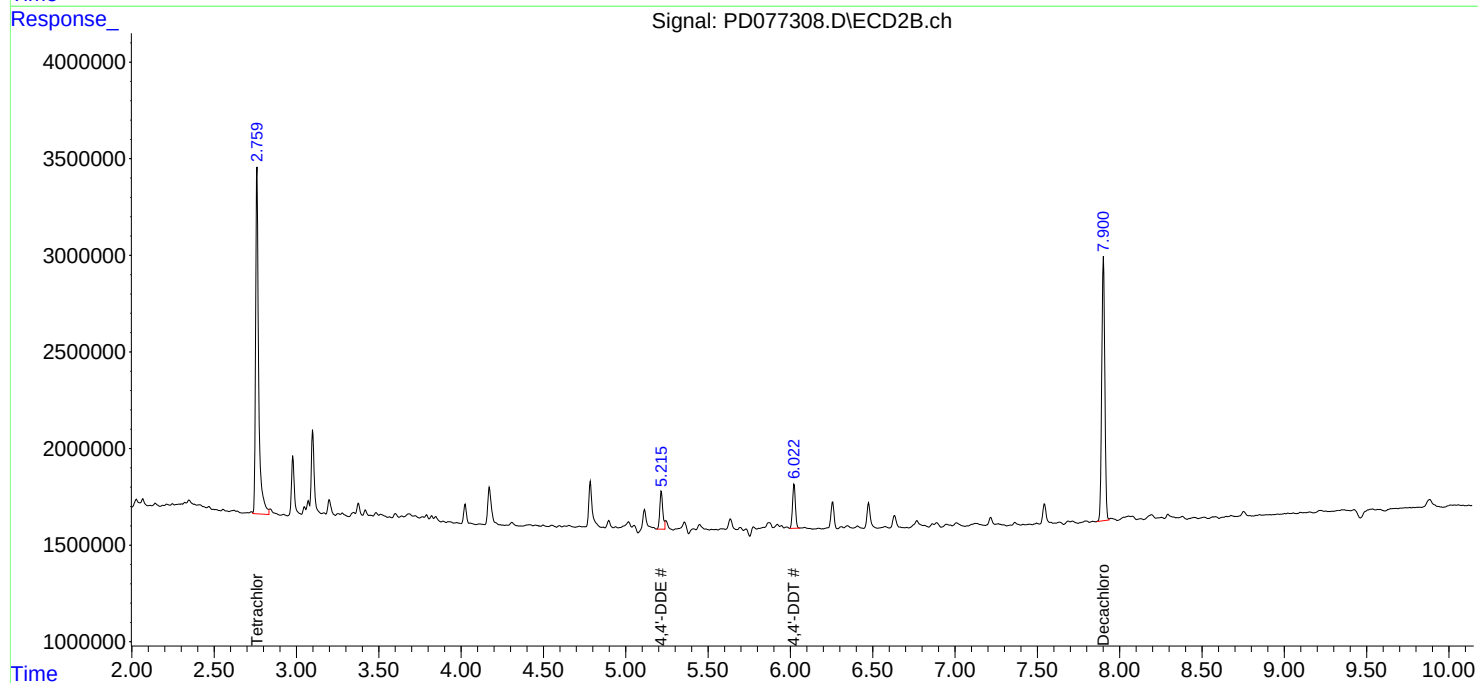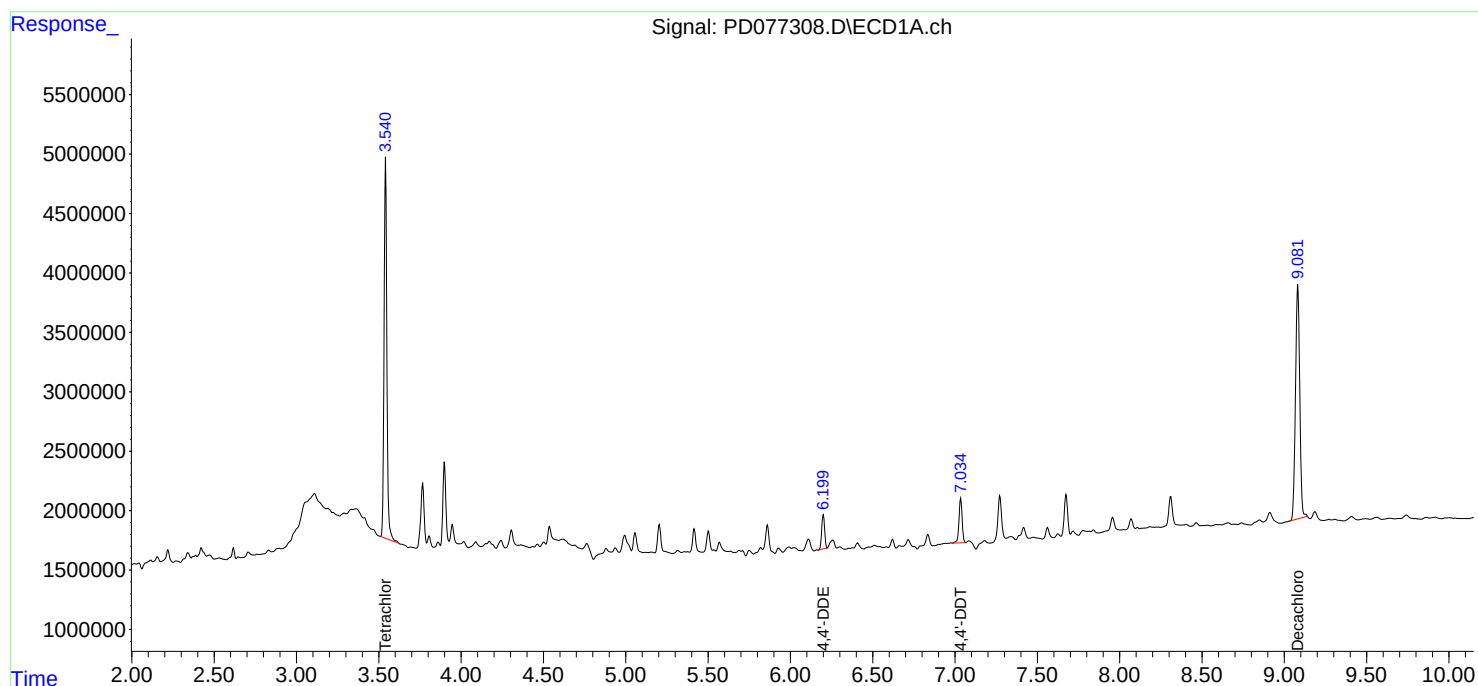


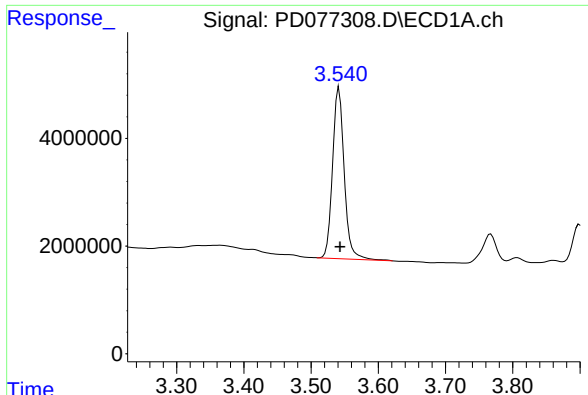

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: -0.001 min
Response: 37846755
Conc: 15.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-A

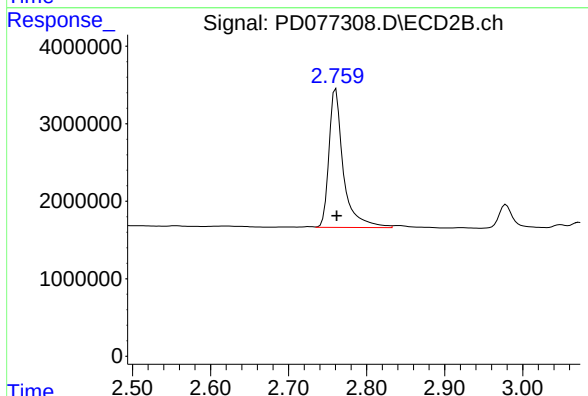


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: -0.001 min
Response: 22955218
Conc: 16.85 ng/ml

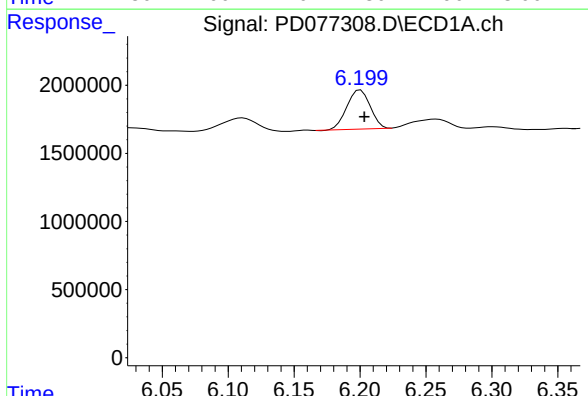


#12 4,4'-DDE

R.T.: 6.200 min
Delta R.T.: -0.003 min
Response: 3525837
Conc: 1.19 ng/ml

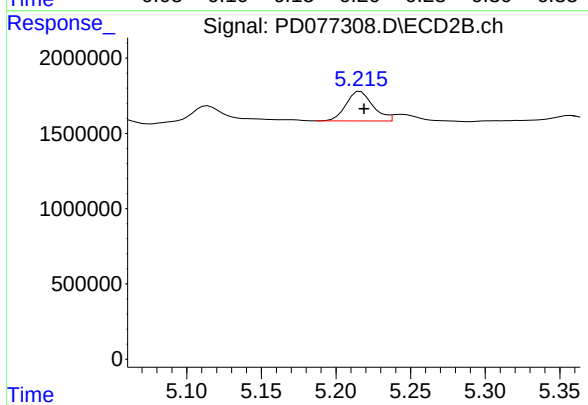

#12 4,4'-DDE


R.T.: 5.216 min
Delta R.T.: -0.002 min
Response: 2462130
Conc: 1.70 ng/ml

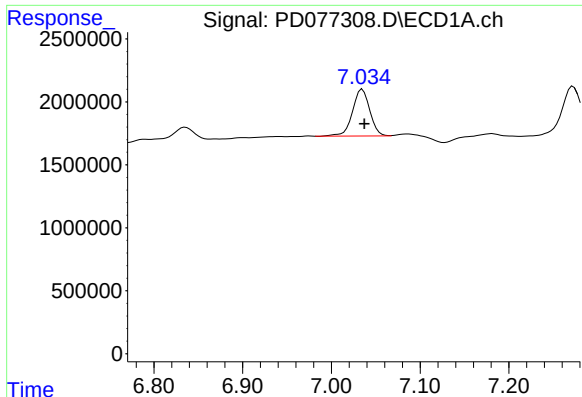

#17 4,4'-DDT


R.T.: 7.035 min
Delta R.T.: -0.002 min
Response: 5049405
Conc: 2.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-A

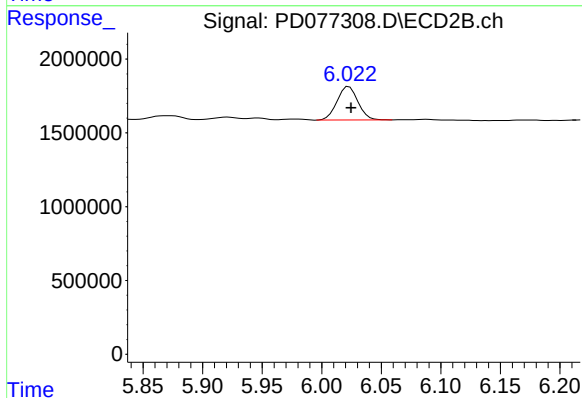


#17 4,4'-DDT

R.T.: 6.023 min
Delta R.T.: -0.002 min
Response: 2767466
Conc: 2.49 ng/ml

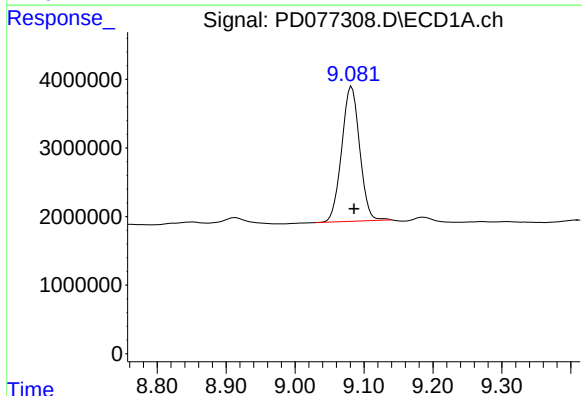

#28 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: -0.004 min
Response: 35637708
Conc: 13.01 ng/ml

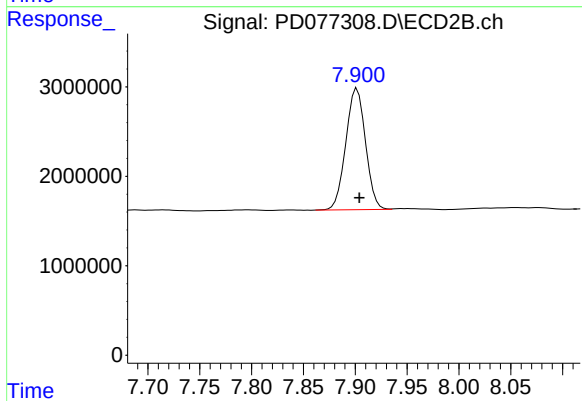

#28 Decachlorobiphenyl

R.T.: 7.902 min
Delta R.T.: -0.002 min
Response: 17923799
Conc: 12.52 ng/ml