

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082123\
 Data File : PD077317.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2023 03:05
 Operator : AR\AJ
 Sample : 04093-03
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 NEVINS-SB04-Z83-84

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/22/2023
 Supervised By : Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 06:13:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.541	2.771	17375834	34389767	7.342m	25.247m#
2) SA Decachlor...	9.081	7.900	25764850	16530602	9.403m	11.551

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082123\
Data File : PD077317.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2023 03:05
Operator : AR\AJ
Sample : 04093-03
Misc :
ALS Vial : 61 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
NEVINS-SB04-Z83-84


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/22/2023
Supervised By : Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 06:13:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

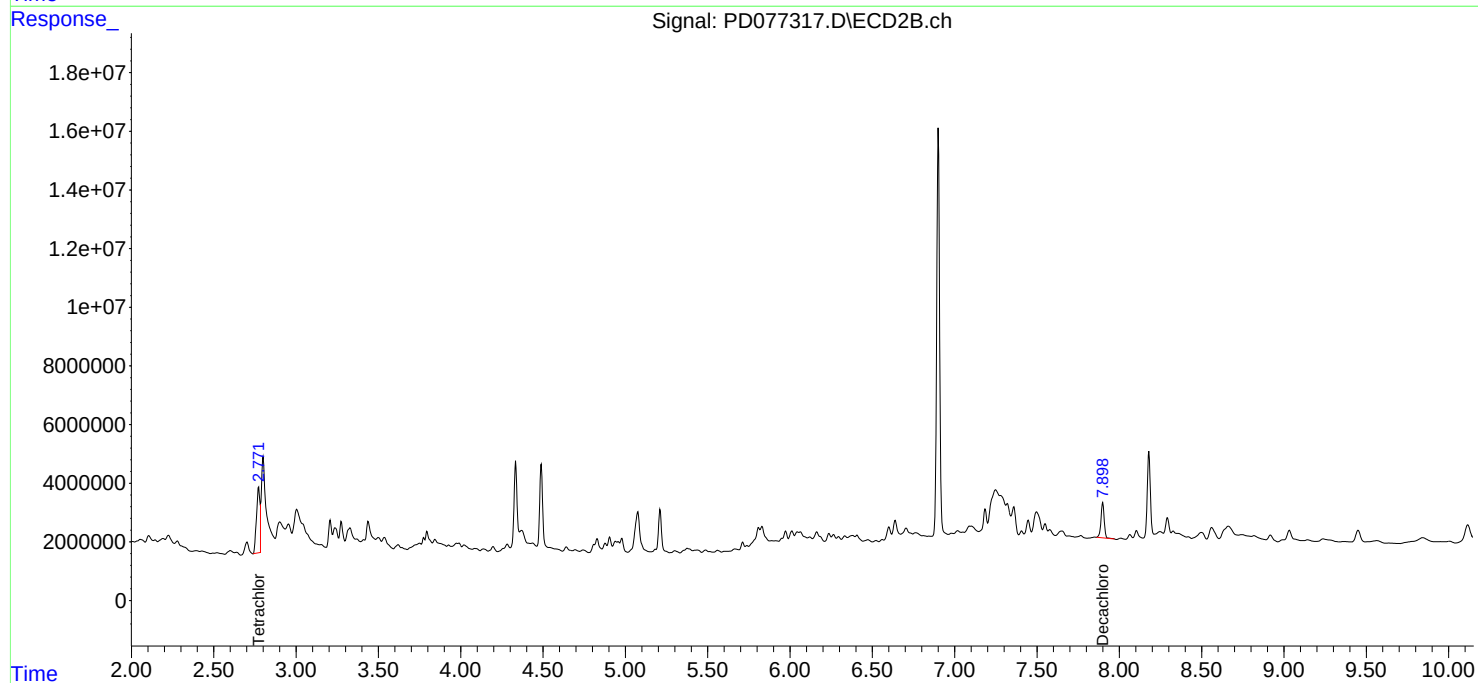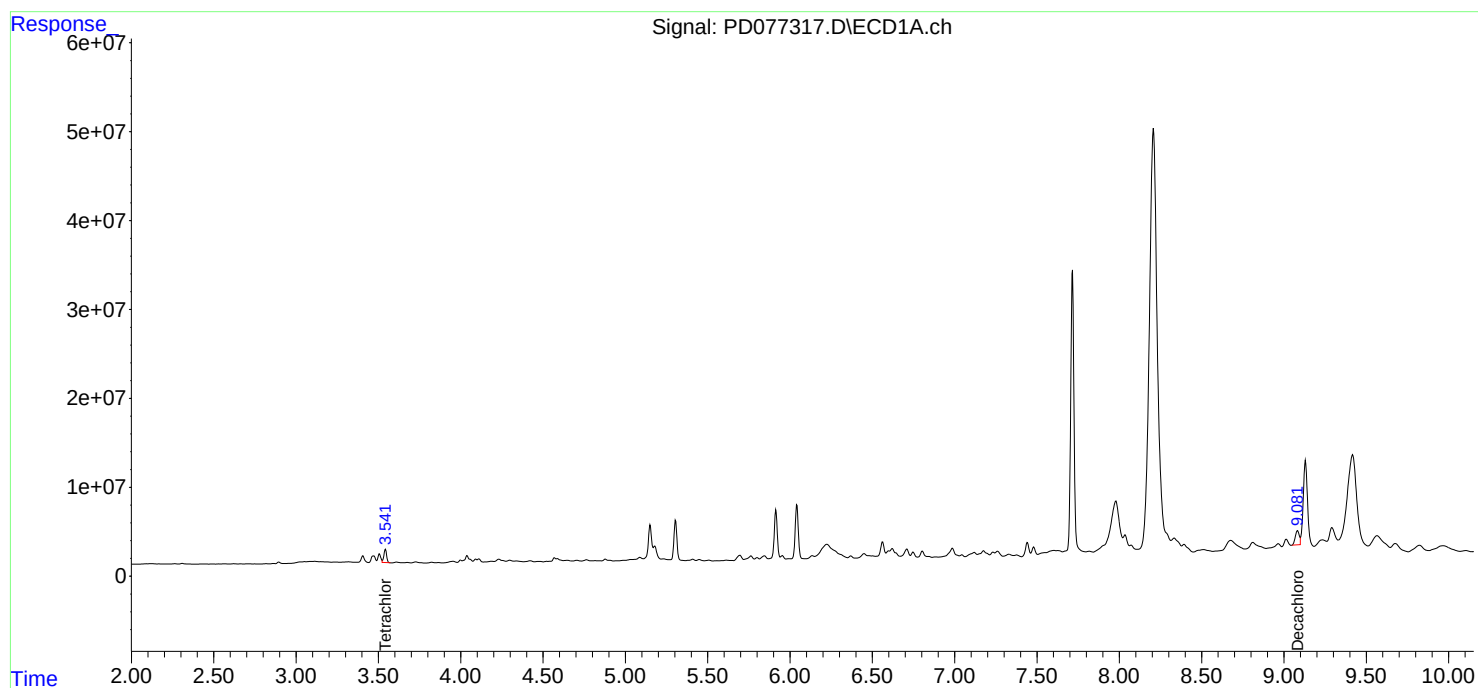

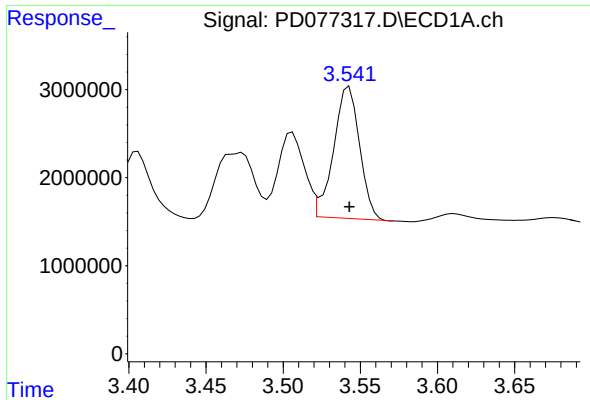


#1 Tetrachloro-m-xylene

R.T.: 3.541 min
Delta R.T.: -0.002 min
Response: 17375834
Conc: 7.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
NEVINS-SB04-Z83-84


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

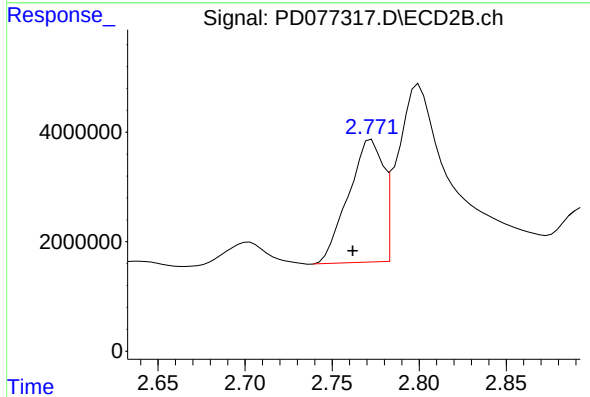


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.009 min
Response: 34389767
Conc: 25.25 ng/ml m

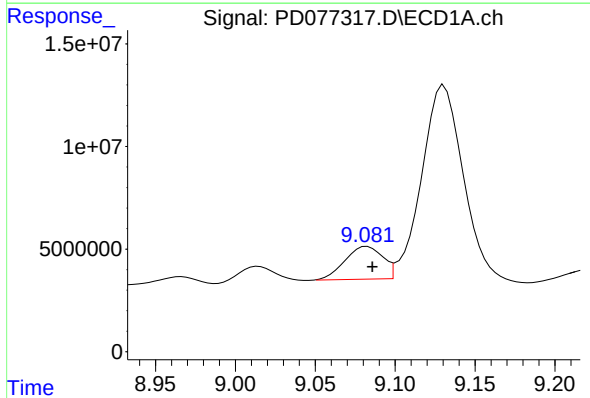

#28 Decachlorobiphenyl

R.T.: 9.081 min
Delta R.T.: -0.005 min
Response: 25764850
Conc: 9.40 ng/ml m

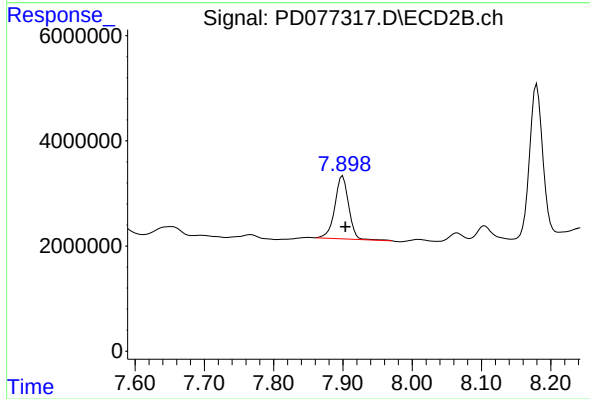

#28 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: -0.004 min
Response: 16530602
Conc: 11.55 ng/ml