

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082218\
 Data File : PD049022.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Aug 2018 13:05
 Operator : AJ\SJ
 Sample : PIBLK10
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 14:18:10 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081618CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 16 13:32:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.370	3.968	23564098	357.5E6	19.306	20.330
27)	SA Decachlor...	8.068	8.996	56822680	635.8E6	39.463	39.278
Target Compounds							
4)	MA Heptachlor	0.000	5.102f	0	1365708	N.D.	<MDL
5)	MB Aldrin	0.000	5.401f	0	1634241	N.D.	<MDL
7)	B delta-BHC	0.000	5.046f	0	6609910	N.D.	0.291


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082218\
Data File : PD049022.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Aug 2018 13:05
Operator : AJ\SJ
Sample : PIBLK10
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 14:18:10 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081618CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 16 13:32:25 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

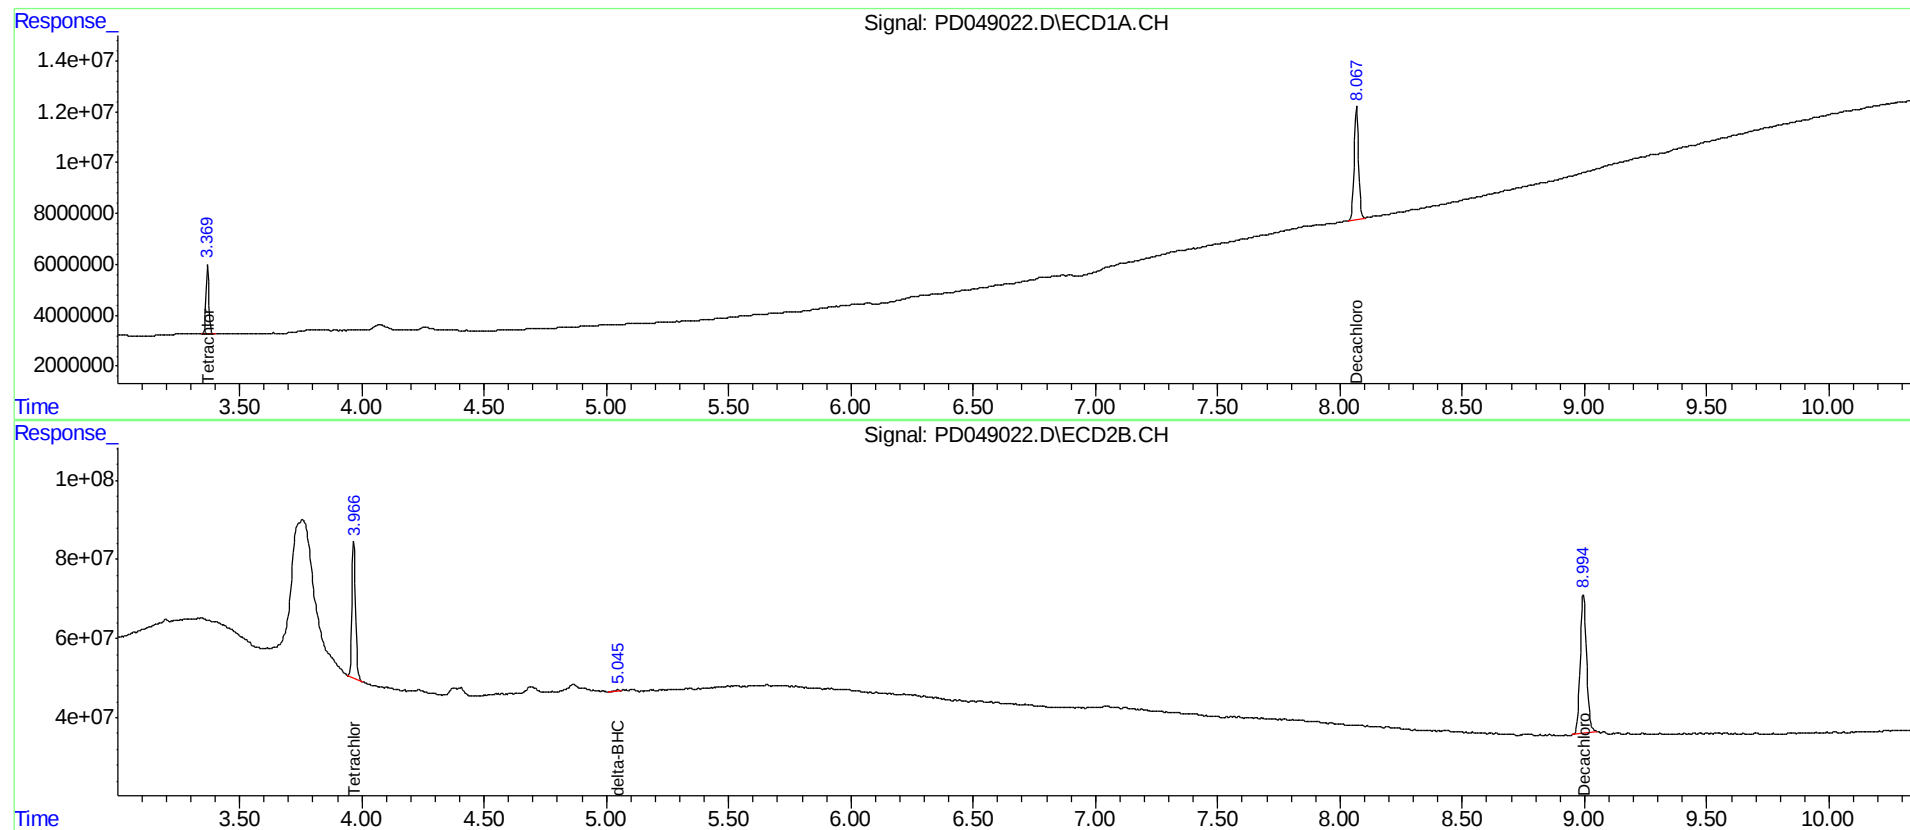


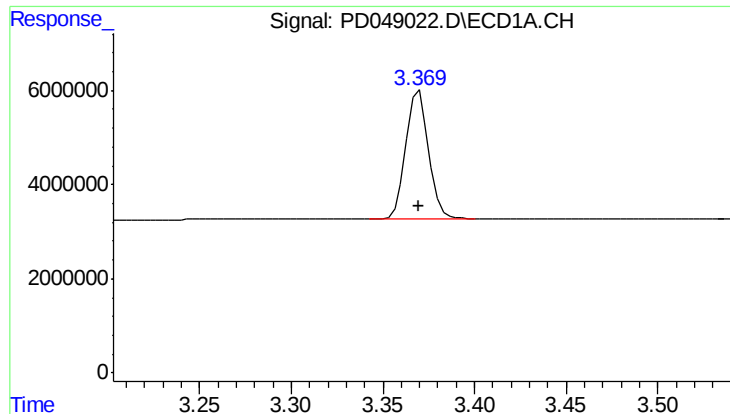

#1 Tetrachloro-m-xylene


R.T.: 3.370 min
Delta R.T.: 0.000 min
Response: 23564098
Conc: 19.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK10

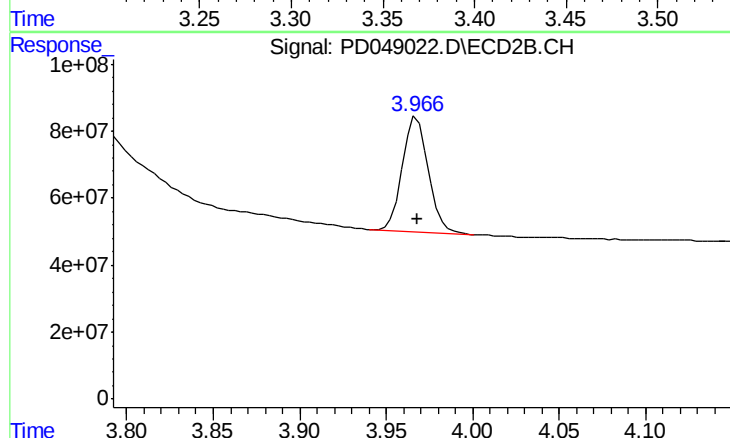


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: 0.000 min
Response: 357454419
Conc: 20.33 ng/ml

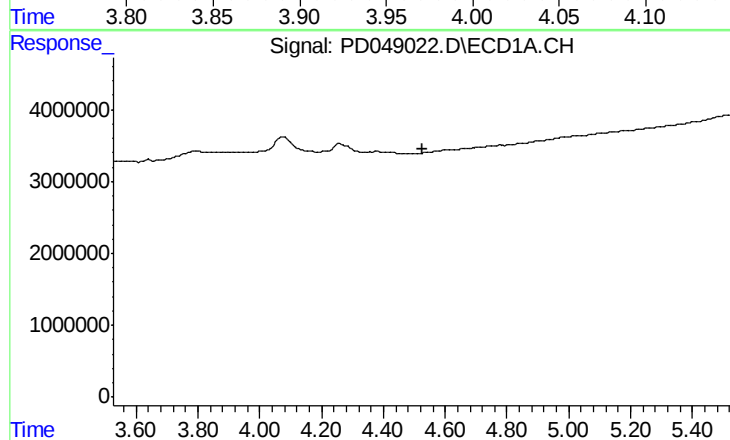


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.526 min
Response: 0
Conc: N.D.

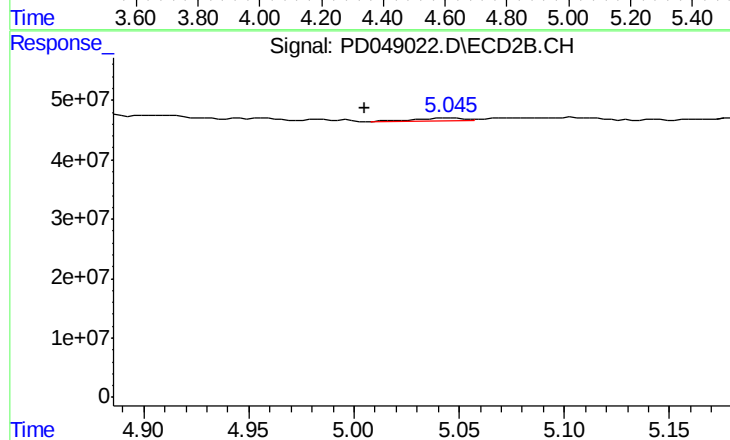

#7 delta-BHC


R.T.: 5.046 min
Delta R.T.: 0.041 min
Response: 6609910
Conc: 0.29 ng/ml

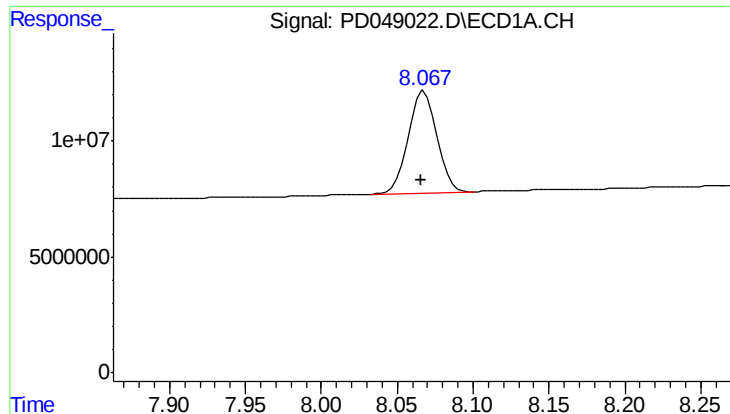

#27 Decachlorobiphenyl

R.T.: 8.068 min
Delta R.T.: 0.002 min
Response: 56822680
Conc: 39.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK10

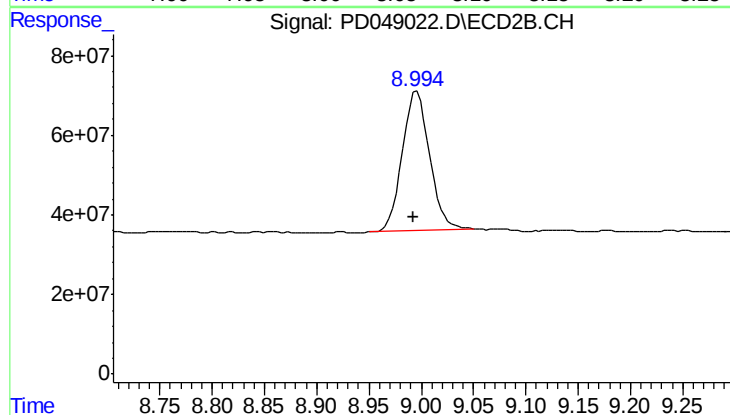

#27 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: 0.003 min
Response: 635847639
Conc: 39.28 ng/ml