

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082219\
 Data File : PD054374.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Aug 2019 15:01
 Operator : SG\AJ
 Sample : K4464-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 04:58:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081619CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 16 15:23:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.982	9466487	12050868	13.636	12.344
27)	SA Decachlor...	8.005	9.025	16270691	22187823	23.549	22.805


Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082219\
Data File : PD054374.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Aug 2019 15:01
Operator : SG\AJ
Sample : K4464-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 04:58:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081619CLP.M
Quant Title : GC Extractables
QLast Update : Fri Aug 16 15:23:53 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

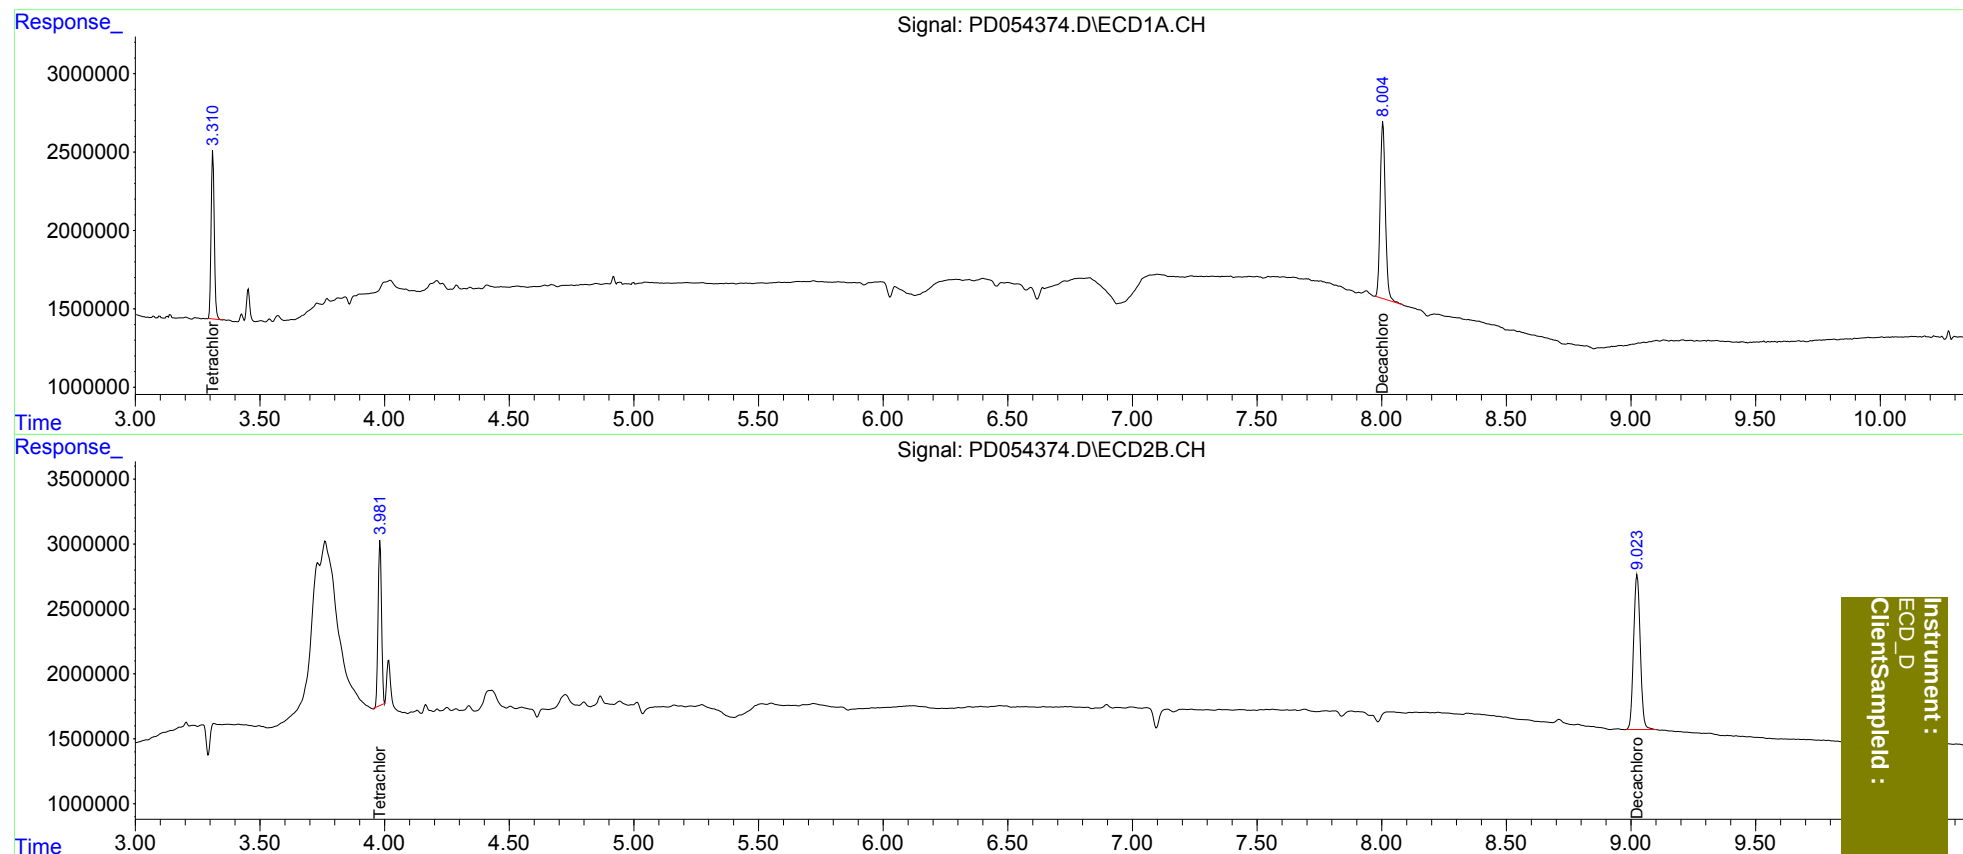


Instrument :
ECD_D
ClientSampleId :

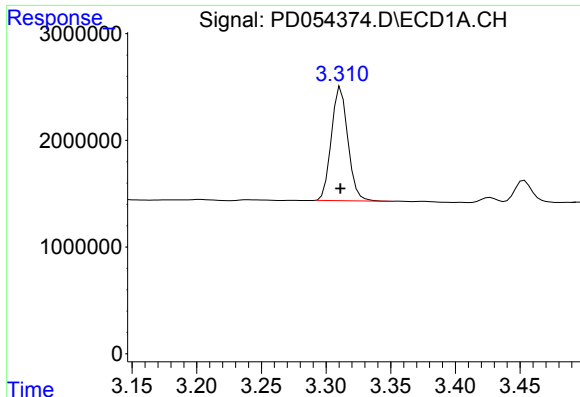

#1 Tetrachloro-m-xylene


R.T.: 3.312 min
Delta R.T.: 0.000 min
Response: 9466487
Conc: 13.64 ng/ml

Instrument :
ECD_D
ClientSampleId :

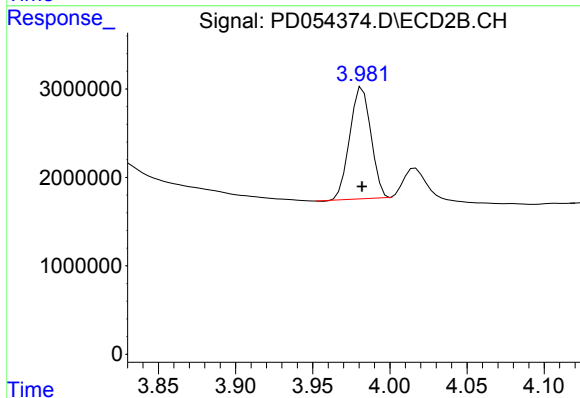


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 12050868
Conc: 12.34 ng/ml

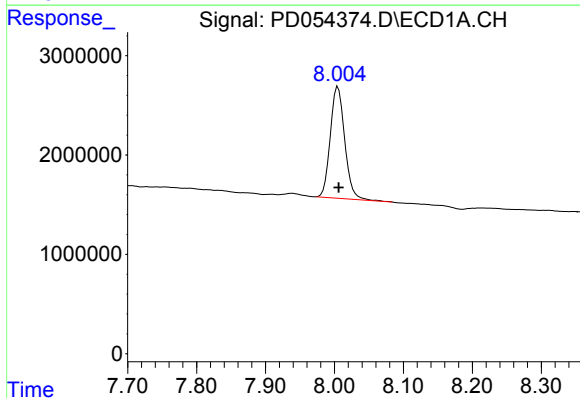

#27 Decachlorobiphenyl

R.T.: 8.005 min
Delta R.T.: -0.001 min
Response: 16270691
Conc: 23.55 ng/ml

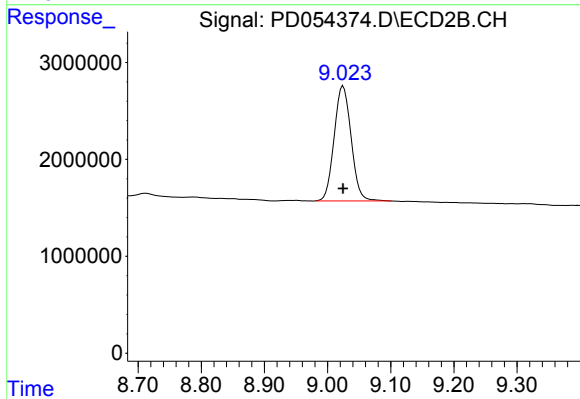

#27 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.000 min
Response: 22187823
Conc: 22.81 ng/ml