

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082223\
 Data File : PD077322.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2023 10:19
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 00:47:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.762	49177503	28850666	20.781	21.181
28)	SA Decachlor...	9.082	7.901	60173216	27788280	21.960	19.418
Target Compounds							
4)	MA Heptachlor	4.912	0.000	335908	0	0.093	N.D. #
6)	B beta-BHC	4.560f	0.000	337957	0	0.225	N.D. #
7)	B delta-BHC	4.767	0.000	1787278	0	0.512	N.D. #
8)	B Heptachlo...	5.688	0.000	4453795	0	1.345	N.D. #
14)	MA Endrin	0.000	5.643f	0	295511	N.D.	0.202 #
15)	B Endosulfa...	6.835f	0.000	200627	0	0.063	N.D. #
22)	Mirex	8.162f	0.000	608489	0	0.267	N.D. #
24)	Chlordane-2	0.000	4.331	0	1981655	N.D.	35.238 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082223\
Data File : PD077322.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2023 10:19
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 00:47:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

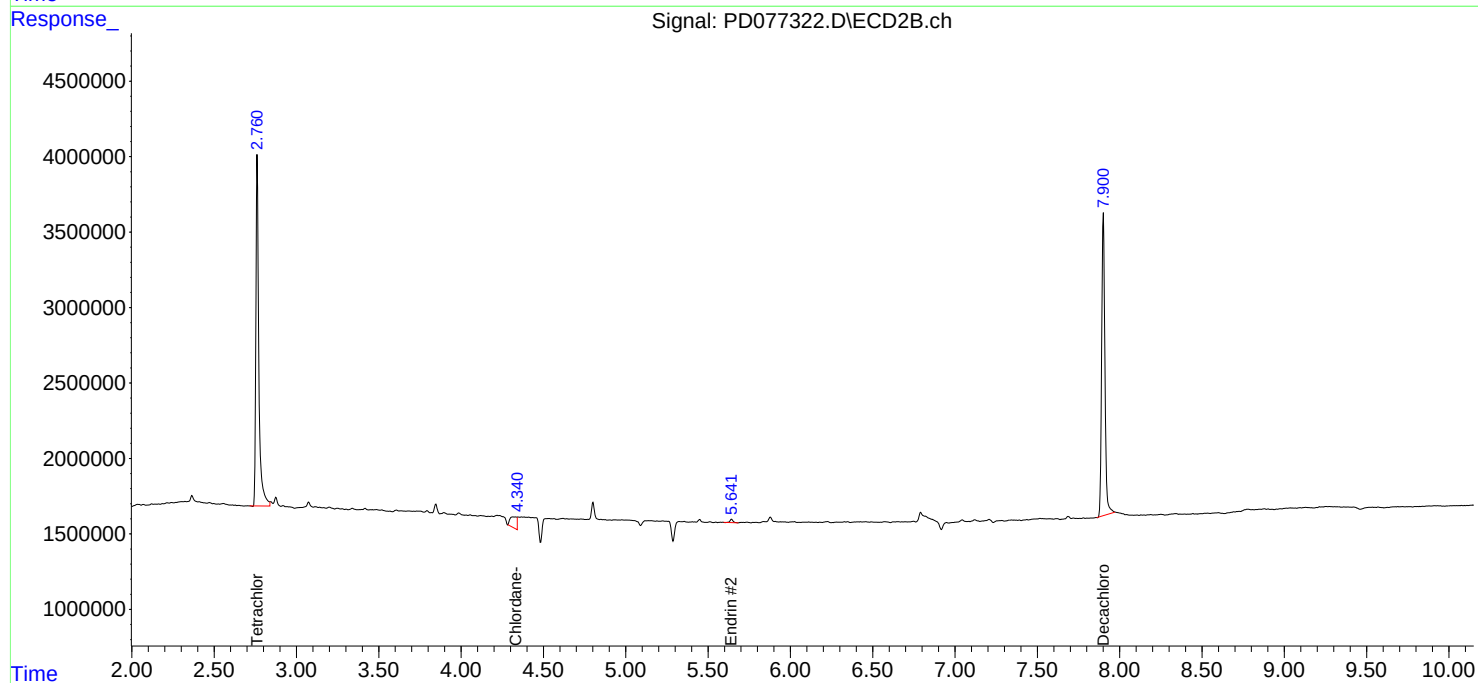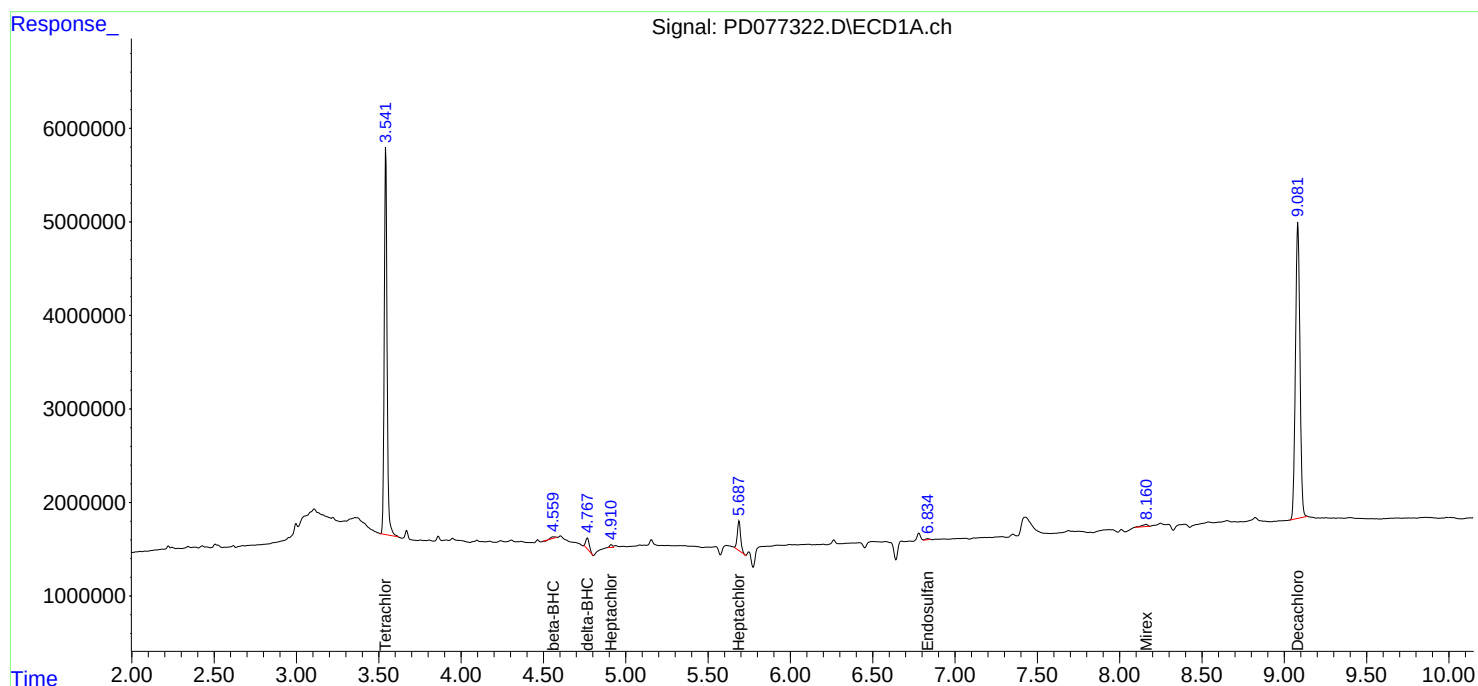


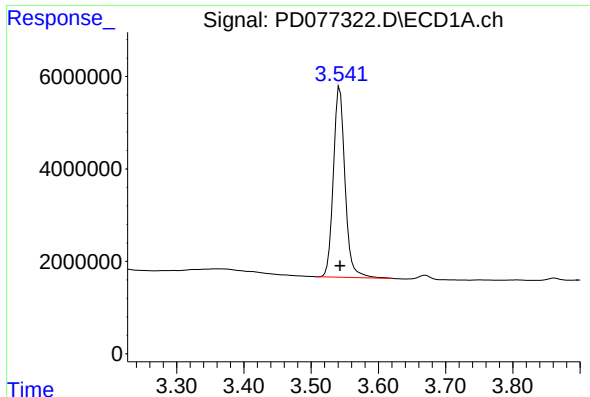

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 49177503
Conc: 20.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

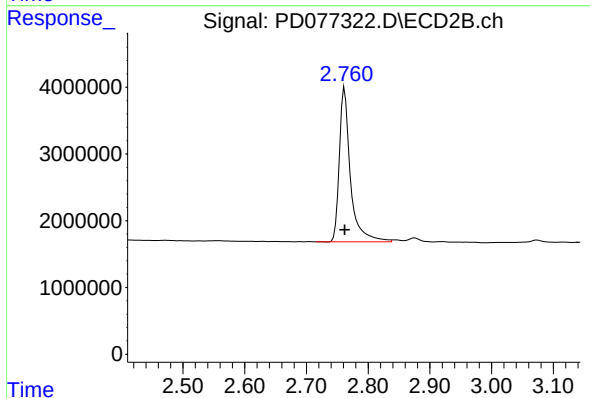


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 28850666
Conc: 21.18 ng/ml

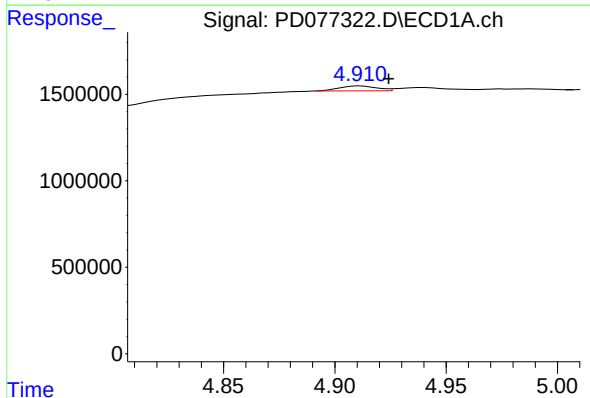


#4 Heptachlor

R.T.: 4.912 min
Delta R.T.: -0.013 min
Response: 335908
Conc: 0.09 ng/ml

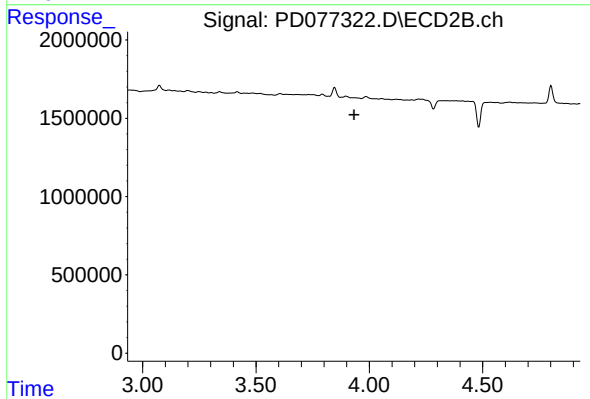

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 3.933 min
Response: 0
Conc: N.D.

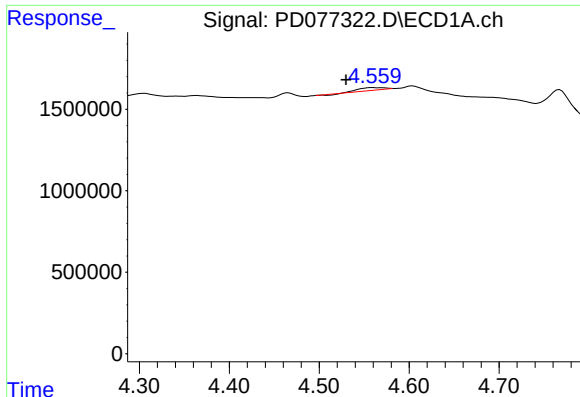

#6 beta-BHC


R.T.: 4.560 min
Delta R.T.: 0.030 min
Response: 337957
Conc: 0.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

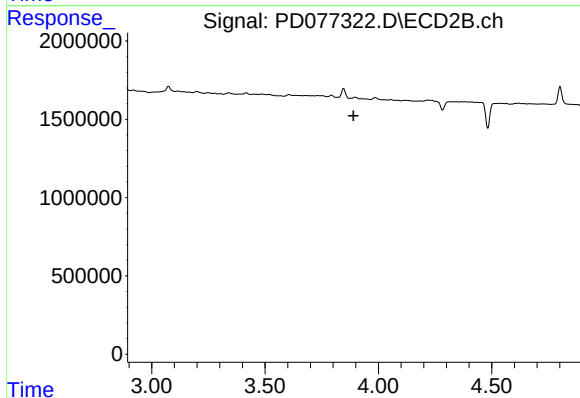


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 3.890 min
Response: 0
Conc: N.D.

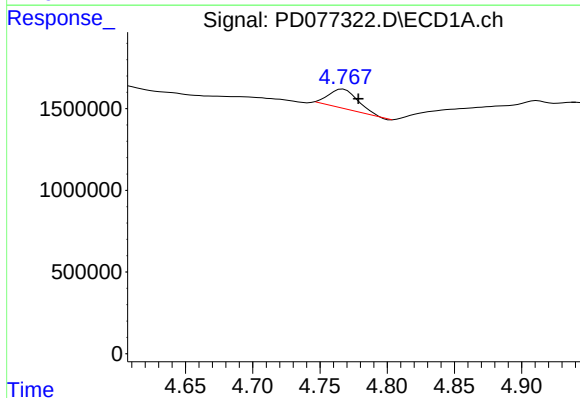


#7 delta-BHC

R.T.: 4.767 min
Delta R.T.: -0.011 min
Response: 1787278
Conc: 0.51 ng/ml

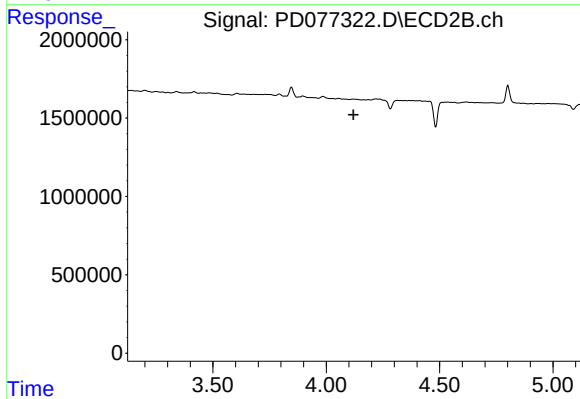

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.120 min
Response: 0
Conc: N.D.

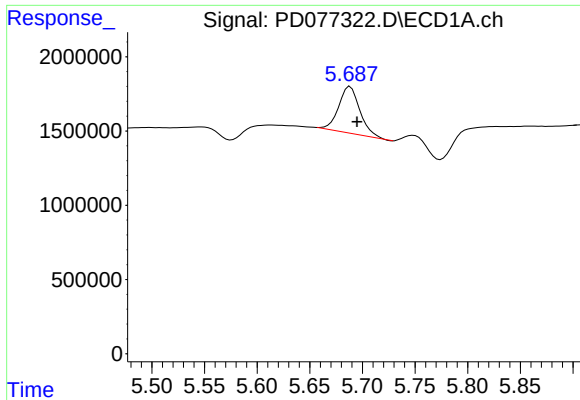

#8 Heptachlor epoxide


R.T.: 5.688 min
Delta R.T.: -0.006 min
Response: 4453795
Conc: 1.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

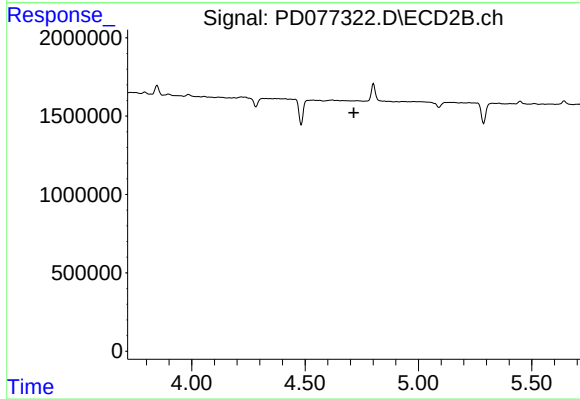


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.716 min
Response: 0
Conc: N.D.

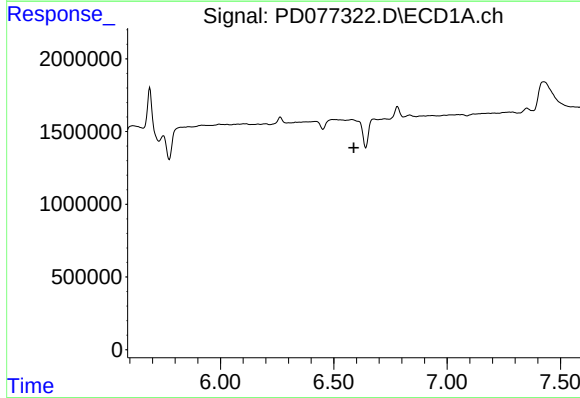


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.588 min
Response: 0
Conc: N.D.

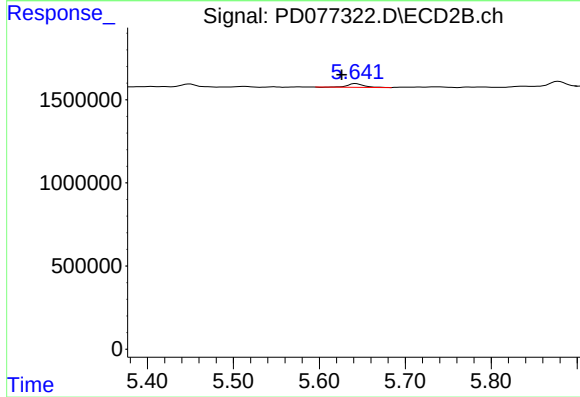

#14 Endrin


R.T.: 5.643 min
Delta R.T.: 0.017 min
Response: 295511
Conc: 0.20 ng/ml

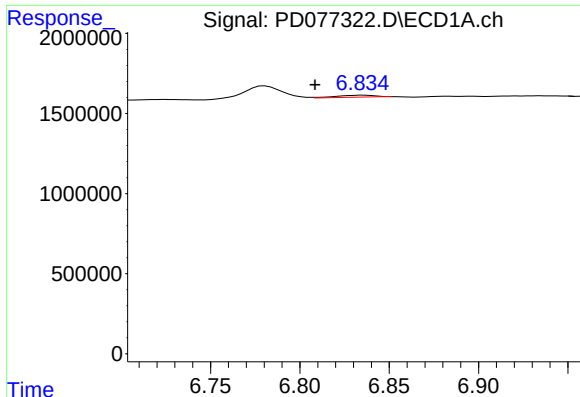

#15 Endosulfan II


R.T.: 6.835 min
Delta R.T.: 0.027 min
Response: 200627
Conc: 0.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

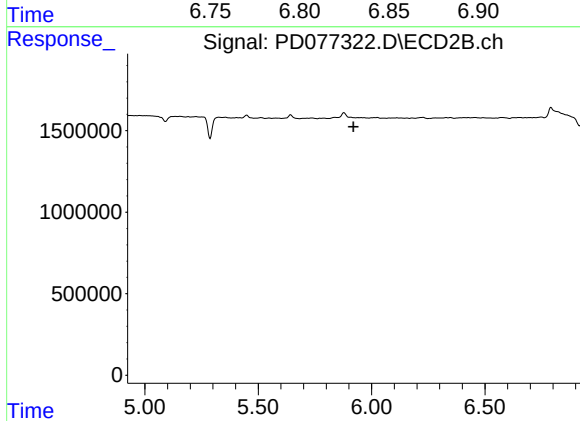


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.920 min
Response: 0
Conc: N.D.

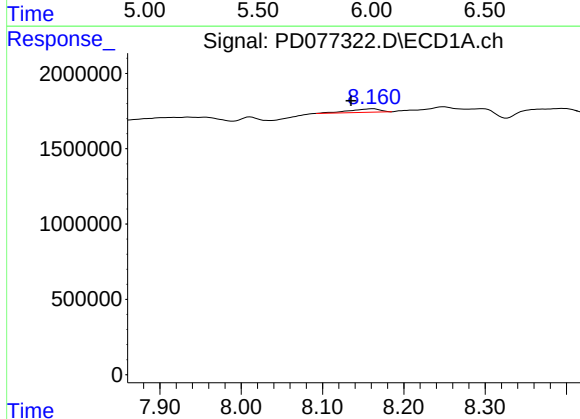


#22 Mirex

R.T.: 8.162 min
Delta R.T.: 0.026 min
Response: 608489
Conc: 0.27 ng/ml

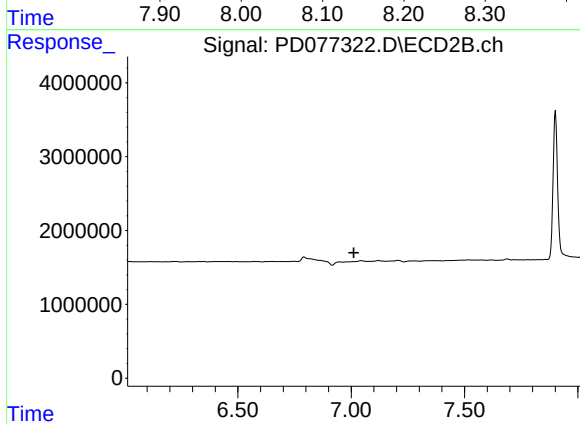

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 7.011 min
Response: 0
Conc: N.D.

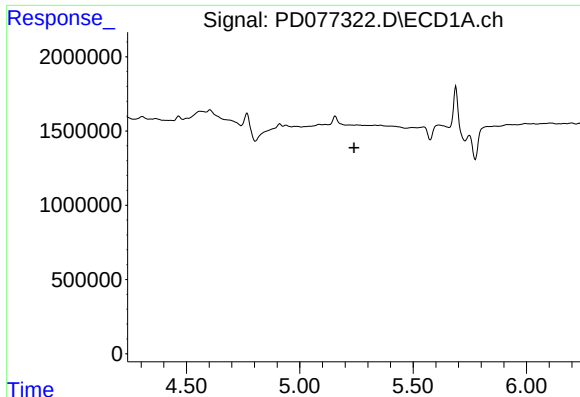

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.240 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

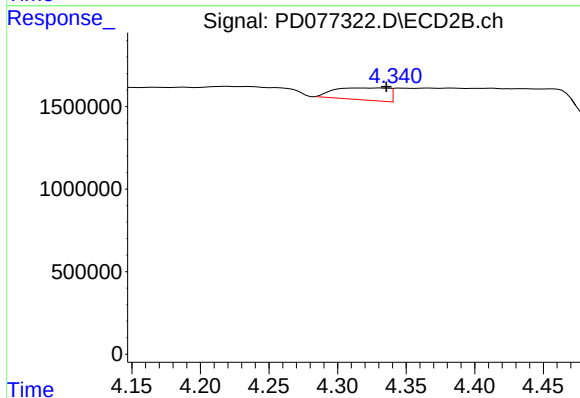


#24 Chlordane-2

R.T.: 4.331 min
Delta R.T.: -0.005 min
Response: 1981655
Conc: 35.24 ng/ml

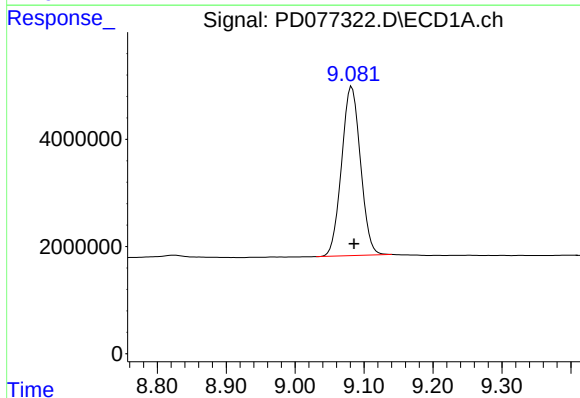

#28 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: -0.003 min
Response: 60173216
Conc: 21.96 ng/ml

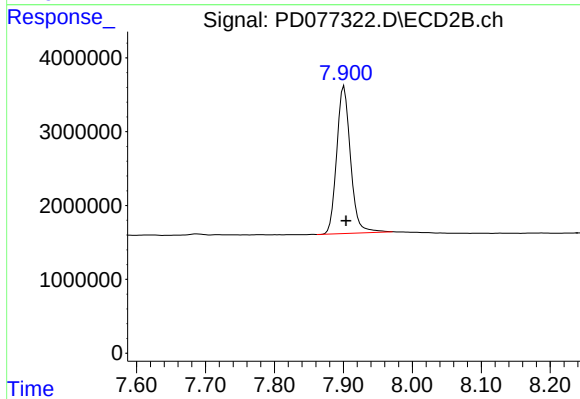

#28 Decachlorobiphenyl

R.T.: 7.901 min
Delta R.T.: -0.003 min
Response: 27788280
Conc: 19.42 ng/ml