

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082223\
 Data File : PD077327.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2023 12:13
 Operator : AR\AJ
 Sample : PB154988BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 00:49:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.761	44296012	25595516	18.718	18.791
28)	SA Decachlor...	9.090	7.904	57775236	25618991	21.084	17.902
Target Compounds							
3)	MA gamma-BHC...	0.000	3.603	0	314824	N.D.	0.169 #
4)	MA Heptachlor	4.945f	0.000	274746	0	0.076	N.D. #
7)	B delta-BHC	4.778	0.000	1150995	0	0.330	N.D. #
8)	B Heptachlo...	5.695	0.000	1800543	0	0.544	N.D. #
14)	MA Endrin	0.000	5.644f	0	248679	N.D.	0.170 #
15)	B Endosulfa...	6.824	0.000	346605	0	0.109	N.D. #
21)	B Endrin ke...	7.687f	0.000	609763	0	0.202	N.D. #
24)	Chlordane-2	0.000	4.321f	0	1910629	N.D.	33.975 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082223\
Data File : PD077327.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2023 12:13
Operator : AR\AJ
Sample : PB154988BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 00:49:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

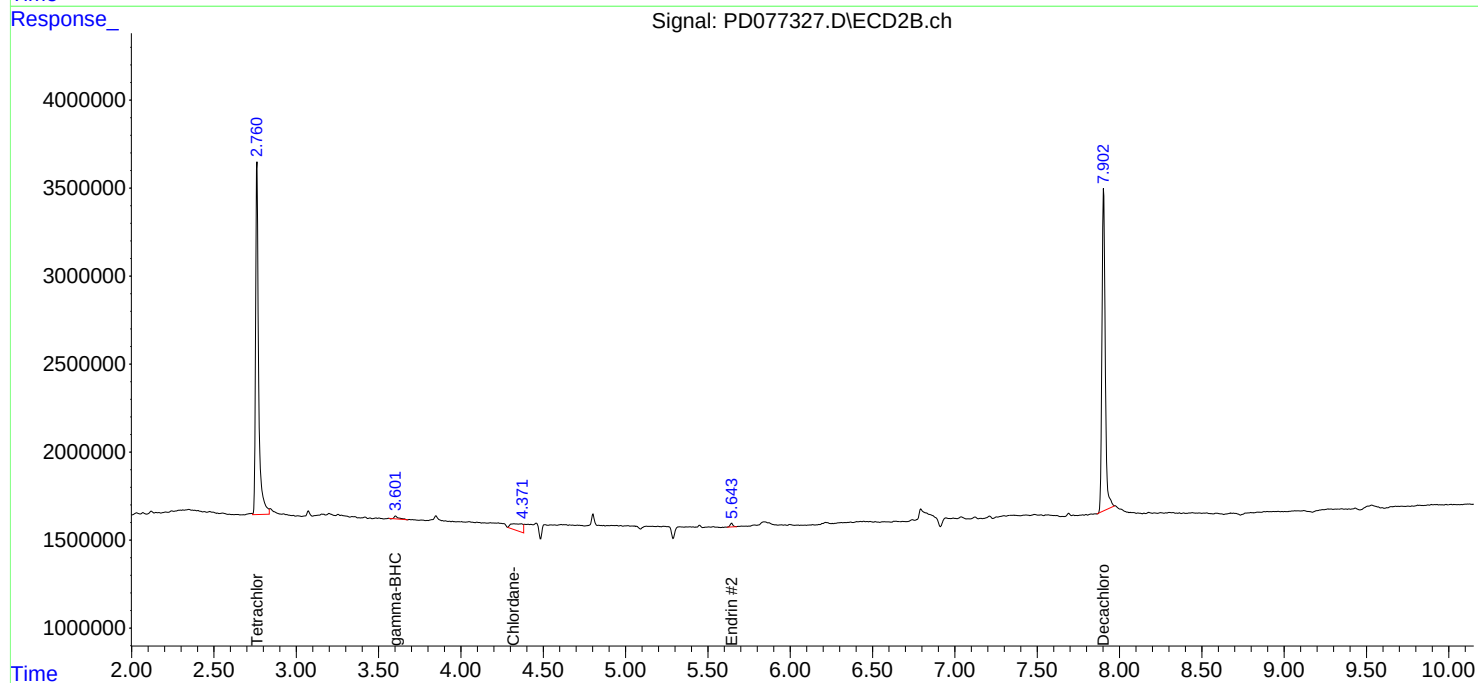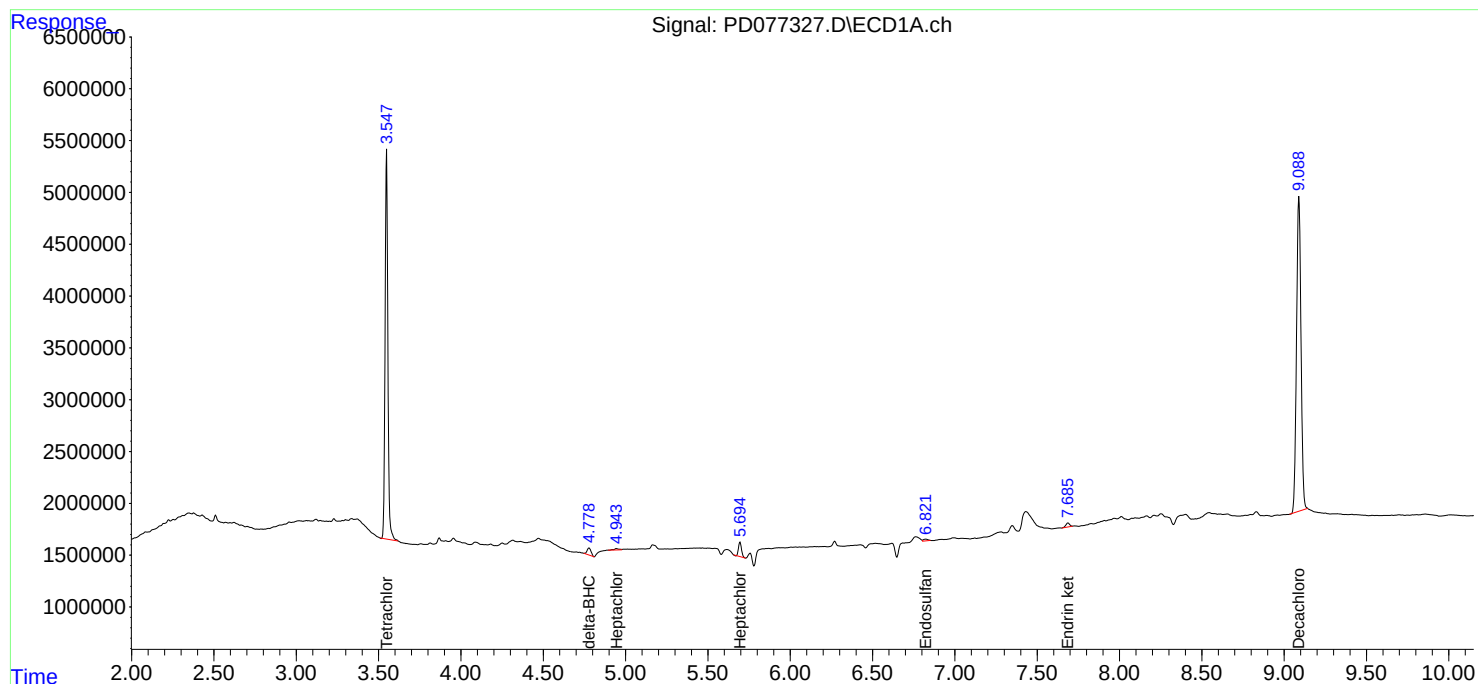


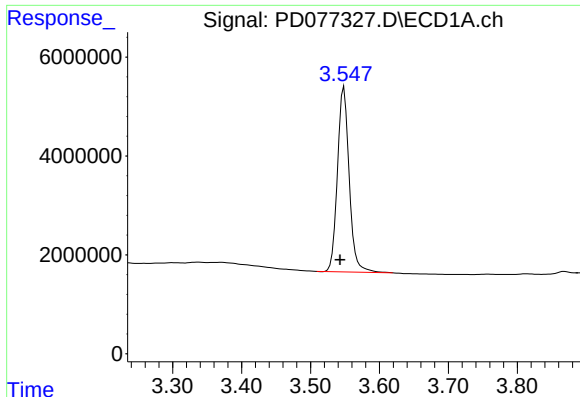

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.005 min
Response: 44296012
Conc: 18.72 ng/ml

Instrument :
ECD_D
ClientSampleId :

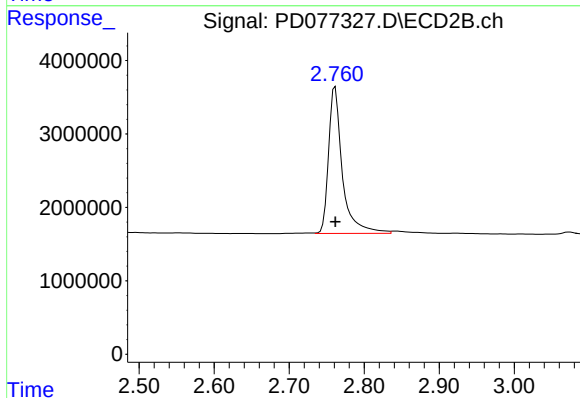


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 25595516
Conc: 18.79 ng/ml

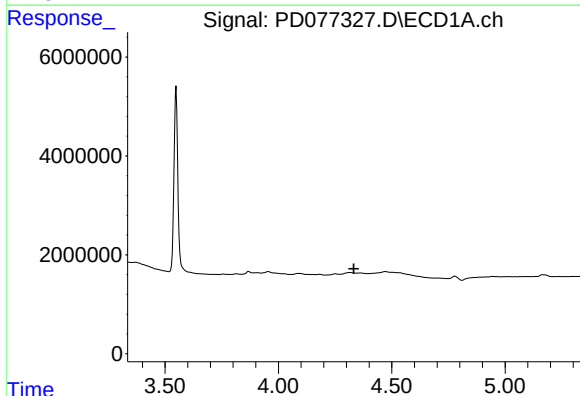


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.333 min
Response: 0
Conc: N.D.

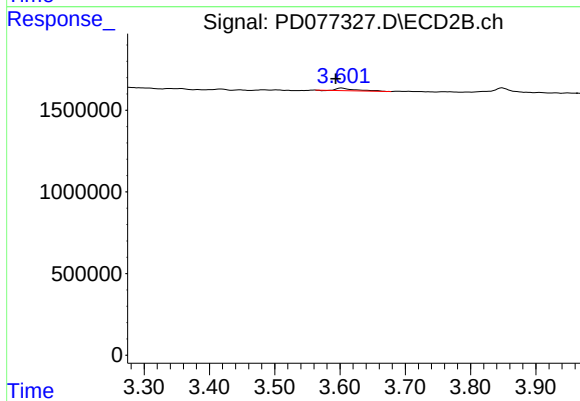

#3 gamma-BHC (Lindane)


R.T.: 3.603 min
Delta R.T.: 0.009 min
Response: 314824
Conc: 0.17 ng/ml

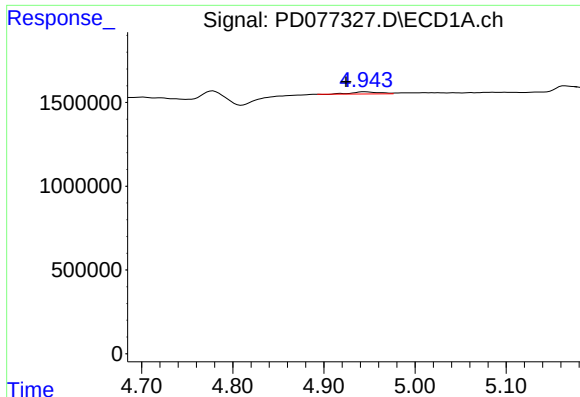

#4 Heptachlor


R.T.: 4.945 min
Delta R.T.: 0.021 min
Response: 274746
Conc: 0.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

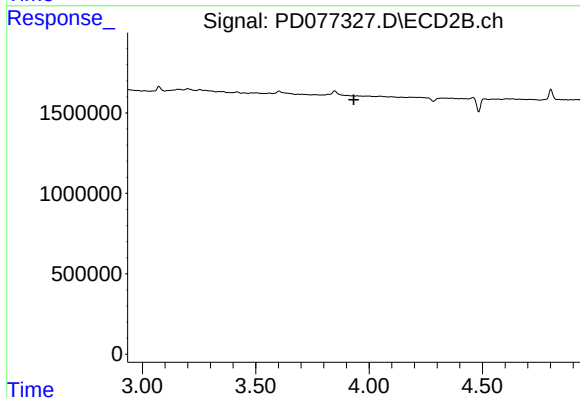


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 3.933 min
Response: 0
Conc: N.D.

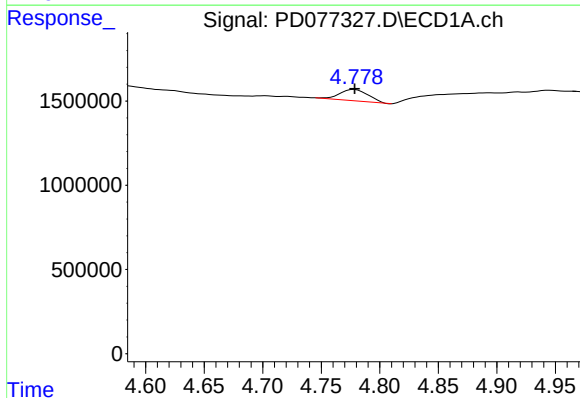


#7 delta-BHC

R.T.: 4.778 min
Delta R.T.: 0.000 min
Response: 1150995
Conc: 0.33 ng/ml

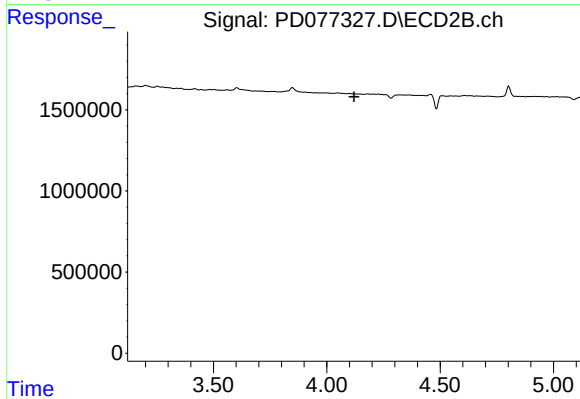

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.120 min
Response: 0
Conc: N.D.

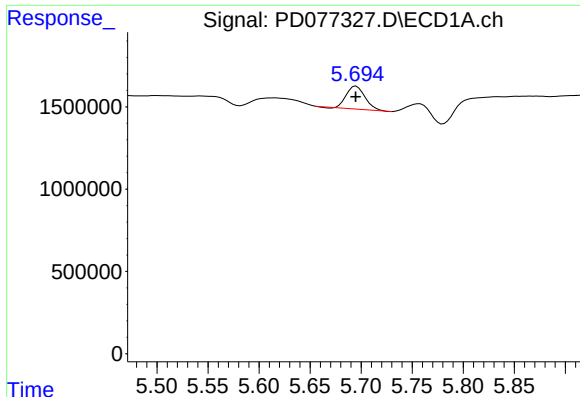

#8 Heptachlor epoxide


R.T.: 5.695 min
Delta R.T.: 0.000 min
Response: 1800543
Conc: 0.54 ng/ml

Instrument :
ECD_D
ClientSampleId :

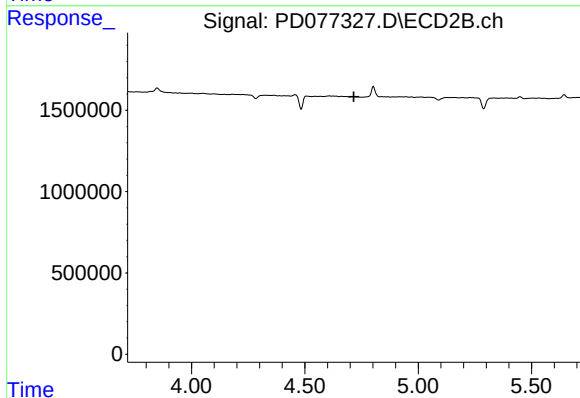


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.716 min
Response: 0
Conc: N.D.

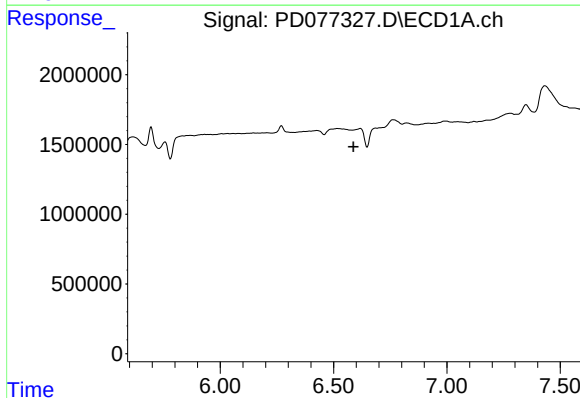


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.588 min
Response: 0
Conc: N.D.

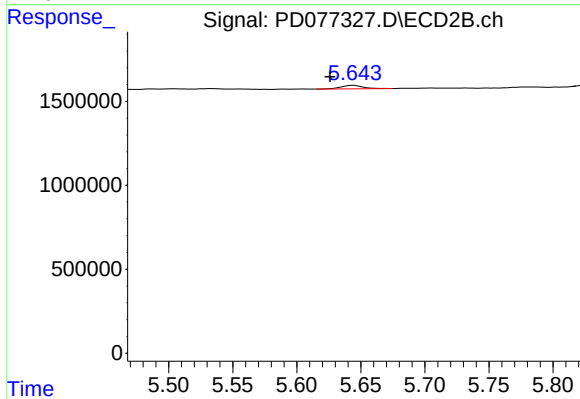

#14 Endrin


R.T.: 5.644 min
Delta R.T.: 0.018 min
Response: 248679
Conc: 0.17 ng/ml

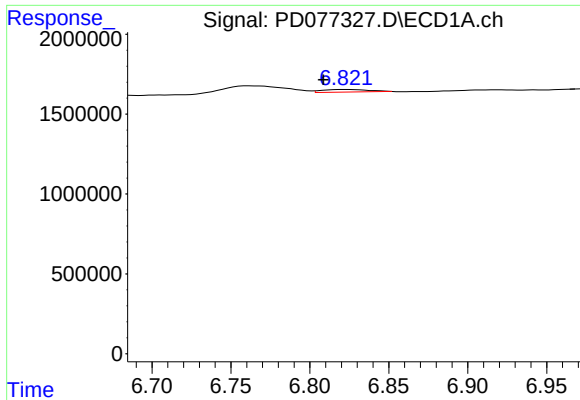

#15 Endosulfan II


R.T.: 6.824 min
Delta R.T.: 0.015 min
Response: 346605
Conc: 0.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

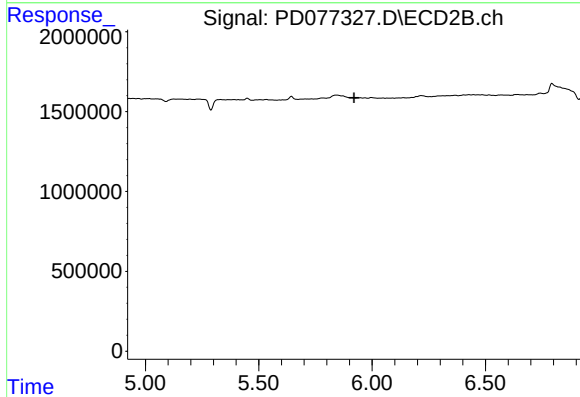


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.920 min
Response: 0
Conc: N.D.

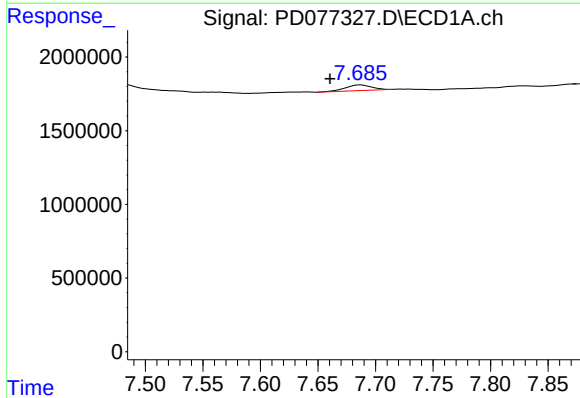


#21 Endrin ketone

R.T.: 7.687 min
Delta R.T.: 0.027 min
Response: 609763
Conc: 0.20 ng/ml

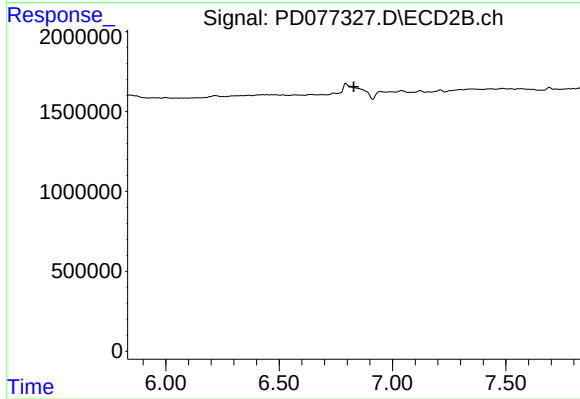

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.830 min
Response: 0
Conc: N.D.

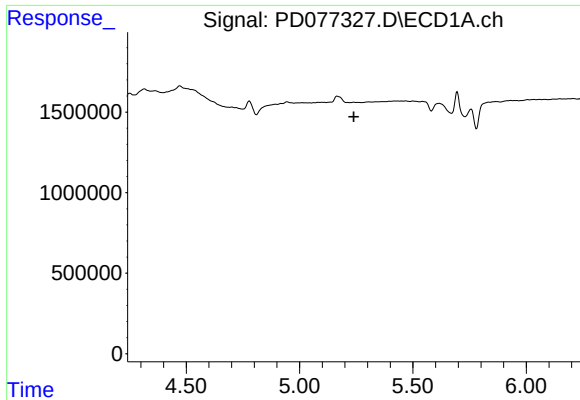

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.240 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

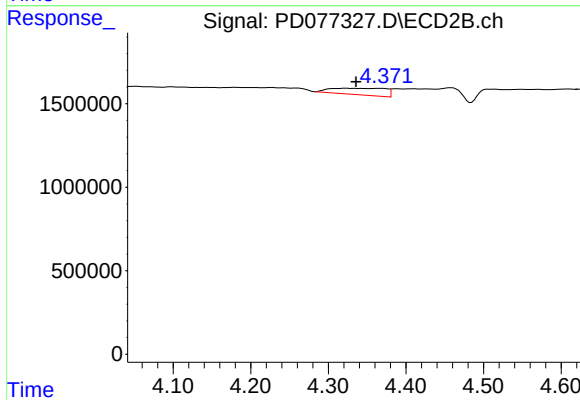


#24 Chlordane-2

R.T.: 4.321 min
Delta R.T.: -0.015 min
Response: 1910629
Conc: 33.98 ng/ml

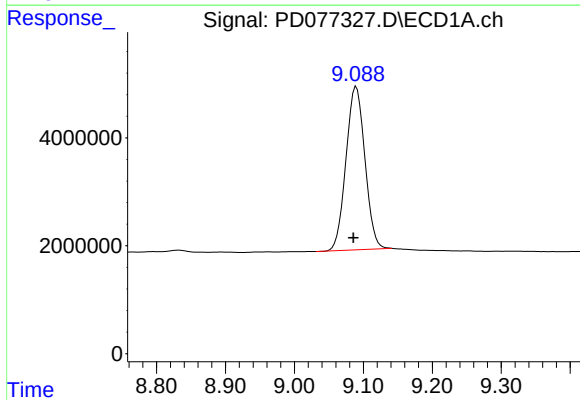

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: 0.004 min
Response: 57775236
Conc: 21.08 ng/ml

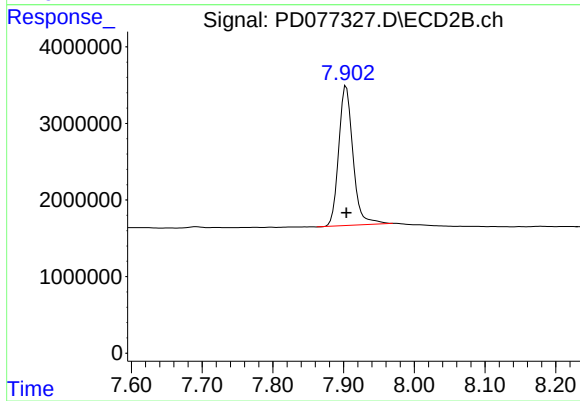

#28 Decachlorobiphenyl

R.T.: 7.904 min
Delta R.T.: 0.000 min
Response: 25618991
Conc: 17.90 ng/ml