

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082223\
 Data File : PD077329.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2023 12:54
 Operator : AR\AJ
 Sample : 04100-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 WC-1

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/23/2023
 Supervised By : Ankita Jodhani 08/23/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 00:50:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.760	22408548	12219752	9.469	8.971m
2)	SA Decachlor...	9.088	7.903	32044104	14336756	11.694m	10.018m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082223\
Data File : PD077329.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2023 12:54
Operator : AR\AJ
Sample : 04100-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
WC-1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/23/2023
Supervised By : Ankita Jodhani 08/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 00:50:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

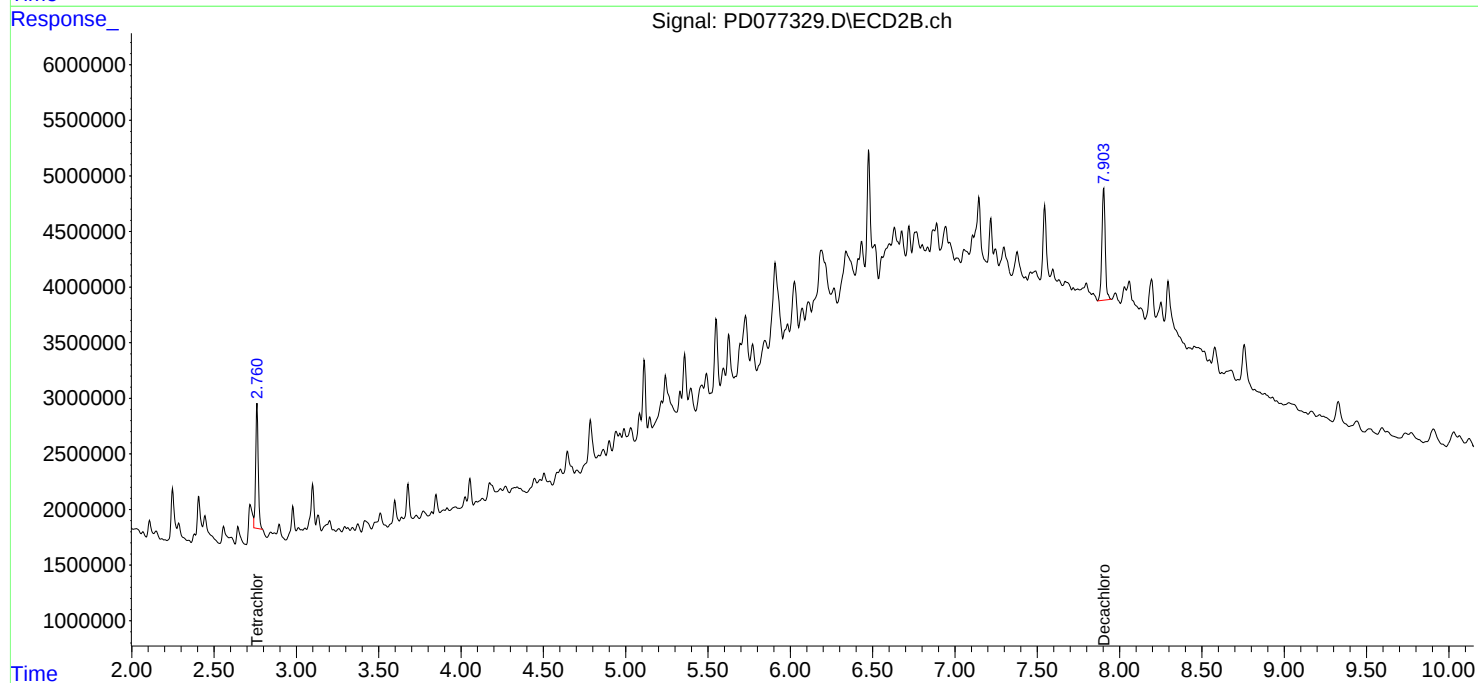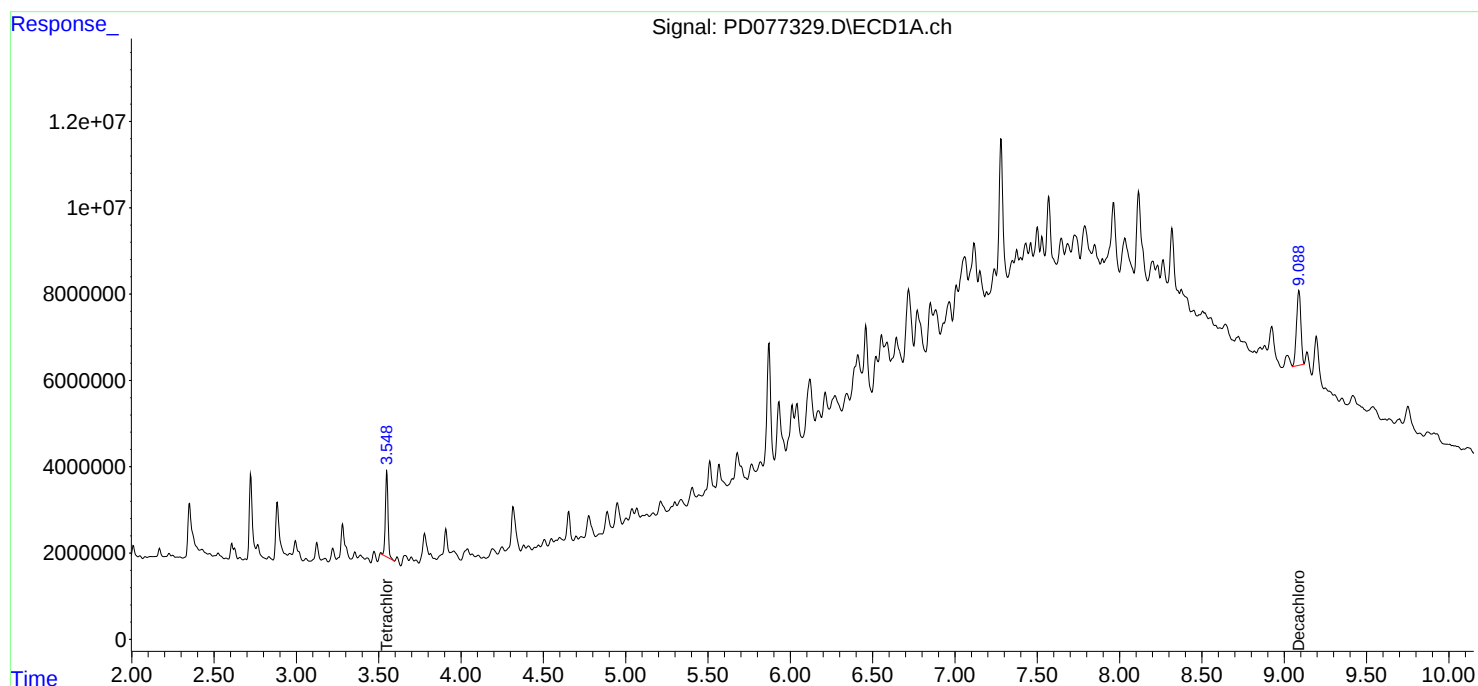

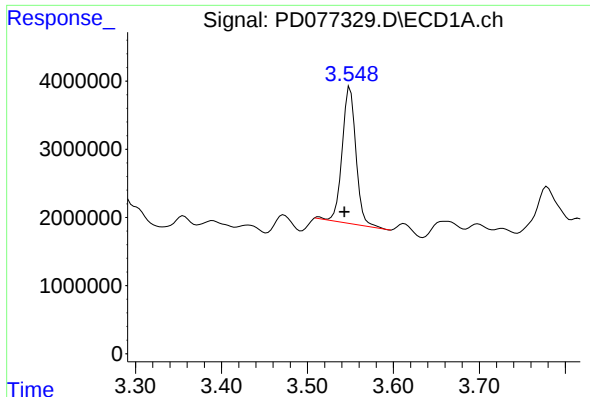


#1 Tetrachloro-m-xylene

R.T.: 3.550 min
Delta R.T.: 0.007 min
Response: 22408548
Conc: 9.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/23/2023
Supervised By :Ankita Jodhani 08/23/2023

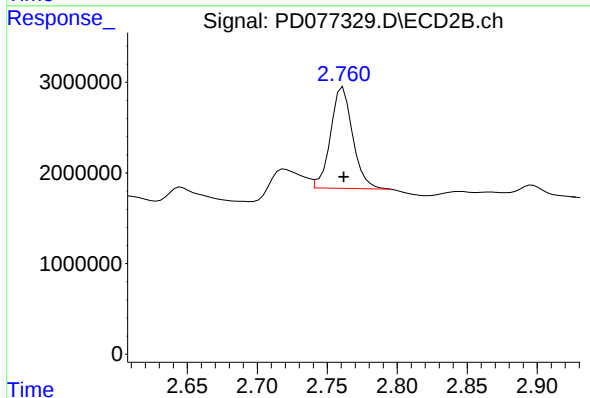


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: -0.002 min
Response: 12219752
Conc: 8.97 ng/ml m

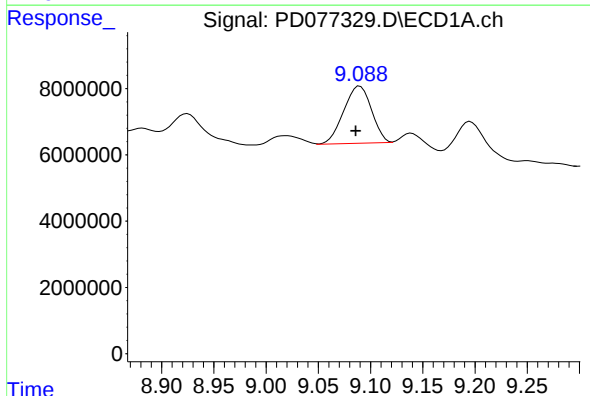

#28 Decachlorobiphenyl

R.T.: 9.088 min
Delta R.T.: 0.003 min
Response: 32044104
Conc: 11.69 ng/ml m

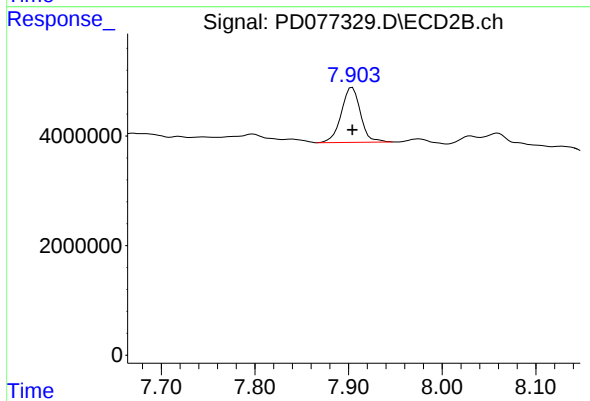

#28 Decachlorobiphenyl

R.T.: 7.903 min
Delta R.T.: -0.001 min
Response: 14336756
Conc: 10.02 ng/ml m