

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082321\
 Data File : PD065231.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2021 09:07
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 04:13:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.498	4.012	22275834	176.6E6	21.671	22.300
28) SA	Decachlor...	8.244	9.086	26860682	102.1E6	23.707	21.578
Target Compounds							
2) A	alpha-BHC	0.000	4.431f	0	9738265	N.D.	0.838 #
7) B	delta-BHC	0.000	5.095	0	937307	N.D.	0.097 #
15) B	Endosulfa...	0.000	6.936	0	2156344	N.D.	0.368 #
23)	Chlordane-1	4.396f	0.000	3908437	0	103.201	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082321\
Data File : PD065231.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2021 09:07
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 04:13:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

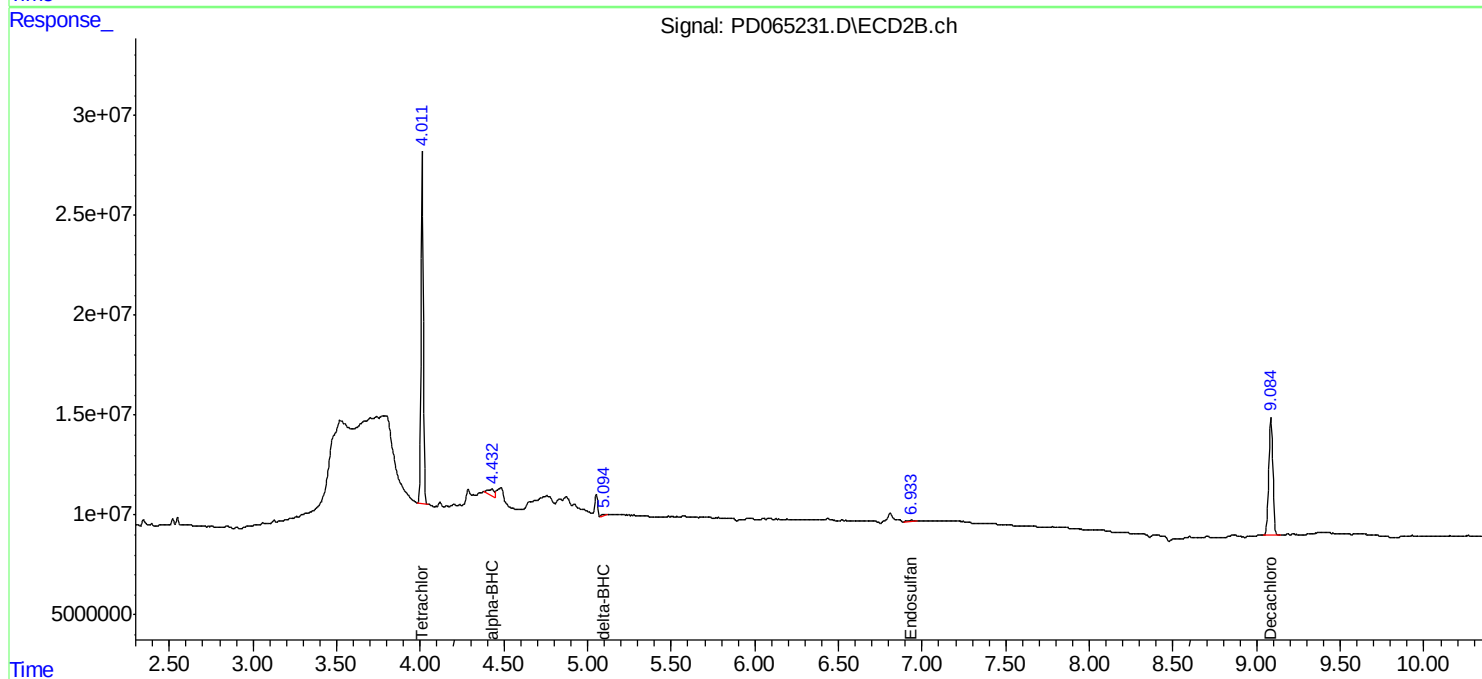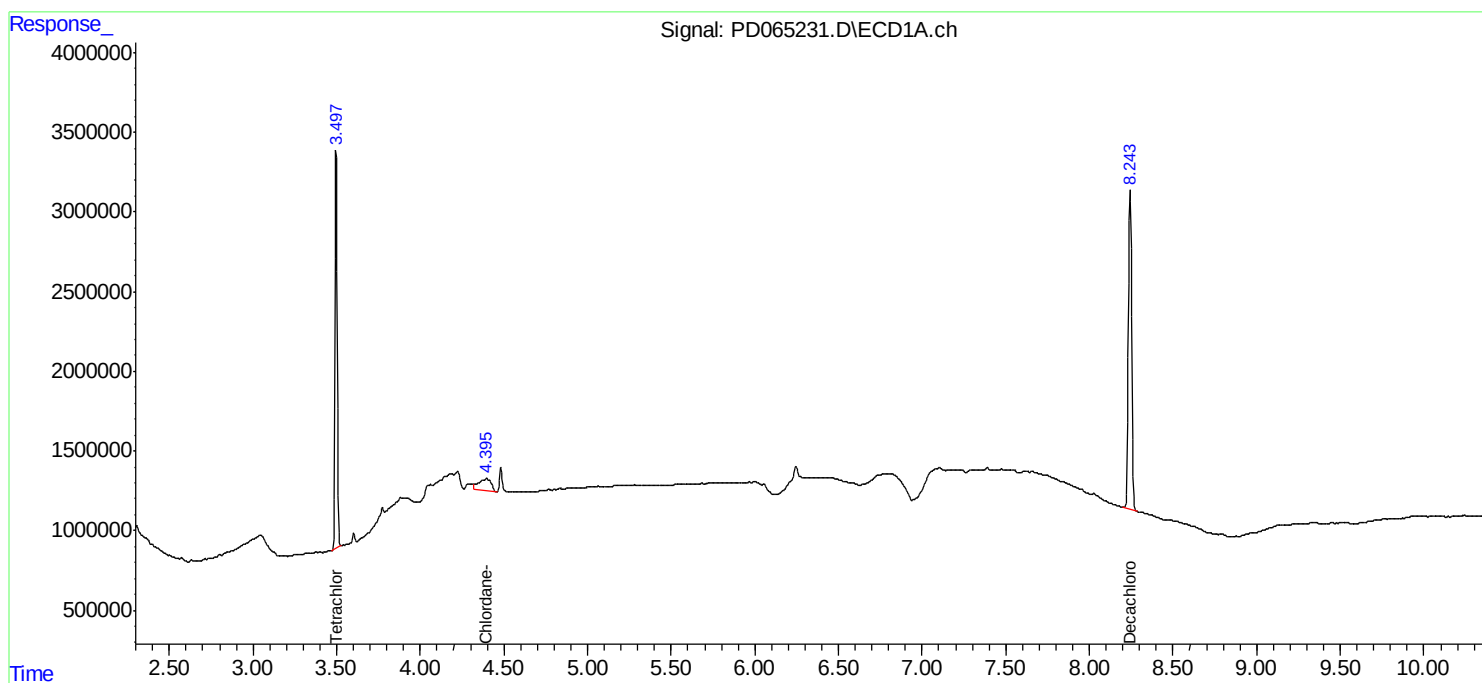


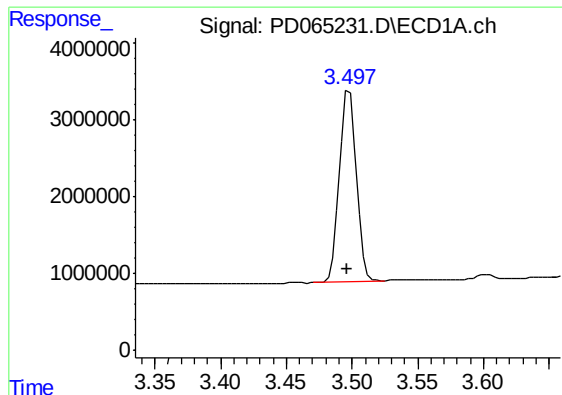

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.002 min
Response: 22275834
Conc: 21.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

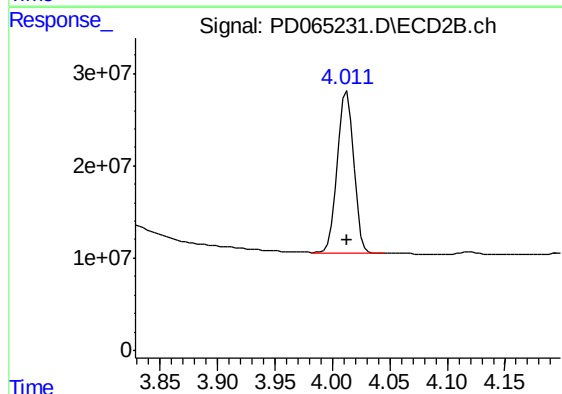


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 176630307
Conc: 22.30 ng/ml

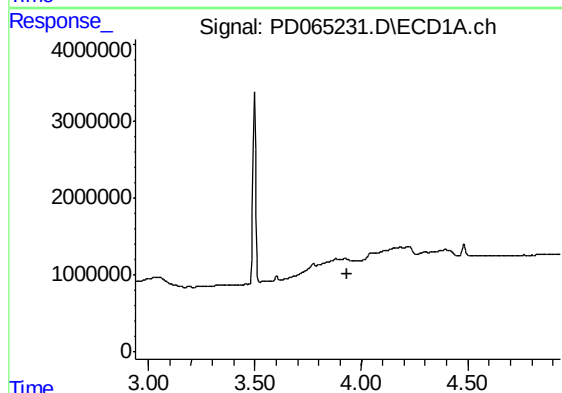


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.935 min
Response: 0
Conc: N.D.

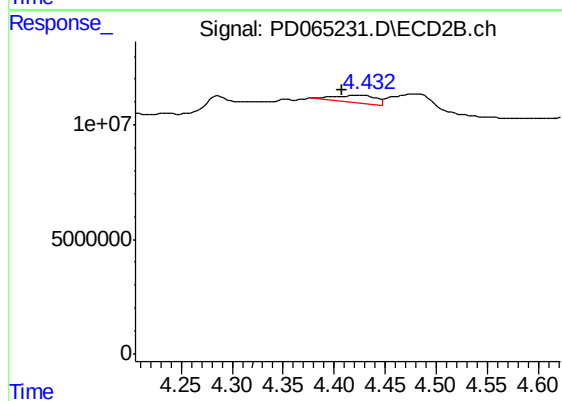

#2 alpha-BHC


R.T.: 4.431 min
Delta R.T.: 0.023 min
Response: 9738265
Conc: 0.84 ng/ml

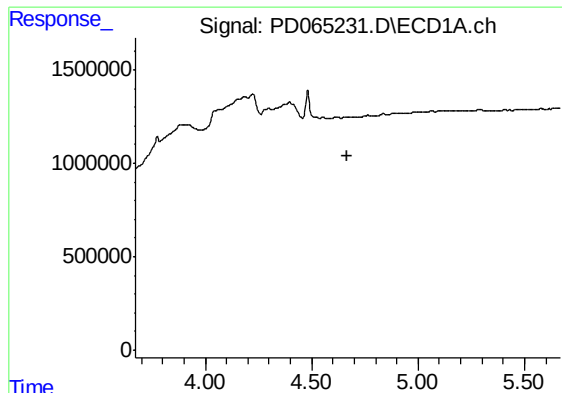

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.670 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

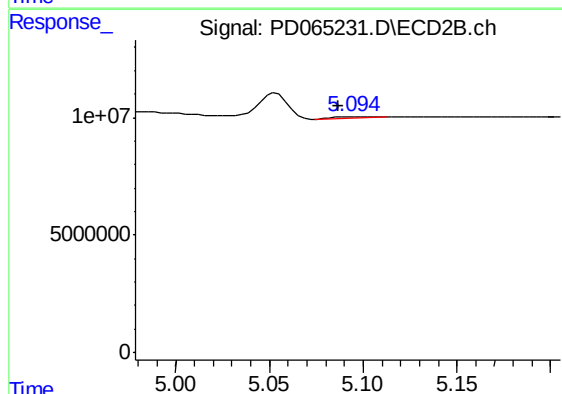


#7 delta-BHC

R.T.: 5.095 min
Delta R.T.: 0.009 min
Response: 937307
Conc: 0.10 ng/ml

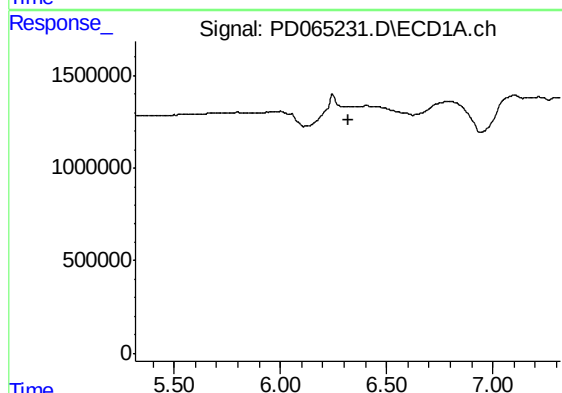


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.319 min
Response: 0
Conc: N.D.

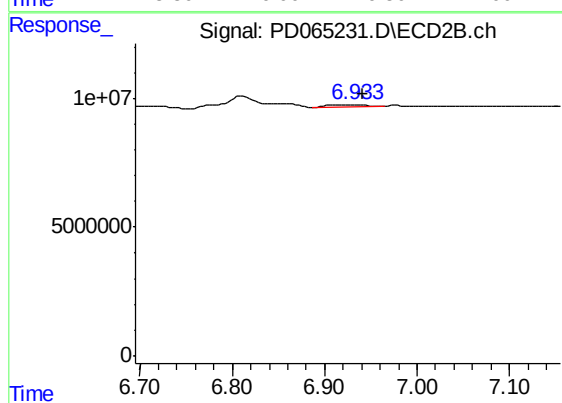

#15 Endosulfan II


R.T.: 6.936 min
Delta R.T.: -0.005 min
Response: 2156344
Conc: 0.37 ng/ml

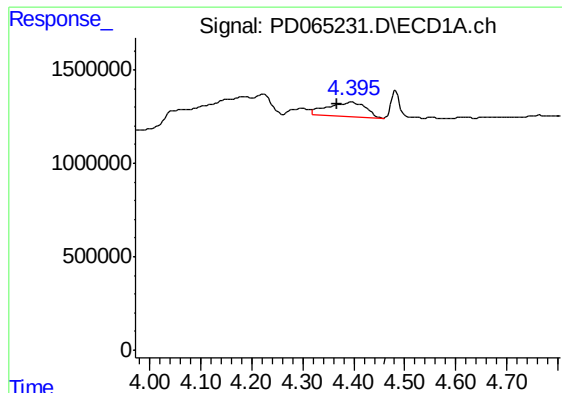

#23 Chlordane-1


R.T.: 4.396 min
Delta R.T.: 0.030 min
Response: 3908437
Conc: 103.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

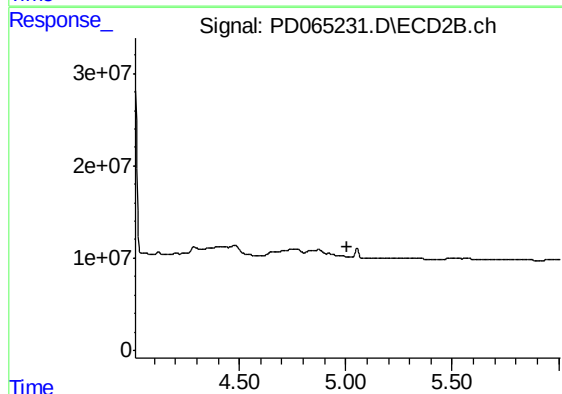


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.009 min
Response: 0
Conc: N.D.

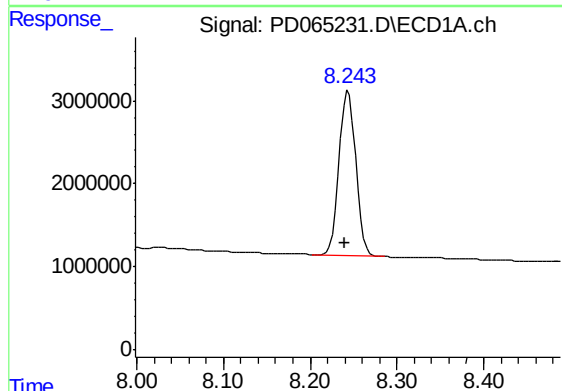

#28 Decachlorobiphenyl

R.T.: 8.244 min
Delta R.T.: 0.004 min
Response: 26860682
Conc: 23.71 ng/ml

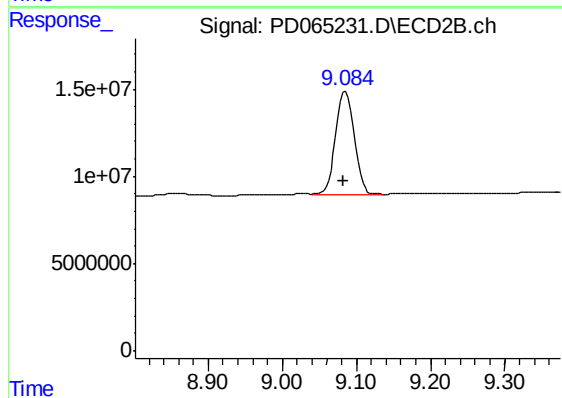

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.003 min
Response: 102118814
Conc: 21.58 ng/ml