

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082321\
 Data File : PD065246.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2021 16:55
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 04:19:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.496	4.013	21856592	165.8E6	21.263	20.935
28) SA	Decachlor...	8.240	9.086	26767837	98349891	23.625	20.782
Target Compounds							
3) MA	gamma-BHC...	4.227	0.000	1072381	0	0.782	N.D. #
20) A	Methoxychlor	0.000	7.620	0	72772042	N.D.	24.048 #
21) B	Endrin ke...	0.000	7.770	0	3912826	N.D.	0.602 #
23)	Chlordane-1	4.394f	0.000	1111577	0	29.351	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082321\
Data File : PD065246.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2021 16:55
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 04:19:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

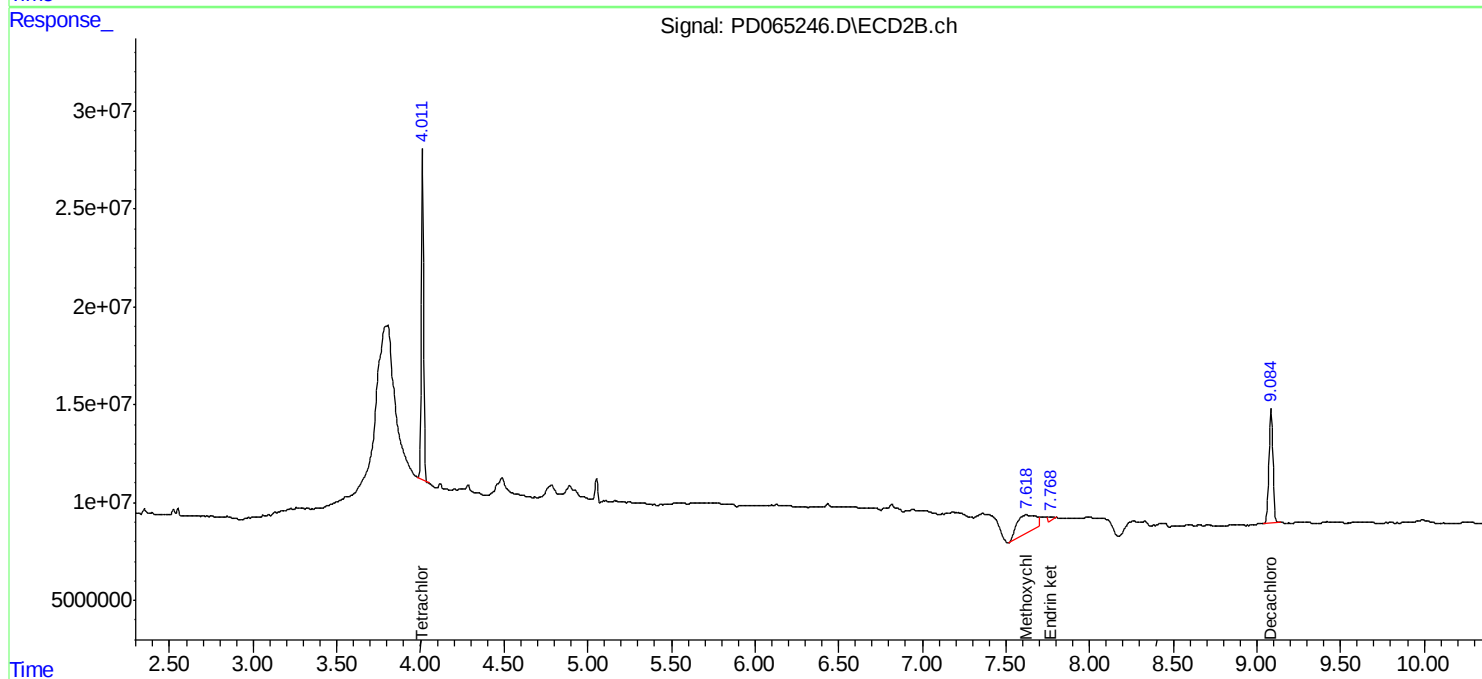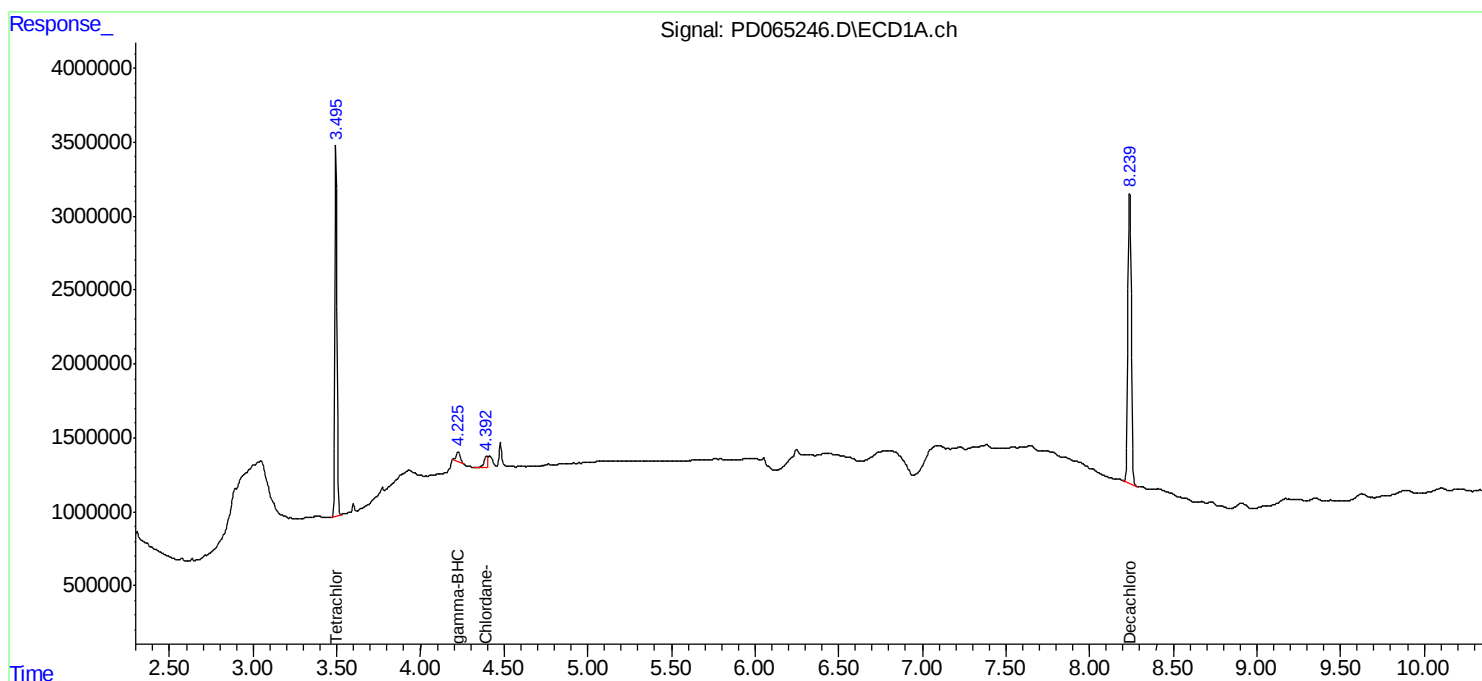


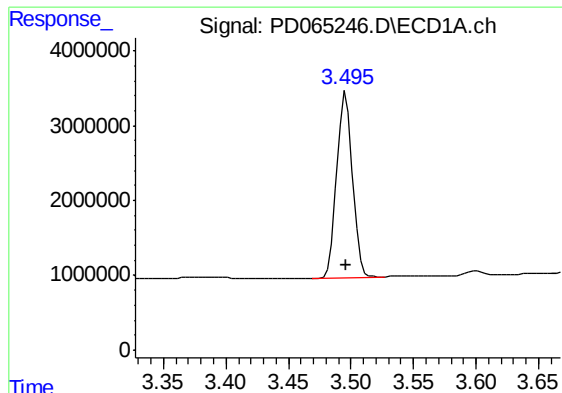

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 21856592
Conc: 21.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

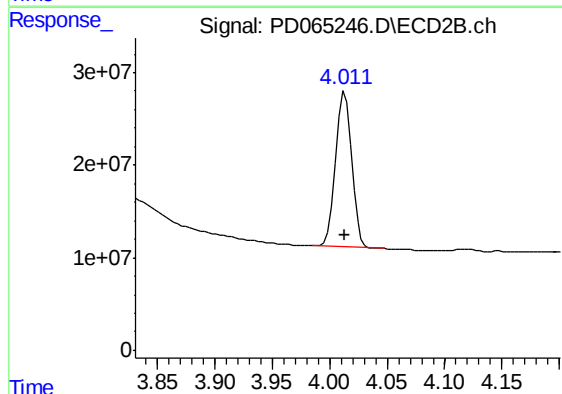


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 165820983
Conc: 20.94 ng/ml

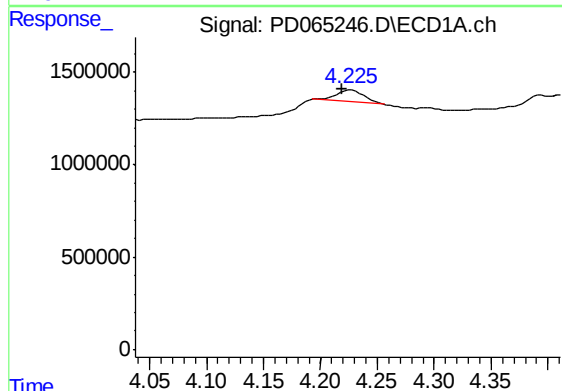


#3 gamma-BHC (Lindane)

R.T.: 4.227 min
Delta R.T.: 0.008 min
Response: 1072381
Conc: 0.78 ng/ml

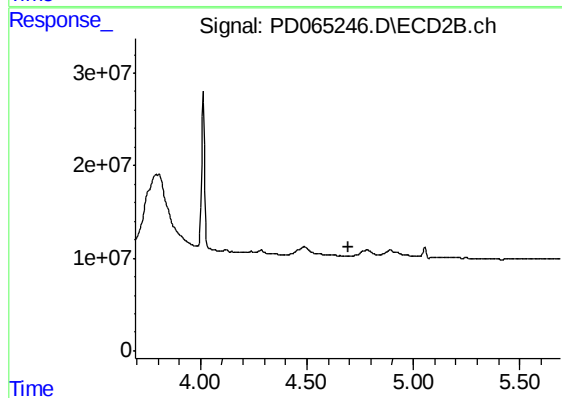

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.694 min
Response: 0
Conc: N.D.

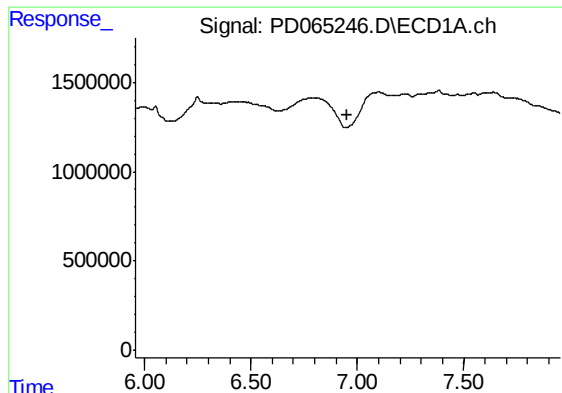

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.955 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

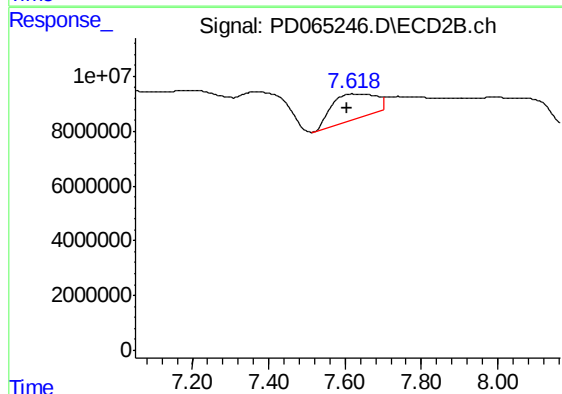


#20 Methoxychlor

R.T.: 7.620 min
Delta R.T.: 0.012 min
Response: 72772042
Conc: 24.05 ng/ml

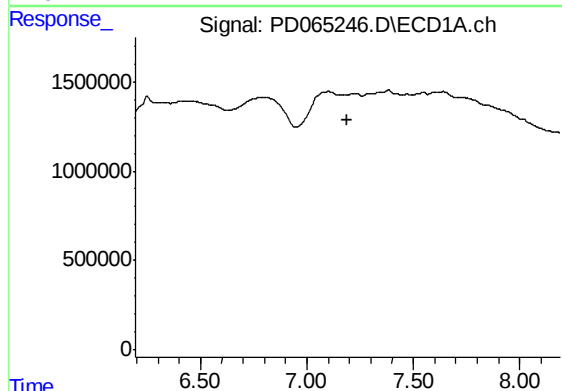


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.192 min
Response: 0
Conc: N.D.

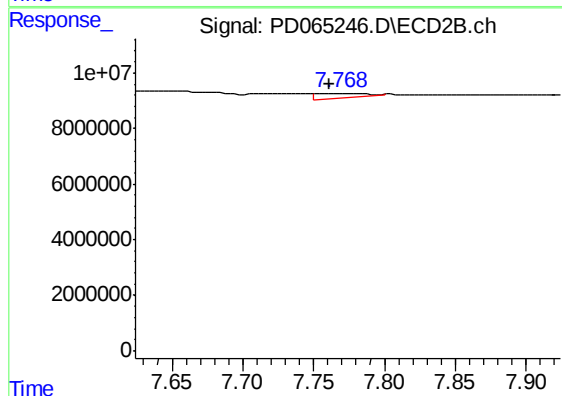

#21 Endrin ketone


R.T.: 7.770 min
Delta R.T.: 0.009 min
Response: 3912826
Conc: 0.60 ng/ml

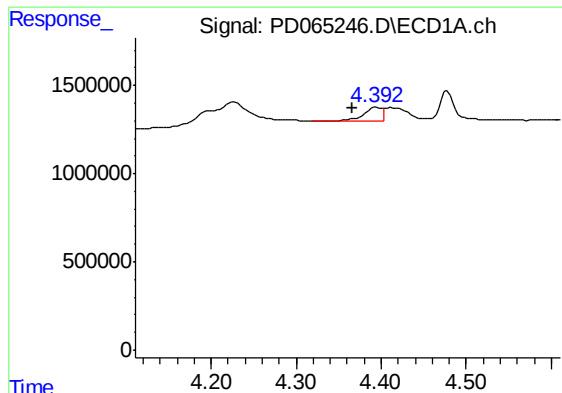

#23 Chlordane-1


R.T.: 4.394 min
Delta R.T.: 0.028 min
Response: 1111577
Conc: 29.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

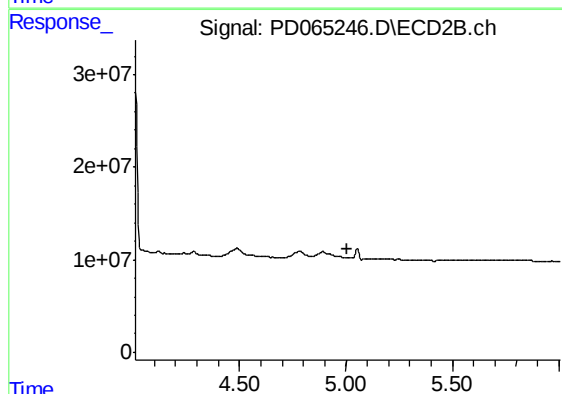


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.009 min
Response: 0
Conc: N.D.

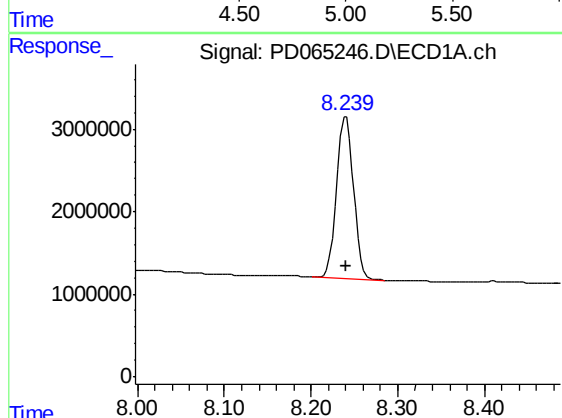

#28 Decachlorobiphenyl

R.T.: 8.240 min
Delta R.T.: 0.000 min
Response: 26767837
Conc: 23.62 ng/ml

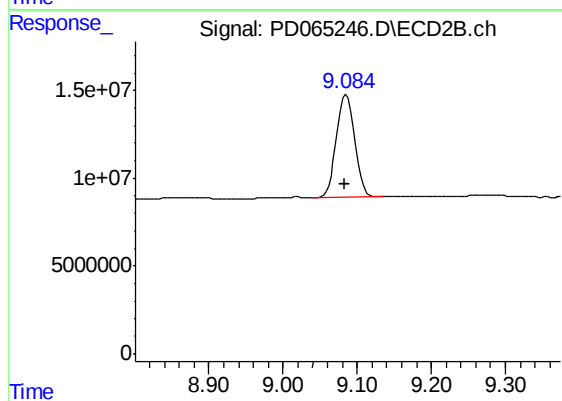

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.003 min
Response: 98349891
Conc: 20.78 ng/ml