

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082321\
 Data File : PD065252.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2021 18:49
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 04:21:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:25:41 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	21505060	164.0E6	20.921	20.706
28)	SA Decachlor...	8.241	9.085	21552578	80473807	19.022	17.004
Target Compounds							
3)	MA gamma-BHC...	4.227	0.000	1126196	0	0.821	N.D. #
7)	B delta-BHC	0.000	5.092	0	1797789	N.D.	0.185 #
17)	MA 4,4'-DDT	0.000	7.144	0	985971	N.D.	0.164 #
23)	Chlordane-1	4.395f	0.000	2314139	0	61.104	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082321\
Data File : PD065252.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2021 18:49
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 04:21:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:25:41 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

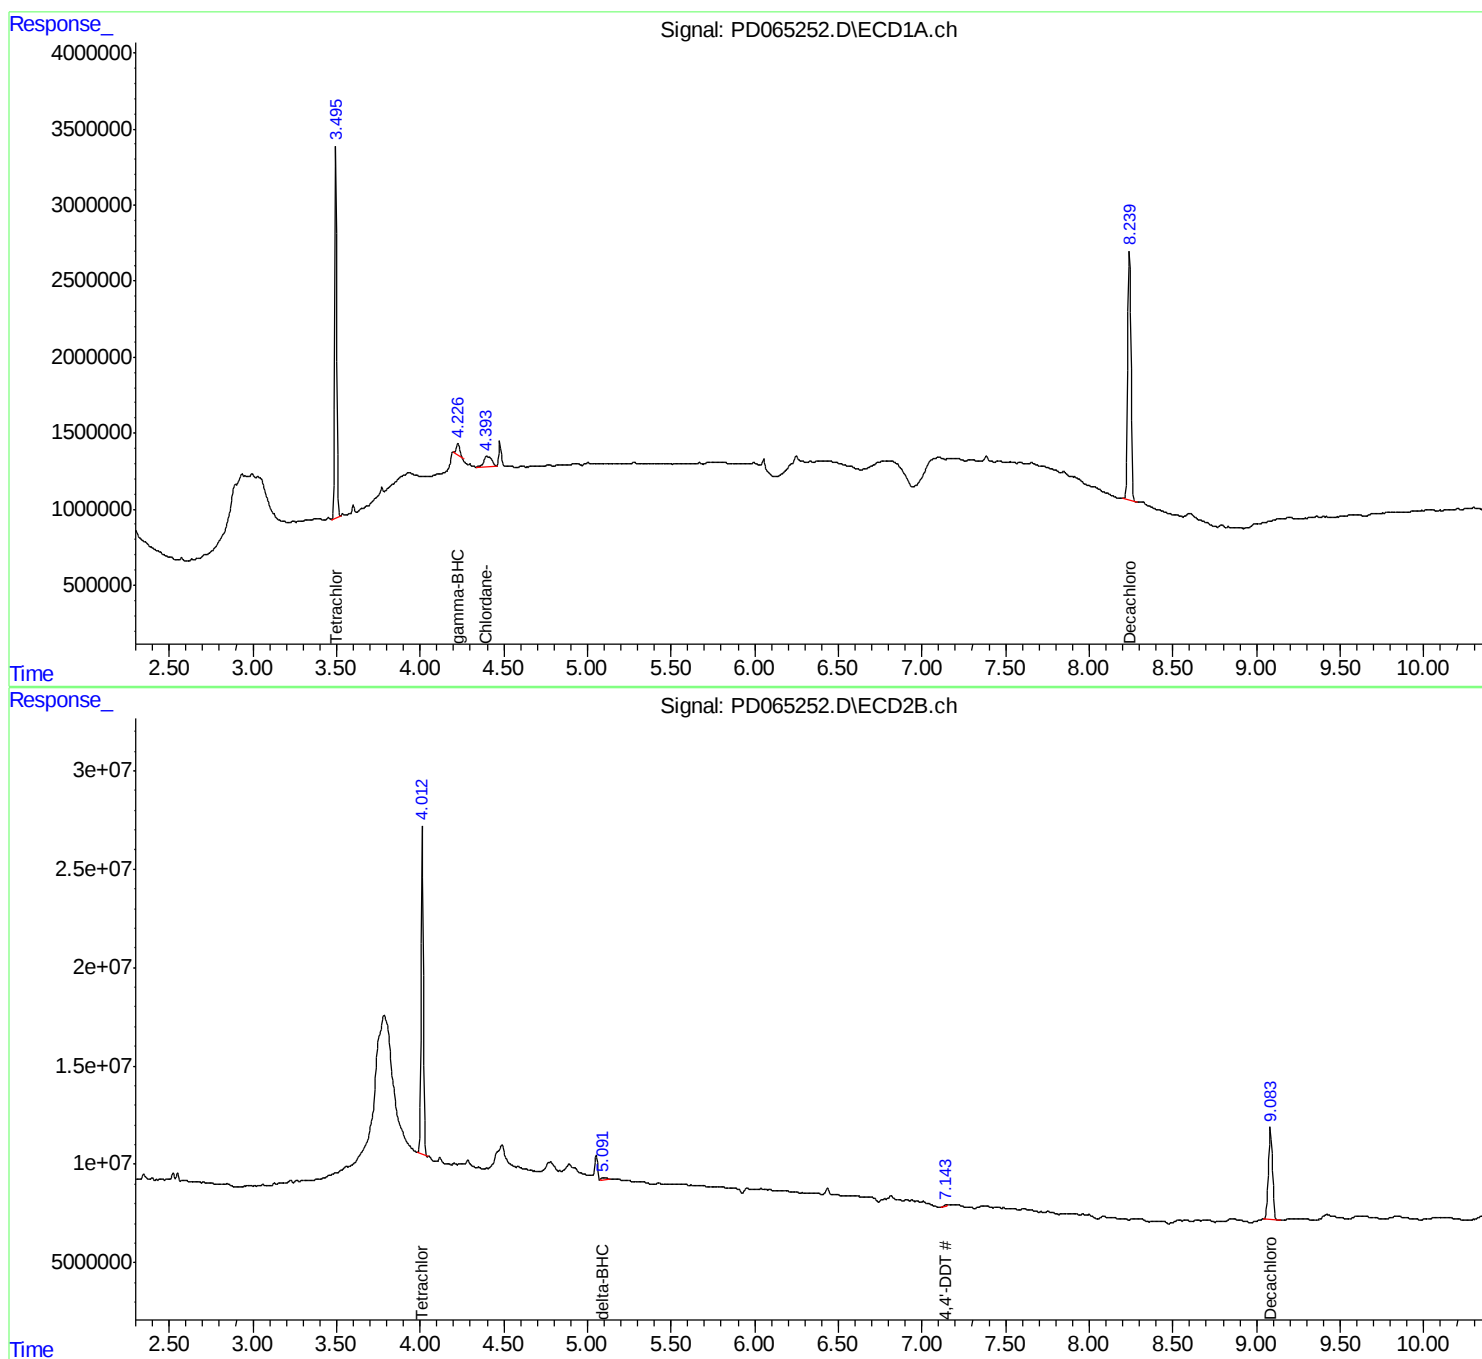


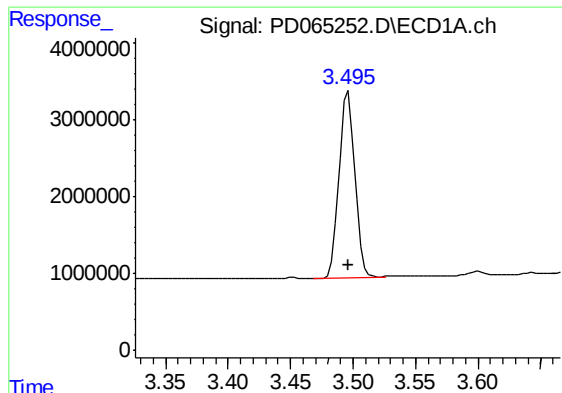

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 21505060
Conc: 20.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

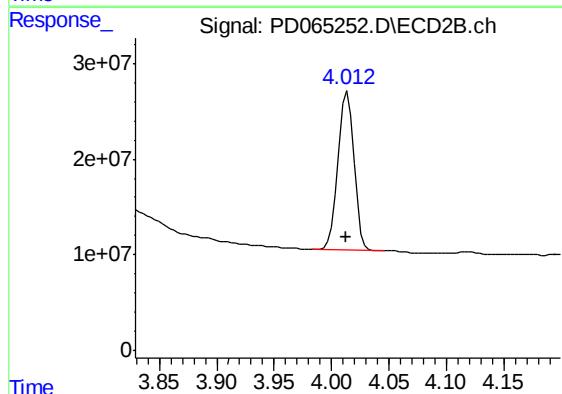


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 164004758
Conc: 20.71 ng/ml

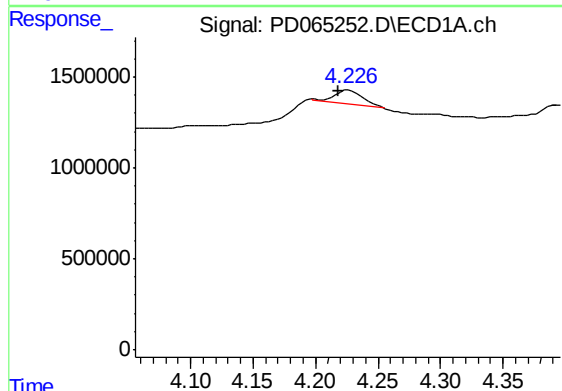


#3 gamma-BHC (Lindane)

R.T.: 4.227 min
Delta R.T.: 0.008 min
Response: 1126196
Conc: 0.82 ng/ml

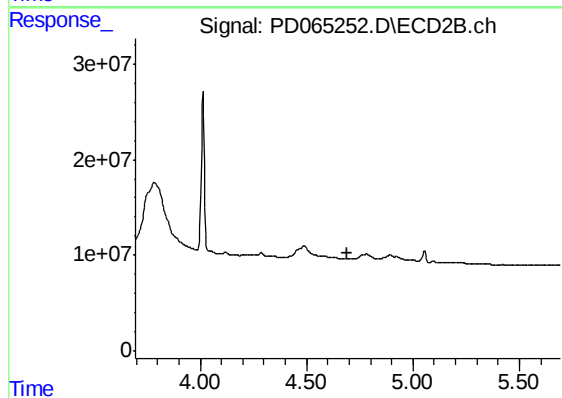

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.694 min
Response: 0
Conc: N.D.

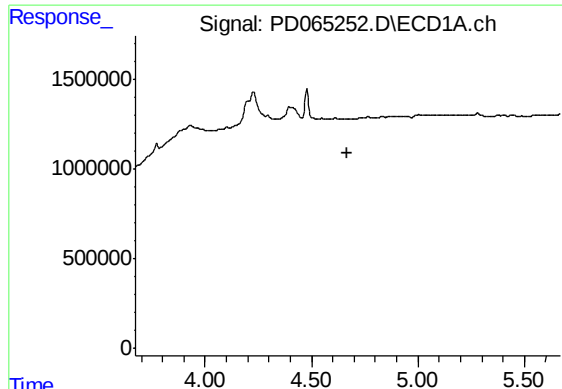

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.670 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

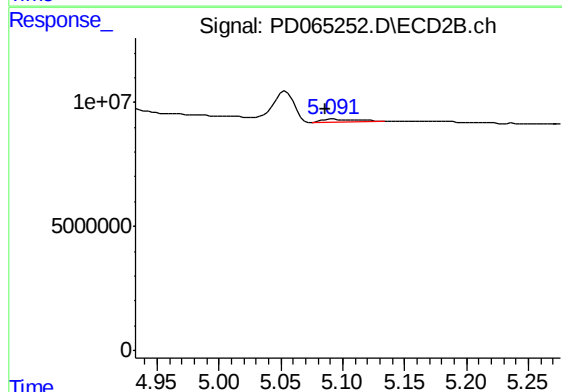


#7 delta-BHC

R.T.: 5.092 min
Delta R.T.: 0.006 min
Response: 1797789
Conc: 0.19 ng/ml

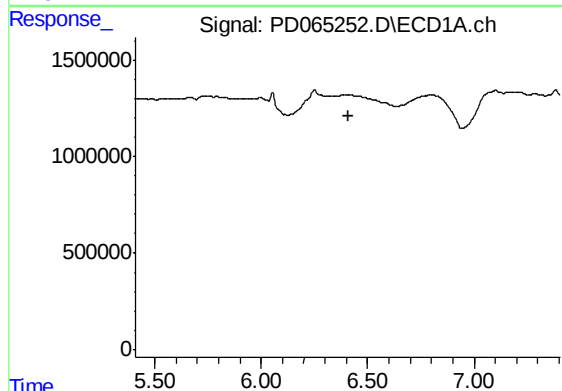


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.409 min
Response: 0
Conc: N.D.

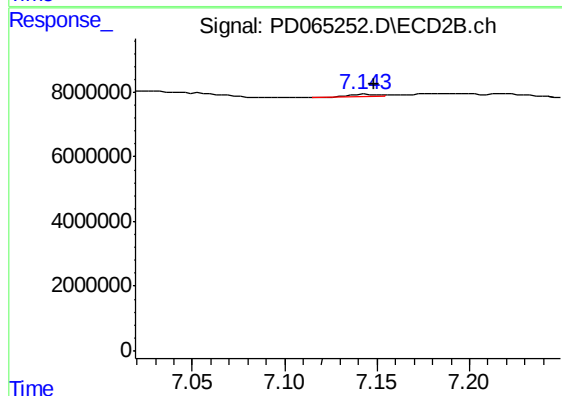

#17 4,4'-DDT


R.T.: 7.144 min
Delta R.T.: -0.004 min
Response: 985971
Conc: 0.16 ng/ml

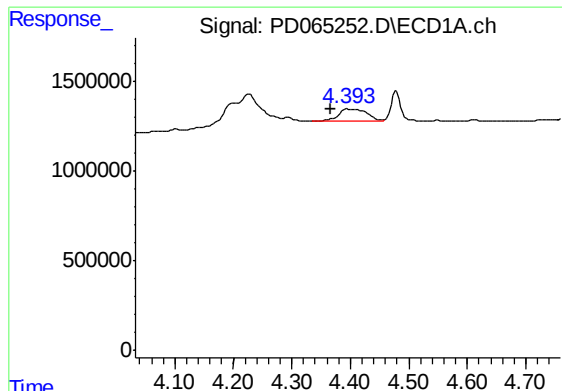

#23 Chlordane-1


R.T.: 4.395 min
Delta R.T.: 0.028 min
Response: 2314139
Conc: 61.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

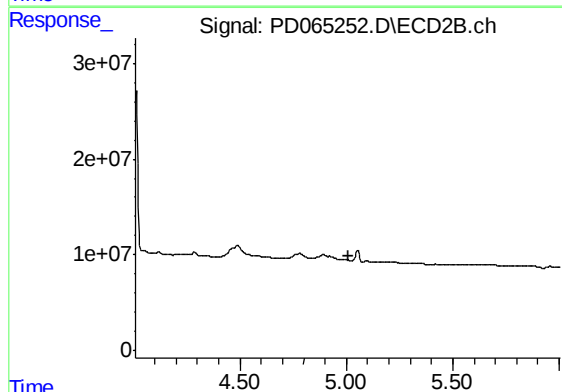


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.009 min
Response: 0
Conc: N.D.

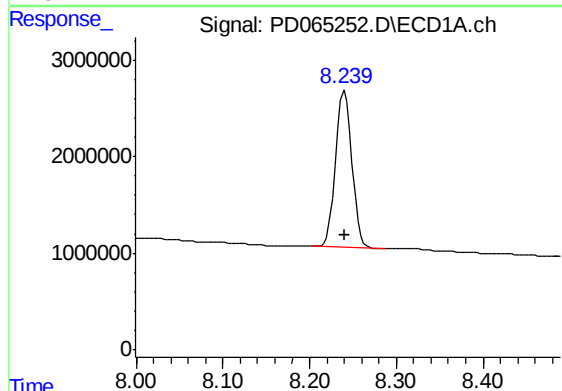

#28 Decachlorobiphenyl

R.T.: 8.241 min
Delta R.T.: 0.000 min
Response: 21552578
Conc: 19.02 ng/ml

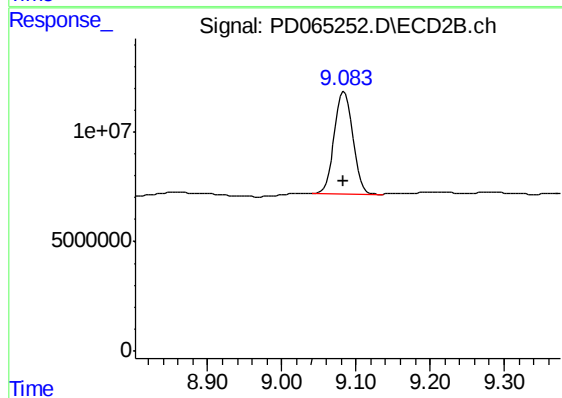

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.002 min
Response: 80473807
Conc: 17.00 ng/ml