

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082321\
 Data File : PD065255.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2021 19:30
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 05:25:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX082021.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 20 02:56:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.496	4.014	52242376	392.7E6	50.603	49.238
7) SA Decachlor...	8.240	9.085	53809315	208.0E6	44.344	42.800
Target Compounds						
2) Toxaphene-1	5.749	6.407	4557567	15481306	515.175	422.259
3) Toxaphene-2	5.910	6.599	4751543	30840695	515.476	507.854
4) Toxaphene-3	6.351	7.182	10902711	47180777	522.389	439.721
5) Toxaphene-4	6.596	7.268	11930115	48768374	530.097	466.342
6) Toxaphene-5	7.083	7.687	12417755	37305767	473.713	441.565

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082321\
Data File : PD065255.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2021 19:30
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 05:25:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX082021.M
Quant Title : GC Extractables
QLast Update : Fri Aug 20 02:56:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

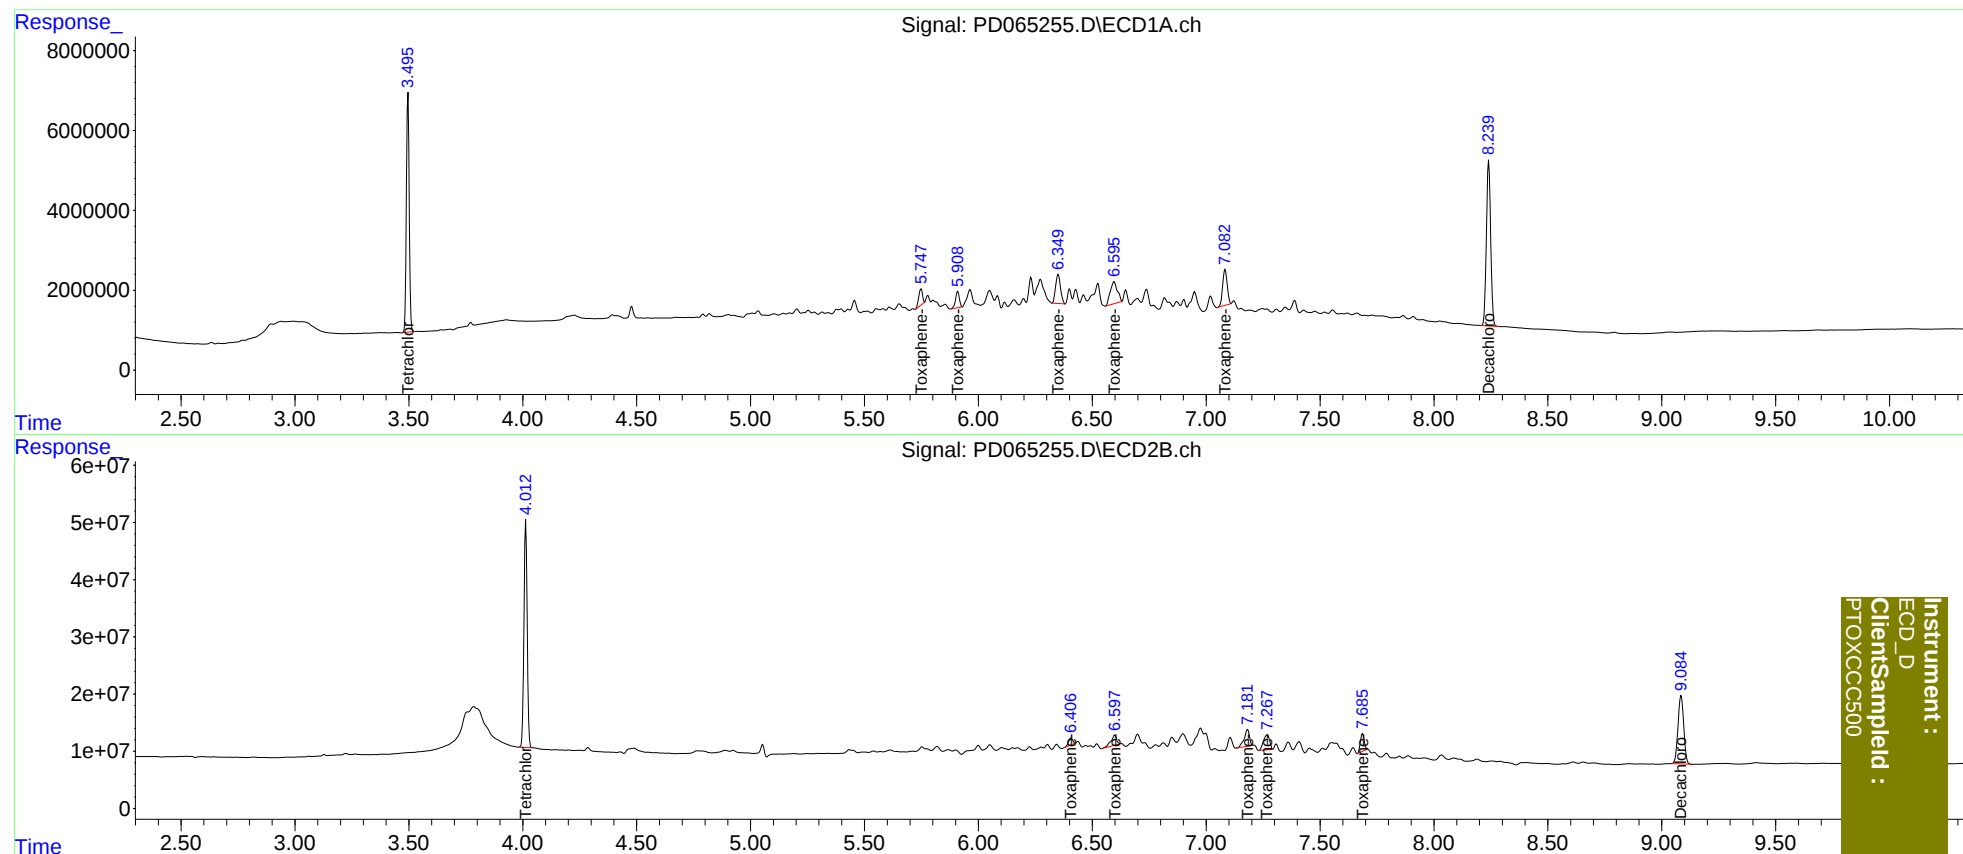

Instrument :
ECD_D
ClientSampled :
PTOXCCC500