

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082323\
 Data File : PD077335.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2023 08:14
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 22:44:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
2) A	alpha-BHC	0.000	3.278	0	40465	N.D. 0.021 #
4) MA	Heptachlor	4.926	0.000	266843	0	0.074 N.D. #
5) MB	Aldrin	5.265	4.195f	190082	298040	0.051 0.161 #
7) B	delta-BHC	4.780	0.000	1249048	0	0.358 N.D. #
8) B	Heptachlo...	5.700	0.000	4382220	0	1.323 N.D. #
14) MA	Endrin	0.000	5.645f	0	3344354	N.D. 2.286 #
15) B	Endosulfa...	6.821	0.000	14941	0	0.005 N.D. #
16) A	4,4'-DDD	6.725	0.000	195748	0	0.083 N.D. #
17) MA	4,4'-DDT	7.062f	0.000	791904	0	0.326 N.D. #
21) B	Endrin ke...	7.663	0.000	253275	0	0.084 N.D. #
24)	Chlordane-2	5.224f	4.358f	44478	10073800	0.367 179.135 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082323\
Data File : PD077335.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2023 08:14
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 22:44:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

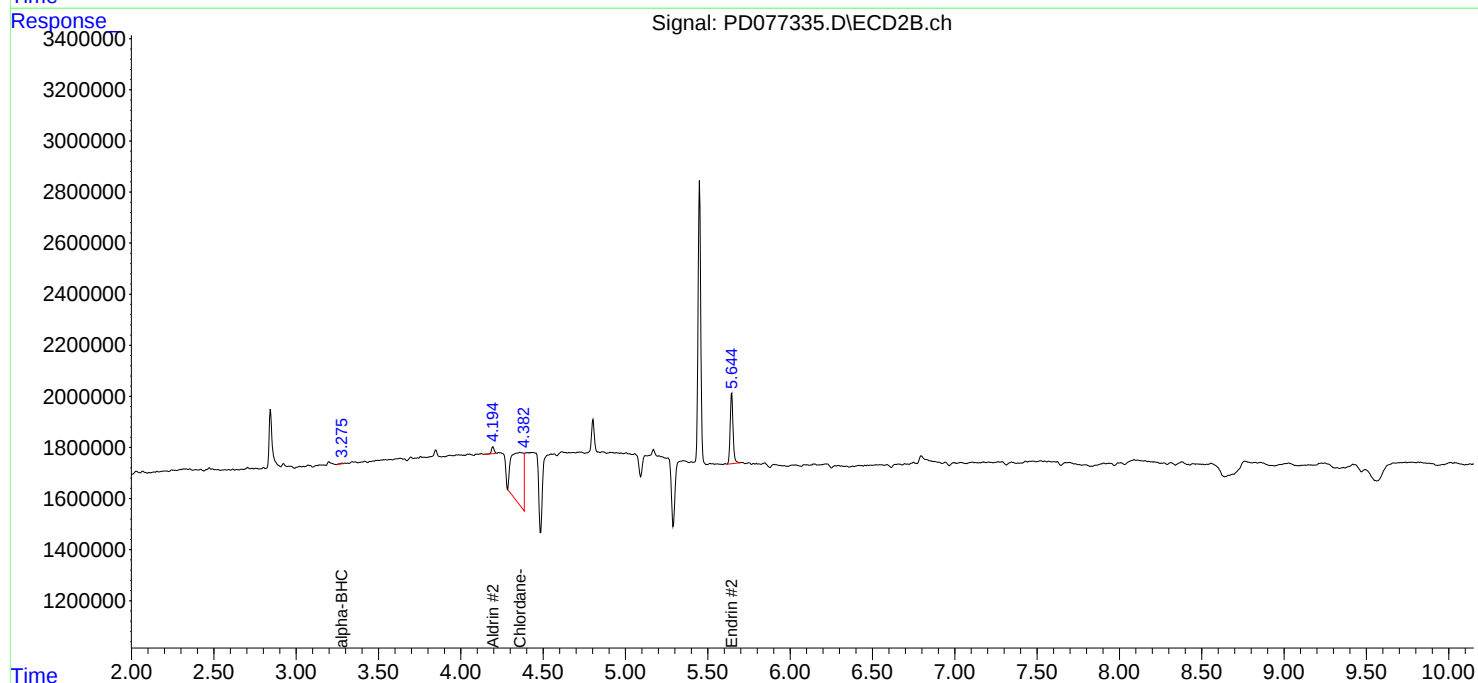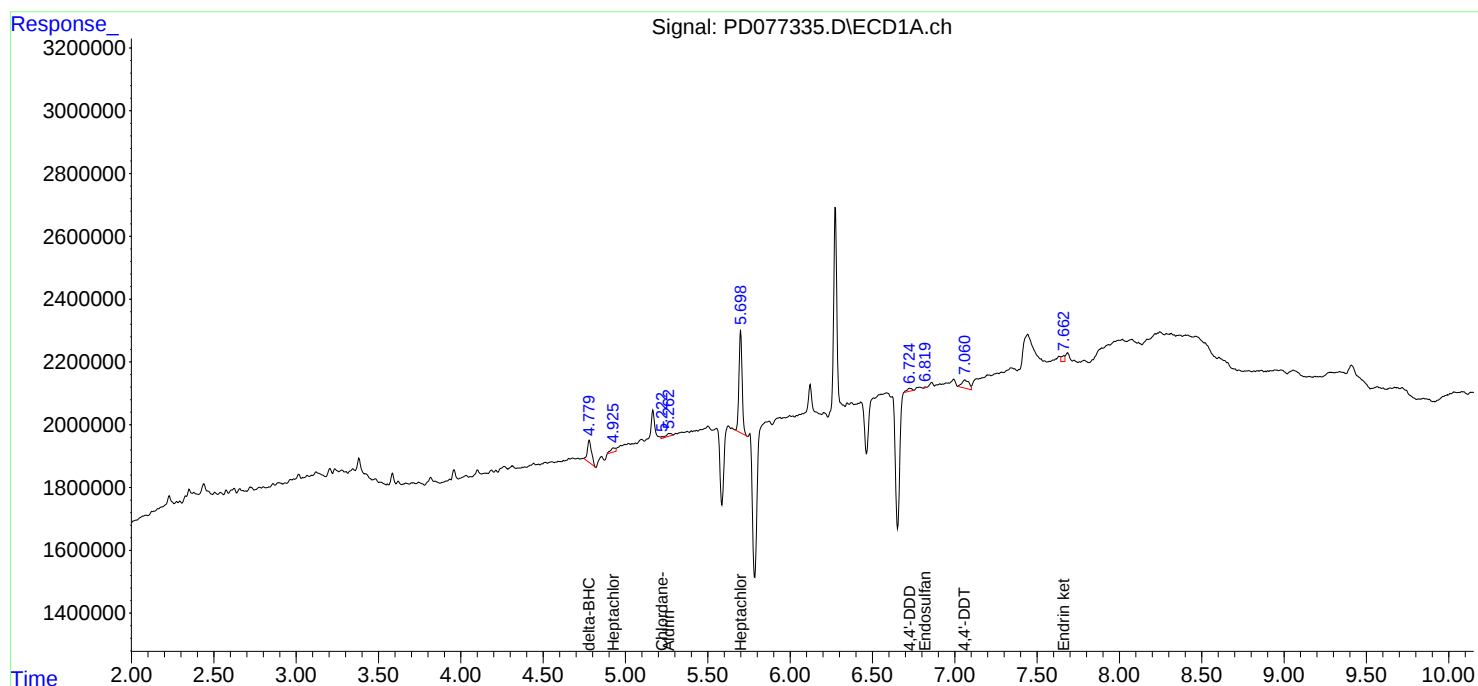


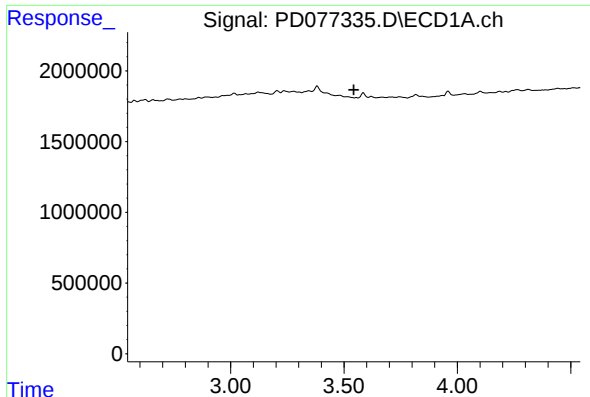

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.543 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

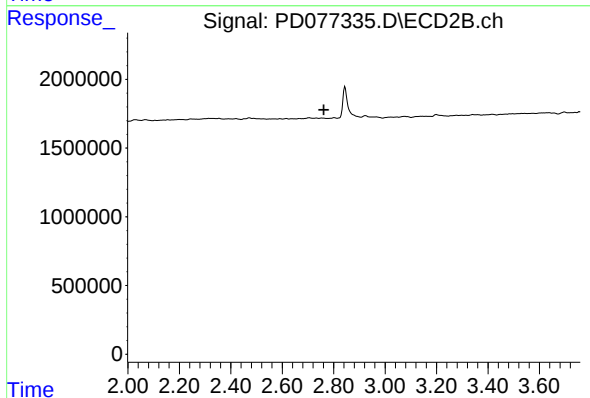


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.762 min
Response: 0
Conc: N.D.

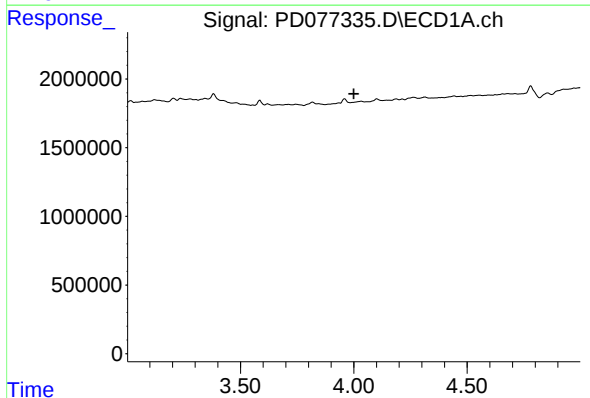


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 4.000 min
Response: 0
Conc: N.D.

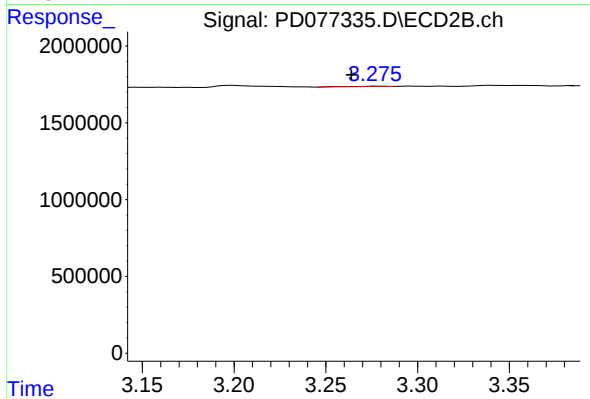

#2 alpha-BHC


R.T.: 3.278 min
Delta R.T.: 0.014 min
Response: 40465
Conc: 0.02 ng/ml

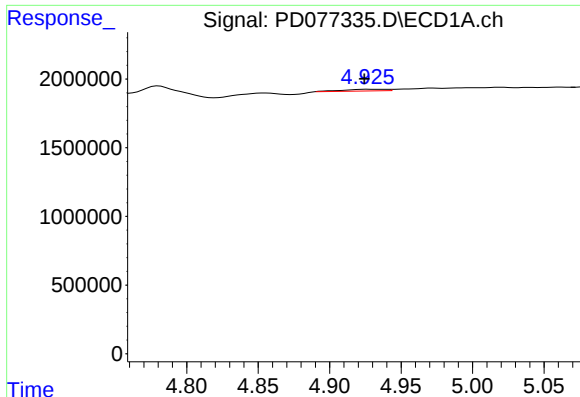

#4 Heptachlor


R.T.: 4.926 min
Delta R.T.: 0.002 min
Response: 266843
Conc: 0.07 ng/ml

Instrument :
ECD_D
ClientSampleId :

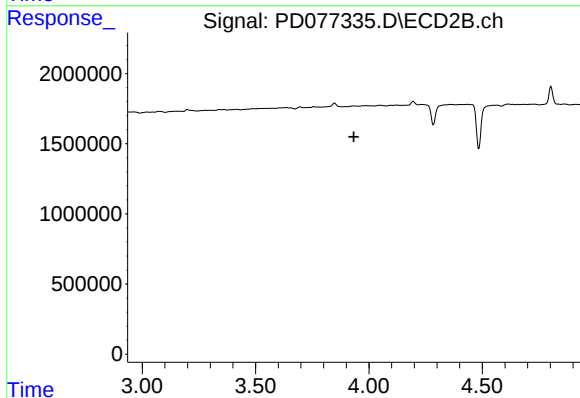


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 3.933 min
Response: 0
Conc: N.D.

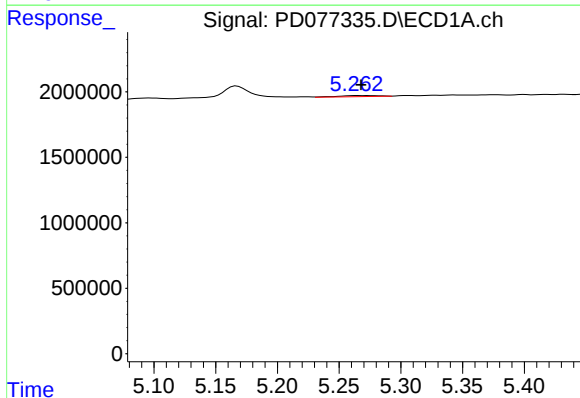


#5 Aldrin

R.T.: 5.265 min
Delta R.T.: -0.003 min
Response: 190082
Conc: 0.05 ng/ml

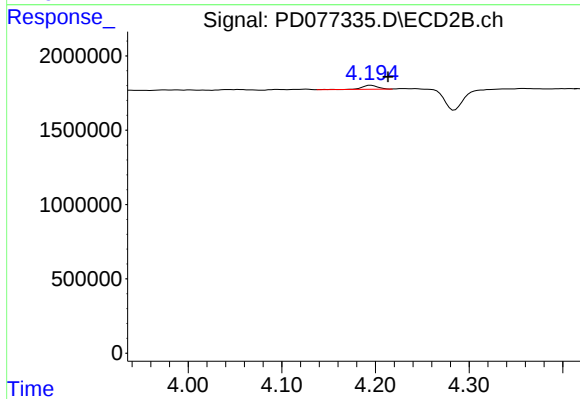

#5 Aldrin


R.T.: 4.195 min
Delta R.T.: -0.018 min
Response: 298040
Conc: 0.16 ng/ml

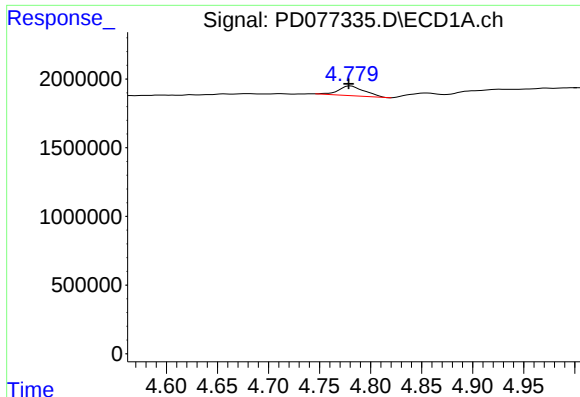

#7 delta-BHC


R.T.: 4.780 min
Delta R.T.: 0.002 min
Response: 1249048
Conc: 0.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

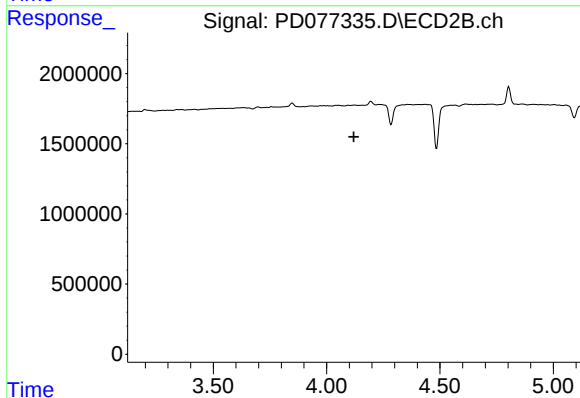


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.120 min
Response: 0
Conc: N.D.

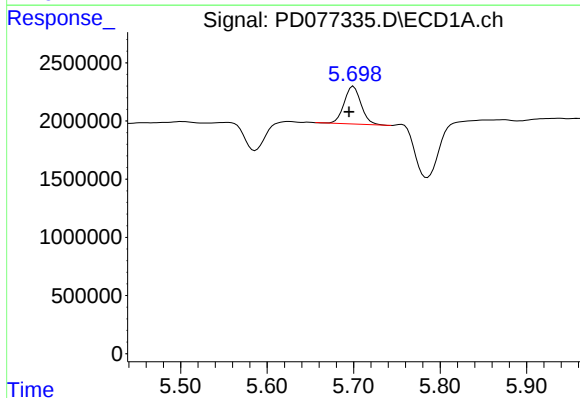


#8 Heptachlor epoxide

R.T.: 5.700 min
Delta R.T.: 0.005 min
Response: 4382220
Conc: 1.32 ng/ml

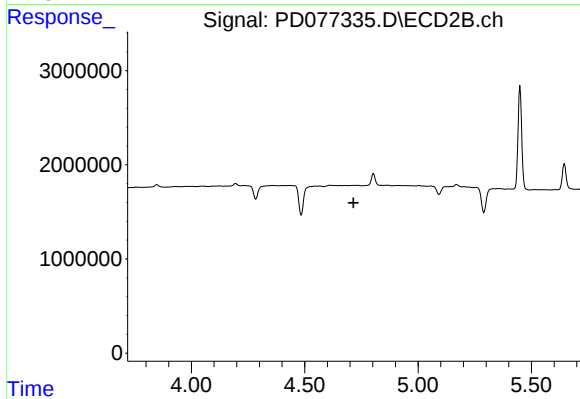

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.716 min
Response: 0
Conc: N.D.

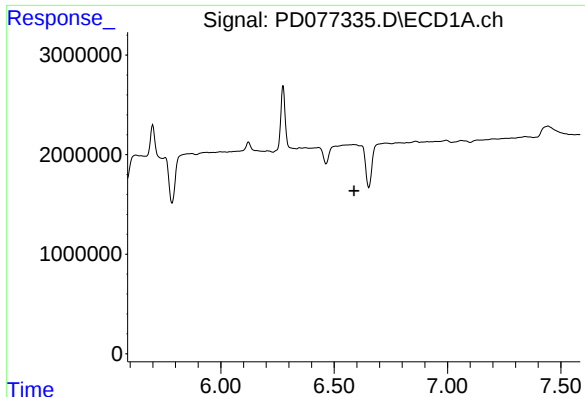

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.588 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

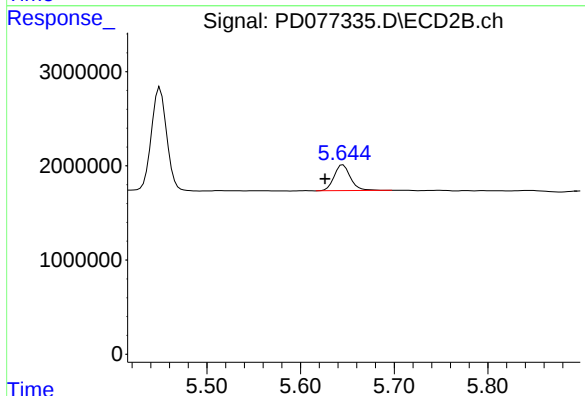


#14 Endrin

R.T.: 5.645 min
Delta R.T.: 0.019 min
Response: 3344354
Conc: 2.29 ng/ml

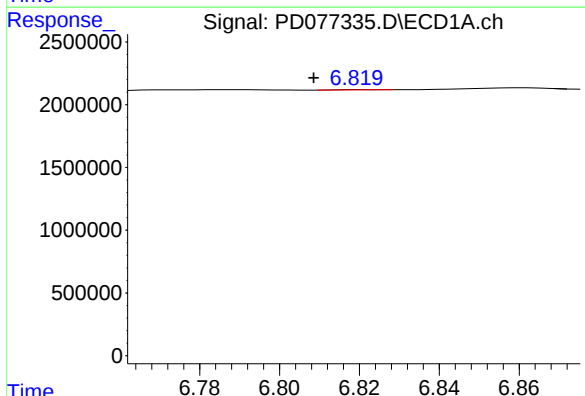


#15 Endosulfan II

R.T.: 6.821 min
Delta R.T.: 0.012 min
Response: 14941
Conc: 0.00 ng/ml

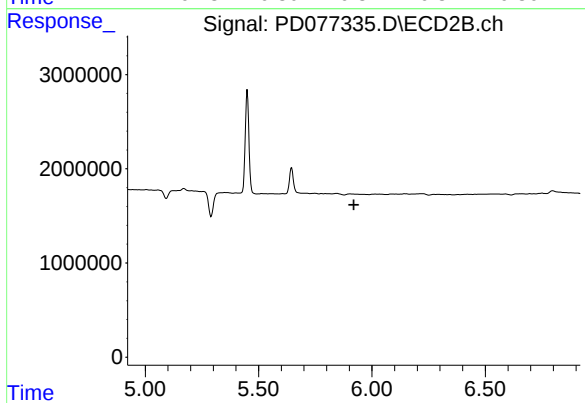

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.920 min
Response: 0
Conc: N.D.

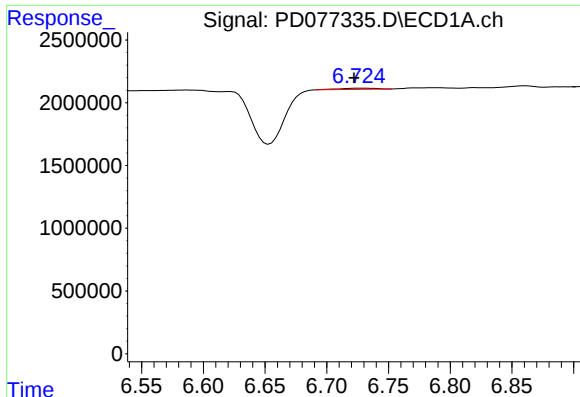

#16 4,4'-DDD


R.T.: 6.725 min
Delta R.T.: 0.003 min
Response: 195748
Conc: 0.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

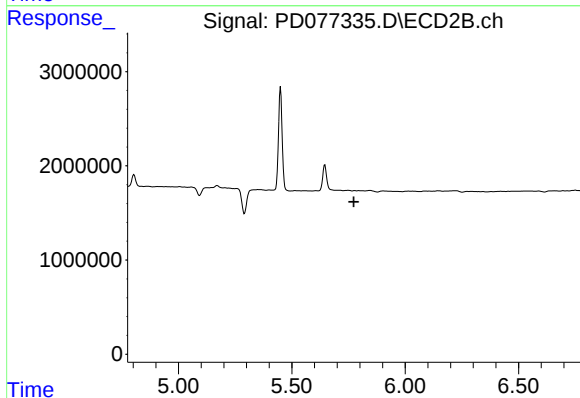


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.773 min
Response: 0
Conc: N.D.

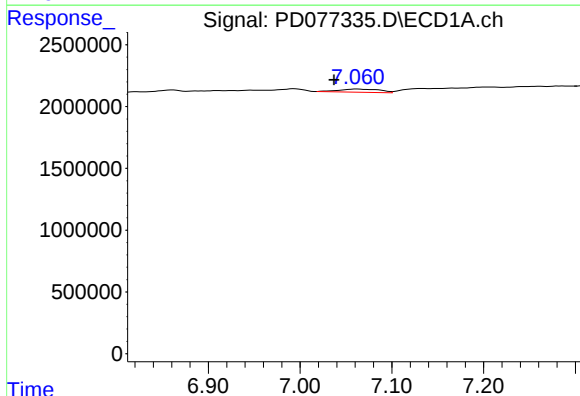


#17 4,4'-DDT

R.T.: 7.062 min
Delta R.T.: 0.025 min
Response: 791904
Conc: 0.33 ng/ml

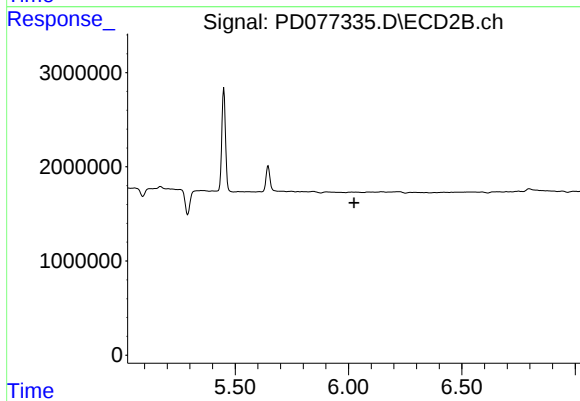

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.025 min
Response: 0
Conc: N.D.

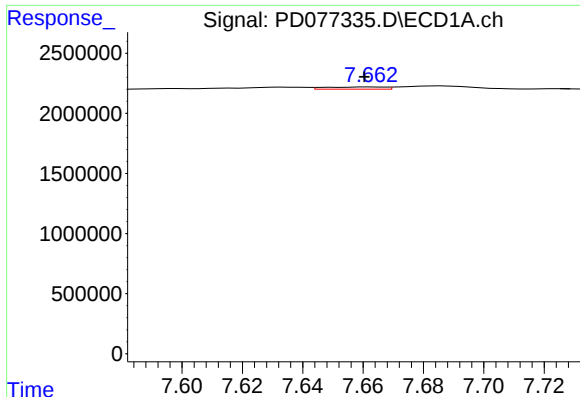

#21 Endrin ketone


R.T.: 7.663 min
Delta R.T.: 0.003 min
Response: 253275
Conc: 0.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

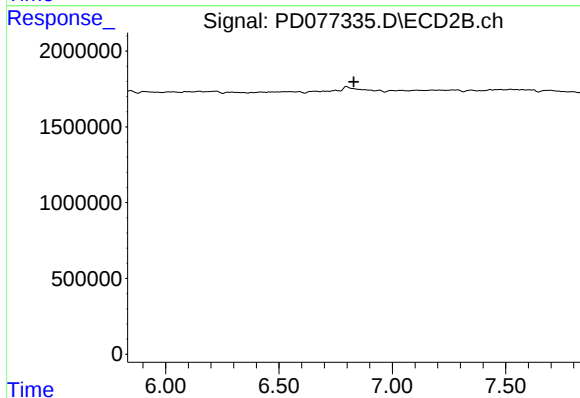


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.830 min
Response: 0
Conc: N.D.

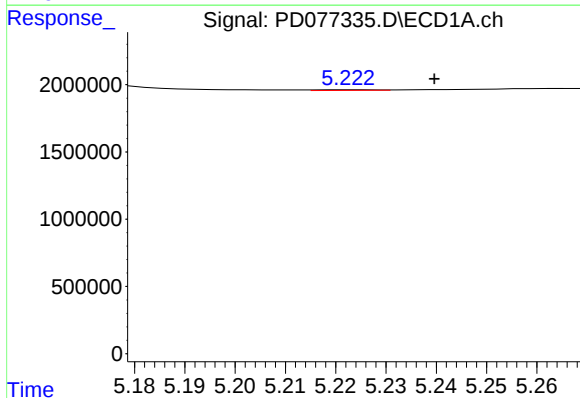


#24 Chlordane-2

R.T.: 5.224 min
Delta R.T.: -0.016 min
Response: 44478
Conc: 0.37 ng/ml

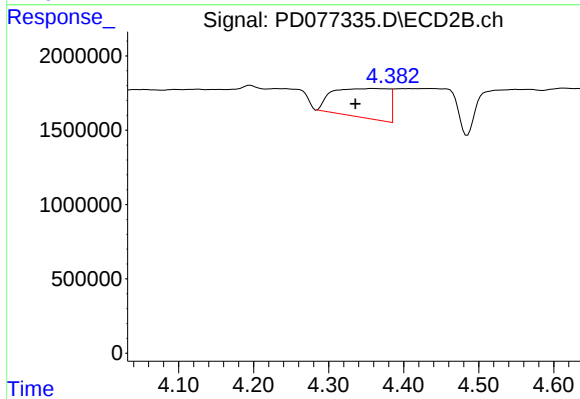

#24 Chlordane-2


R.T.: 4.358 min
Delta R.T.: 0.023 min
Response: 10073800
Conc: 179.14 ng/ml

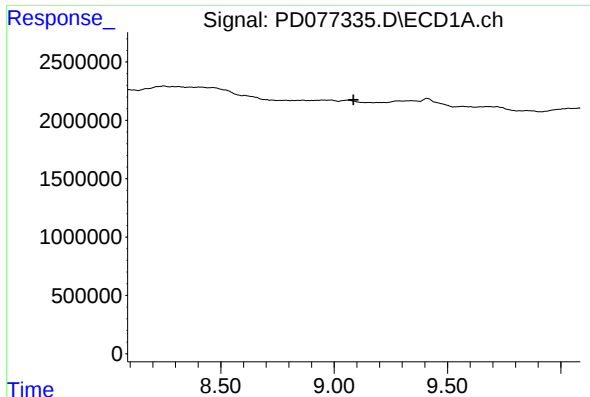

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.086 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

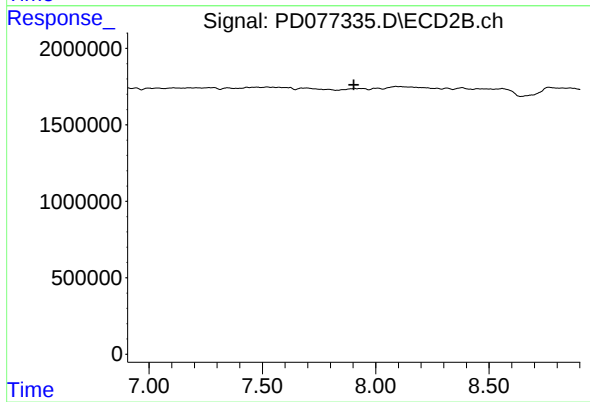

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.904 min
Response: 0
Conc: N.D.