

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082323\
 Data File : PD077336.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2023 08:27
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 22:44:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.761	54437610	31229540	23.004	22.927
28)	SA Decachlor...	9.087	7.902	62988851	30691812	22.987	21.446
Target Compounds							
4)	MA Heptachlor	4.912	0.000	374205	0	0.104	N.D. #
7)	B delta-BHC	4.770	0.000	2737793	0	0.785	N.D. #
8)	B Heptachlo...	5.691	0.000	2663030	0	0.804	N.D. #
9)	A Endosulfan I	6.082	0.000	63460	0	0.021	N.D. #
14)	MA Endrin	0.000	5.642f	0	1364802	N.D.	0.933 #
15)	B Endosulfa...	6.784f	0.000	867684	0	0.273	N.D. #
21)	B Endrin ke...	7.689f	0.000	1383099	0	0.459	N.D. #
22)	Mirex	8.160f	0.000	813500	0	0.357	N.D. #
24)	Chlordane-2	0.000	4.354f	0	1060170	N.D.	18.852 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082323\
Data File : PD077336.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2023 08:27
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 22:44:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

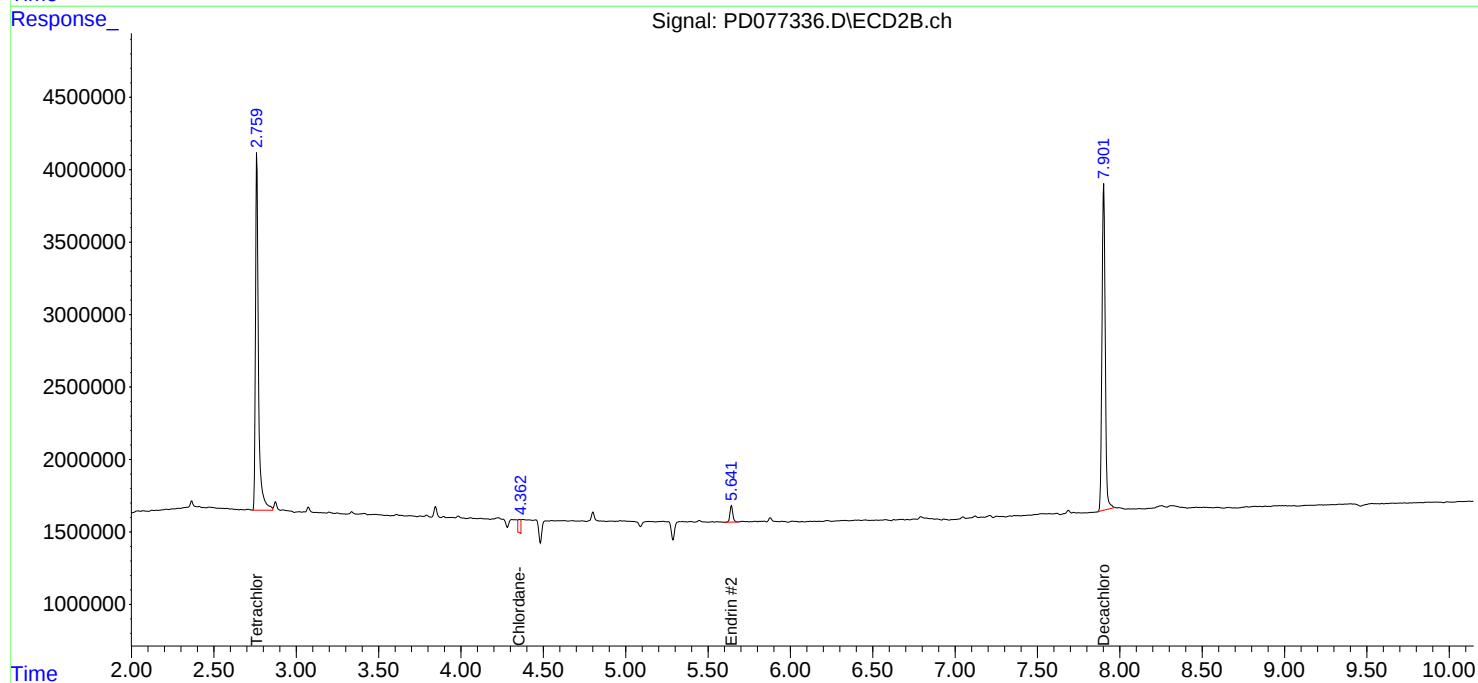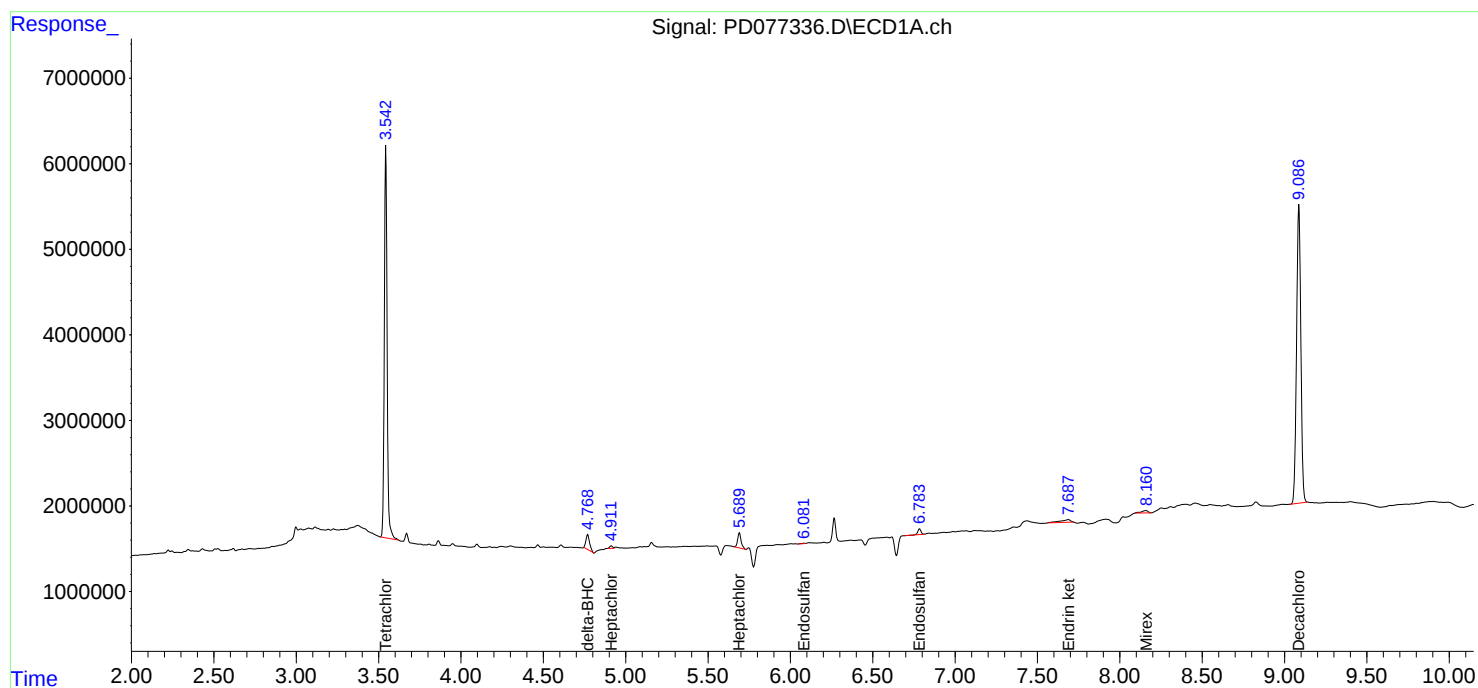


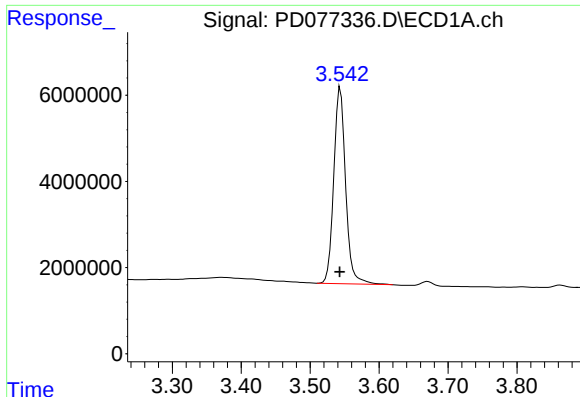

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 54437610
Conc: 23.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

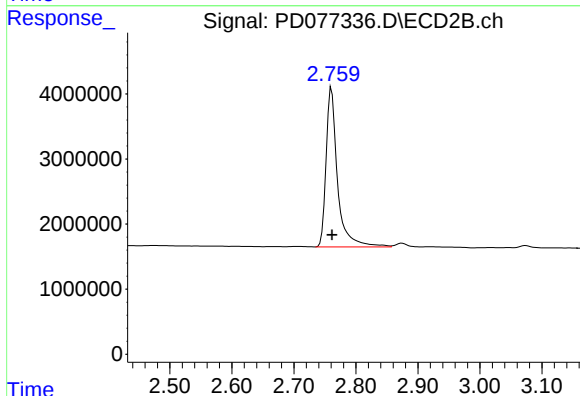


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 31229540
Conc: 22.93 ng/ml

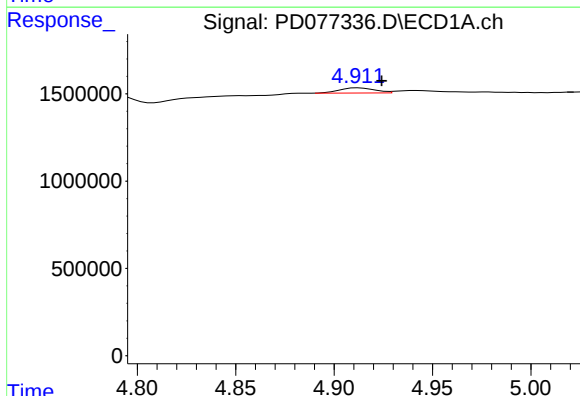


#4 Heptachlor

R.T.: 4.912 min
Delta R.T.: -0.012 min
Response: 374205
Conc: 0.10 ng/ml

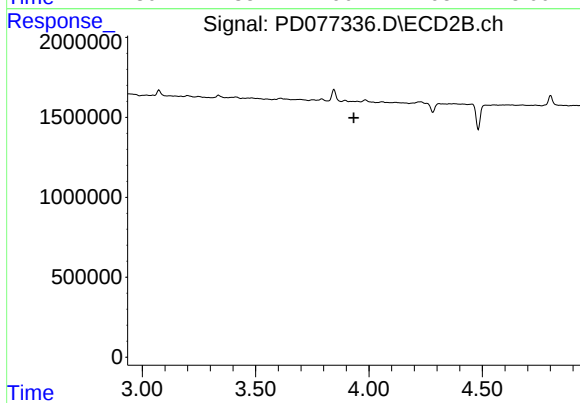

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 3.933 min
Response: 0
Conc: N.D.

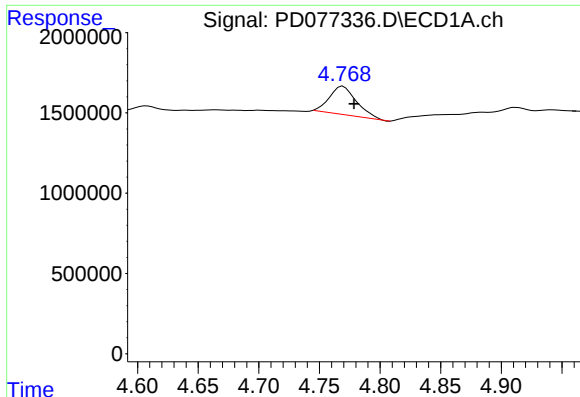

#7 delta-BHC


R.T.: 4.770 min
Delta R.T.: -0.009 min
Response: 2737793
Conc: 0.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

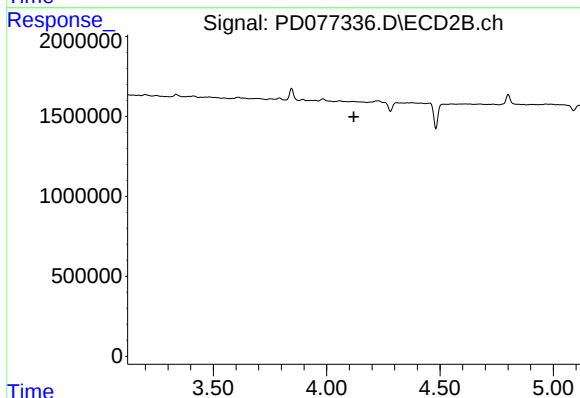


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.120 min
Response: 0
Conc: N.D.

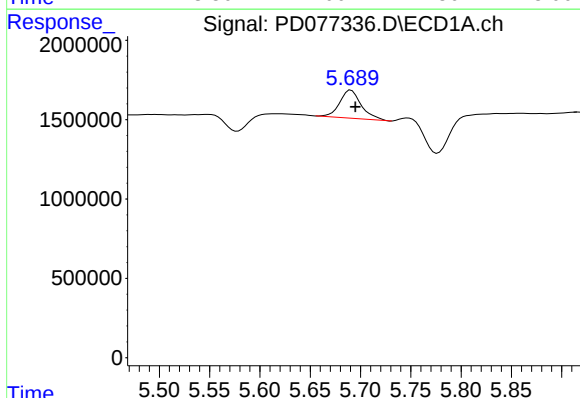


#8 Heptachlor epoxide

R.T.: 5.691 min
Delta R.T.: -0.004 min
Response: 2663030
Conc: 0.80 ng/ml

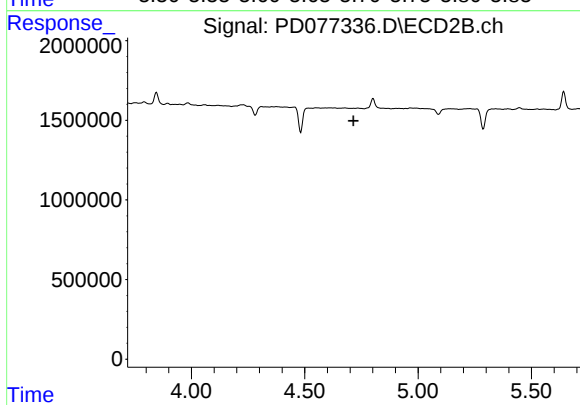

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.716 min
Response: 0
Conc: N.D.

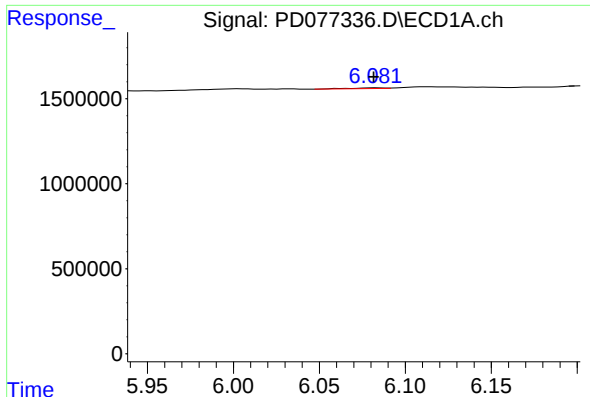

#9 Endosulfan I


R.T.: 6.082 min
Delta R.T.: 0.000 min
Response: 63460
Conc: 0.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

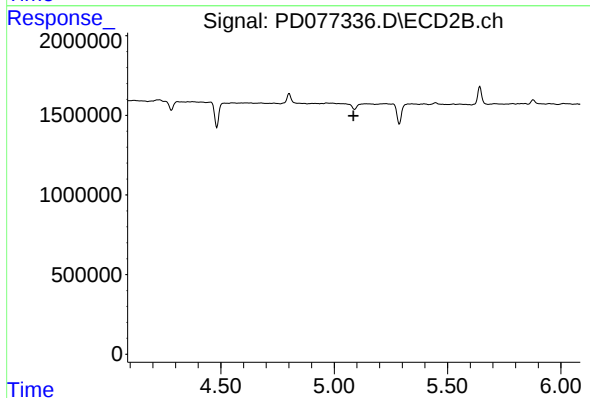


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.086 min
Response: 0
Conc: N.D.

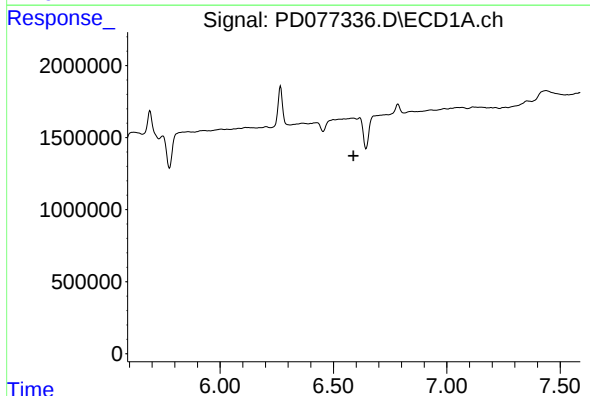


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.588 min
Response: 0
Conc: N.D.

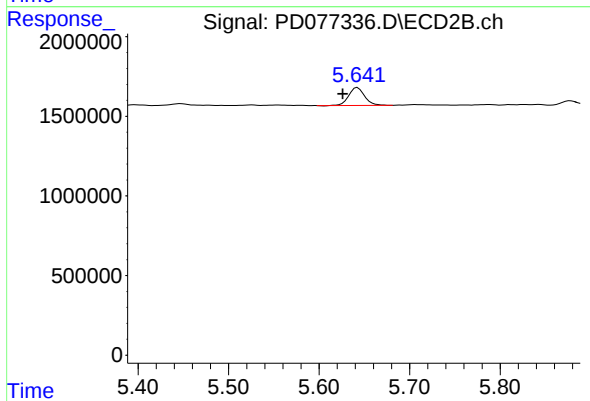

#14 Endrin


R.T.: 5.642 min
Delta R.T.: 0.016 min
Response: 1364802
Conc: 0.93 ng/ml

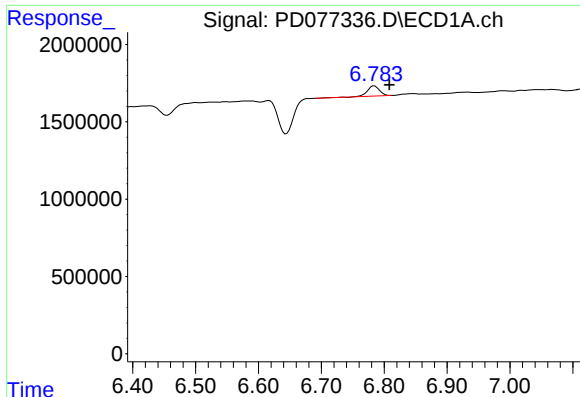

#15 Endosulfan II


R.T.: 6.784 min
Delta R.T.: -0.024 min
Response: 867684
Conc: 0.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

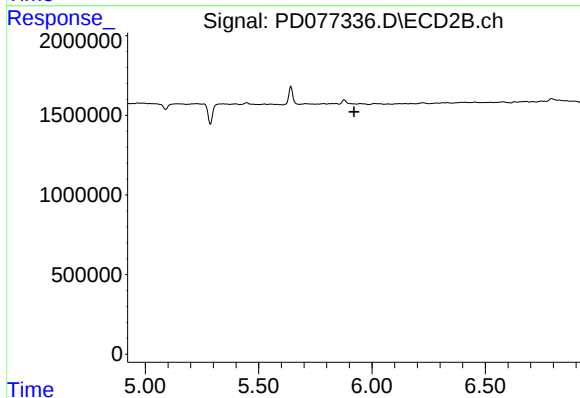


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.920 min
Response: 0
Conc: N.D.

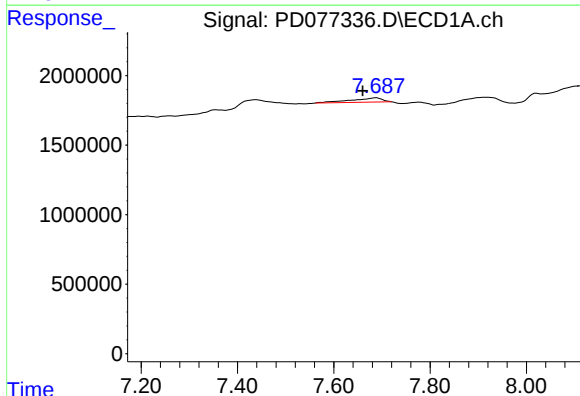


#21 Endrin ketone

R.T.: 7.689 min
Delta R.T.: 0.028 min
Response: 1383099
Conc: 0.46 ng/ml

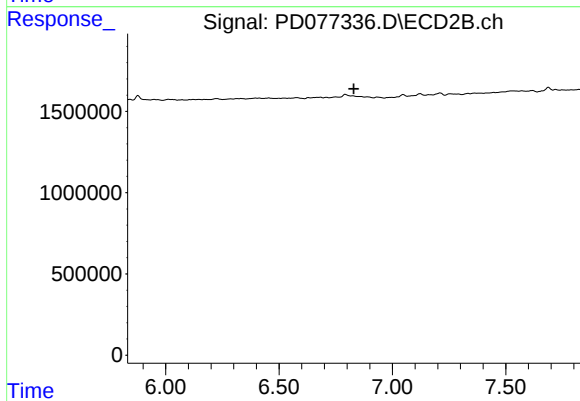

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.830 min
Response: 0
Conc: N.D.

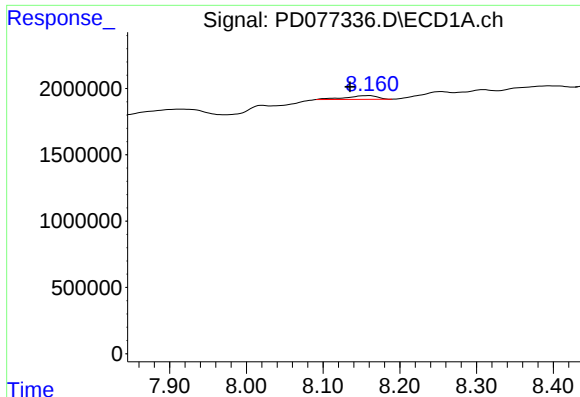

#22 Mirex


R.T.: 8.160 min
Delta R.T.: 0.025 min
Response: 813500
Conc: 0.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

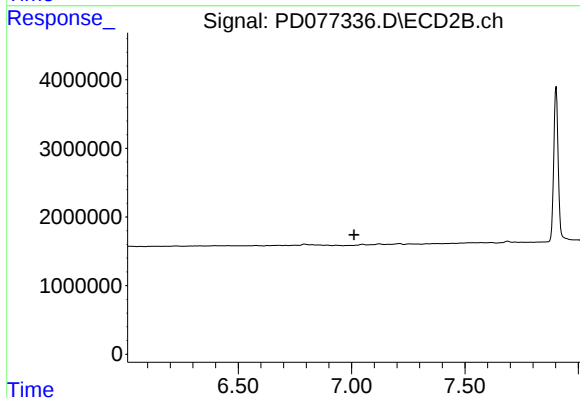


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.011 min
Response: 0
Conc: N.D.

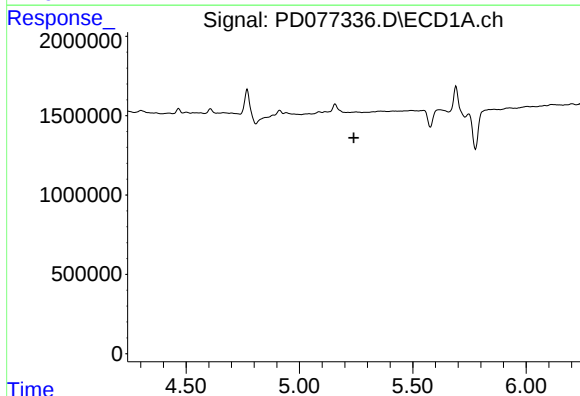


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.240 min
Response: 0
Conc: N.D.

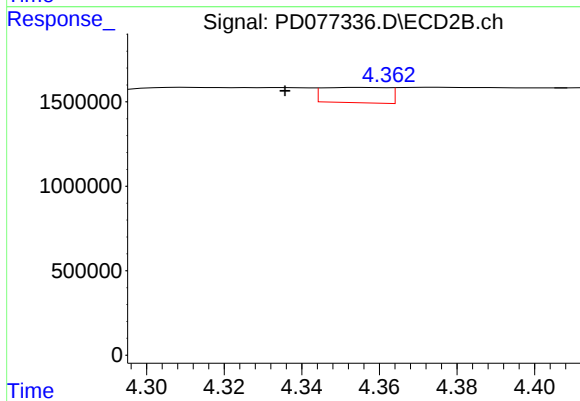

#24 Chlordane-2


R.T.: 4.354 min
Delta R.T.: 0.018 min
Response: 1060170
Conc: 18.85 ng/ml

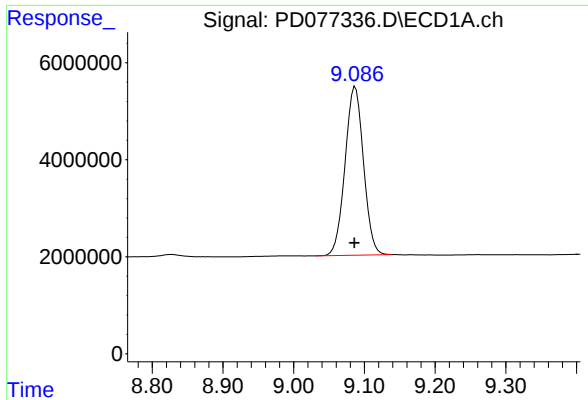

#28 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: 0.002 min
Response: 62988851
Conc: 22.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

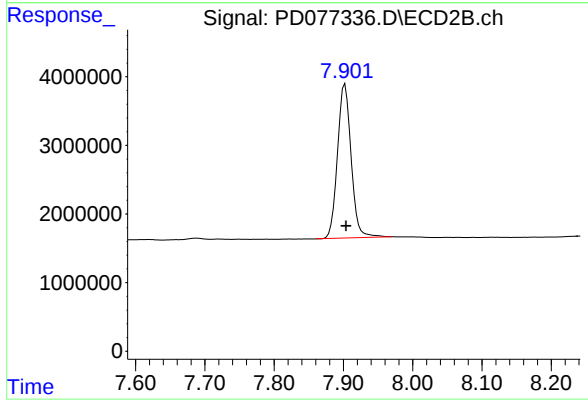

#28 Decachlorobiphenyl

R.T.: 7.902 min
Delta R.T.: -0.002 min
Response: 30691812
Conc: 21.45 ng/ml