

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082323\
 Data File : PD077357.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2023 17:30
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 22:50:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.762	53907428	31847218	22.780	23.381
28)	SA Decachlor...	9.085	7.902	62733767	32031372	22.894	22.383
Target Compounds							
4)	MA Heptachlor	4.912	0.000	363947	0	0.101	N.D. #
7)	B delta-BHC	4.769	0.000	2316797	0	0.664	N.D. #
8)	B Heptachlo...	5.689	0.000	3450273	0	1.042	N.D. #
9)	A Endosulfan I	6.111f	0.000	302106	0	0.099	N.D. #
14)	MA Endrin	0.000	5.643f	0	1929841	N.D.	1.319 #
15)	B Endosulfa...	6.782f	0.000	966585	0	0.304	N.D. #
21)	B Endrin ke...	7.690f	0.000	245990	0	0.082	N.D. #
22)	Mirex	8.152f	0.000	354067	0	0.155	N.D. #
24)	Chlordane-2	0.000	4.334	0	681230	N.D.	12.114 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082323\
Data File : PD077357.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2023 17:30
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 22:50:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

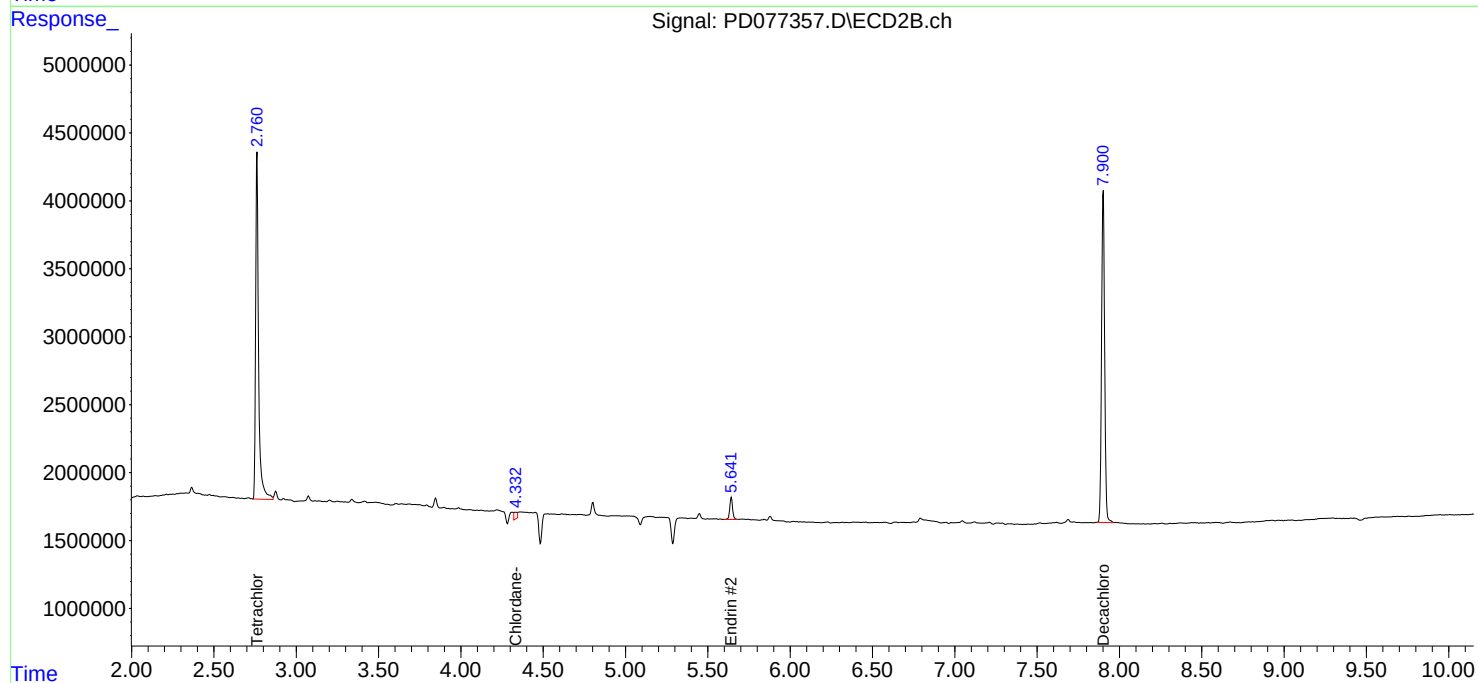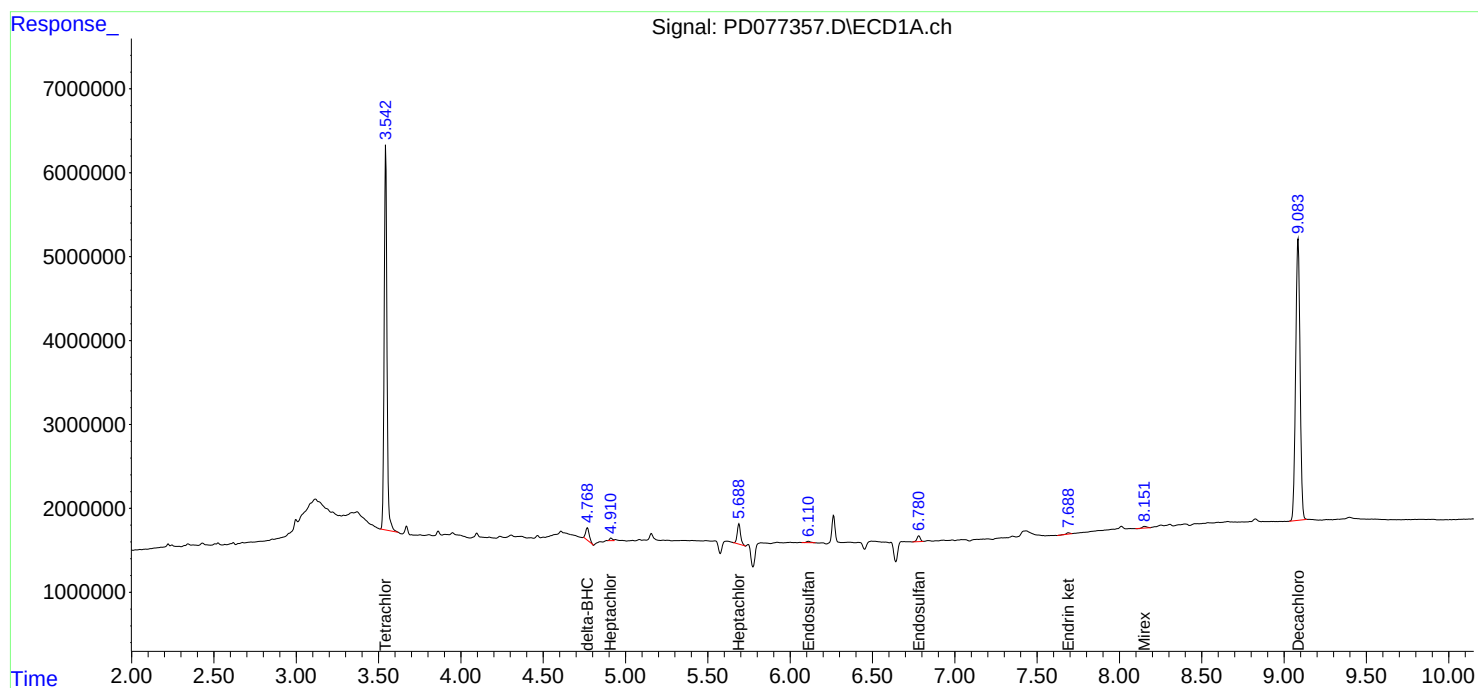


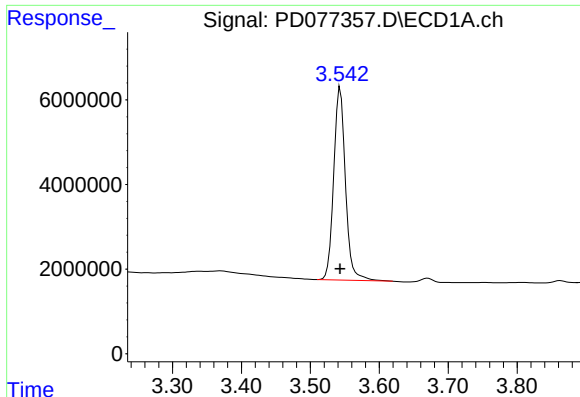

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 53907428
Conc: 22.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

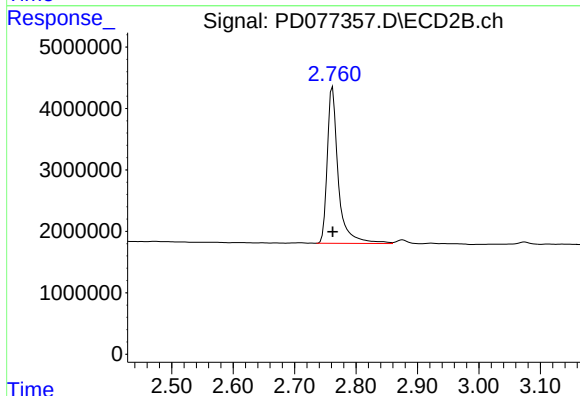


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 31847218
Conc: 23.38 ng/ml

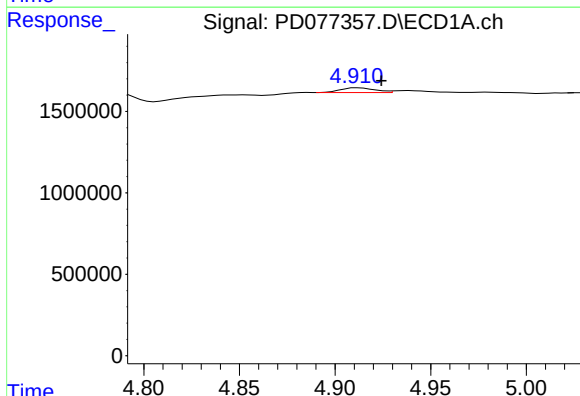


#4 Heptachlor

R.T.: 4.912 min
Delta R.T.: -0.012 min
Response: 363947
Conc: 0.10 ng/ml

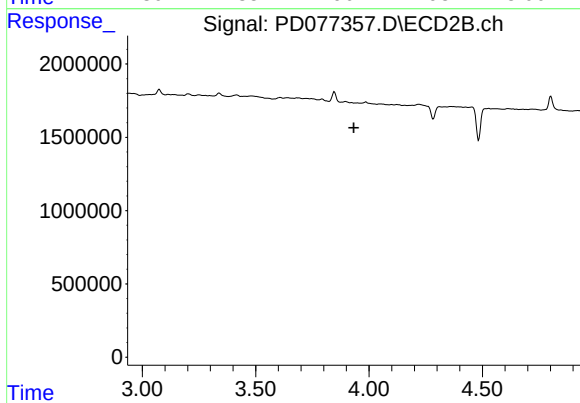

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 3.933 min
Response: 0
Conc: N.D.

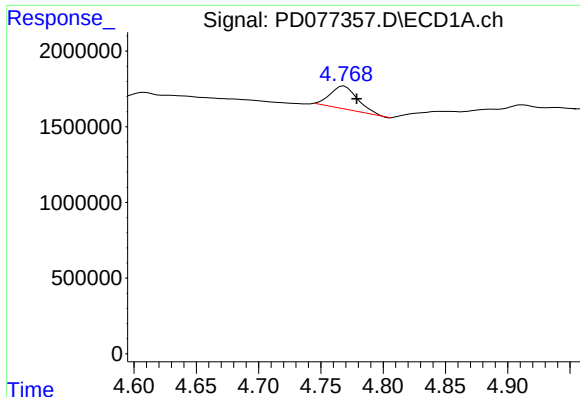

#7 delta-BHC


R.T.: 4.769 min
Delta R.T.: -0.010 min
Response: 2316797
Conc: 0.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

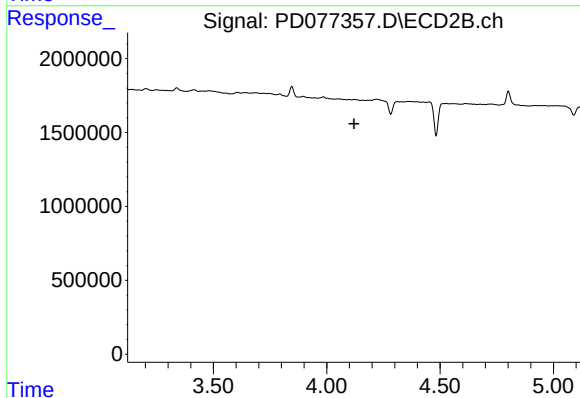


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.120 min
Response: 0
Conc: N.D.

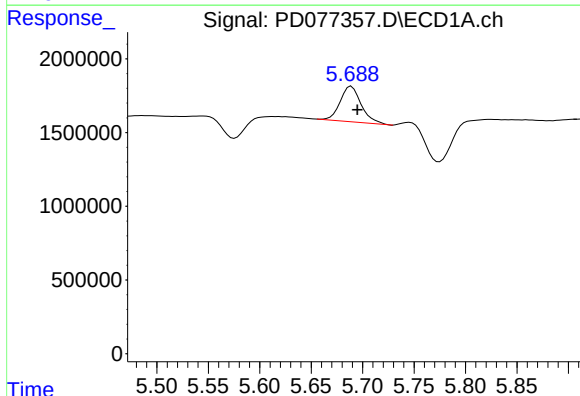


#8 Heptachlor epoxide

R.T.: 5.689 min
Delta R.T.: -0.006 min
Response: 3450273
Conc: 1.04 ng/ml

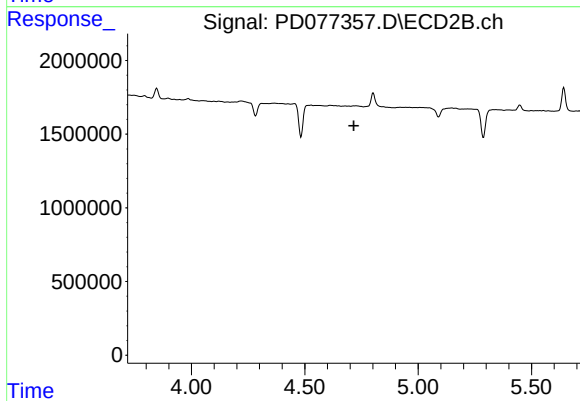

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.716 min
Response: 0
Conc: N.D.

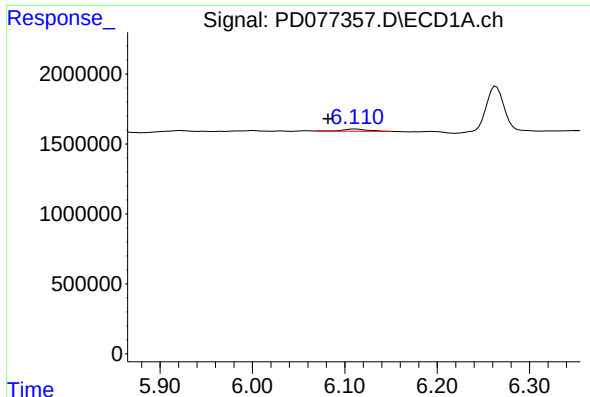

#9 Endosulfan I


R.T.: 6.111 min
Delta R.T.: 0.030 min
Response: 302106
Conc: 0.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

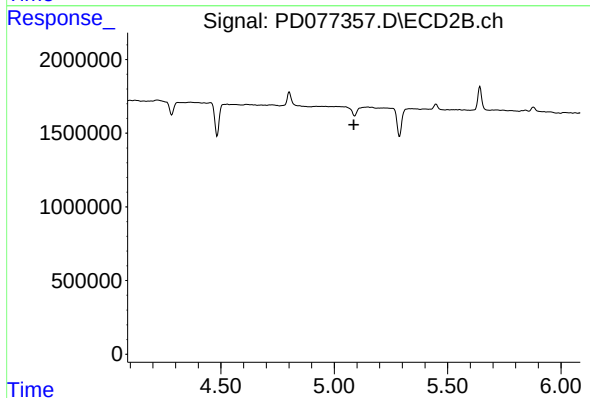


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.086 min
Response: 0
Conc: N.D.

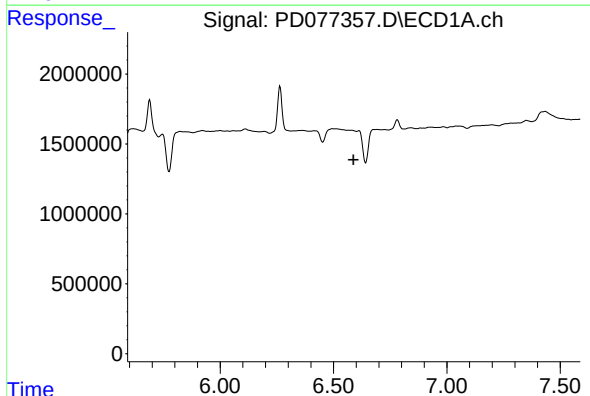


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.588 min
Response: 0
Conc: N.D.

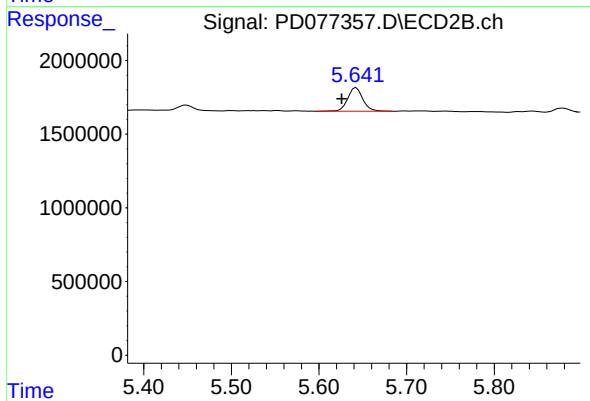

#14 Endrin


R.T.: 5.643 min
Delta R.T.: 0.016 min
Response: 1929841
Conc: 1.32 ng/ml

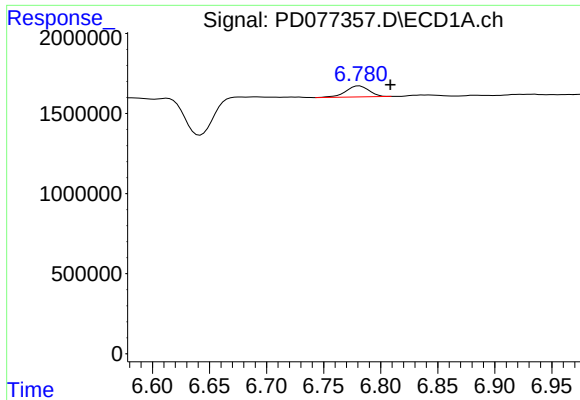

#15 Endosulfan II


R.T.: 6.782 min
Delta R.T.: -0.027 min
Response: 966585
Conc: 0.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

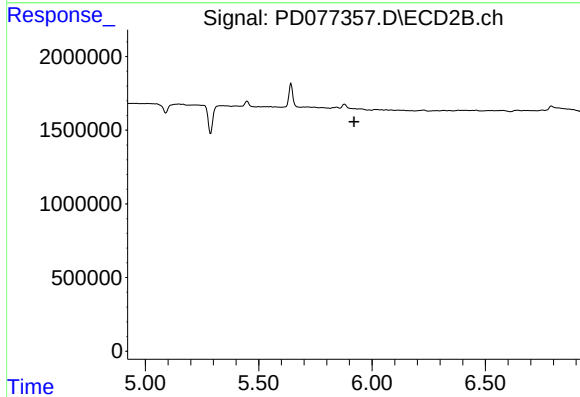


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.920 min
Response: 0
Conc: N.D.

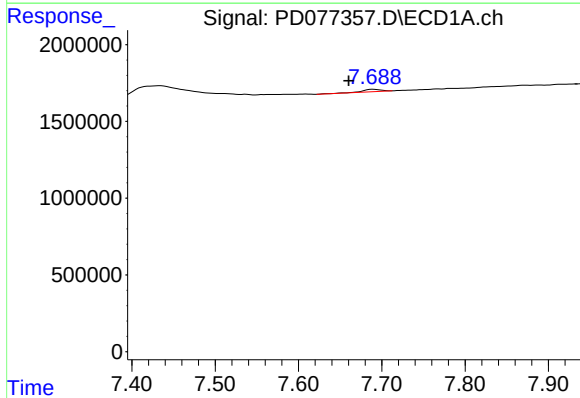


#21 Endrin ketone

R.T.: 7.690 min
Delta R.T.: 0.030 min
Response: 245990
Conc: 0.08 ng/ml

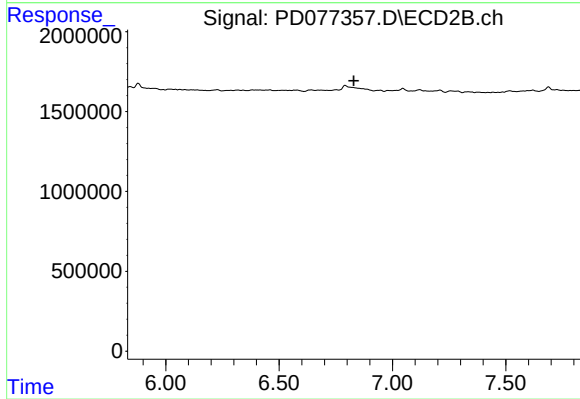

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.830 min
Response: 0
Conc: N.D.

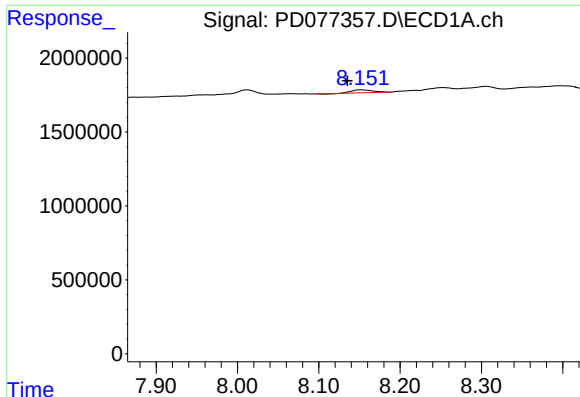

#22 Mirex


R.T.: 8.152 min
Delta R.T.: 0.017 min
Response: 354067
Conc: 0.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

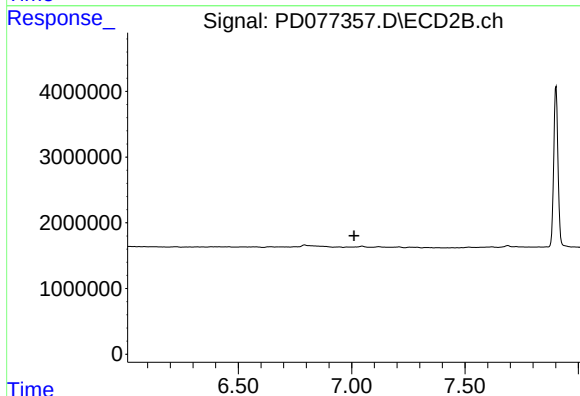


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.011 min
Response: 0
Conc: N.D.

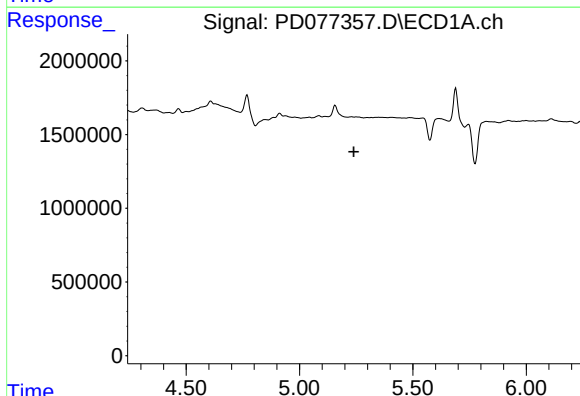


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.240 min
Response: 0
Conc: N.D.

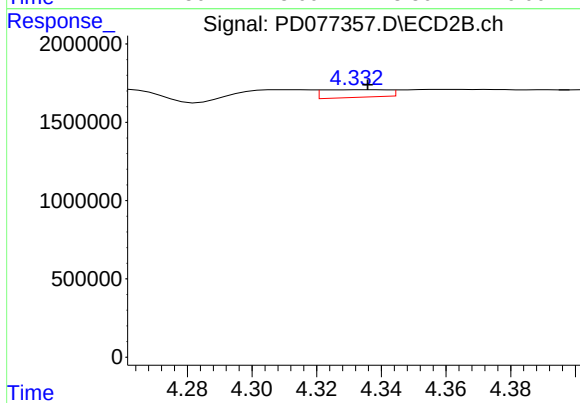

#24 Chlordane-2


R.T.: 4.334 min
Delta R.T.: -0.002 min
Response: 681230
Conc: 12.11 ng/ml

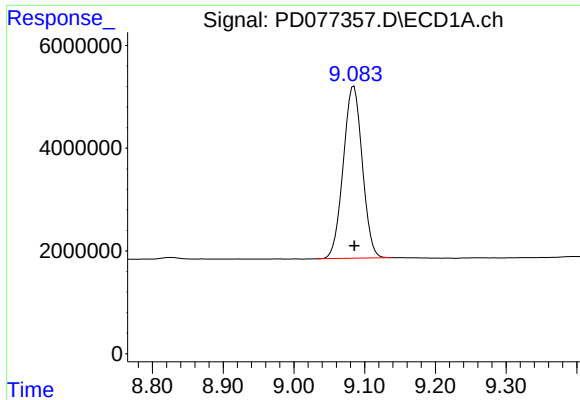

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 62733767
Conc: 22.89 ng/ml

Instrument :
ECD_D
ClientSampleId :

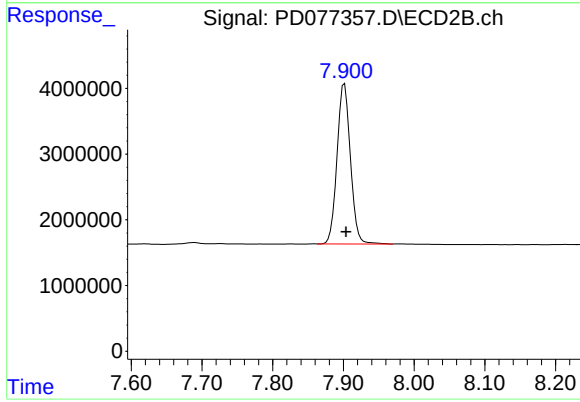

#28 Decachlorobiphenyl

R.T.: 7.902 min
Delta R.T.: -0.002 min
Response: 32031372
Conc: 22.38 ng/ml