

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082323\
 Data File : PD077344.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2023 12:44
 Operator : AR\AJ
 Sample : 04116-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 22:46:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.543	2.762	22246450	13870959	9.401	10.183
28) SA Decachlor...	9.083	7.901	25217046	11217708	9.203	7.839
Target Compounds						
12) B 4,4'-DDE	6.202	5.217	3599640	1826019	1.213	1.259



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082323\
Data File : PD077344.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2023 12:44
Operator : AR\AJ
Sample : 04116-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 22:46:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

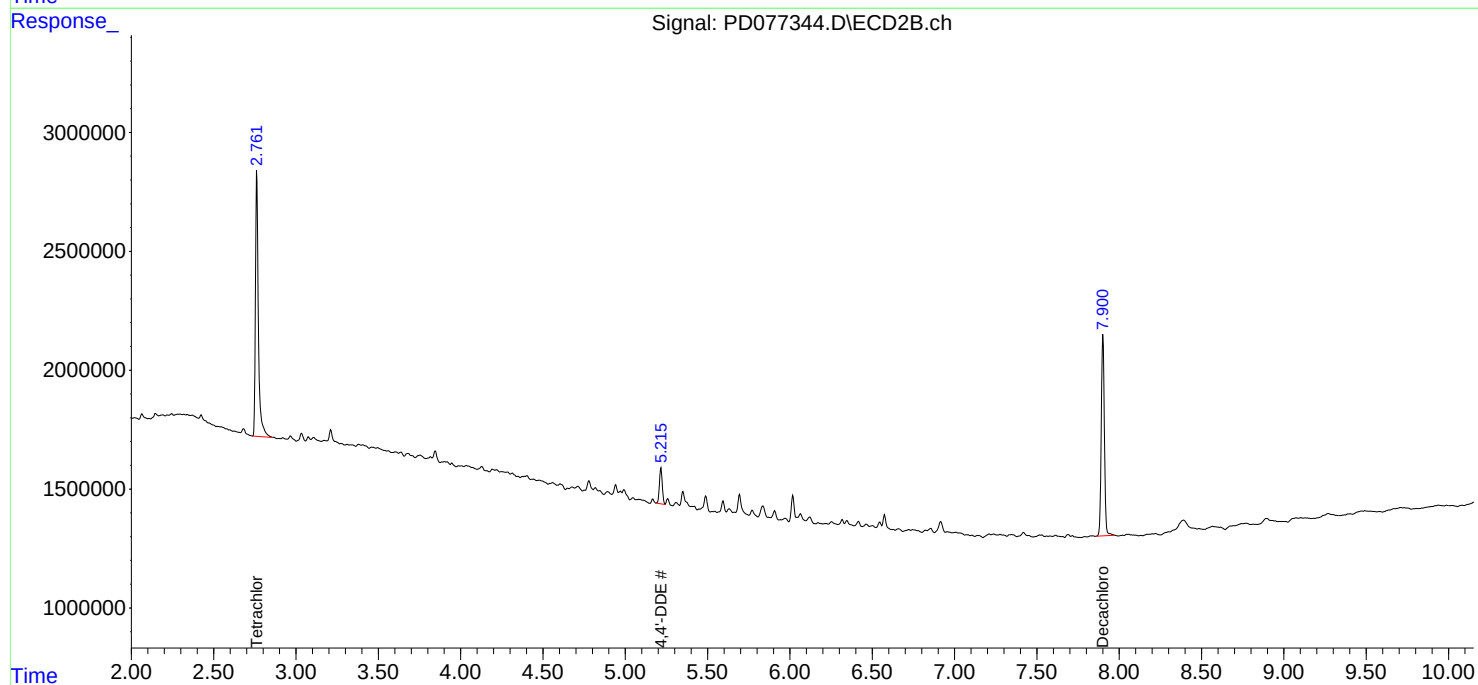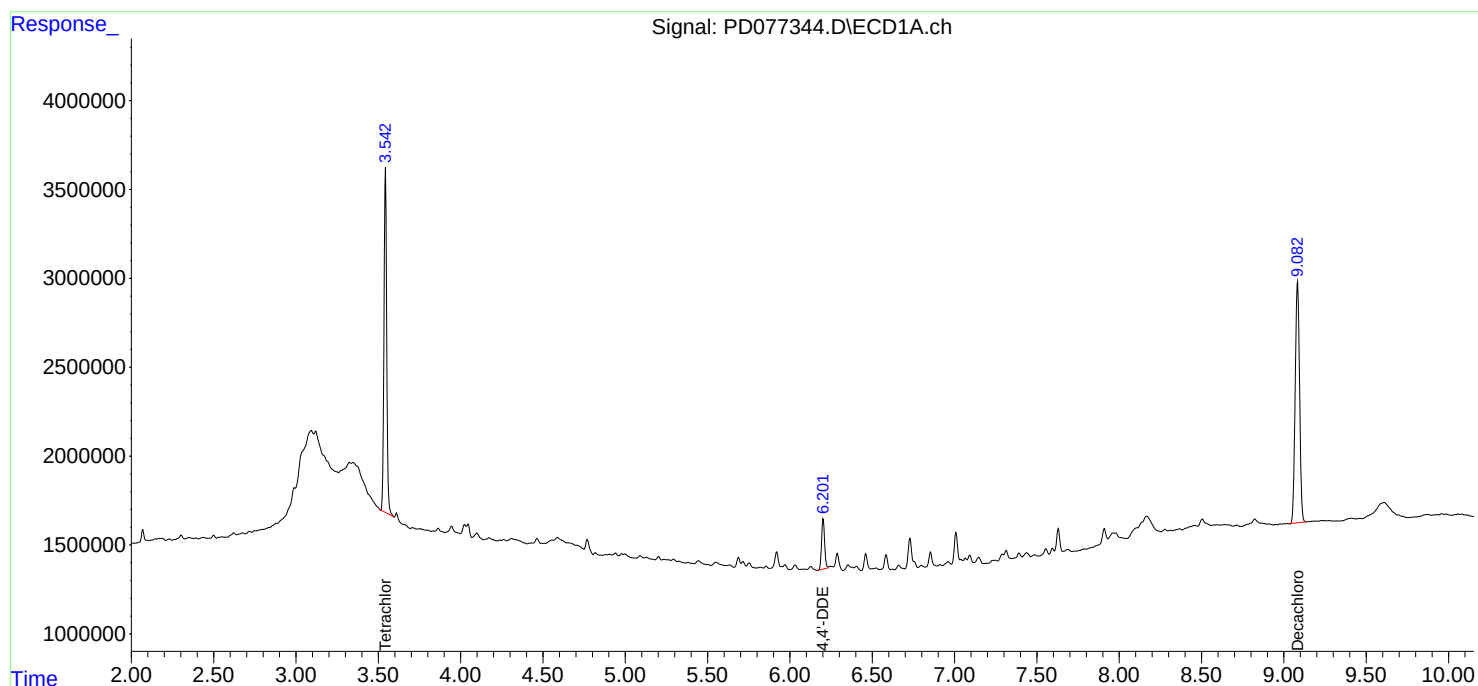


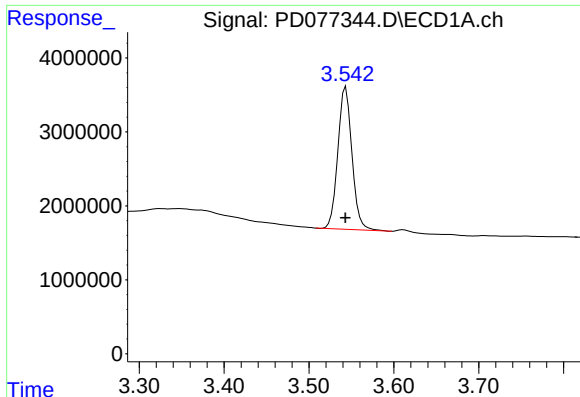

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 22246450
Conc: 9.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-3

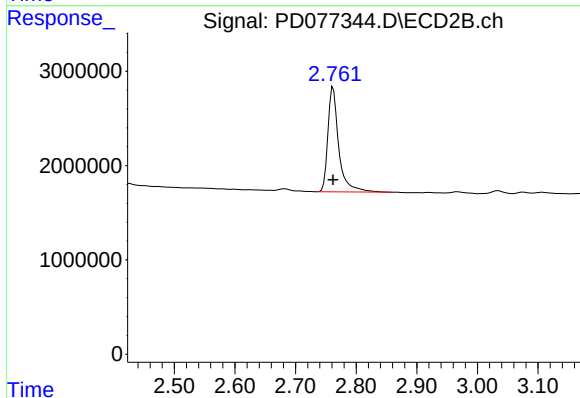


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 13870959
Conc: 10.18 ng/ml

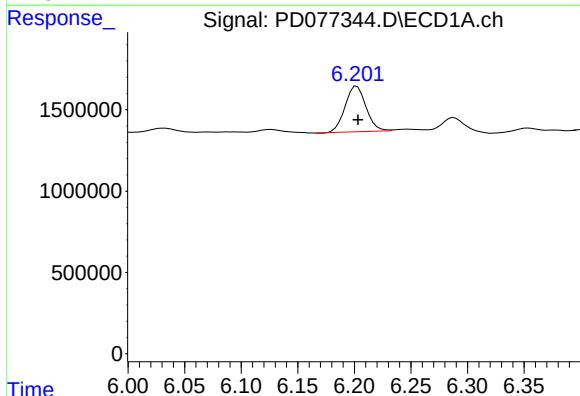


#12 4,4'-DDE

R.T.: 6.202 min
Delta R.T.: -0.001 min
Response: 3599640
Conc: 1.21 ng/ml

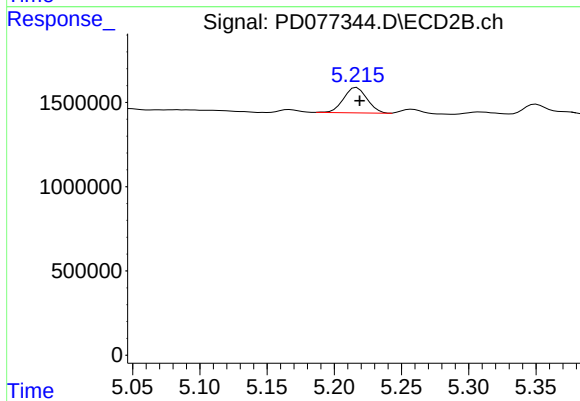

#12 4,4'-DDE


R.T.: 5.217 min
Delta R.T.: -0.002 min
Response: 1826019
Conc: 1.26 ng/ml

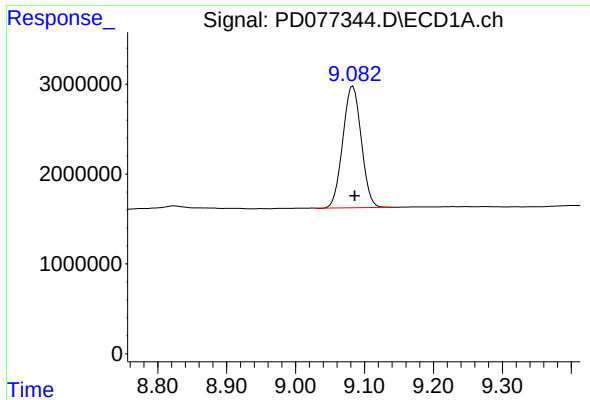

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: -0.003 min
Response: 25217046
Conc: 9.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-3

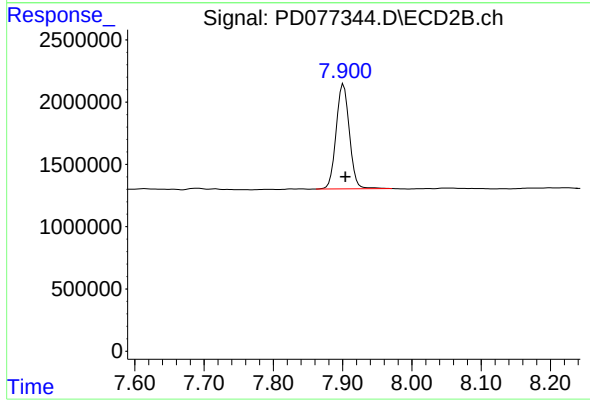

#28 Decachlorobiphenyl

R.T.: 7.901 min
Delta R.T.: -0.003 min
Response: 11217708
Conc: 7.84 ng/ml