

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082424\
 Data File : PD084624.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2024 17:13
 Operator : AR\AJ
 Sample : RESC042
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC047

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 06:24:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082424CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 23 06:21:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.907	18478981	69006311	19.359	20.443
27)	SA Decachlor...	9.034	8.110	46926014	133.5E6	38.950	40.238
Target Compounds							
2)	A alpha-BHC	3.984	3.418	15193131	52825081	8.942	10.401
3)	MA gamma-BHC...	4.313	3.753	14595916	51192951	9.075	10.653
4)	MA Heptachlor	4.910	4.108	14014850	43327195	9.266	10.328
5)	MB Aldrin	5.252	4.395	13749634	43861988	8.805	10.059
6)	B beta-BHC	4.495	4.046	6521167	20990580	9.356	9.836
7)	B delta-BHC	4.743	4.284	13784800	47073327	8.403	9.619
8)	B Heptachlo...	5.671	4.899	12479856	40640427	8.716	9.872
9)	A Endosulfan I	6.053	5.275	12732732	38753437	9.623	10.160
10)	B trans-Chl...	5.925	5.152	11784561	37646751	8.662	9.804
11)	B cis-Chlor...	6.006	5.218	12186251	38148251	8.670	9.470
12)	B 4,4'-DDE	6.174	5.403	20085208	73969133	16.244	19.255
13)	MA Dieldrin	6.325	5.542	26462583	89403671	18.398	21.194
14)	MA Endrin	6.552	5.819	20374365	78456803	18.505	21.536
15)	B Endosulfa...	6.763	6.111	22461312	70167610	17.862	19.464
16)	A 4,4'-DDD	6.682	5.959	17119538	68592082	18.099	21.440
17)	MA 4,4'-DDT	6.998	6.215	15576091	65791114	17.520	20.753
18)	B Endrin al...	6.892	6.290	14769457	52979509	17.719	19.930
19)	B Endosulfa...	7.125	6.514	19239352	68225571	17.544	19.875
20)	A Methoxychlor	7.469	6.788	49594025	180.6E6	97.027	113.281
21)	B Endrin ke...	7.605	7.025	21437485	90722349	18.399	21.479

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082424\
Data File : PD084624.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2024 17:13
Operator : AR\AJ
Sample : RESC042
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 06:24:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082424CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Aug 23 06:21:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

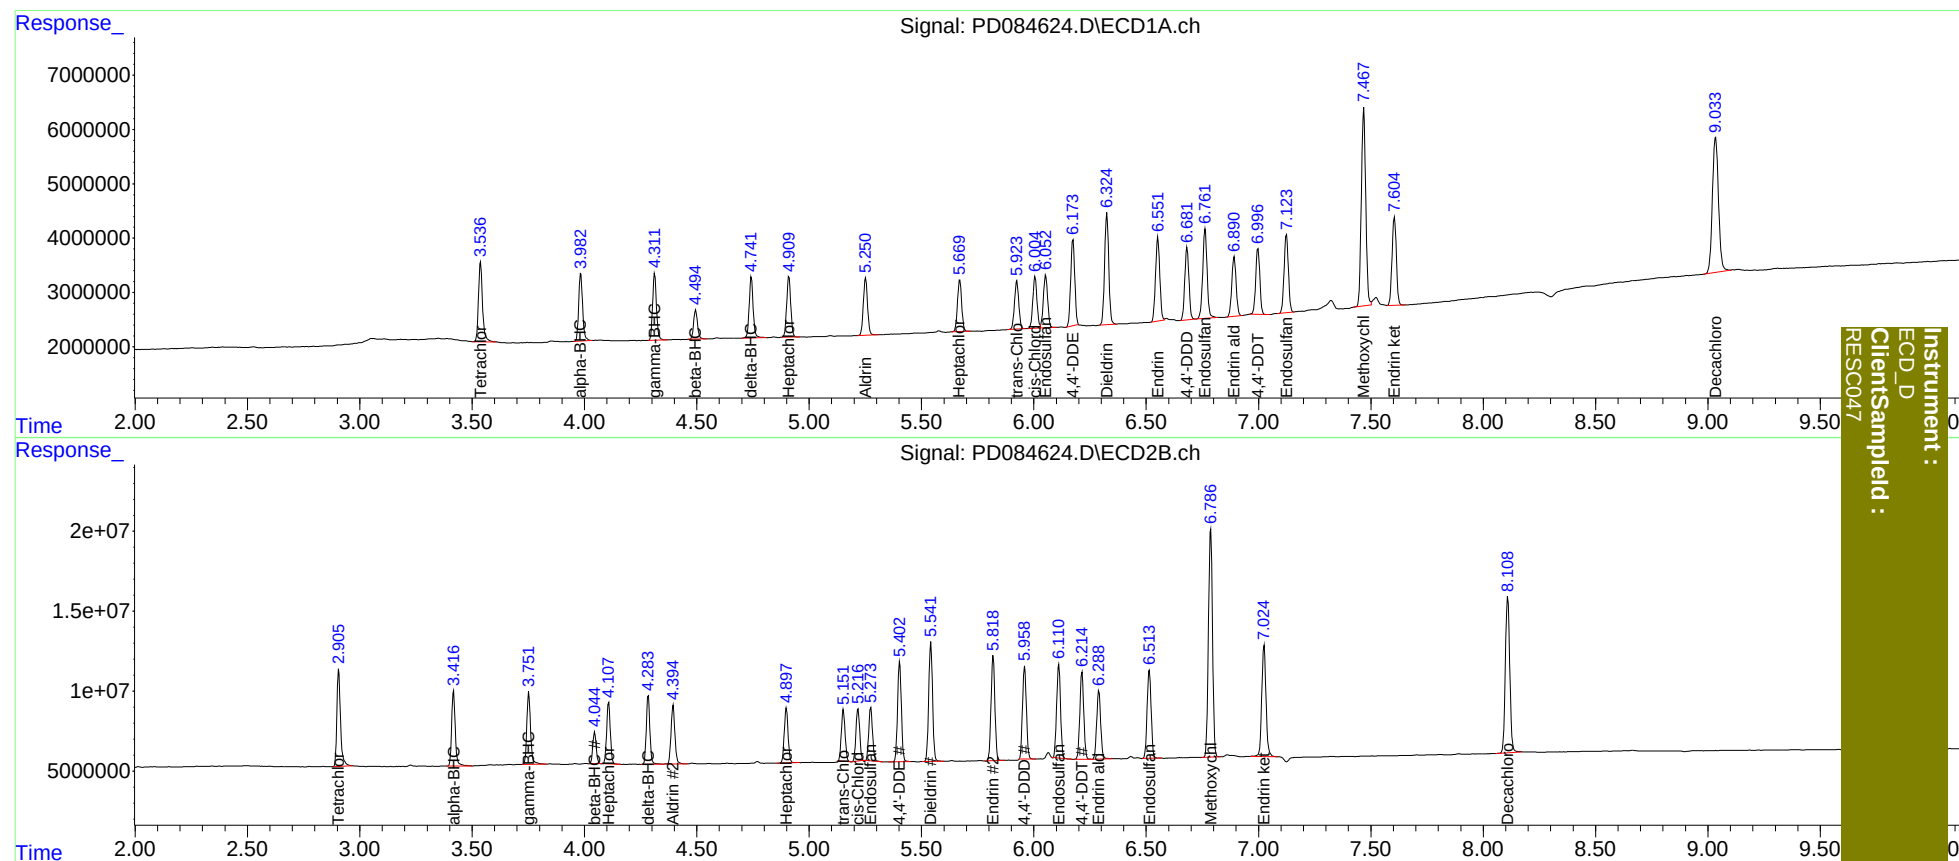

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082424\
Data File : PD084624.D
Acq On : 22 Aug 2024 17:13
Operator : AR\AJ
Sample : RESCH042
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC047

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082424CLP-TCLP.M
Title : GC Extractables
Last Update : Fri Aug 23 06:21:54 2024
Integrator: ChemStation

RT#1	RT#2	Resolution
3.538	3.984	100.00%
3.984	4.313	100.00%
4.313	4.495	100.00%
4.495	4.743	100.00%
4.743	4.910	100.00%
4.910	5.252	100.00%
5.252	5.671	100.00%
5.671	5.925	100.00%
5.925	6.006	100.00%
6.006	6.053	95.04%
6.053	6.174	100.00%
6.174	6.325	100.00%
6.325	6.552	100.00%
6.552	6.682	100.00%
6.682	6.763	100.00%
6.763	6.892	100.00%
6.892	6.998	100.00%
6.998	7.125	100.00%
7.125	7.324	100.00%
7.324	7.469	100.00%
7.469	7.605	100.00%
7.605	9.034	100.00%

Signal #2


2.907	3.418	100.00%
3.418	3.753	100.00%
3.753	4.046	100.00%
4.046	4.108	100.00%
4.108	4.284	100.00%
4.284	4.395	100.00%
4.395	4.899	100.00%
4.899	5.152	100.00%
5.152	5.218	100.00%
5.218	5.275	100.00%
5.275	5.403	100.00%
5.403	5.542	100.00%
5.542	5.819	100.00%
5.819	5.959	100.00%
5.959	6.065	100.00%
6.065	6.111	100.00%
6.111	6.215	100.00%
6.215	6.290	100.00%
6.290	6.514	100.00%
6.514	6.788	100.00%
6.788	7.025	100.00%
7.025	8.110	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082424\
Data File : PD084624.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2024 17:13
Operator : AR\AJ
Sample : RESCH042
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC047

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 06:24:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082424CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Aug 23 06:21:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

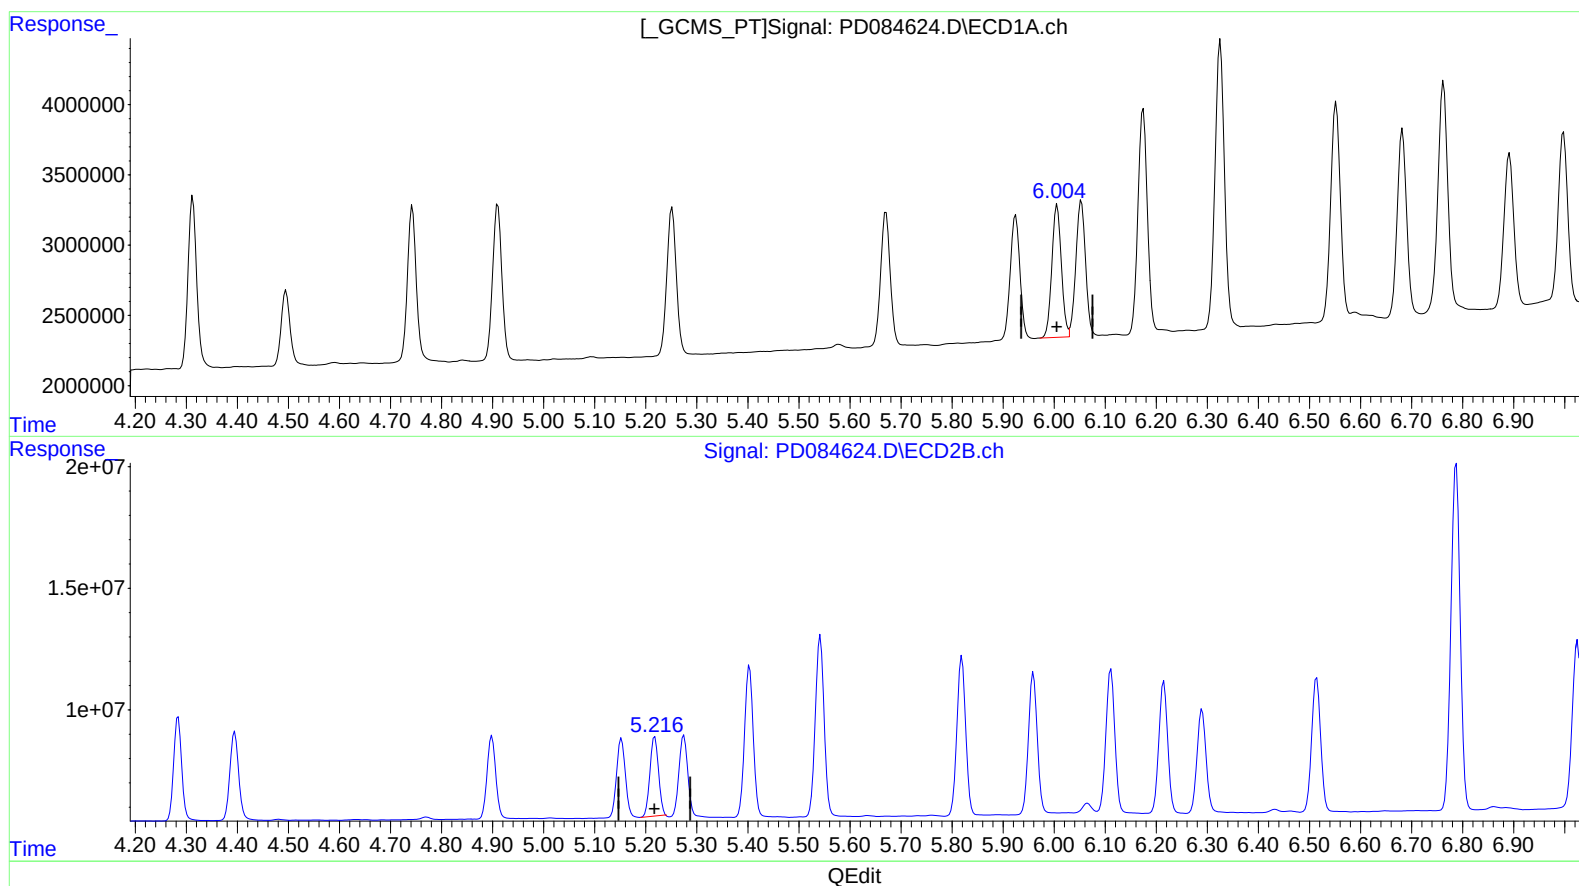

(11) cis-Chlordane (B)

6.006min 8.670 ng/ml

response 12186251

(11) cis-Chlordane #2 (B)

5.218min 9.470 ng/ml

response 38148251