

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082521\
 Data File : PD065271.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2021 19:16
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 06:12:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082521.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 25 05:44:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
3) MA	gamma-BHC...	4.226	4.695	3534033	840643	2.327 0.093 #
10) B	gamma-Chl...	0.000	6.130	0	6951247	N.D. 1.056 #
11) B	alpha-Chl...	0.000	6.196	0	3855231	N.D. 0.597 #
14) MA	Endrin	6.052	0.000	1793016	0	1.497 N.D. #
17) MA	4,4'-DDT	0.000	7.147	0	2340285	N.D. 0.435 #
20) A	Methoxychlor	6.954	7.606	689445	2310968	0.982 0.827
25)	Chlordane-3	0.000	6.130	0	6951247	N.D. 7.923 #
26)	Chlordane-4	0.000	6.196	0	3855231	N.D. 3.773 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082521\
Data File : PD065271.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2021 19:16
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 06:12:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082521.M
Quant Title : GC Extractables
QLast Update : Wed Aug 25 05:44:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

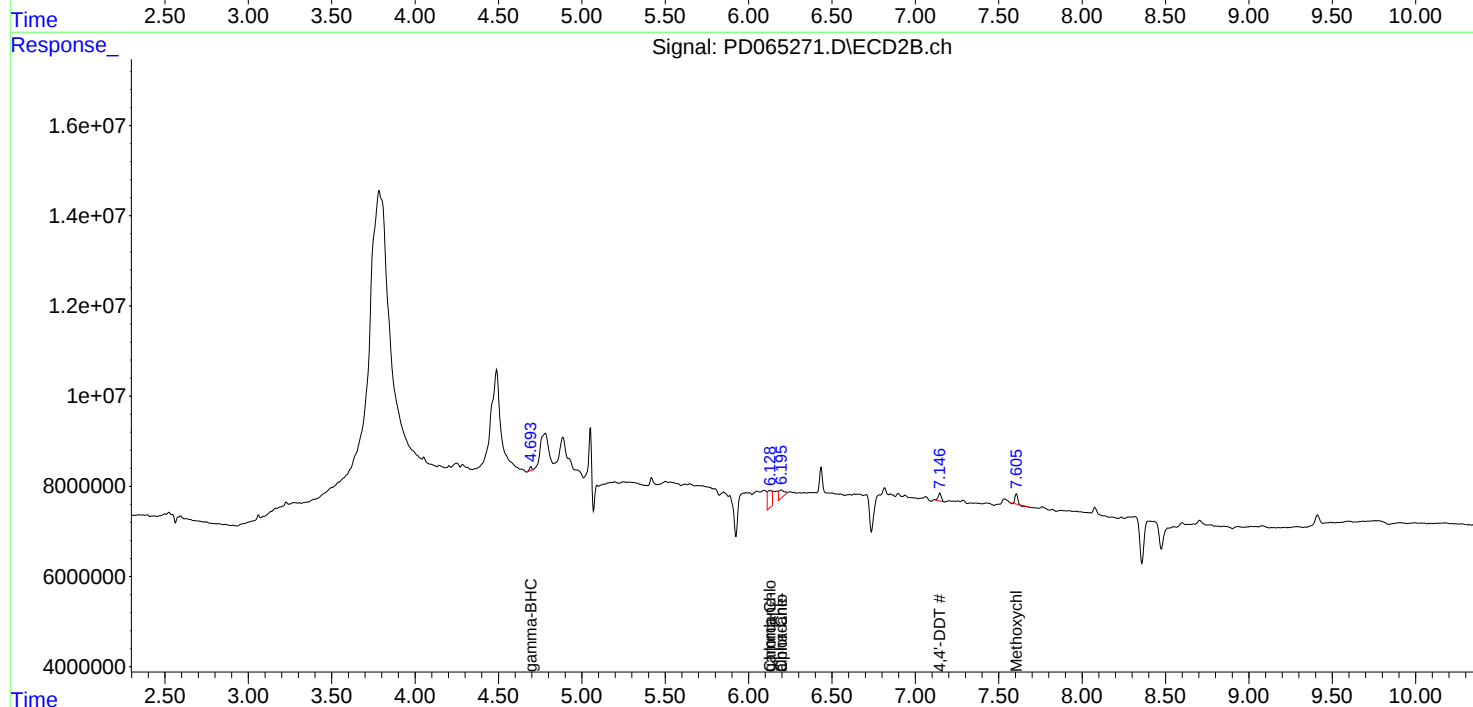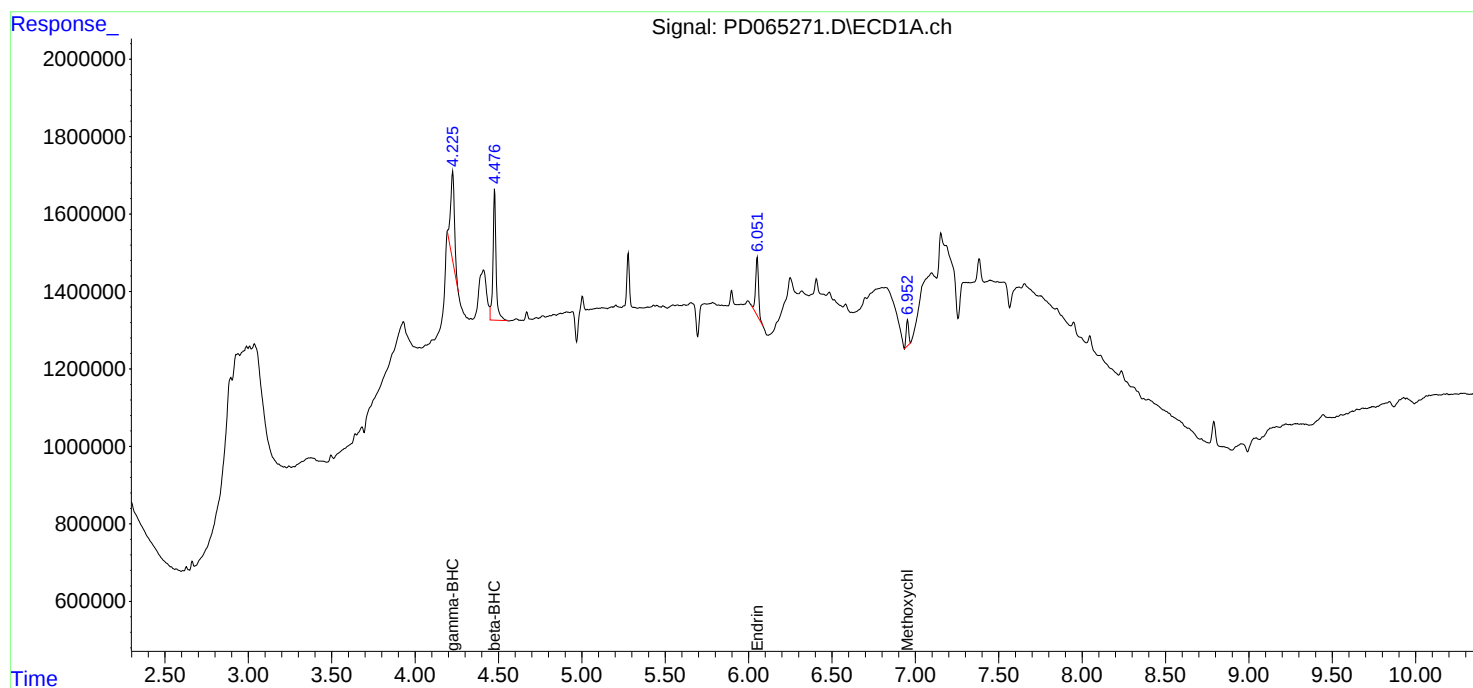


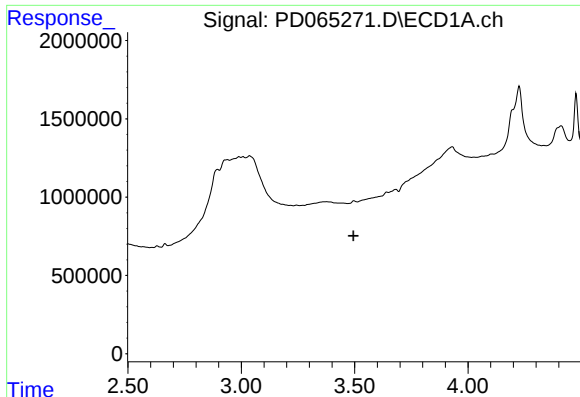

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

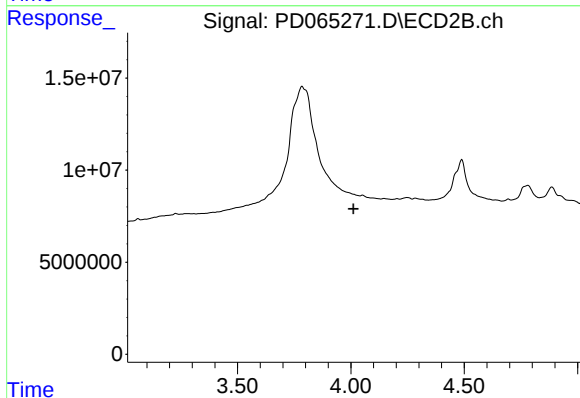


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.012 min
Response: 0
Conc: N.D.

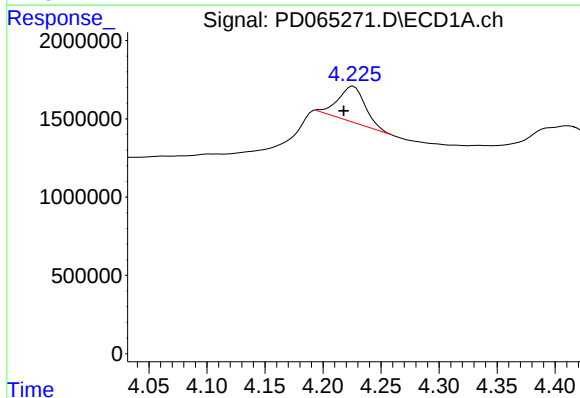


#3 gamma-BHC (Lindane)

R.T.: 4.226 min
Delta R.T.: 0.009 min
Response: 3534033
Conc: 2.33 ng/ml

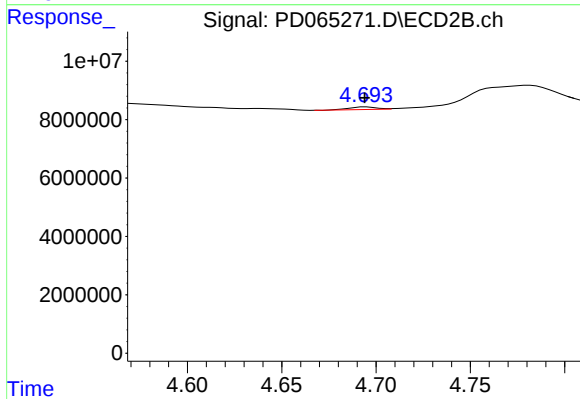

#3 gamma-BHC (Lindane)


R.T.: 4.695 min
Delta R.T.: 0.000 min
Response: 840643
Conc: 0.09 ng/ml

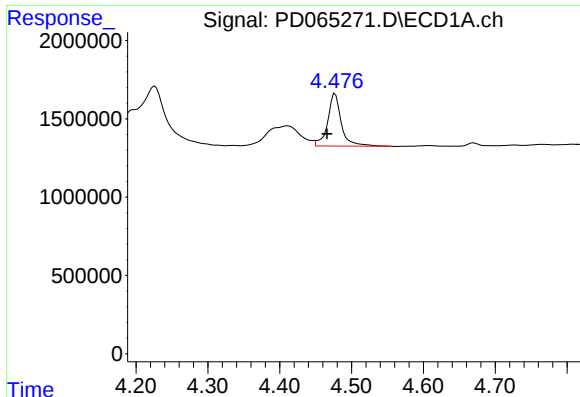

#6 beta-BHC


R.T.: 4.477 min
Delta R.T.: 0.012 min
Response: 4436550
Conc: 0.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

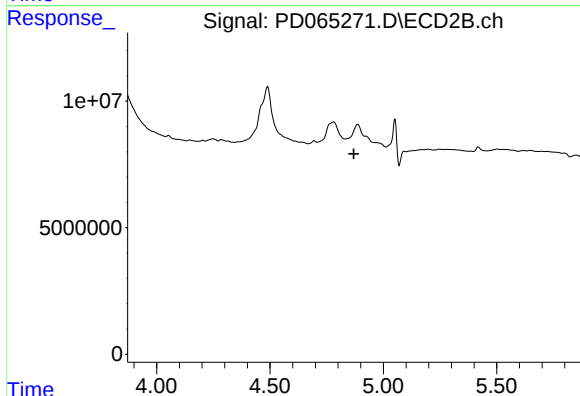


#6 beta-BHC

R.T.: 4.887 min
Delta R.T.: 0.017 min
Response: 8439192
Conc: N.D.

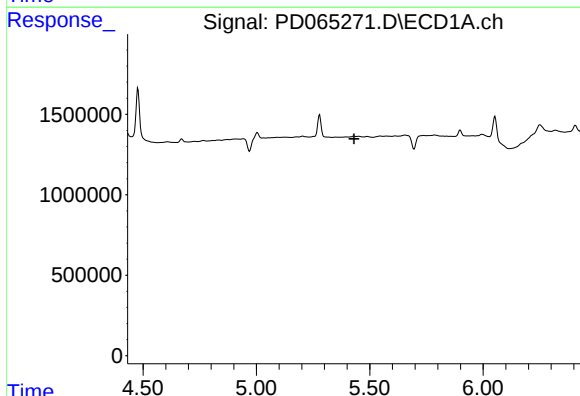


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.431 min
Response: 0
Conc: N.D.

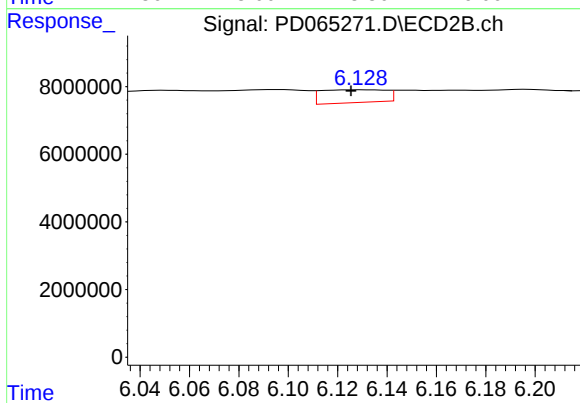

#10 gamma-Chlordane


R.T.: 6.130 min
Delta R.T.: 0.005 min
Response: 6951247
Conc: 1.06 ng/ml

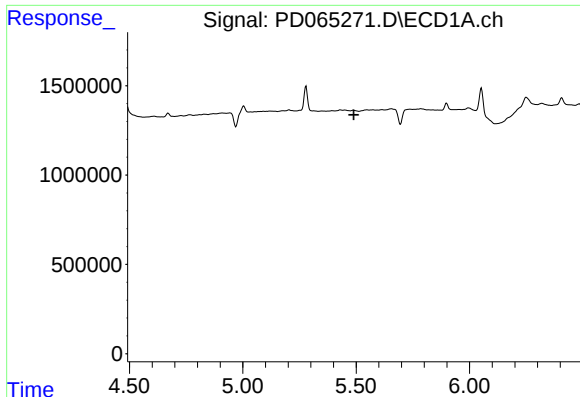

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.490 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

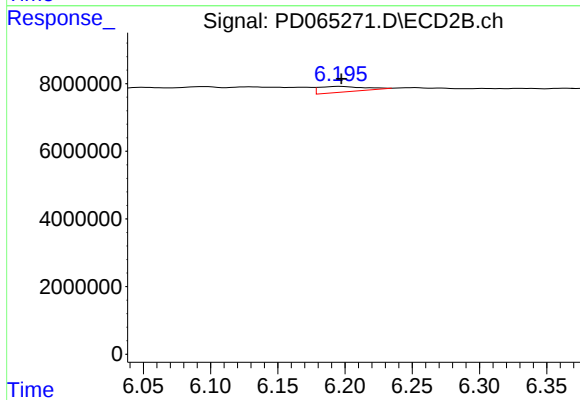


#11 alpha-Chlordane

R.T.: 6.196 min
Delta R.T.: -0.001 min
Response: 3855231
Conc: 0.60 ng/ml

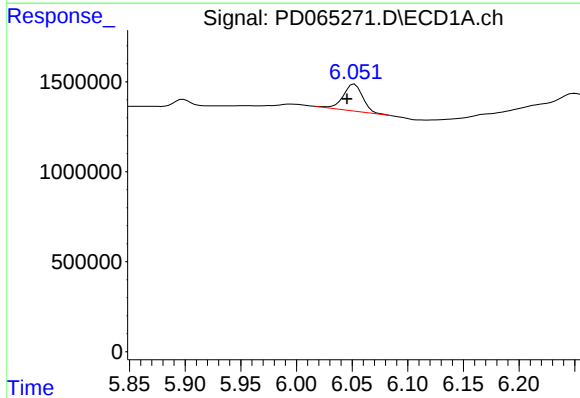


#14 Endrin

R.T.: 6.052 min
Delta R.T.: 0.007 min
Response: 1793016
Conc: 1.50 ng/ml

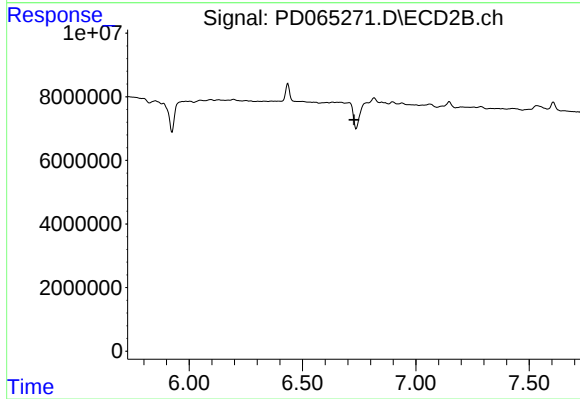

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.727 min
Response: 0
Conc: N.D.

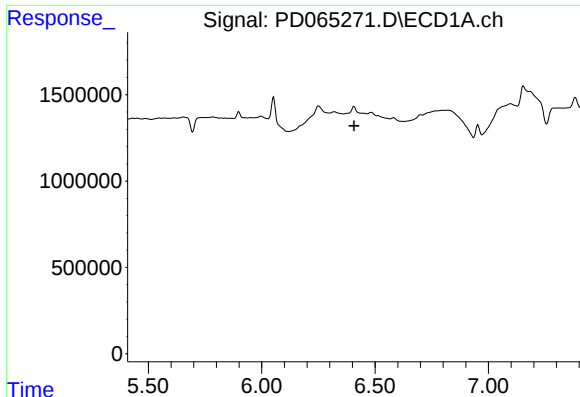

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

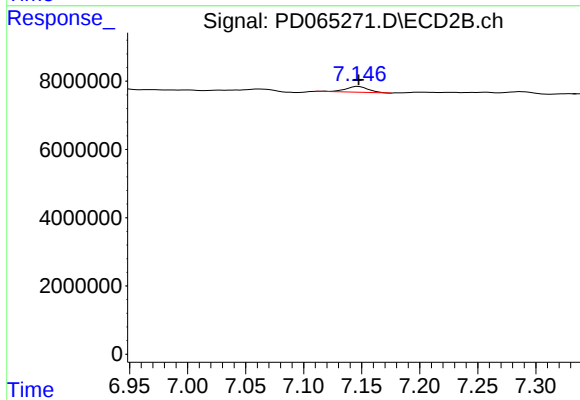


#17 4,4'-DDT

R.T.: 7.147 min
Delta R.T.: 0.000 min
Response: 2340285
Conc: 0.44 ng/ml

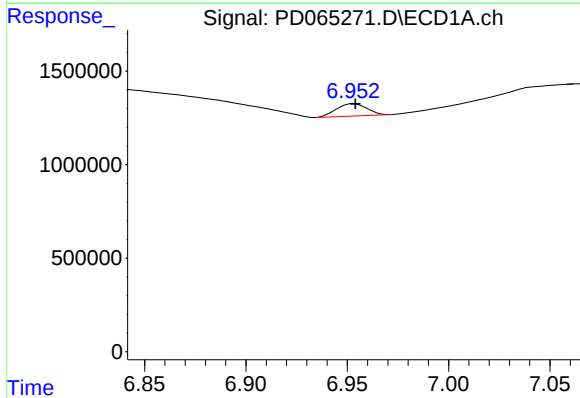


#20 Methoxychlor

R.T.: 6.954 min
Delta R.T.: 0.000 min
Response: 689445
Conc: 0.98 ng/ml

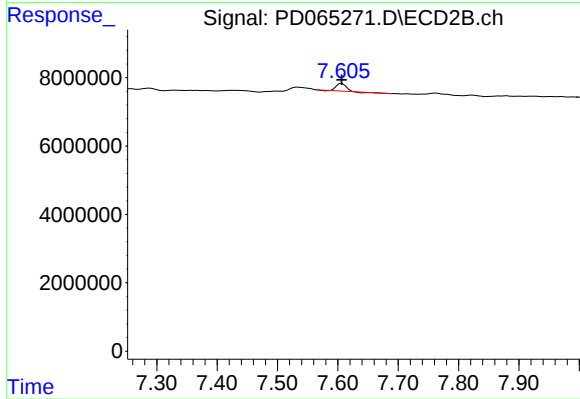

#20 Methoxychlor


R.T.: 7.606 min
Delta R.T.: 0.000 min
Response: 2310968
Conc: 0.83 ng/ml

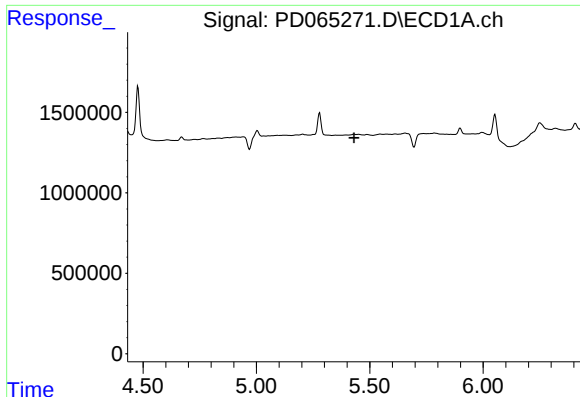

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

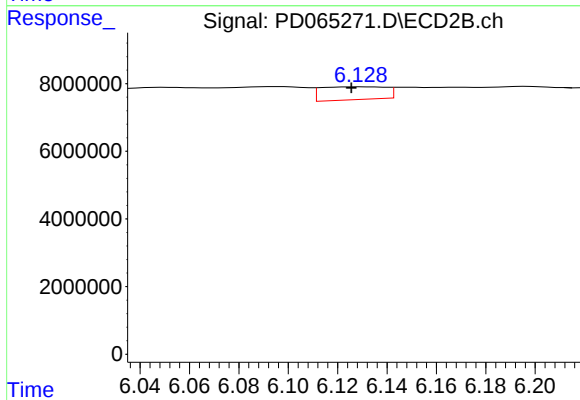


#25 Chlordane-3

R.T.: 6.130 min
Delta R.T.: 0.005 min
Response: 6951247
Conc: 7.92 ng/ml

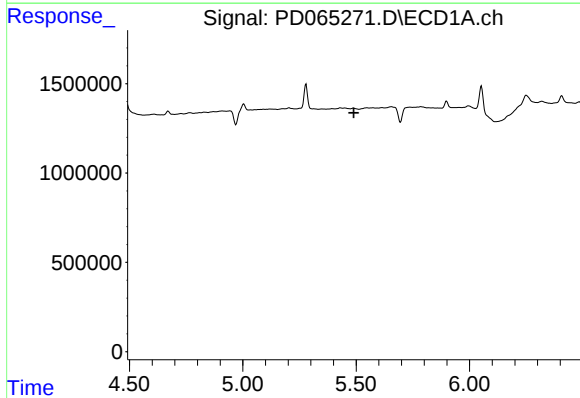


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.490 min
Response: 0
Conc: N.D.

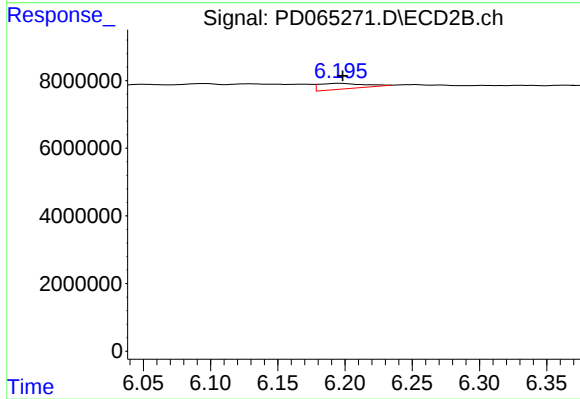

#26 Chlordane-4


R.T.: 6.196 min
Delta R.T.: -0.002 min
Response: 3855231
Conc: 3.77 ng/ml

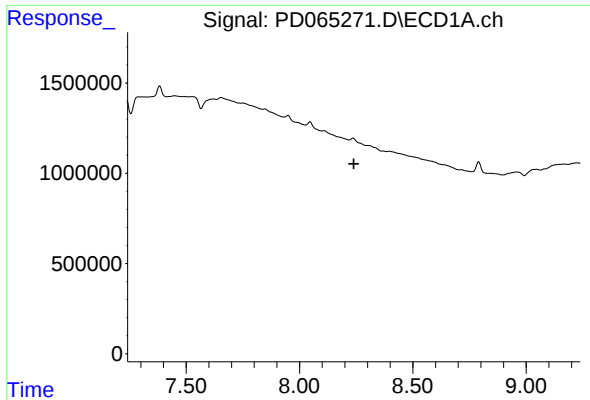

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

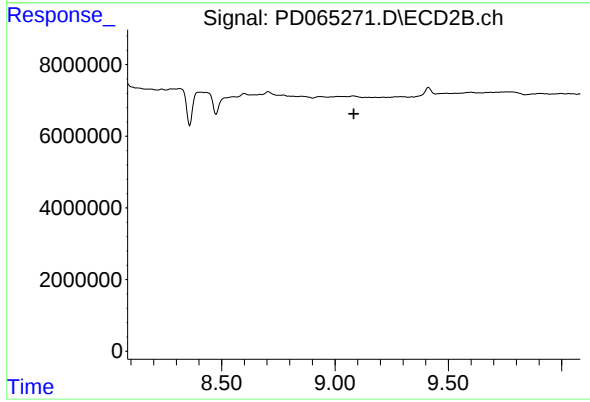

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.083 min
Response: 0
Conc: N.D.