

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082521\
 Data File : PD065280.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2021 21:21
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 05:30:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082521.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 25 05:29:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.495	4.013	121.5E6	647.8E6	96.393	94.392
28)	SA Decachlor...	8.240	9.083	121.3E6	402.8E6	91.448	91.644
Target Compounds							
23)	Chlordane-1	4.366	5.009	36187154	244.6E6	942.445	943.253
24)	Chlordane-2	4.866	5.478	41666280	220.1E6	904.698	912.514
25)	Chlordane-3	5.432	6.126	113.8E6	829.7E6	963.610	951.428
26)	Chlordane-4	5.490	6.198	93611787	957.3E6	945.251	943.382
27)	Chlordane-5	6.327	7.009	45523633	199.6E6	940.532	945.751



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082521\
Data File : PD065280.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2021 21:21
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 05:30:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082521.M
Quant Title : GC Extractables
QLast Update : Wed Aug 25 05:29:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

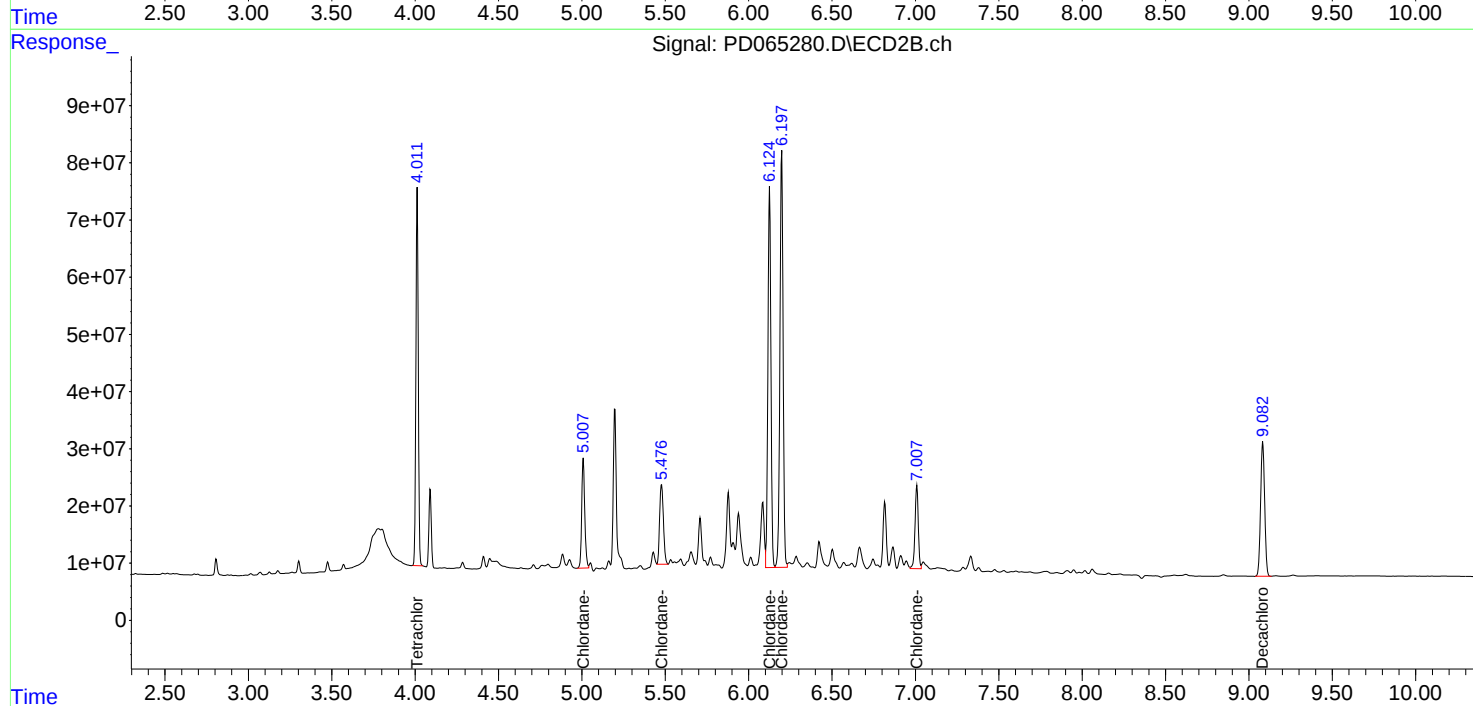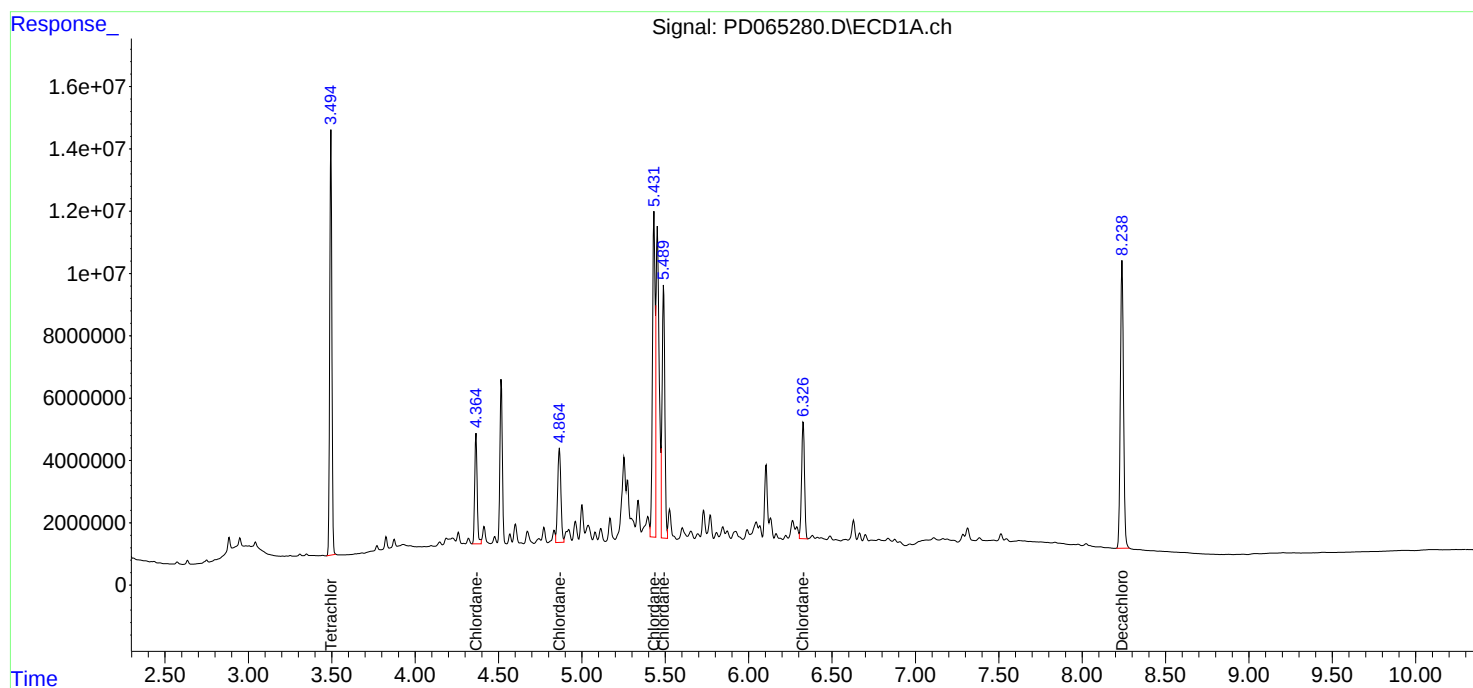


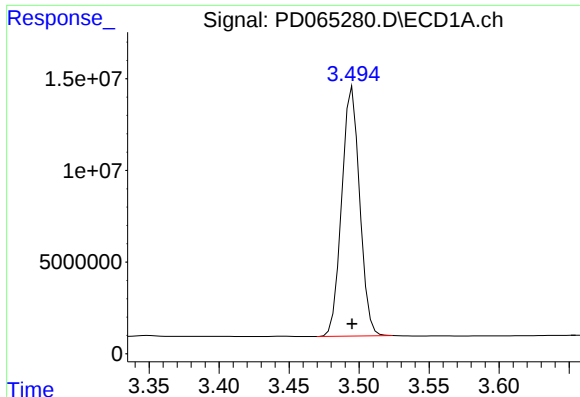

#1 Tetrachloro-m-xylene


R.T.: 3.495 min
Delta R.T.: 0.000 min
Response: 121500155
Conc: 96.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

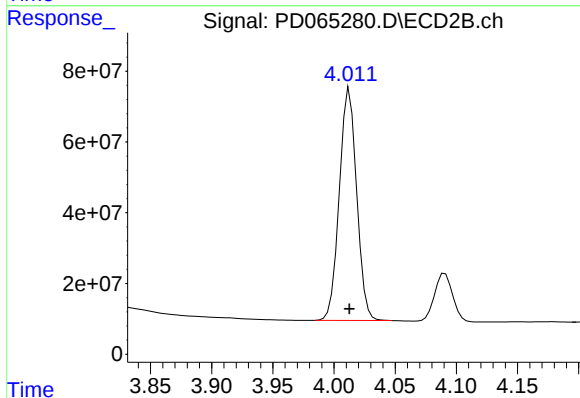


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 647826206
Conc: 94.39 ng/ml

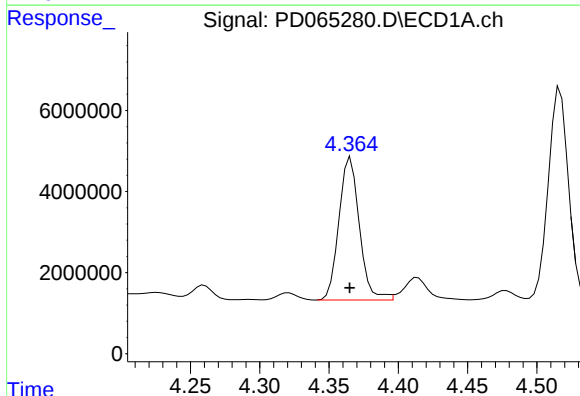


#23 Chlordane-1

R.T.: 4.366 min
Delta R.T.: 0.000 min
Response: 36187154
Conc: 942.45 ng/ml

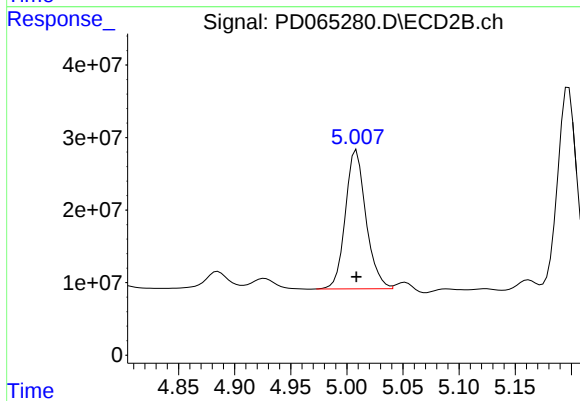

#23 Chlordane-1


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 244614964
Conc: 943.25 ng/ml

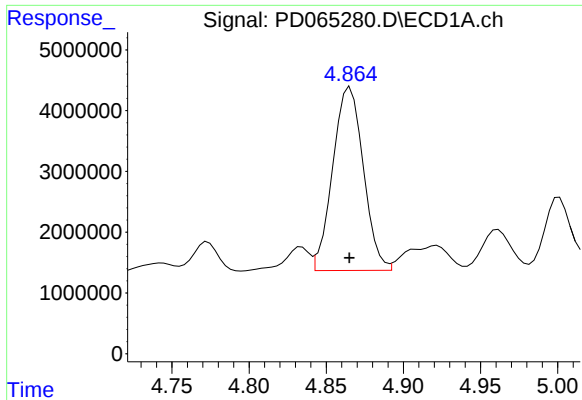

#24 Chlordane-2


R.T.: 4.866 min
Delta R.T.: 0.000 min
Response: 41666280
Conc: 904.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

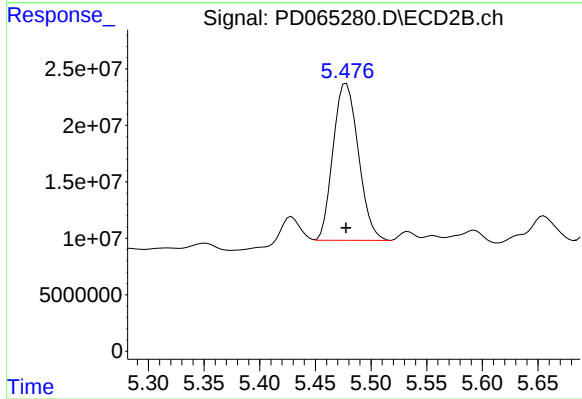


#24 Chlordane-2

R.T.: 5.478 min
Delta R.T.: 0.000 min
Response: 220060321
Conc: 912.51 ng/ml

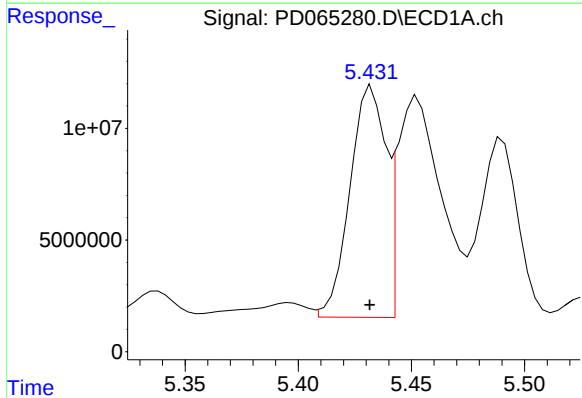


#25 Chlordane-3

R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 113828779
Conc: 963.61 ng/ml

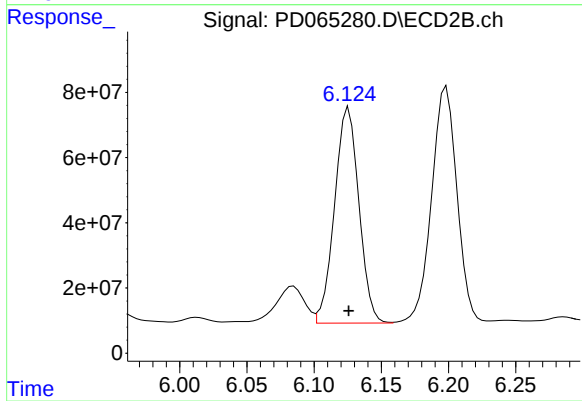

#25 Chlordane-3


R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 829679407
Conc: 951.43 ng/ml

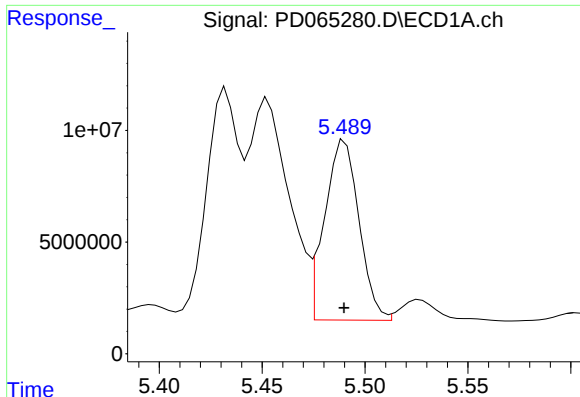

#26 Chlordane-4


R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 93611787
Conc: 945.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

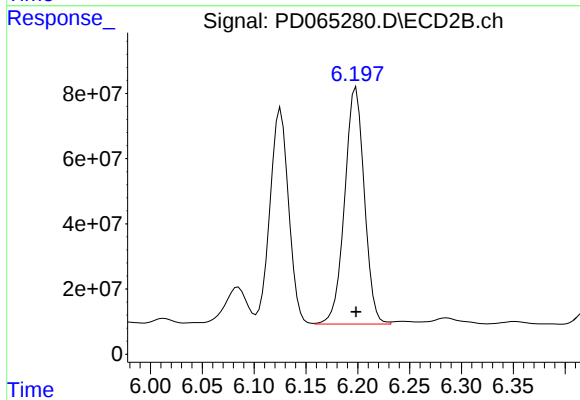


#26 Chlordane-4

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 957263549
Conc: 943.38 ng/ml

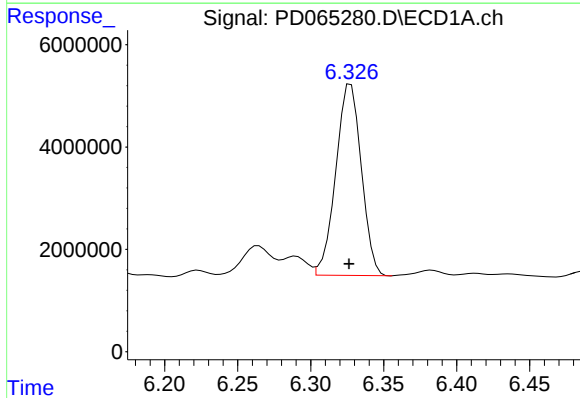


#27 Chlordane-5

R.T.: 6.327 min
Delta R.T.: 0.001 min
Response: 45523633
Conc: 940.53 ng/ml

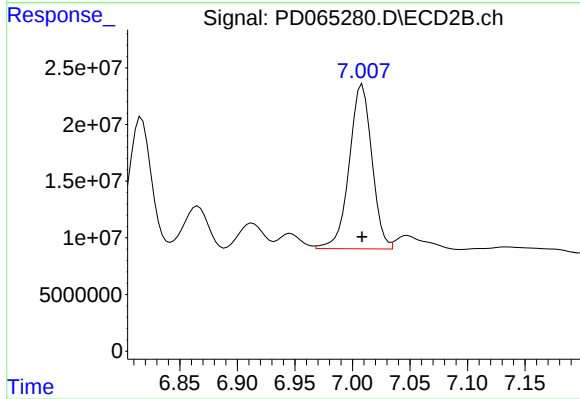

#27 Chlordane-5


R.T.: 7.009 min
Delta R.T.: 0.000 min
Response: 199612392
Conc: 945.75 ng/ml

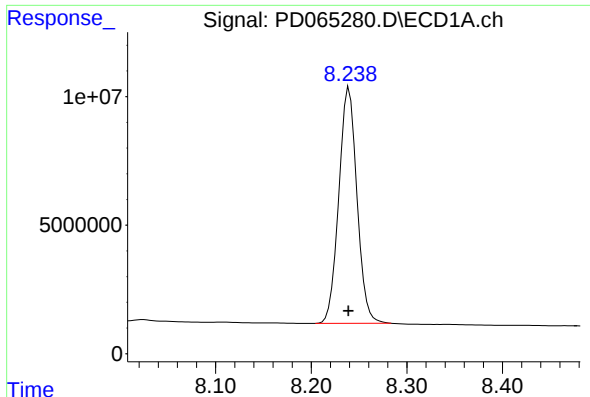

#28 Decachlorobiphenyl

R.T.: 8.240 min
Delta R.T.: 0.000 min
Response: 121261779
Conc: 91.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

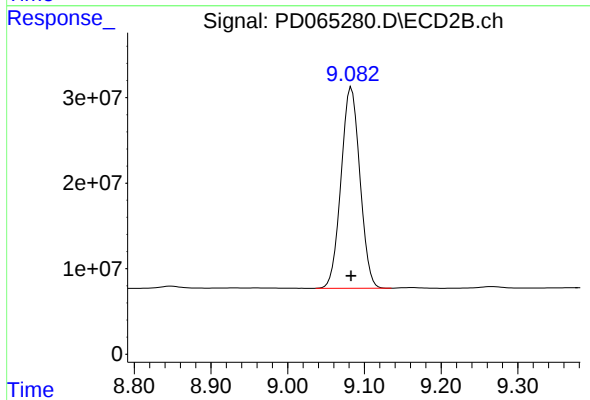

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: 0.000 min
Response: 402804084
Conc: 91.64 ng/ml