

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082521\
 Data File : PD065283.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2021 22:02
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 05:31:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082521.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 25 05:29:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.495	4.013	31663289	176.2E6	25.120	25.677
28)	SA Decachlor...	8.239	9.082	34817339	114.3E6	26.257	26.015
Target Compounds							
23)	Chlordane-1	4.365	5.008	9977011	69271032	259.838	267.114
24)	Chlordane-2	4.865	5.478	12353740	63503408	268.236	263.327
25)	Chlordane-3	5.431	6.125	29511063	221.5E6	249.824	253.965
26)	Chlordane-4	5.490	6.198	25346676	259.5E6	255.940	255.729
27)	Chlordane-5	6.326	7.009	12526119	52561951	258.793	249.035



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082521\
Data File : PD065283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2021 22:02
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 05:31:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082521.M
Quant Title : GC Extractables
QLast Update : Wed Aug 25 05:29:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

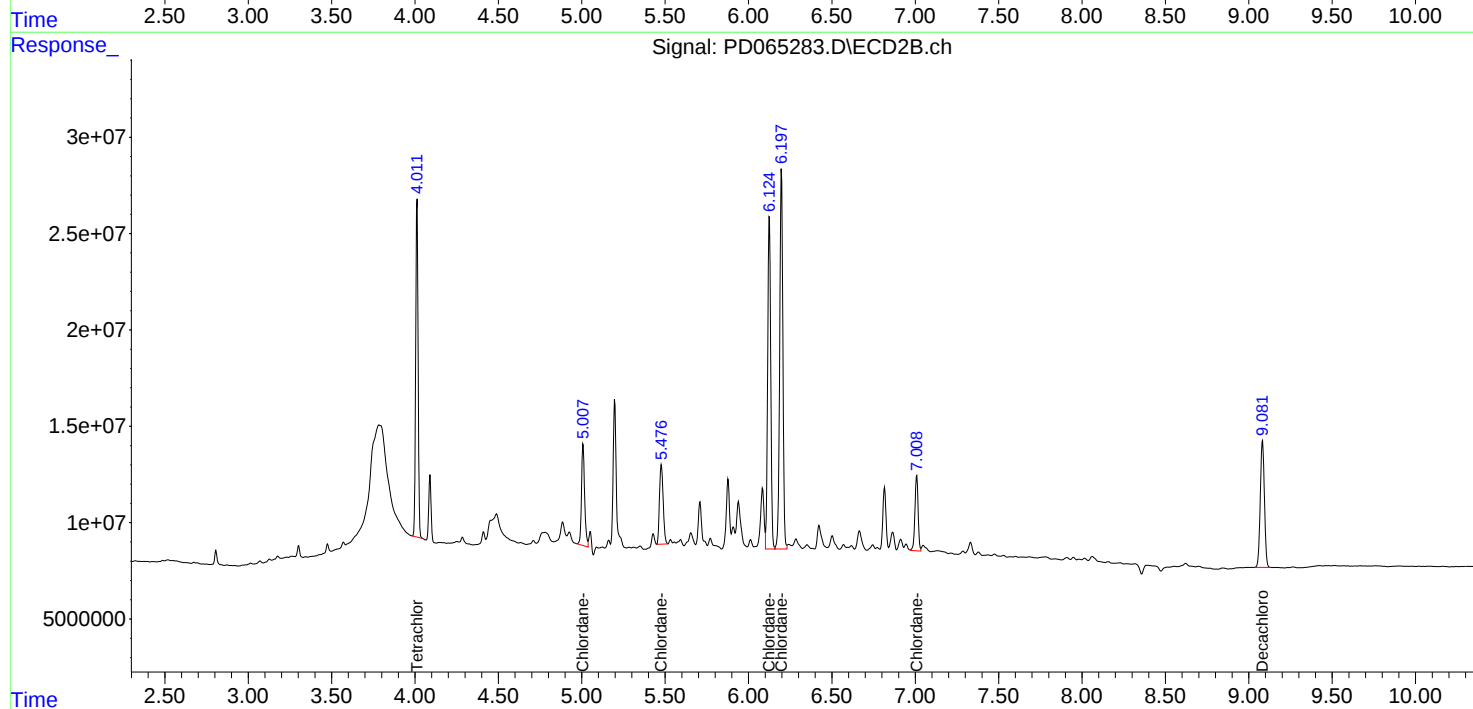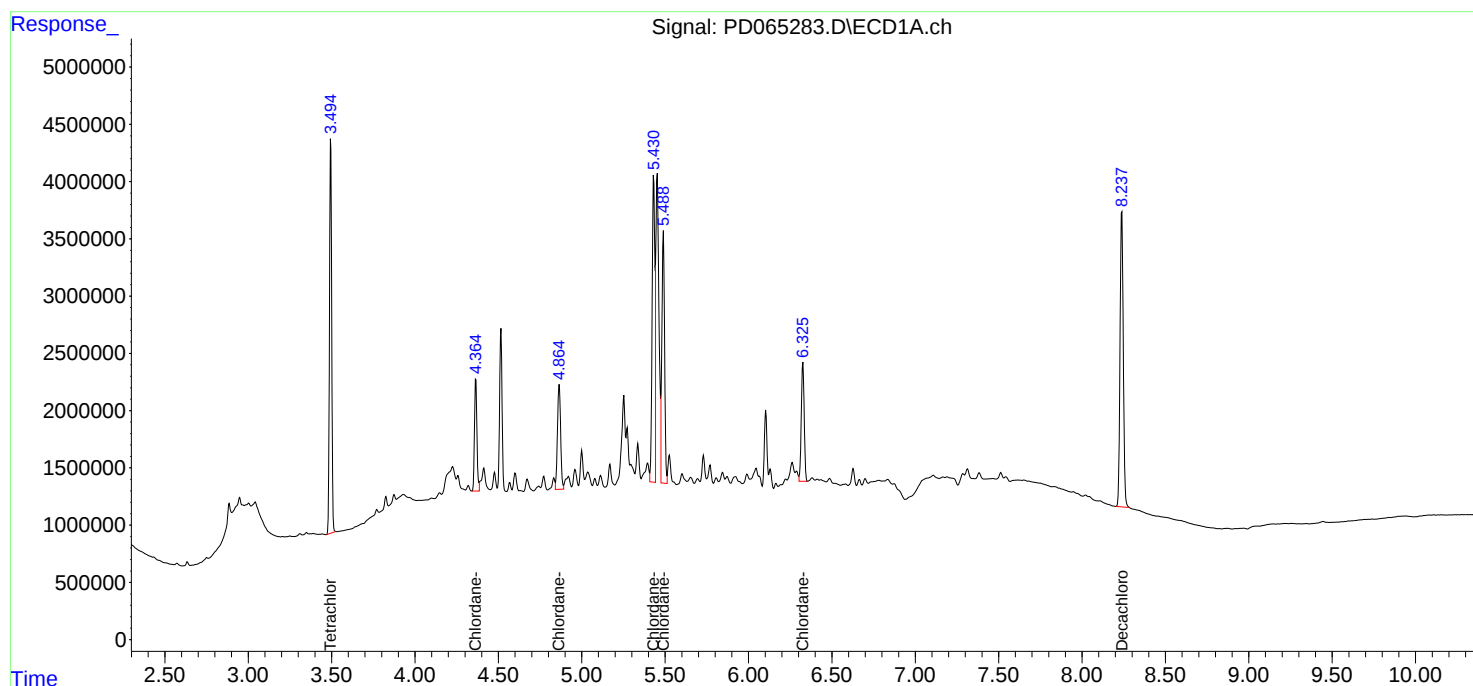


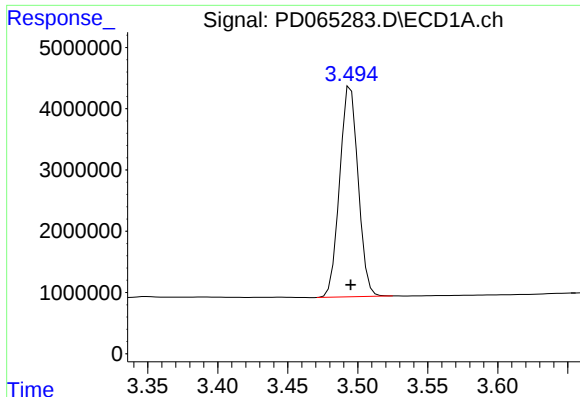

#1 Tetrachloro-m-xylene


R.T.: 3.495 min
Delta R.T.: 0.000 min
Response: 31663289
Conc: 25.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

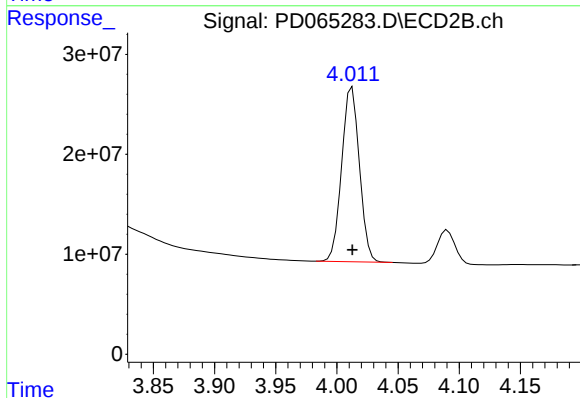


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 176221320
Conc: 25.68 ng/ml

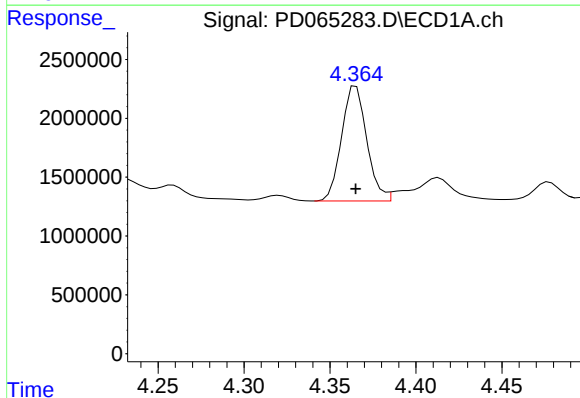


#23 Chlordane-1

R.T.: 4.365 min
Delta R.T.: 0.000 min
Response: 9977011
Conc: 259.84 ng/ml

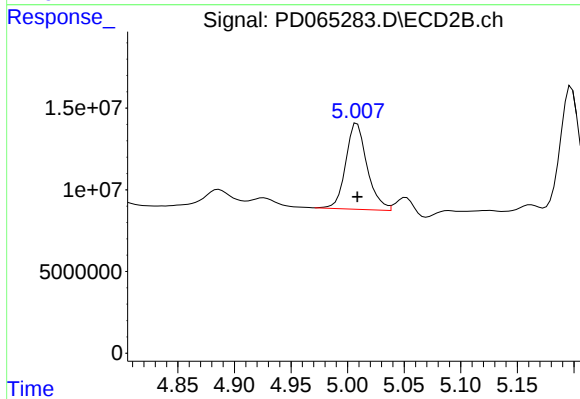

#23 Chlordane-1


R.T.: 5.008 min
Delta R.T.: 0.000 min
Response: 69271032
Conc: 267.11 ng/ml

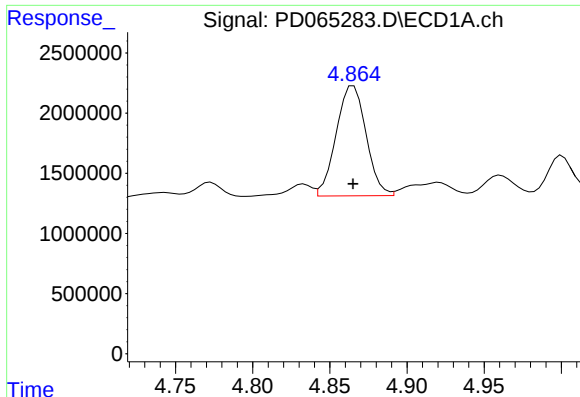

#24 Chlordane-2


R.T.: 4.865 min
Delta R.T.: 0.000 min
Response: 12353740
Conc: 268.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

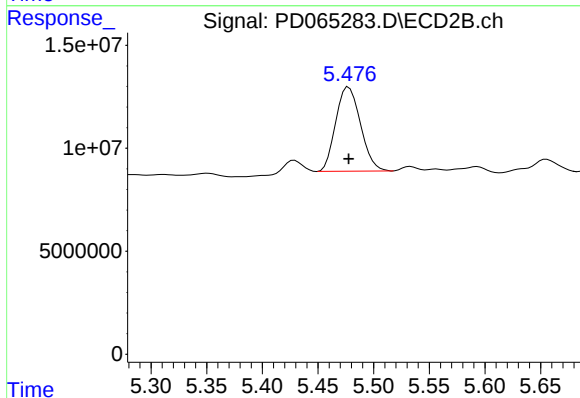


#24 Chlordane-2

R.T.: 5.478 min
Delta R.T.: 0.000 min
Response: 63503408
Conc: 263.33 ng/ml

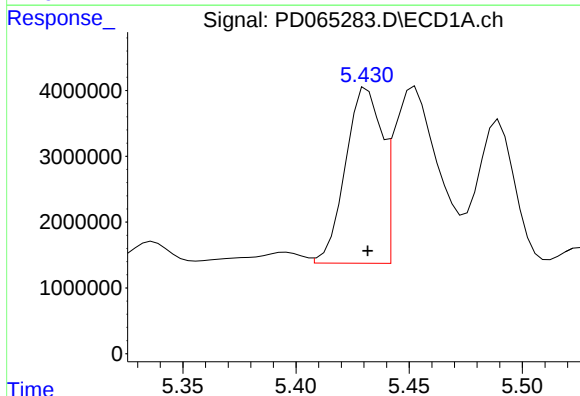


#25 Chlordane-3

R.T.: 5.431 min
Delta R.T.: 0.000 min
Response: 29511063
Conc: 249.82 ng/ml

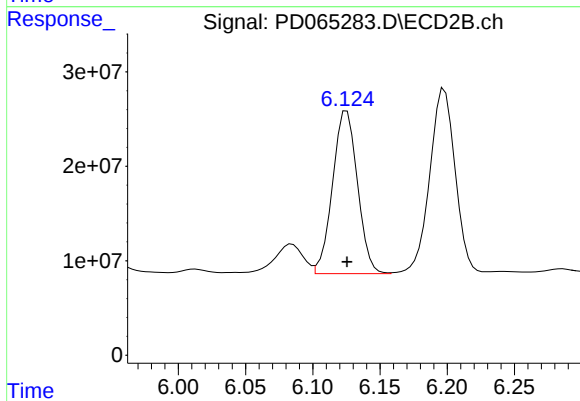

#25 Chlordane-3


R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 221466446
Conc: 253.96 ng/ml

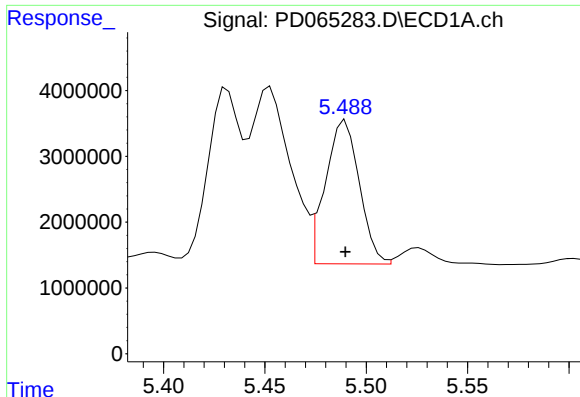

#26 Chlordane-4


R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 25346676
Conc: 255.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

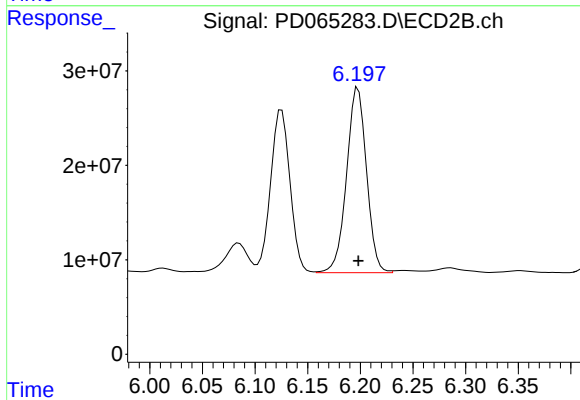


#26 Chlordane-4

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 259492358
Conc: 255.73 ng/ml

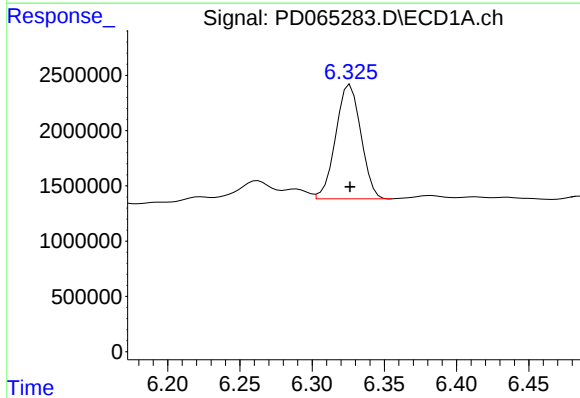


#27 Chlordane-5

R.T.: 6.326 min
Delta R.T.: 0.000 min
Response: 12526119
Conc: 258.79 ng/ml

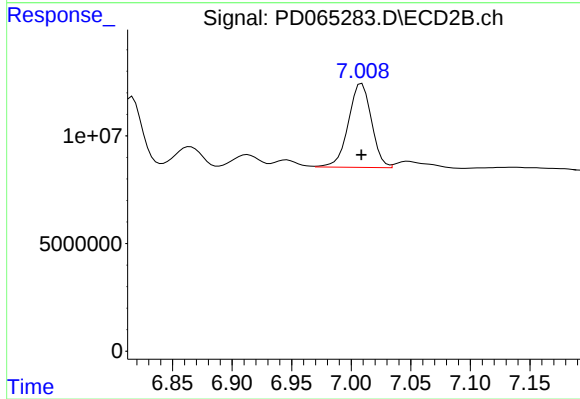

#27 Chlordane-5


R.T.: 7.009 min
Delta R.T.: 0.000 min
Response: 52561951
Conc: 249.04 ng/ml

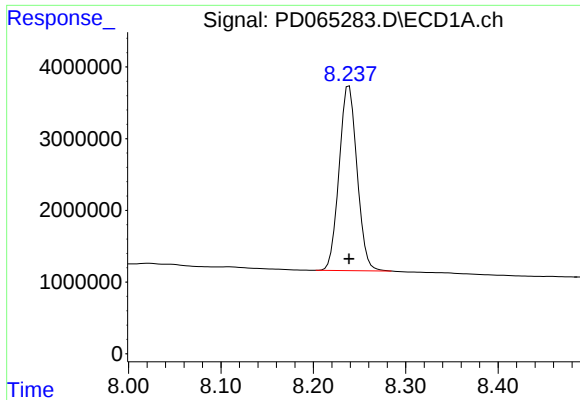

#28 Decachlorobiphenyl

R.T.: 8.239 min
Delta R.T.: 0.000 min
Response: 34817339
Conc: 26.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

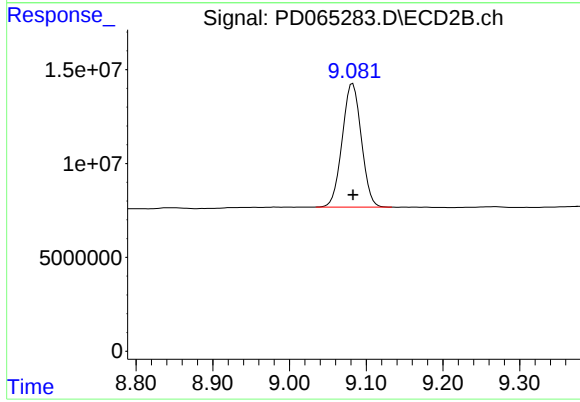

#28 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: 0.000 min
Response: 114344570
Conc: 26.02 ng/ml