

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082521\
 Data File : PD065307.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Aug 2021 14:29
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 26 03:39:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082521.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 25 05:44:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	22252913	152.6E6	20.640	22.326
28)	SA Decachlor...	8.238	9.083	27849061	82660357	20.524	19.087
Target Compounds							
3)	MA gamma-BHC...	4.228	0.000	942519	0	0.621	N.D. #
8)	B Heptachlo...	0.000	5.880	0	7879370	N.D.	1.238 #
12)	B 4,4'-DDE	0.000	6.369	0	860651	N.D.	0.139 #
15)	B Endosulfa...	0.000	6.946	0	12920604	N.D.	2.474 #
19)	B Endosulfa...	6.723f	0.000	529583	0	0.429	N.D. #
22)	Mirex	7.367	8.224	6869822	8373954	1.330	2.028 #
23)	Chlordane-1	4.394f	0.000	532349	0	13.562	N.D. #
27)	Chlordane-5	0.000	7.000	0	2710068	N.D.	13.308 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082521\
Data File : PD065307.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Aug 2021 14:29
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 26 03:39:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082521.M
Quant Title : GC Extractables
QLast Update : Wed Aug 25 05:44:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

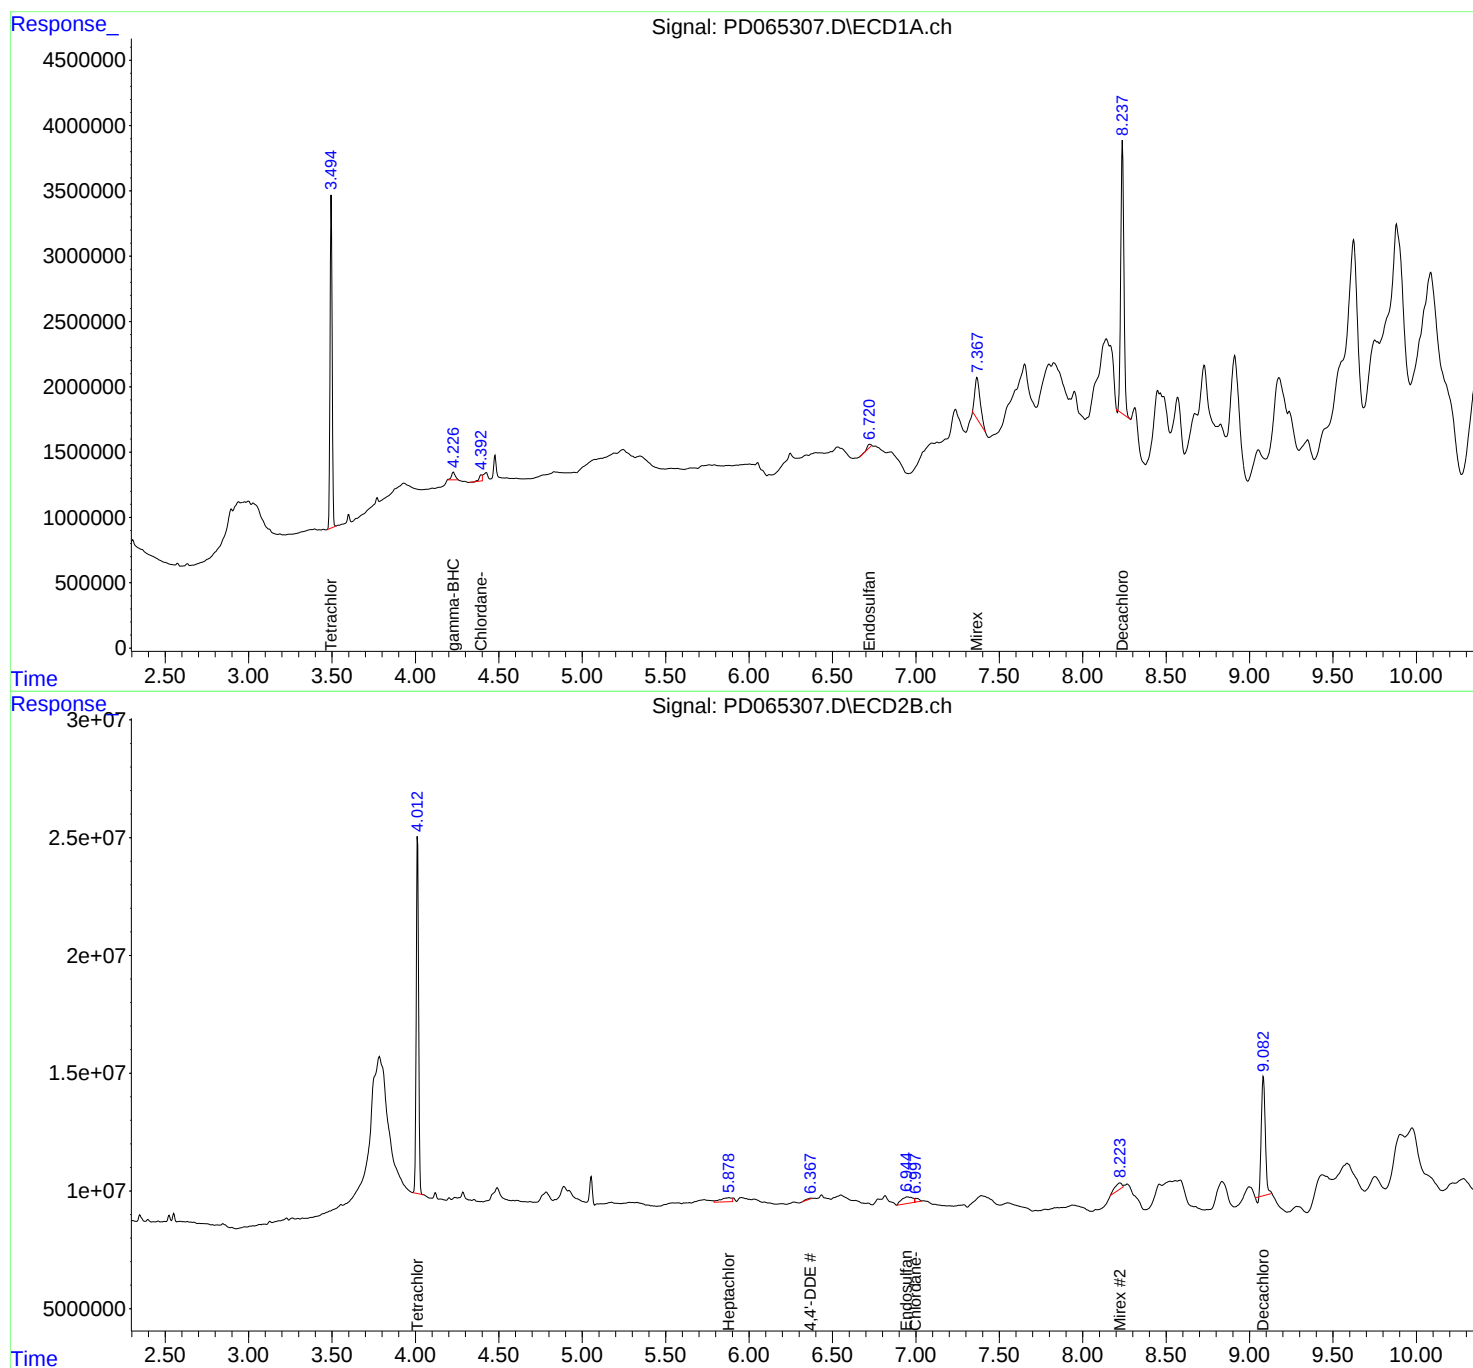


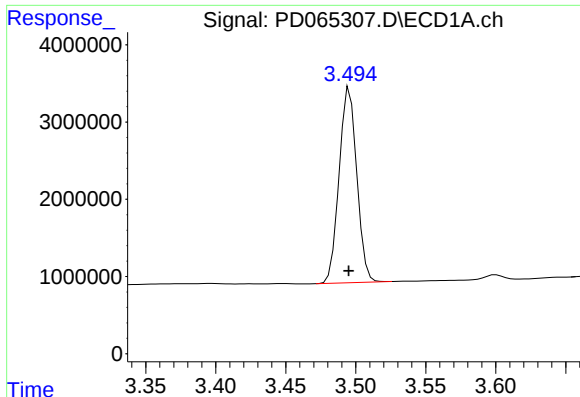

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 22252913
Conc: 20.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

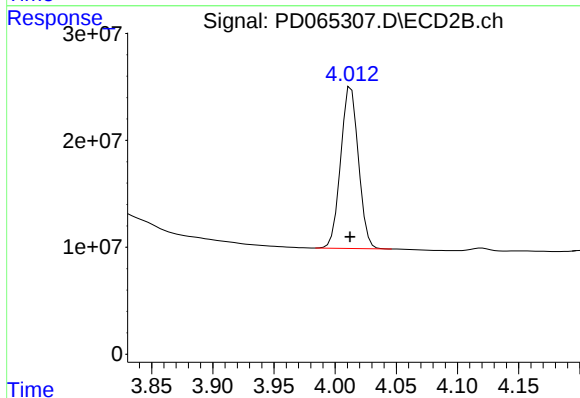


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 152649265
Conc: 22.33 ng/ml

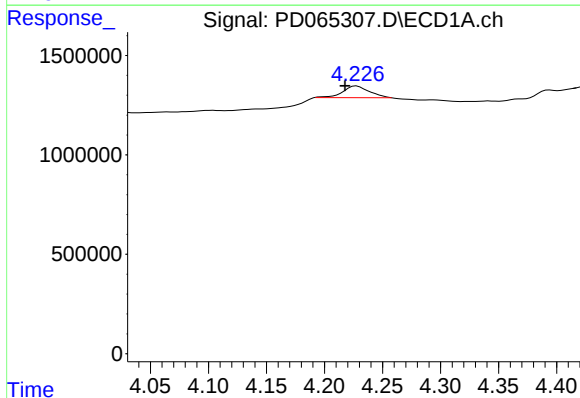


#3 gamma-BHC (Lindane)

R.T.: 4.228 min
Delta R.T.: 0.010 min
Response: 942519
Conc: 0.62 ng/ml

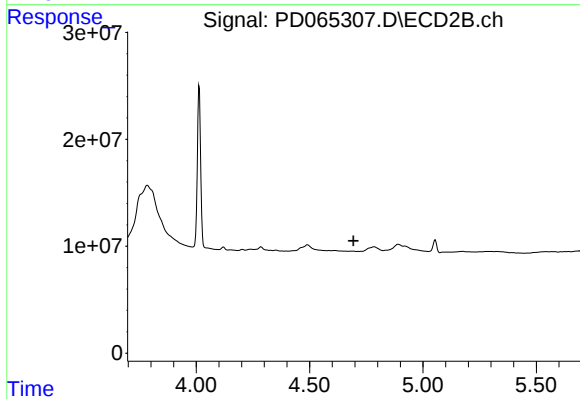

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.694 min
Response: 0
Conc: N.D.

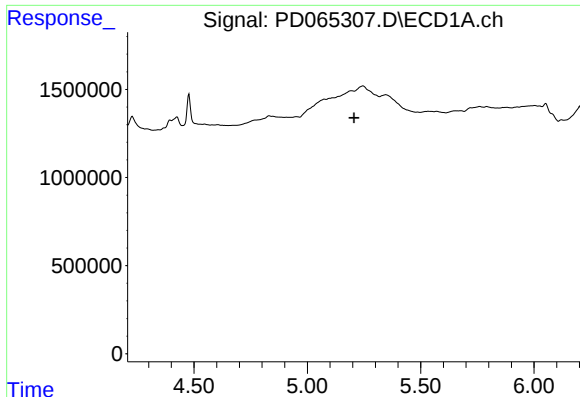

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.206 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

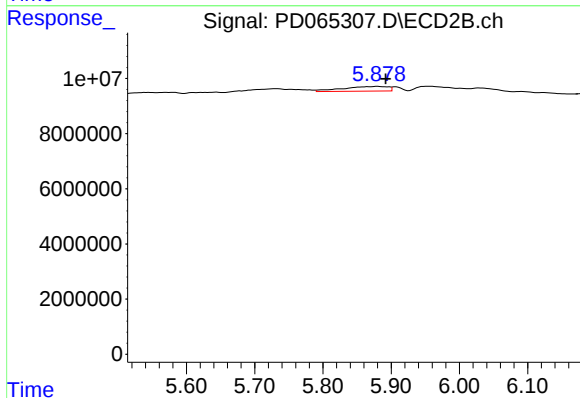


#8 Heptachlor epoxide

R.T.: 5.880 min
Delta R.T.: -0.012 min
Response: 7879370
Conc: 1.24 ng/ml

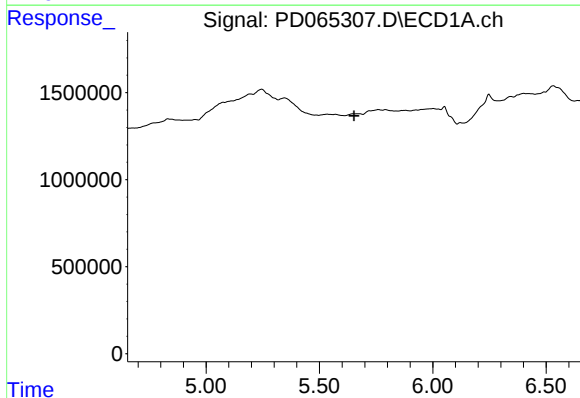


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.653 min
Response: 0
Conc: N.D.

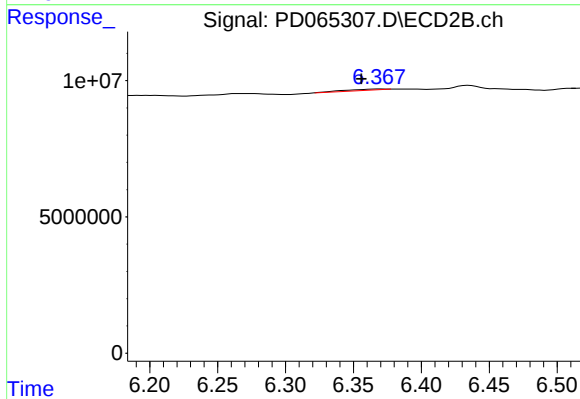

#12 4,4'-DDE


R.T.: 6.369 min
Delta R.T.: 0.013 min
Response: 860651
Conc: 0.14 ng/ml

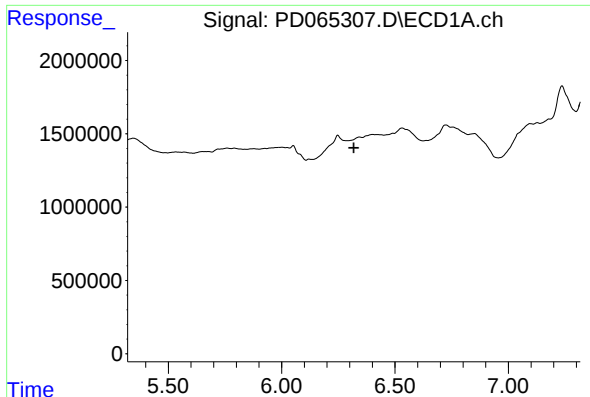

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

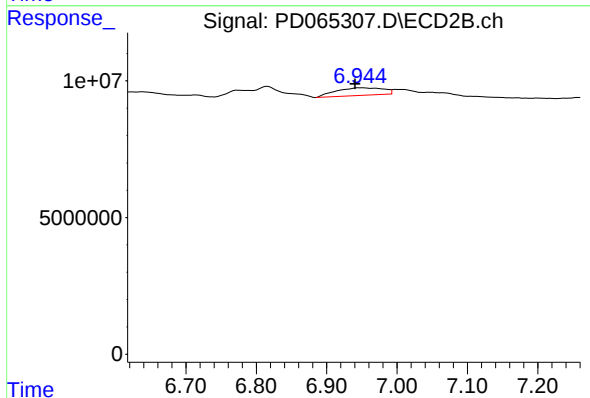


#15 Endosulfan II

R.T.: 6.946 min
Delta R.T.: 0.005 min
Response: 12920604
Conc: 2.47 ng/ml

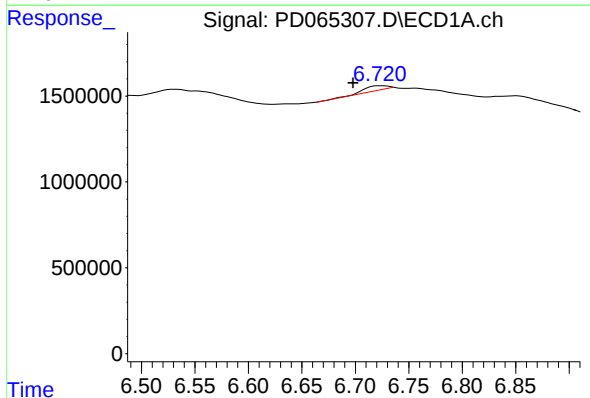


#19 Endosulfan Sulfate

R.T.: 6.723 min
Delta R.T.: 0.025 min
Response: 529583
Conc: 0.43 ng/ml

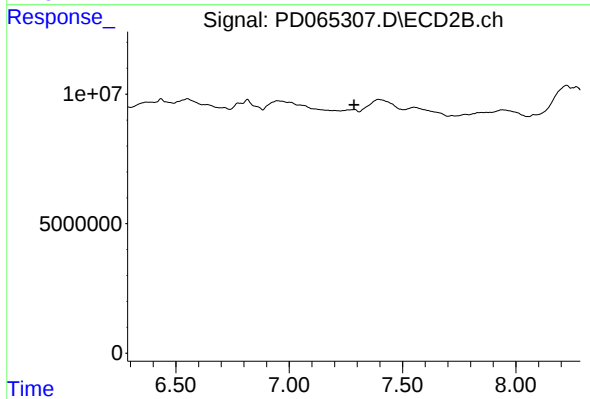

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.287 min
Response: 0
Conc: N.D.

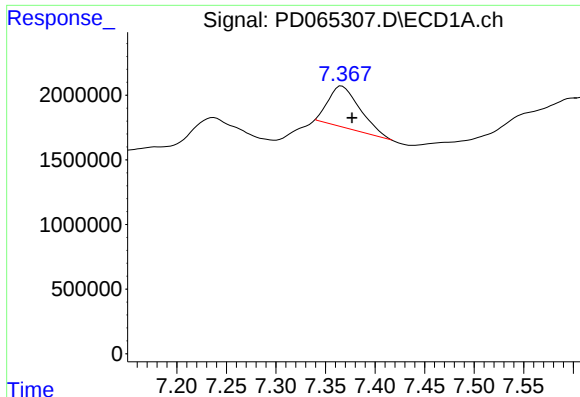

#22 Mirex


R.T.: 7.367 min
Delta R.T.: -0.010 min
Response: 6869822
Conc: 1.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

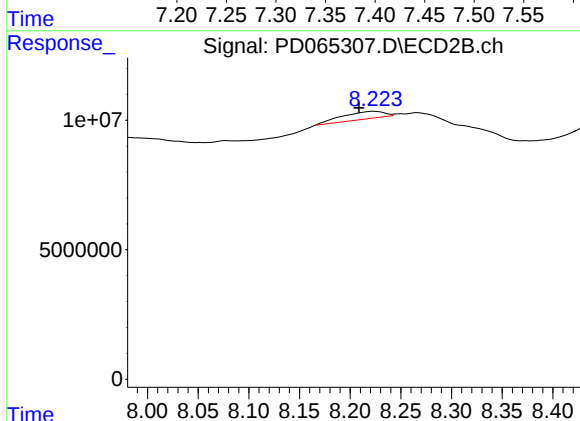


#22 Mirex

R.T.: 8.224 min
Delta R.T.: 0.015 min
Response: 8373954
Conc: 2.03 ng/ml

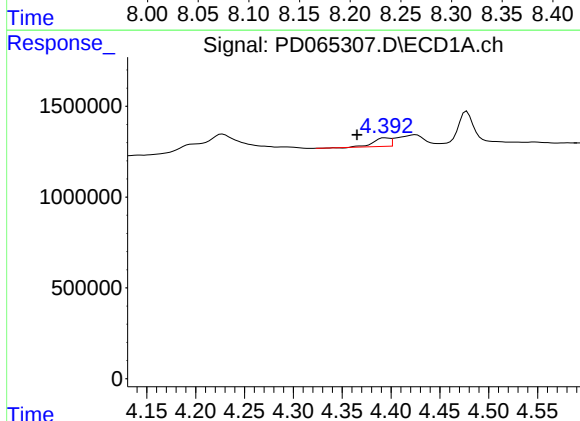


#23 Chlordane-1

R.T.: 4.394 min
Delta R.T.: 0.029 min
Response: 532349
Conc: 13.56 ng/ml

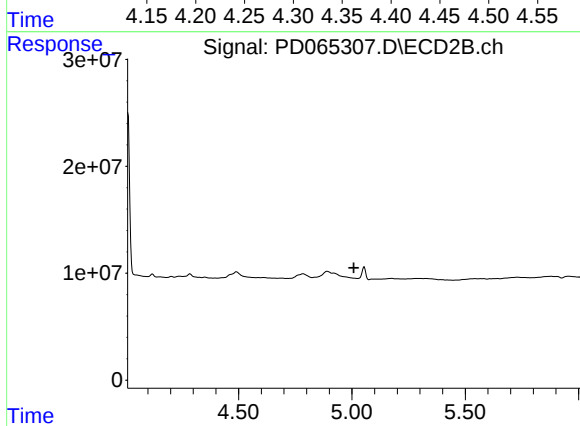

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.009 min
Response: 0
Conc: N.D.

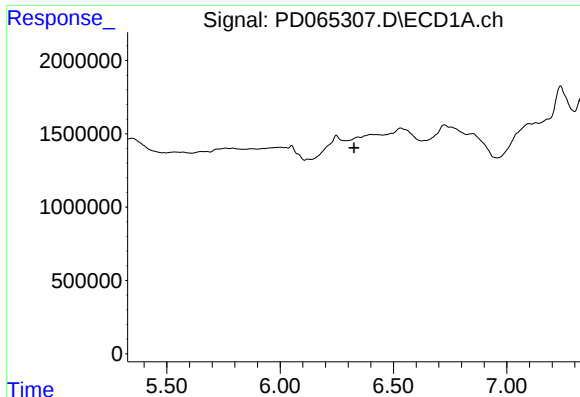

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.326 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

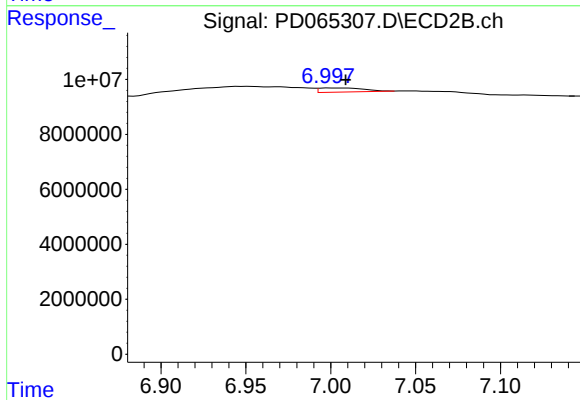


#27 Chlordane-5

R.T.: 7.000 min
Delta R.T.: -0.009 min
Response: 2710068
Conc: 13.31 ng/ml

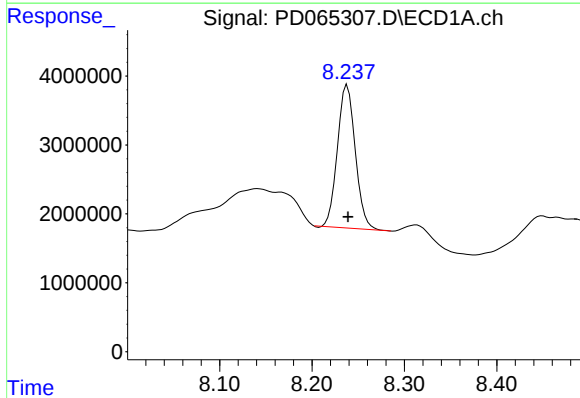

#28 Decachlorobiphenyl

R.T.: 8.238 min
Delta R.T.: 0.000 min
Response: 27849061
Conc: 20.52 ng/ml

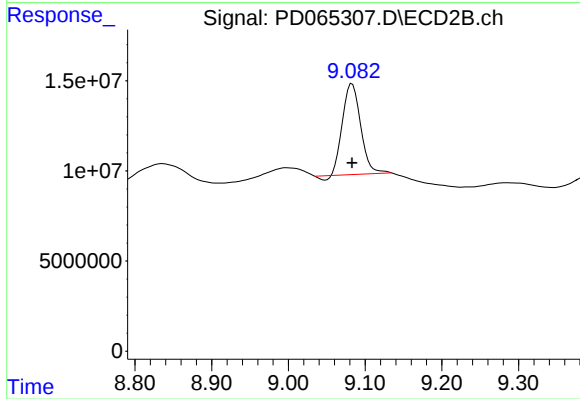

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: 0.000 min
Response: 82660357
Conc: 19.09 ng/ml