

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082521\
 Data File : PD065292.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Aug 2021 00:06
 Operator : AR\AJ
 Sample : PTOXICV500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD082521TOX

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 05:56:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX082521.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 25 05:53:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.496	4.013	51481555	335.5E6	48.032	48.750
7) SA Decachlor...	8.240	9.083	64598475	214.2E6	47.328	47.725
Target Compounds						
2) Toxaphene-1	5.748	6.406	4789573	15802450	492.007	515.634
3) Toxaphene-2	5.910	6.599	5064876	25857366	496.244	464.087
4) Toxaphene-3	6.351	7.182	11071620	45915685	483.693	470.029
5) Toxaphene-4	6.596	7.268	12133996	46936987	483.008	485.690
6) Toxaphene-5	7.083	7.686	13934872	36797898	480.186	474.894

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082521\
Data File : PD065292.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Aug 2021 00:06
Operator : AR\AJ
Sample : PTOXICV500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 05:56:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX082521.M
Quant Title : GC Extractables
QLast Update : Wed Aug 25 05:53:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

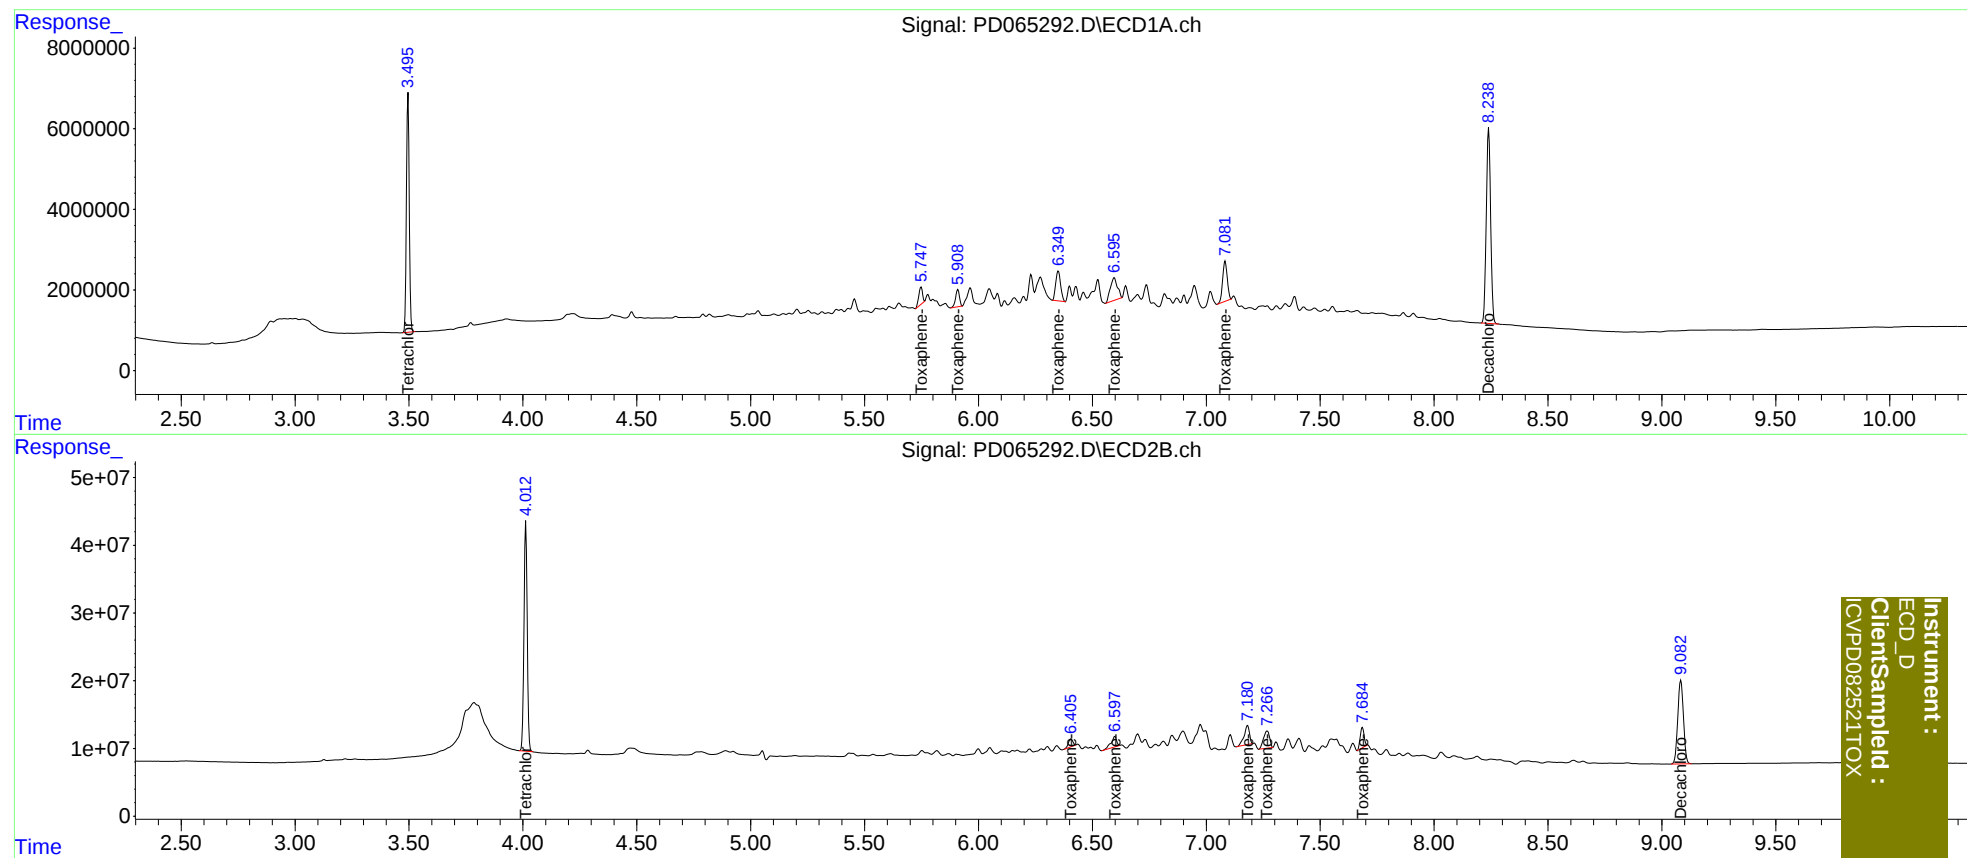

Instrument :
ECD_D
Client Sample :
ICV/PD082521TOX