

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082521\
 Data File : PD065281.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2021 21:35
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 05:30:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082521.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 25 05:29:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	91363019	491.7E6	72.483	71.649
28)	SA Decachlor...	8.239	9.084	92468904	308.4E6	69.734	70.166
Target Compounds							
23)	Chlordane-1	4.366	5.009	27715221	182.8E6	721.805	705.027
24)	Chlordane-2	4.866	5.479	32046338	168.3E6	695.820	697.688
25)	Chlordane-3	5.433	6.126	85050952	625.0E6	719.994	716.685
26)	Chlordane-4	5.490	6.199	70431909	721.6E6	711.191	711.107
27)	Chlordane-5	6.327	7.009	34604336	149.9E6	714.936	710.249



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082521\
Data File : PD065281.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2021 21:35
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 05:30:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082521.M
Quant Title : GC Extractables
QLast Update : Wed Aug 25 05:29:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

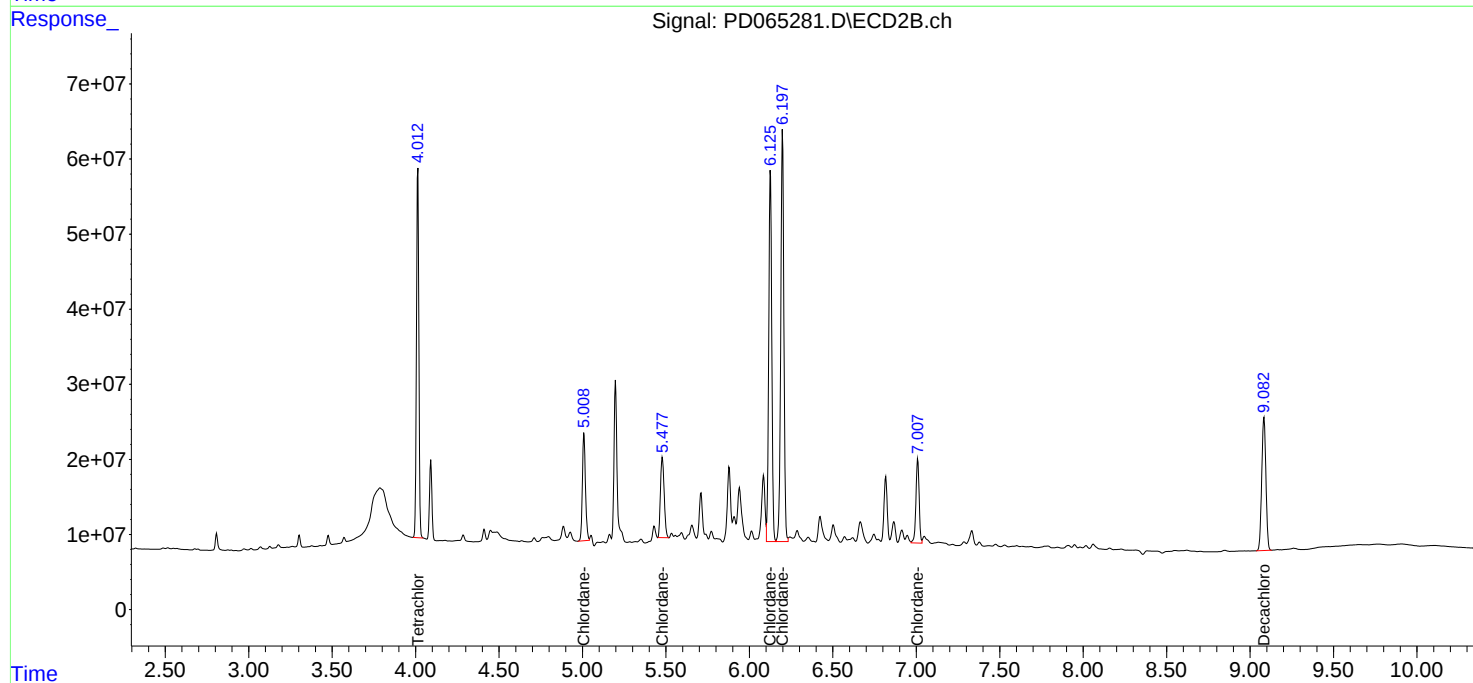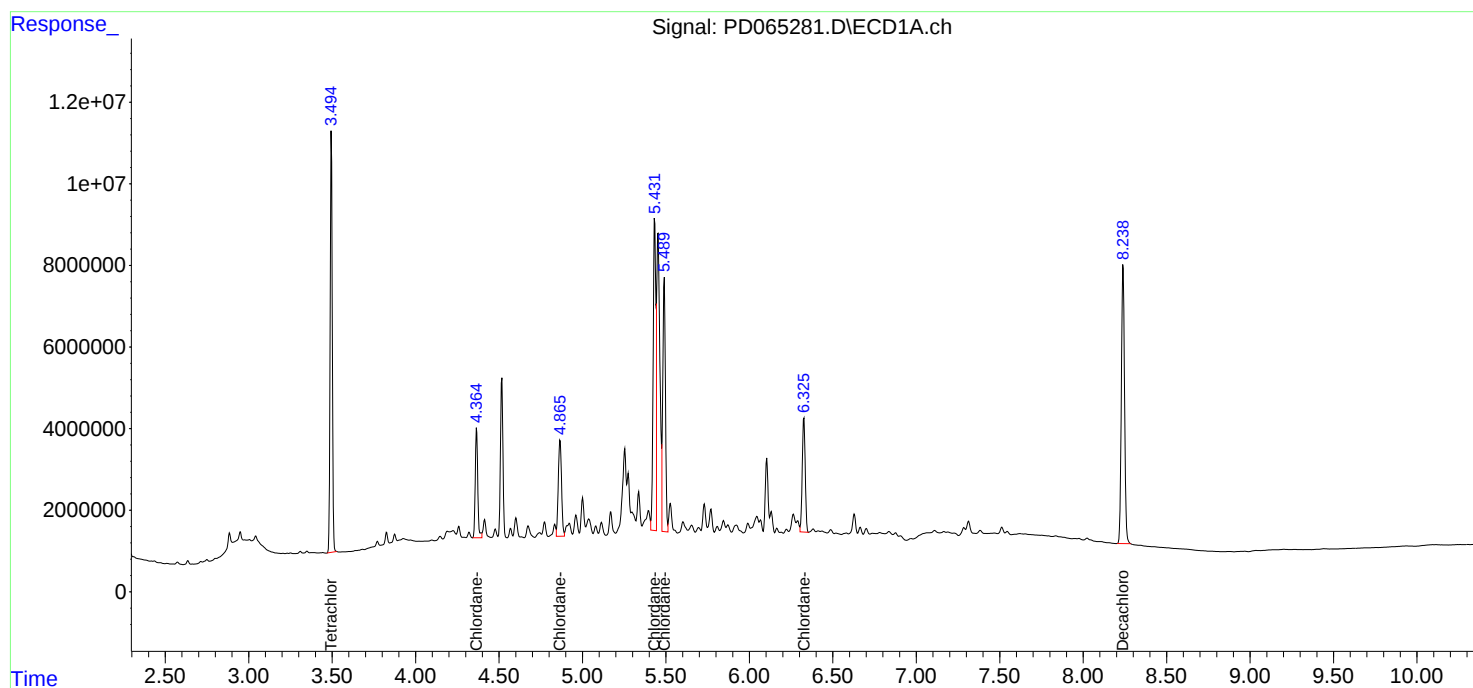


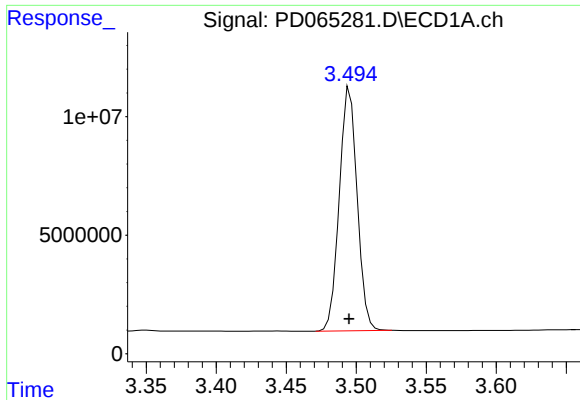

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 91363019
Conc: 72.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

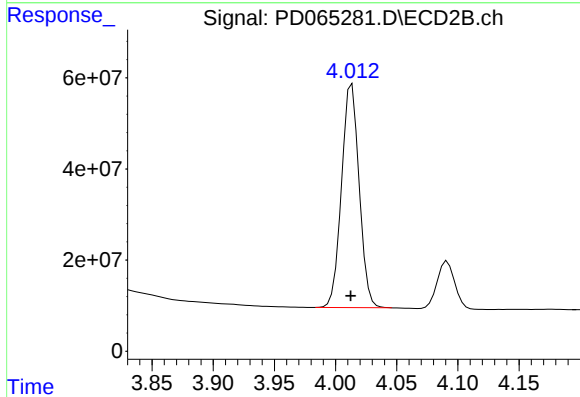


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 491737621
Conc: 71.65 ng/ml

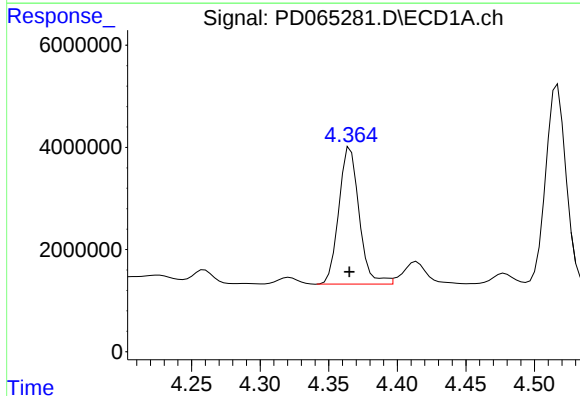


#23 Chlordane-1

R.T.: 4.366 min
Delta R.T.: 0.000 min
Response: 27715221
Conc: 721.81 ng/ml

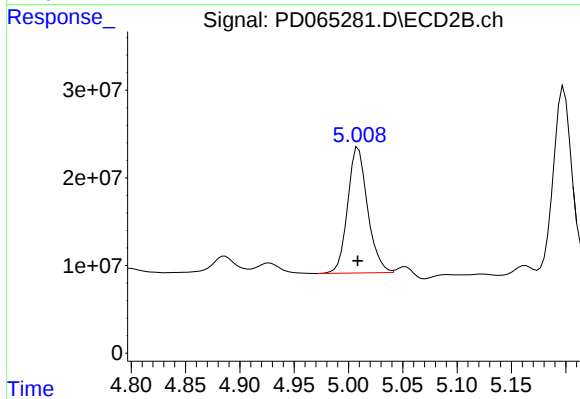

#23 Chlordane-1


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 182835571
Conc: 705.03 ng/ml

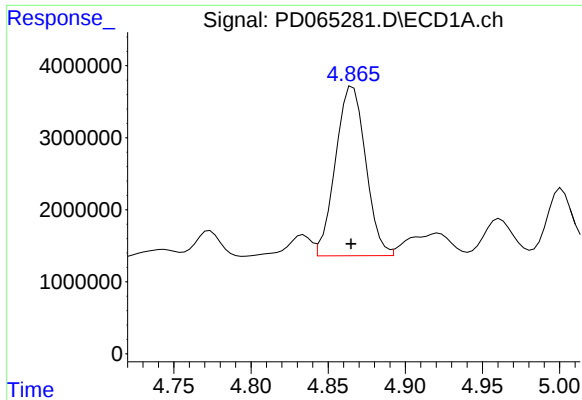

#24 Chlordane-2


R.T.: 4.866 min
Delta R.T.: 0.001 min
Response: 32046338
Conc: 695.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

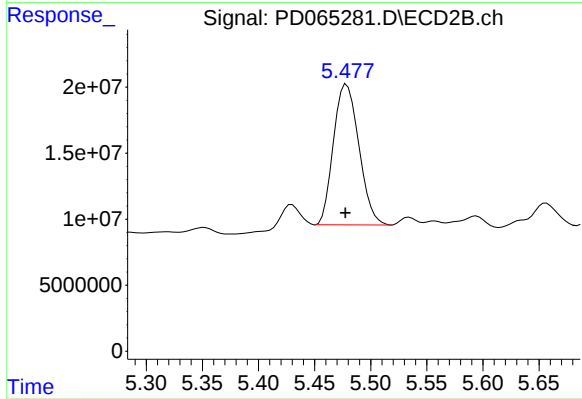


#24 Chlordane-2

R.T.: 5.479 min
Delta R.T.: 0.001 min
Response: 168253173
Conc: 697.69 ng/ml

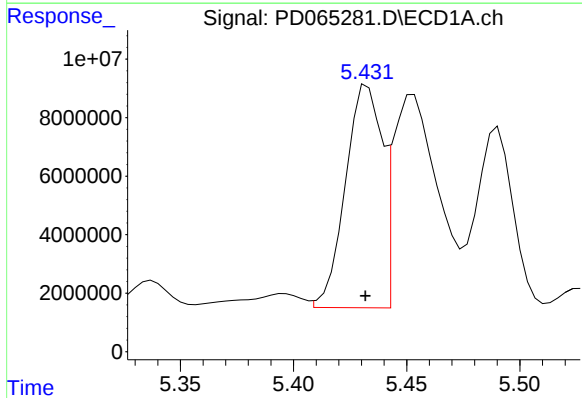


#25 Chlordane-3

R.T.: 5.433 min
Delta R.T.: 0.001 min
Response: 85050952
Conc: 719.99 ng/ml

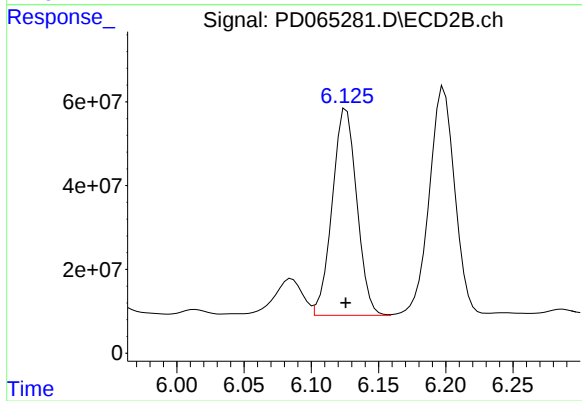

#25 Chlordane-3


R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 624975395
Conc: 716.69 ng/ml

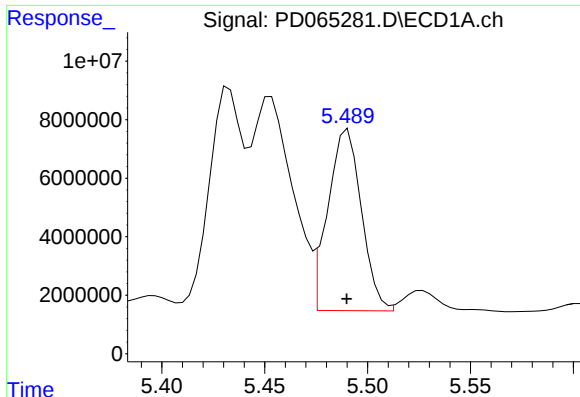

#26 Chlordane-4


R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 70431909
Conc: 711.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

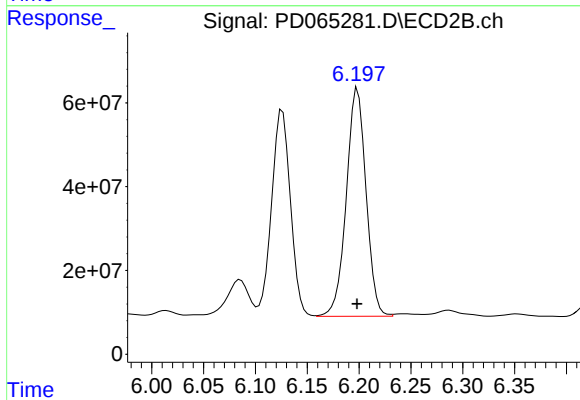


#26 Chlordane-4

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 721570650
Conc: 711.11 ng/ml

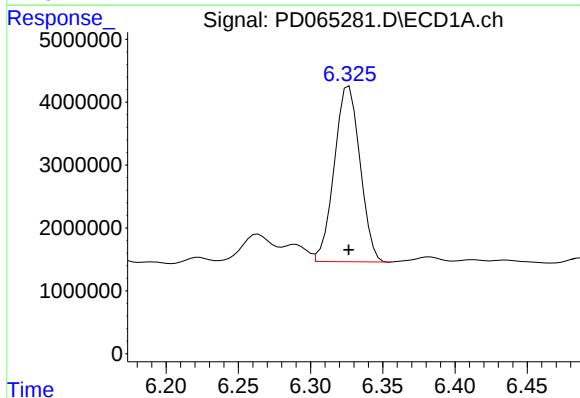


#27 Chlordane-5

R.T.: 6.327 min
Delta R.T.: 0.000 min
Response: 34604336
Conc: 714.94 ng/ml

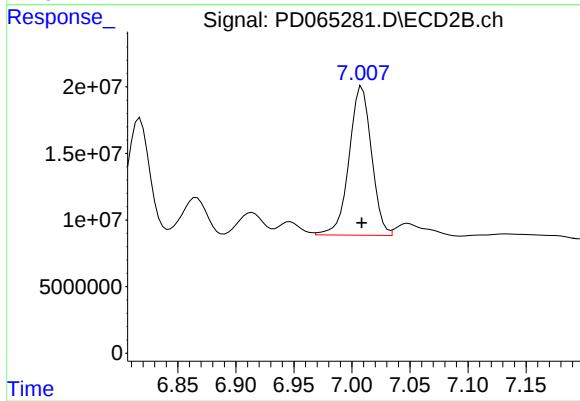

#27 Chlordane-5


R.T.: 7.009 min
Delta R.T.: 0.000 min
Response: 149906931
Conc: 710.25 ng/ml

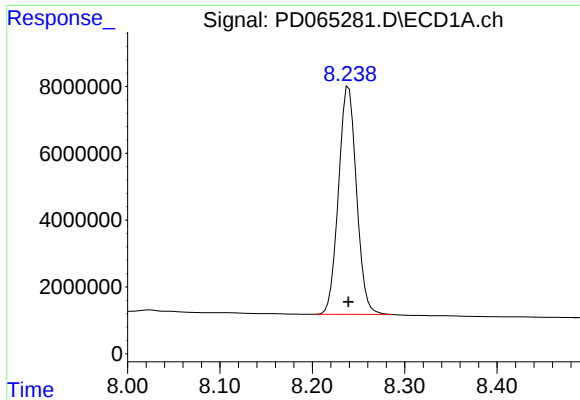

#28 Decachlorobiphenyl

R.T.: 8.239 min
Delta R.T.: 0.000 min
Response: 92468904
Conc: 69.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

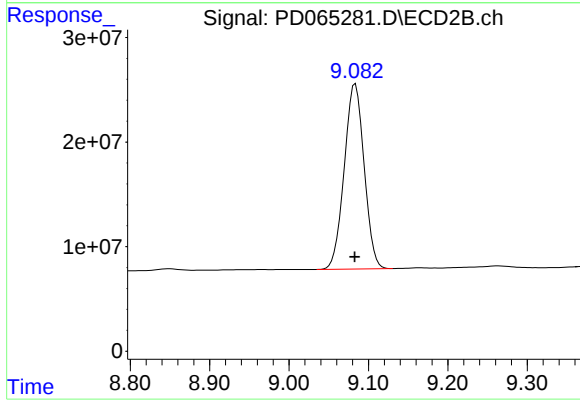

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 308402479
Conc: 70.17 ng/ml