

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD082522\  
 Data File : PD071658.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 25 Aug 2022 16:28  
 Operator : AR\AJ  
 Sample : N4181-04  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 X3C29

Manual Integrations  
 APPROVED

Reviewed By : Abdul Mirza 08/26/2022  
 Supervised By : Ankita Jodhani 08/26/2022

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Aug 26 06:47:44 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD081122CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Aug 11 04:21:34 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml    |
|-----------------------------|-----------------|-------|-------|----------|----------|---------|----------|
| -----                       |                 |       |       |          |          |         |          |
| System Monitoring Compounds |                 |       |       |          |          |         |          |
| 1)                          | SA Tetrachlo... | 2.806 | 3.563 | 59342513 | 868.6E6  | 20.803  | 26.500 # |
| 27)                         | SA Decachlor... | 7.999 | 9.090 | 115.6E6  | 428.0E6  | 41.186  | 44.649   |
| Target Compounds            |                 |       |       |          |          |         |          |
| 2)                          | A alpha-BHC     | 3.316 | 4.030 | 282.0E6  | 2872.7E6 | 68.548  | 68.017   |
| 7)                          | B delta-BHC     | 4.181 | 4.820 | 141.1E6  | 1042.9E6 | 35.539  | 37.188   |
| 11)                         | B cis-Chlor...  | 5.103 | 6.049 | 74046466 | 371.6E6  | 19.017m | 20.802   |
| 12)                         | B 4,4'-DDE      | 5.295 | 6.222 | 99882061 | 487.8E6  | 28.102  | 30.992   |
| 13)                         | MA Dieldrin     | 5.427 | 6.382 | 172.3E6  | 793.7E6  | 45.425  | 47.911   |
| 15)                         | B Endosulfa...  | 5.999 | 6.840 | 3834189  | 21863273 | 1.229   | 1.672 #  |
| 17)                         | MA 4,4'-DDT     | 6.107 | 7.058 | 258.0E6  | 1066.3E6 | 91.313  | 90.133   |
| 18)                         | B Endrin al...  | 6.181 | 6.971 | 128.0E6  | 561.7E6  | 47.728  | 51.087   |
| 21)                         | B Endrin ke...  | 6.915 | 7.696 | 268.0E6  | 1036.0E6 | 78.408  | 78.941   |
| -----                       |                 |       |       |          |          |         |          |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD082522\  
Data File : PD071658.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 25 Aug 2022 16:28  
Operator : AR\AJ  
Sample : N4181-04  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Aug 26 06:47:44 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD081122CLP.M  
Quant Title : GC Extractables  
QLast Update : Thu Aug 11 04:21:34 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

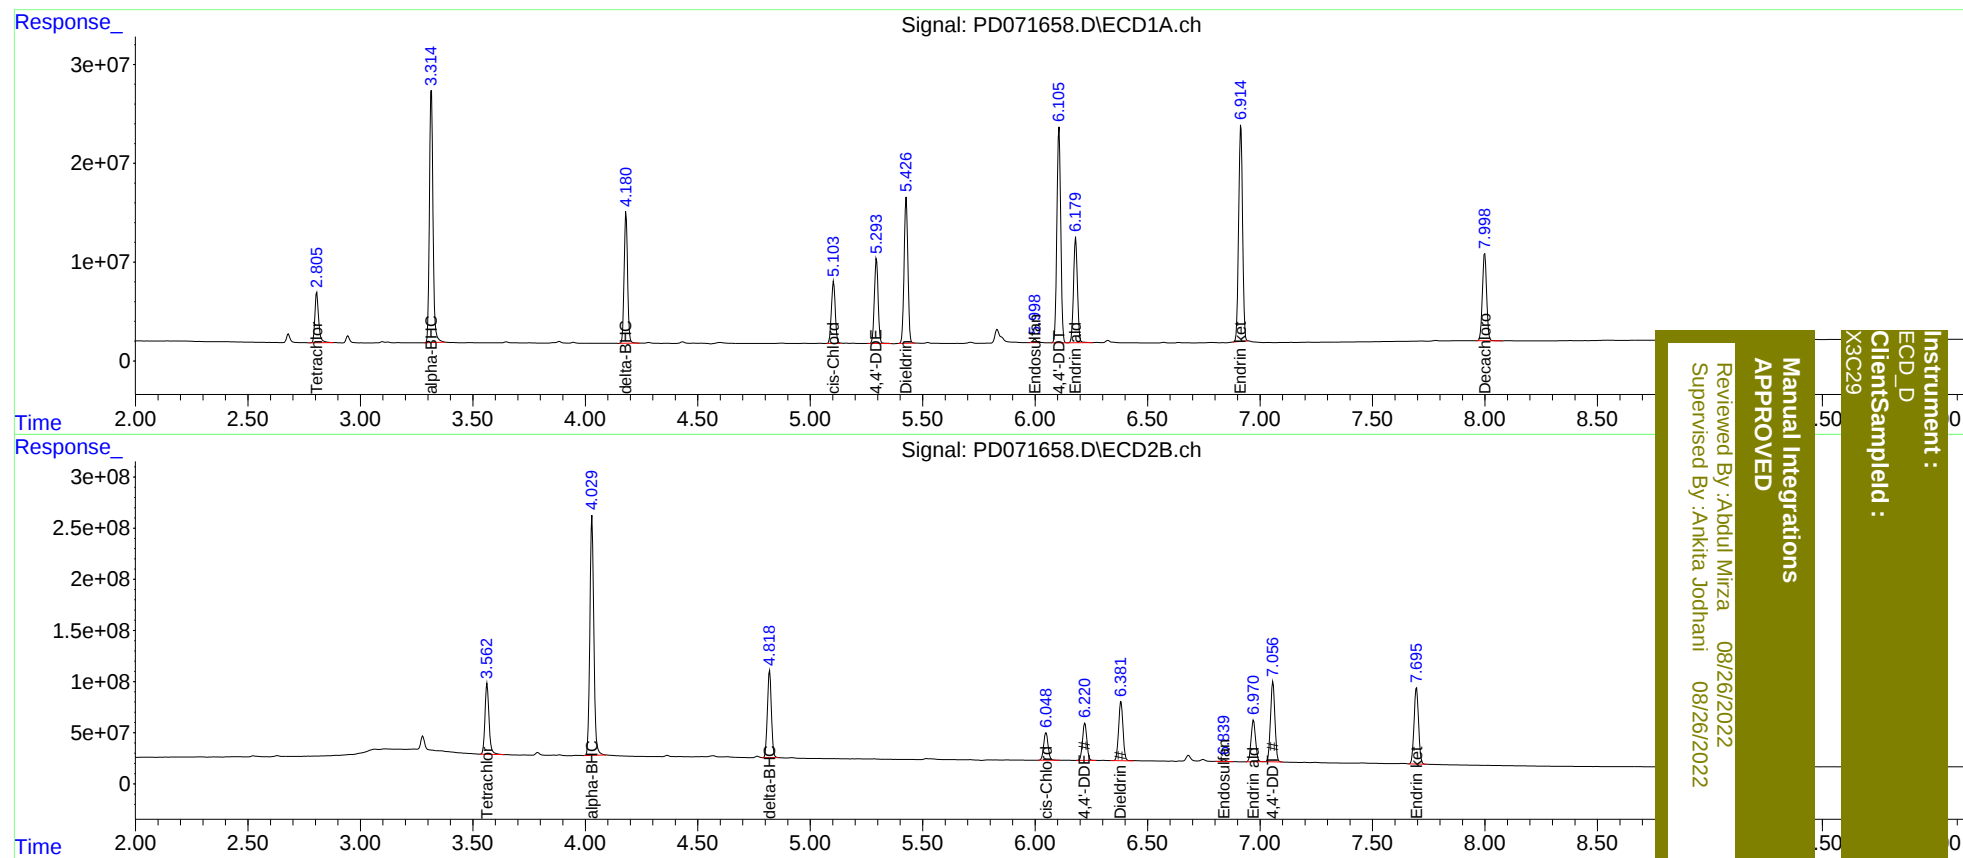

Reviewed By: Abdul Mirza 08/26/2022  
Supervised By: Ankita Jodhani 08/26/2022

Manual Integrations  
APPROVED

Instrument :  
ECD\_D  
Client Sampled :  
X3C29