

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082524\
 Data File : PD084654.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 00:47
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 05:29:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 23 05:28:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.906	5025822	17572733	4.960	4.961
27)	SA Decachlor...	9.031	8.107	13141307	35695070	10.019	10.171
Target Compounds							
2)	A alpha-BHC	3.982	3.417	7165694	23906233	4.304	4.683
3)	MA gamma-BHC...	4.311	3.752	6915270	23402156	4.347	4.811
4)	MA Heptachlor	4.909	4.107	6923303	20624212	4.582	4.805
9)	A Endosulfan I	6.052	5.273	6441718	18961487	4.692	4.889
13)	MA Dieldrin	6.323	5.540	12812698	41948721	8.759	9.674
14)	MA Endrin	6.550	5.818	11082439	36175990	10.133	9.704
16)	A 4,4'-DDD	6.681	5.958	8568969	33298001	8.759	9.725
17)	MA 4,4'-DDT	6.996	6.214	7199960	29708614	8.128	9.191
20)	A Methoxychlor	7.467	6.785	22974377	85801601	43.765	50.880


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082524\
Data File : PD084654.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 00:47
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 05:29:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Aug 23 05:28:46 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

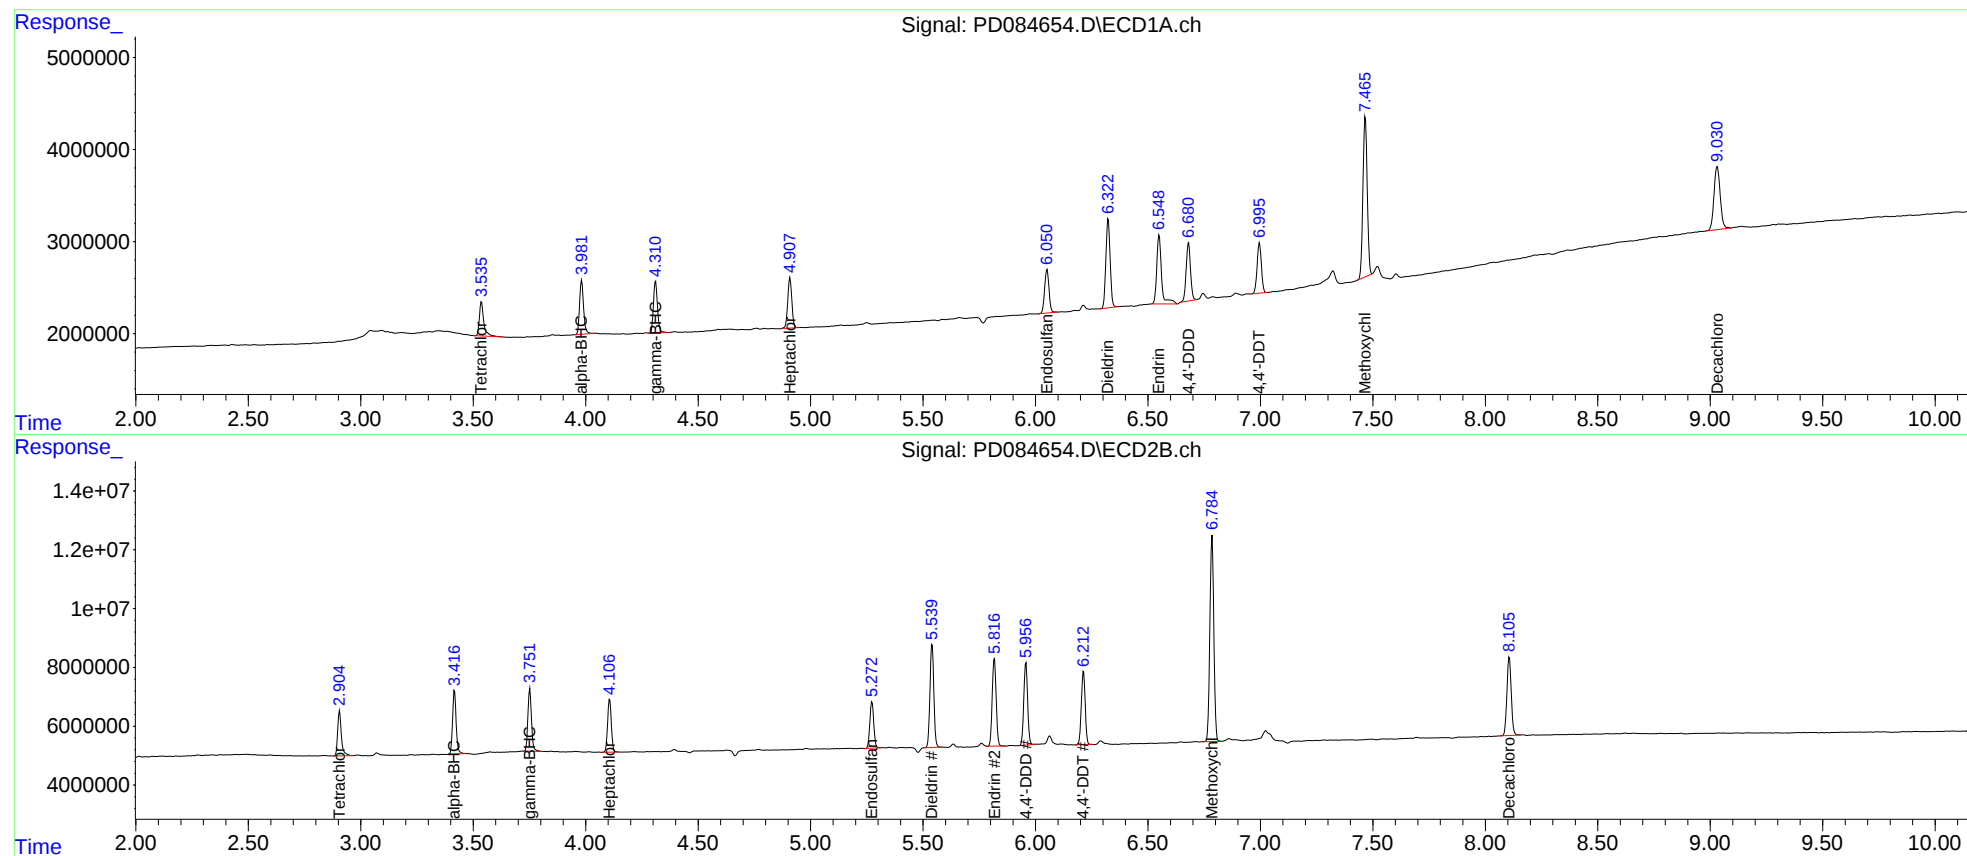

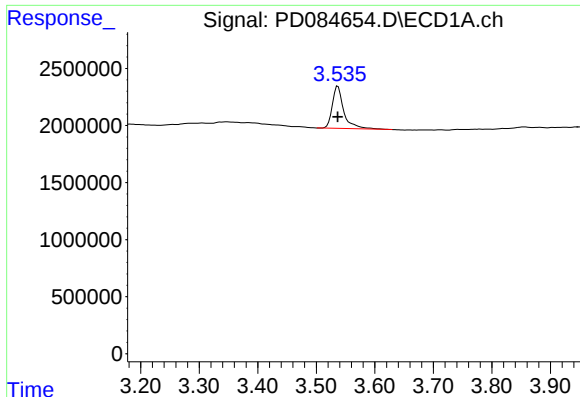


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 5025822
Conc: 4.96 ng/ml

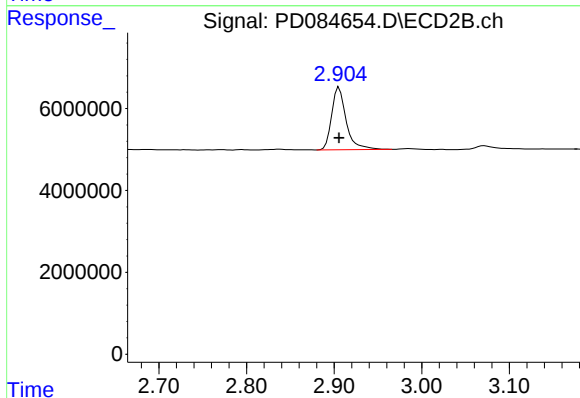


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: 0.000 min
Response: 17572733
Conc: 4.96 ng/ml

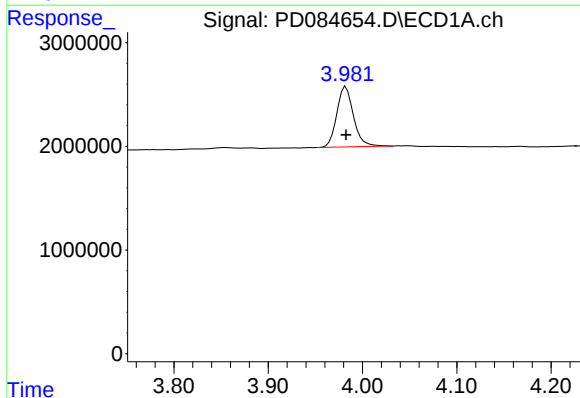


#2 alpha-BHC

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 7165694
Conc: 4.30 ng/ml

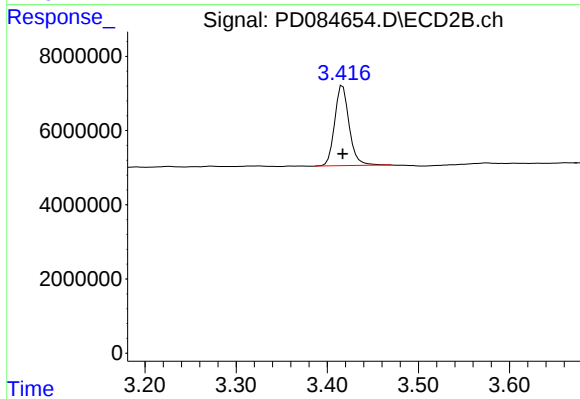


#2 alpha-BHC

R.T.: 3.417 min
Delta R.T.: 0.000 min
Response: 23906233
Conc: 4.68 ng/ml

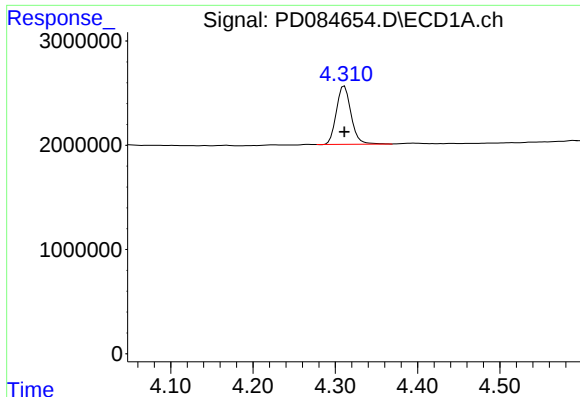


#3 gamma-BHC (Lindane)

R.T.: 4.311 min
Delta R.T.: 0.000 min
Response: 6915270
Conc: 4.35 ng/ml

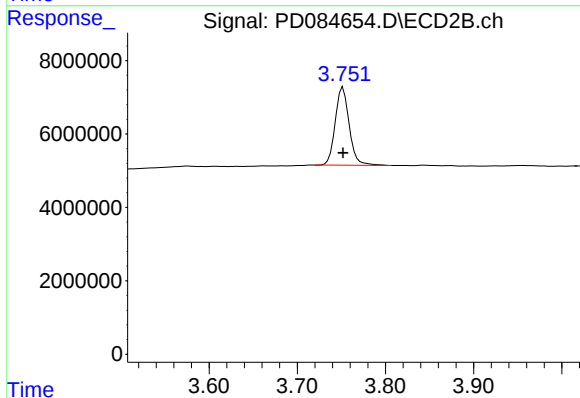


#3 gamma-BHC (Lindane)

R.T.: 3.752 min
Delta R.T.: 0.000 min
Response: 23402156
Conc: 4.81 ng/ml

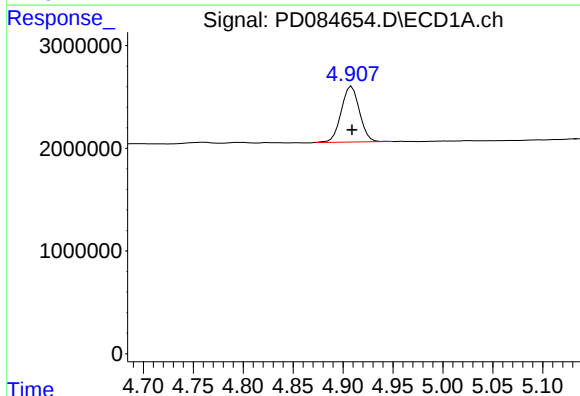


#4 Heptachlor

R.T.: 4.909 min
Delta R.T.: 0.000 min
Response: 6923303
Conc: 4.58 ng/ml

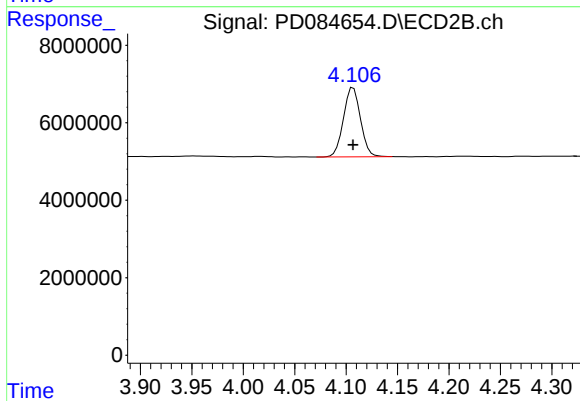


#4 Heptachlor

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 20624212
Conc: 4.81 ng/ml

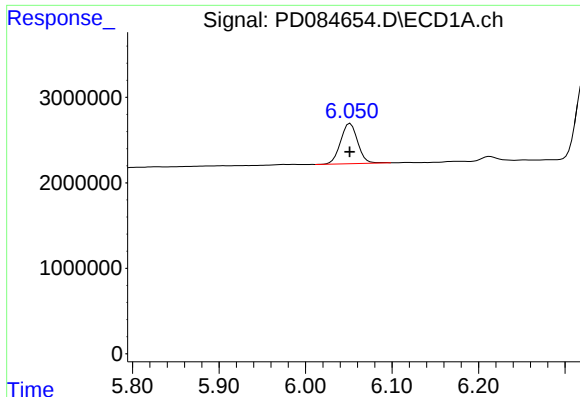


#9 Endosulfan I

R.T.: 6.052 min
Delta R.T.: 0.000 min
Response: 6441718
Conc: 4.69 ng/ml

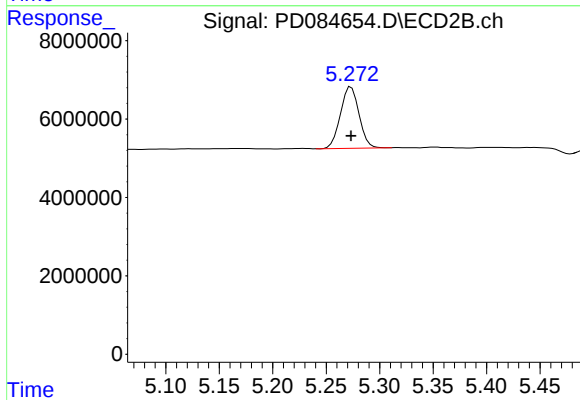


#9 Endosulfan I

R.T.: 5.273 min
Delta R.T.: 0.000 min
Response: 18961487
Conc: 4.89 ng/ml

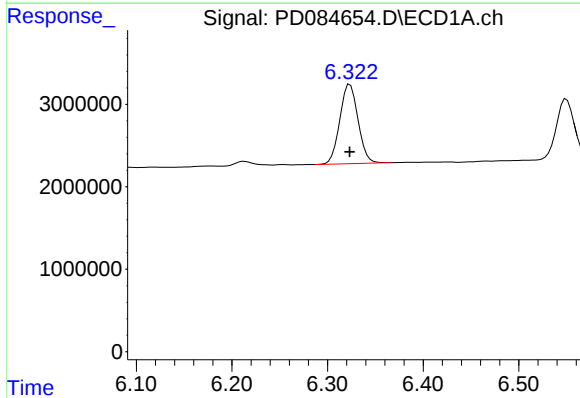


#13 Dieldrin

R.T.: 6.323 min
Delta R.T.: 0.000 min
Response: 12812698
Conc: 8.76 ng/ml

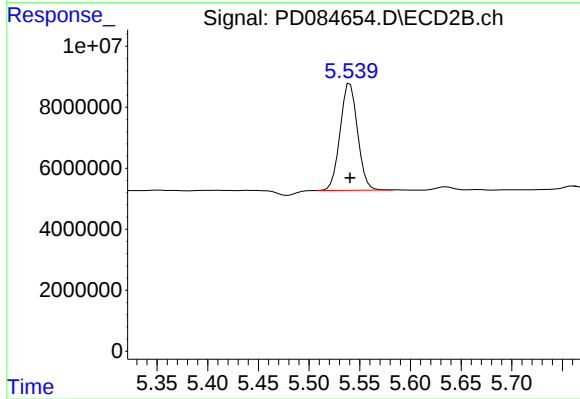


#13 Dieldrin

R.T.: 5.540 min
Delta R.T.: 0.000 min
Response: 41948721
Conc: 9.67 ng/ml

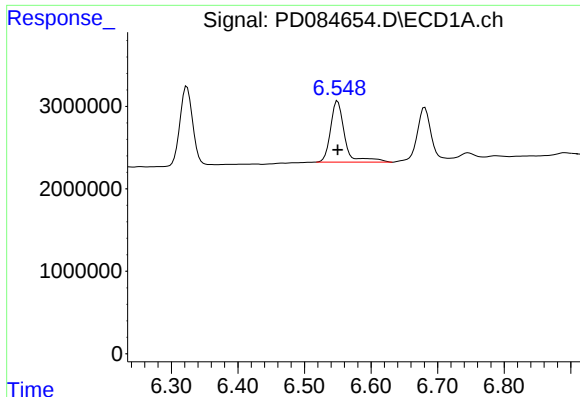


#14 Endrin

R.T.: 6.550 min
Delta R.T.: 0.000 min
Response: 11082439
Conc: 10.13 ng/ml

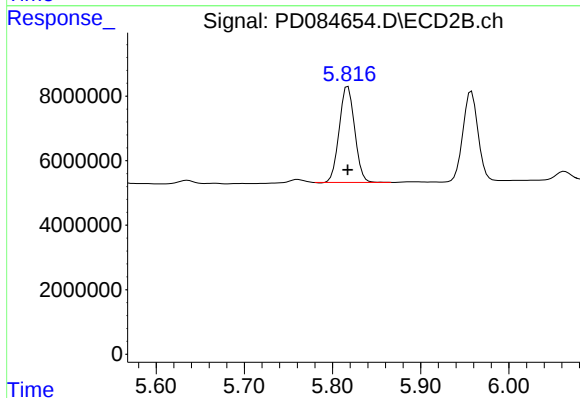


#14 Endrin

R.T.: 5.818 min
Delta R.T.: 0.000 min
Response: 36175990
Conc: 9.70 ng/ml

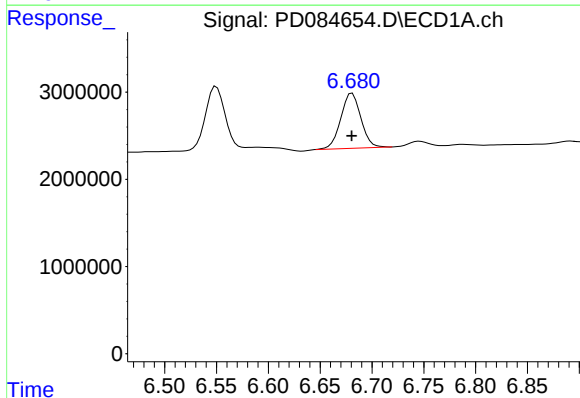


#16 4,4'-DDD

R.T.: 6.681 min
Delta R.T.: 0.000 min
Response: 8568969
Conc: 8.76 ng/ml

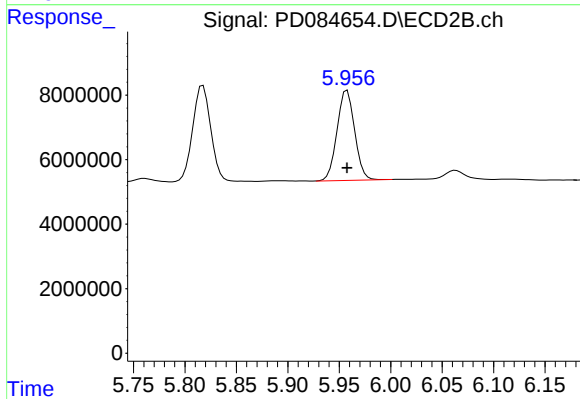


#16 4,4'-DDD

R.T.: 5.958 min
Delta R.T.: 0.000 min
Response: 33298001
Conc: 9.72 ng/ml

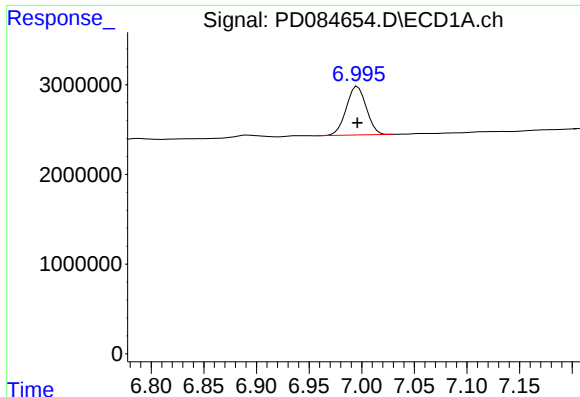


#17 4,4'-DDT

R.T.: 6.996 min
Delta R.T.: 0.000 min
Response: 7199960
Conc: 8.13 ng/ml

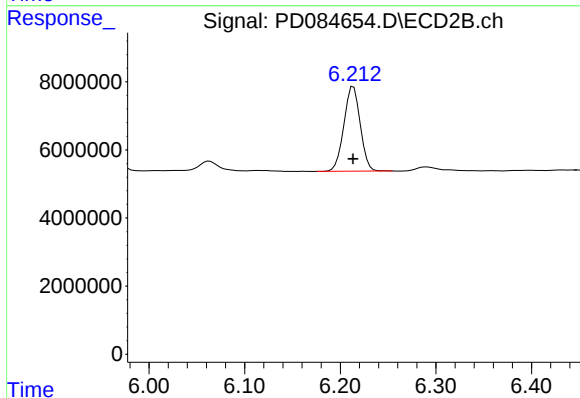


#17 4,4'-DDT

R.T.: 6.214 min
Delta R.T.: 0.000 min
Response: 29708614
Conc: 9.19 ng/ml

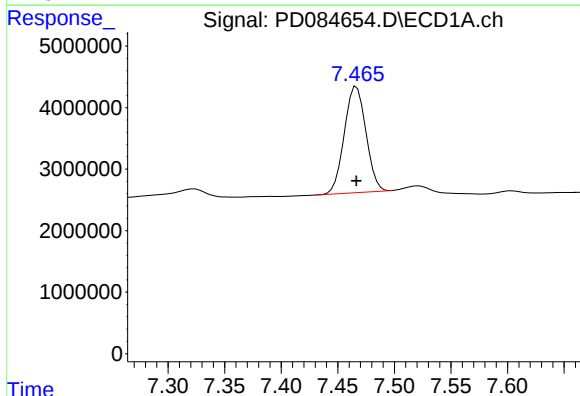


#20 Methoxychlor

R.T.: 7.467 min
Delta R.T.: 0.000 min
Response: 22974377
Conc: 43.76 ng/ml

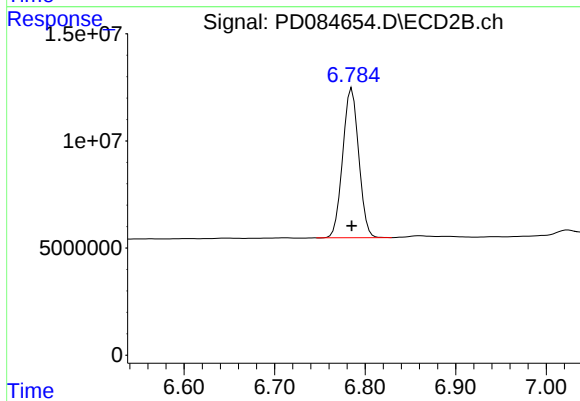


#20 Methoxychlor

R.T.: 6.785 min
Delta R.T.: 0.000 min
Response: 85801601
Conc: 50.88 ng/ml

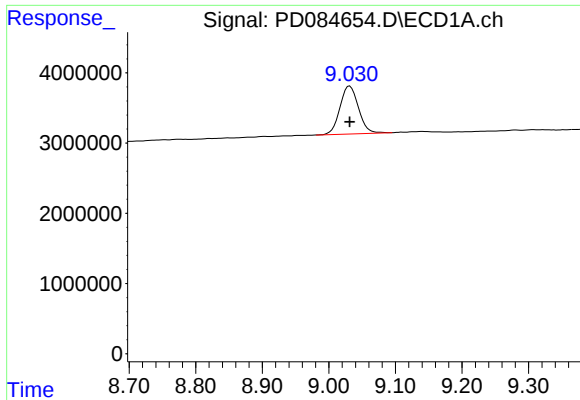

#27 Decachlorobiphenyl

R.T.: 9.031 min
Delta R.T.: 0.000 min
Response: 13141307
Conc: 10.02 ng/ml

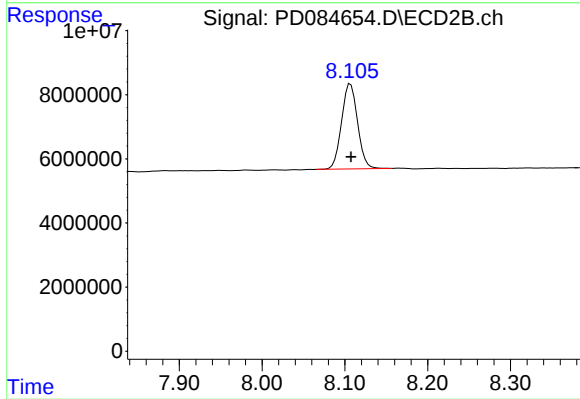

#27 Decachlorobiphenyl

R.T.: 8.107 min
Delta R.T.: 0.000 min
Response: 35695070
Conc: 10.17 ng/ml